

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
 Data File : BN032799.D
 Acq On : 18 Jul 2024 03:31
 Operator : MA/JU
 Sample : P3217-02
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YDZC4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 18 04:24:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 17 02:35:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.536	152	4775	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.305	136	14312	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.188	164	10560	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.953	188	16806m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.168	240	15825m	0.400	ng/ul	0.00
23) Perylene-d12	23.363	264	16604m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	23503	4.099	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.905	152	7528	0.348	ng/ul	-0.03
18) Fluoranthene-d10	18.994	212	15173m	0.294	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.131	88	1778	0.272	ng/ul#	31

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032799.D
Acq On : 18 Jul 2024 03:31
Operator : MA/JU
Sample : P3217-02
Misc :
ALS Vial : 71 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YDZC4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024


Quant Time: Jul 18 04:24:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

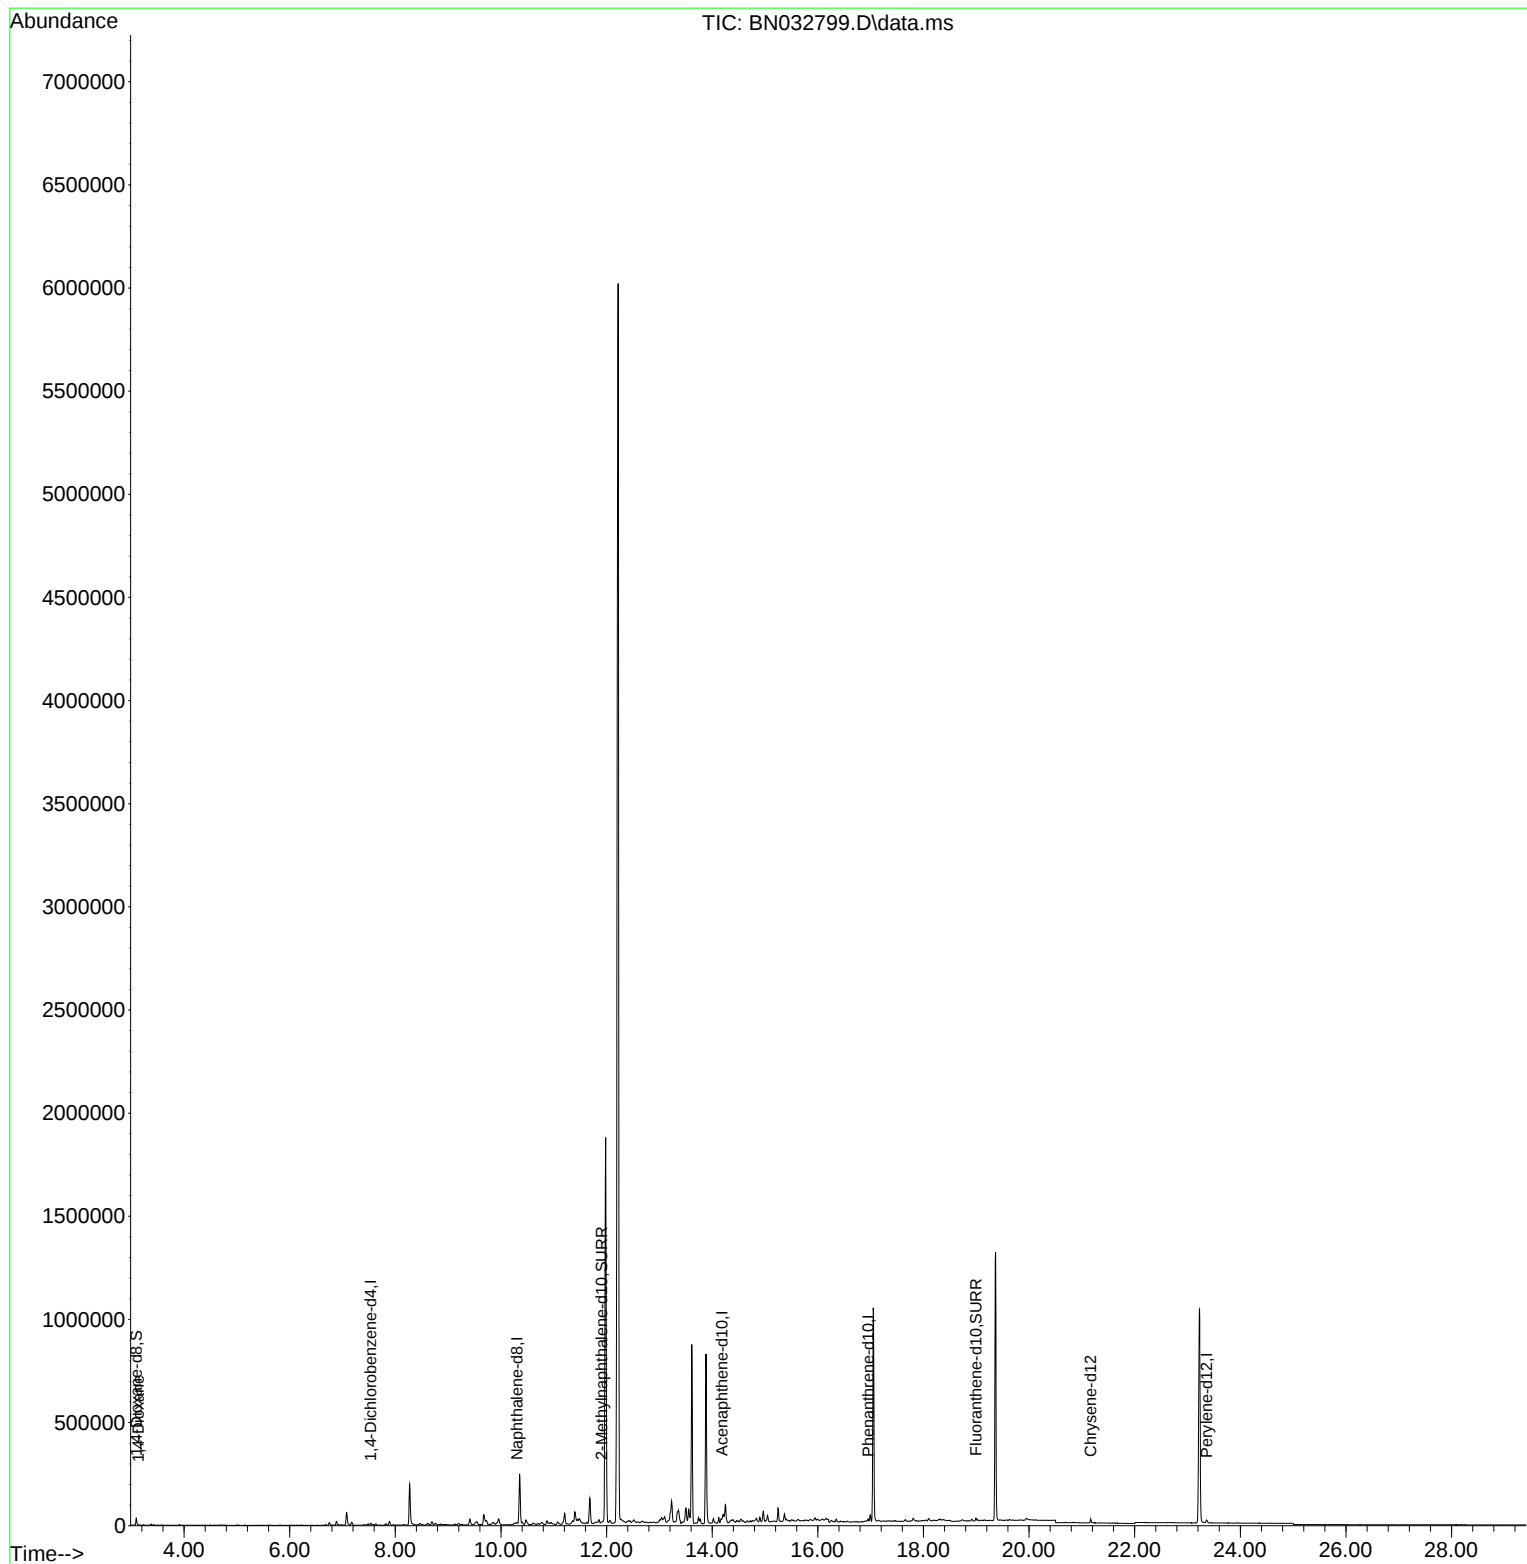

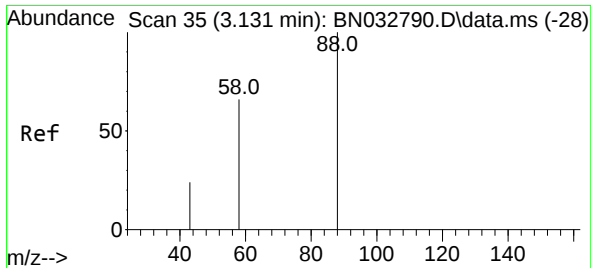

#2
 1,4-Dioxane
 Concen: 0.272 ng/ul
 RT: 3.131 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN032799.D
 Acq: 18 Jul 2024 03:31

Instrument :
 BNA_N
 ClientSampleId :
 YDZC4

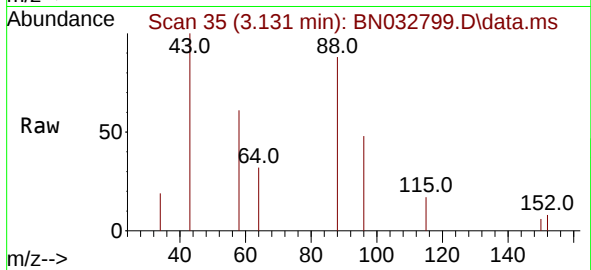

Tgt Ion: 88 Resp: 1778

Ion	Ratio	Lower	Upper
88	100		
43	113.7	24.0	36.0
58	69.9	43.3	64.9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

