

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
 Data File : BN032803.D
 Acq On : 18 Jul 2024 05:56
 Operator : MA/JU
 Sample : P3237-07
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GD1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 18 06:20:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 17 02:35:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	3563	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.310	136	10685	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.188	164	6368	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.953	188	11869m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.173	240	10921m	0.400	ng/ul	0.00
23) Perylene-d12	23.362	264	11154m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	19689	4.602	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.916	152	4862	0.301	ng/ul	-0.02
18) Fluoranthene-d10	18.994	212	10509	0.295	ng/ul	0.00
Target Compounds					Qvalue	
5) Naphthalene	10.360	128	1426	0.050	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032803.D
Acq On : 18 Jul 2024 05:56
Operator : MA/JU
Sample : P3237-07
Misc :
ALS Vial : 75 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GD1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024


Quant Time: Jul 18 06:20:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

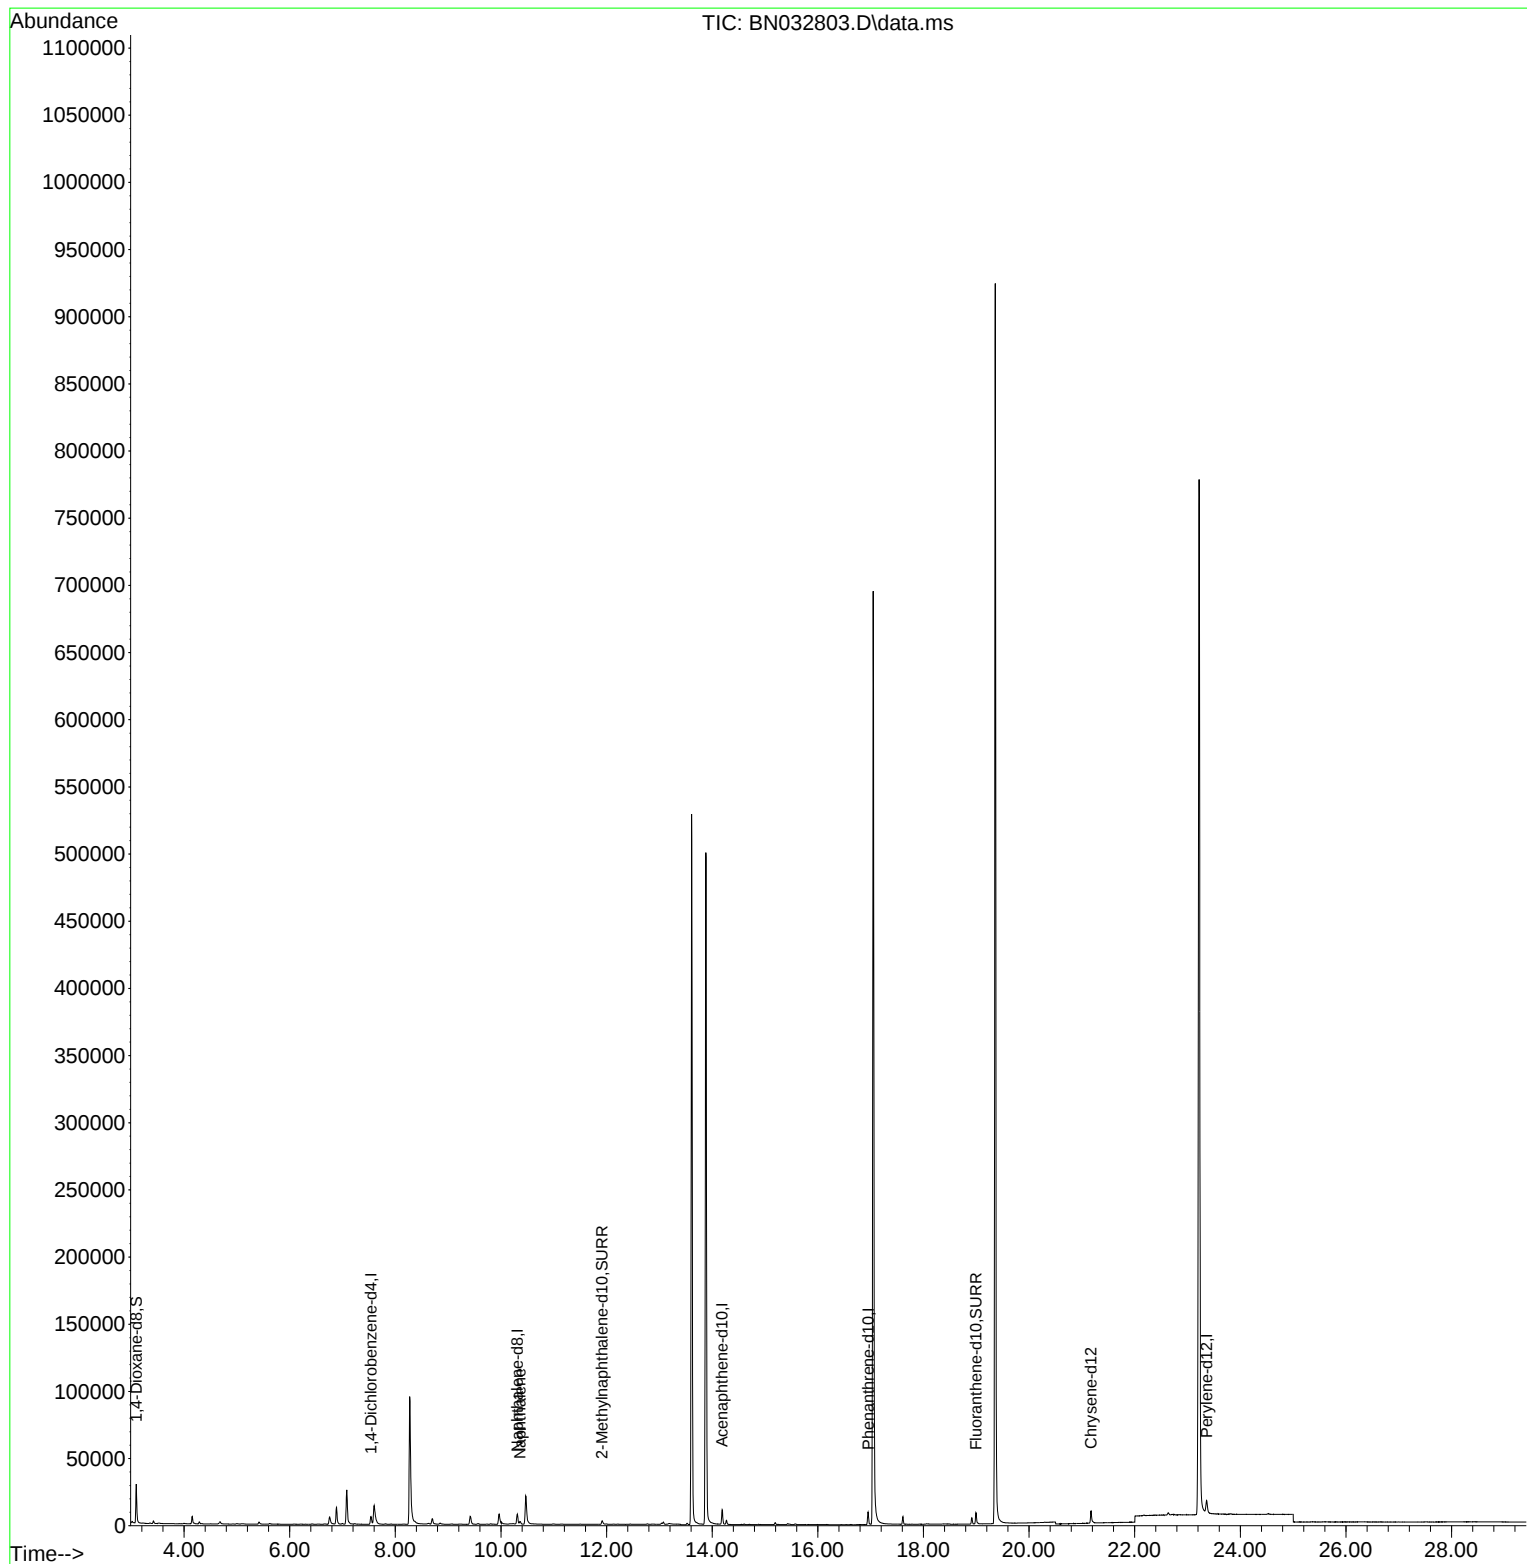

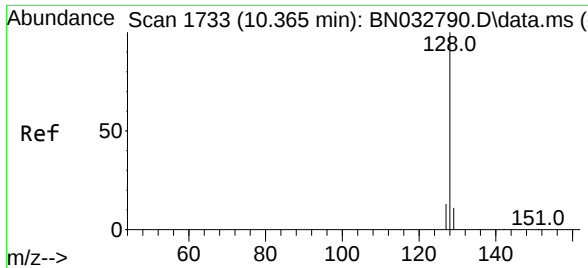

#5
Naphthalene
Concen: 0.050 ng/ul
RT: 10.360 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN032803.D
Acq: 18 Jul 2024 05:56

Instrument :
BNA_N
ClientSampleId :
E1GD1

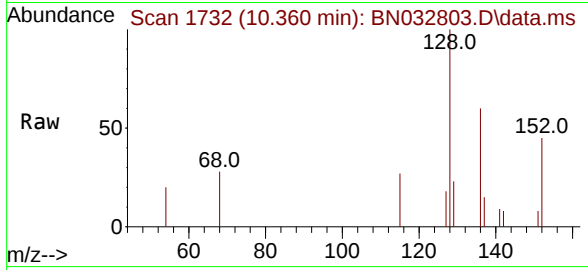

Tgt Ion:128 Resp: 1420

Ion	Ratio	Lower	Upper
128	100		
129	22.7	10.0	15.0
127	18.3	11.6	17.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

