

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
 Data File : BN032811.D
 Acq On : 18 Jul 2024 11:23
 Operator : MA/JU
 Sample : P3217-17
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YDZL4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 18 11:54:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 17 02:35:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.536	152	3926	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.305	136	11570	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.188	164	6421	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.948	188	11413m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.171	240	10378m	0.400	ng/ul	0.00
23) Perylene-d12	23.360	264	10332m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	19547	4.147	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.911	152	6240	0.357	ng/ul	-0.02
18) Fluoranthene-d10	18.994	212	11422	0.338	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.127	88	1577	0.294	ng/ul#	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032811.D
Acq On : 18 Jul 2024 11:23
Operator : MA/JU
Sample : P3217-17
Misc :
ALS Vial : 84 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
YDZL4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/18/2024
Supervised By :mohammad ahmed 07/19/2024


Quant Time: Jul 18 11:54:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

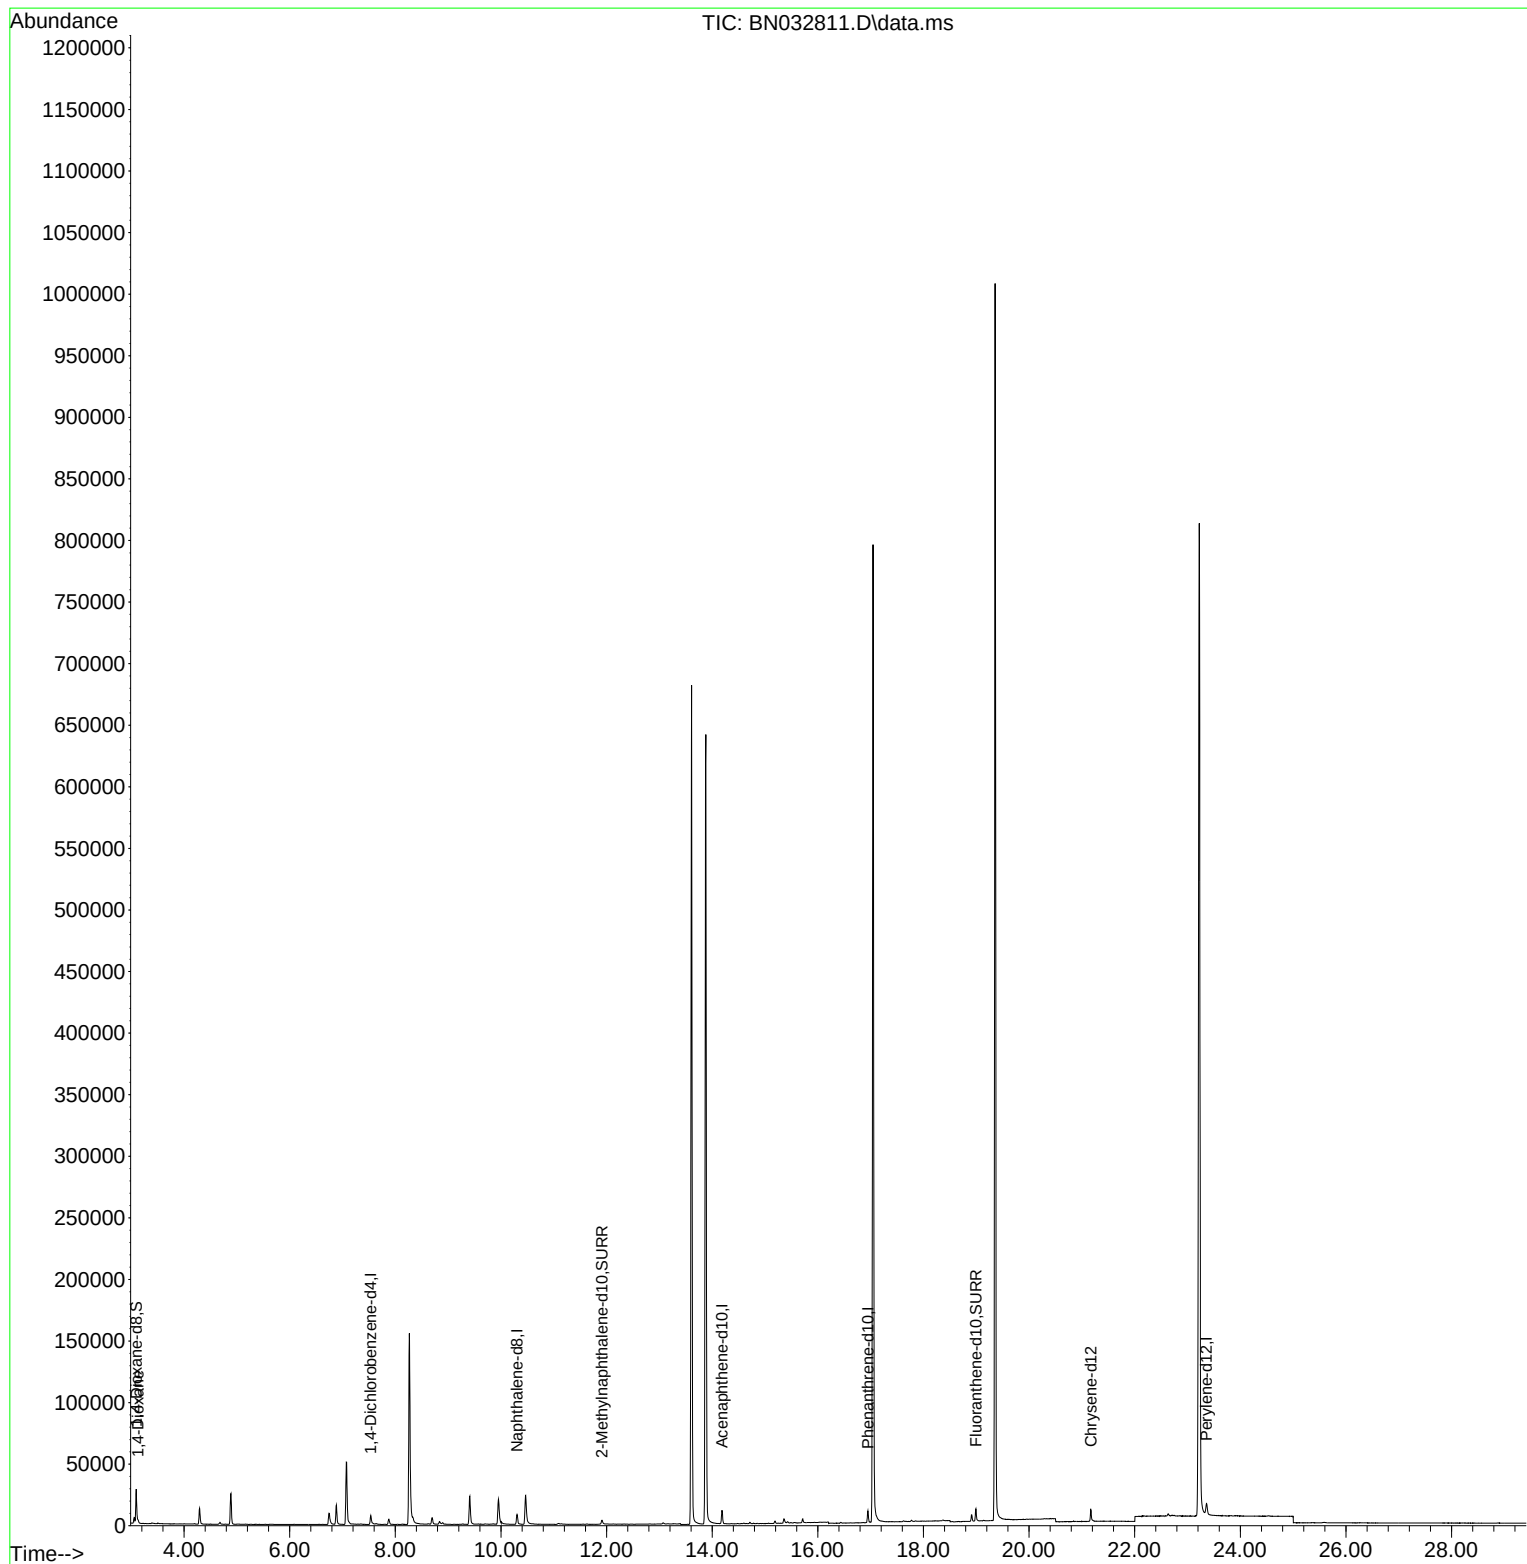

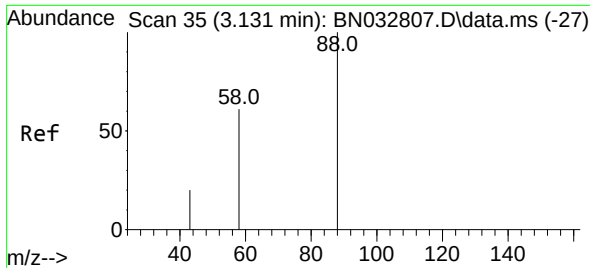

#2
 1,4-Dioxane
 Concen: 0.294 ng/ul
 RT: 3.127 min Scan# 34
 Delta R.T. -0.009 min
 Lab File: BN032811.D
 Acq: 18 Jul 2024 11:23

Instrument :
 BNA_N
 ClientSampleId :
 YDZL4

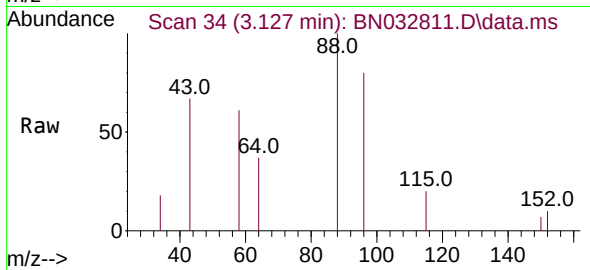

Tgt Ion: 88 Resp: 157
 Ion Ratio Lower Upper
 88 100
 43 67.1 24.0 36.0
 58 60.6 43.3 64.9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

