

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
 Data File : BN032815.D
 Acq On : 18 Jul 2024 13:47
 Operator : MA/JU
 Sample : P3237-03
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1GD0

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/18/2024
 Supervised By :mohammad ahmed 07/19/2024

Quant Time: Jul 18 14:15:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 17 02:35:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.536	152	3893	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.304	136	11509	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.187	164	6571	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.947	188	11641m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.175	240	10100m	0.400	ng/ul	0.00
23) Perylene-d12	23.361	264	10283m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	20790	4.448	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.915	152	6264	0.360	ng/ul	-0.02
18) Fluoranthene-d10	18.993	212	11722	0.356	ng/ul	-0.01
Target Compounds						
					Qvalue	
5) Naphthalene	10.353	128	1176	0.038	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071624\
Data File : BN032815.D
Acq On : 18 Jul 2024 13:47
Operator : MA/JU
Sample : P3237-03
Misc :
ALS Vial : 88 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E1GD0

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/18/2024
Supervised By :mohammad ahmed 07/19/2024


Quant Time: Jul 18 14:15:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN071224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 17 02:35:25 2024
Response via : Initial Calibration

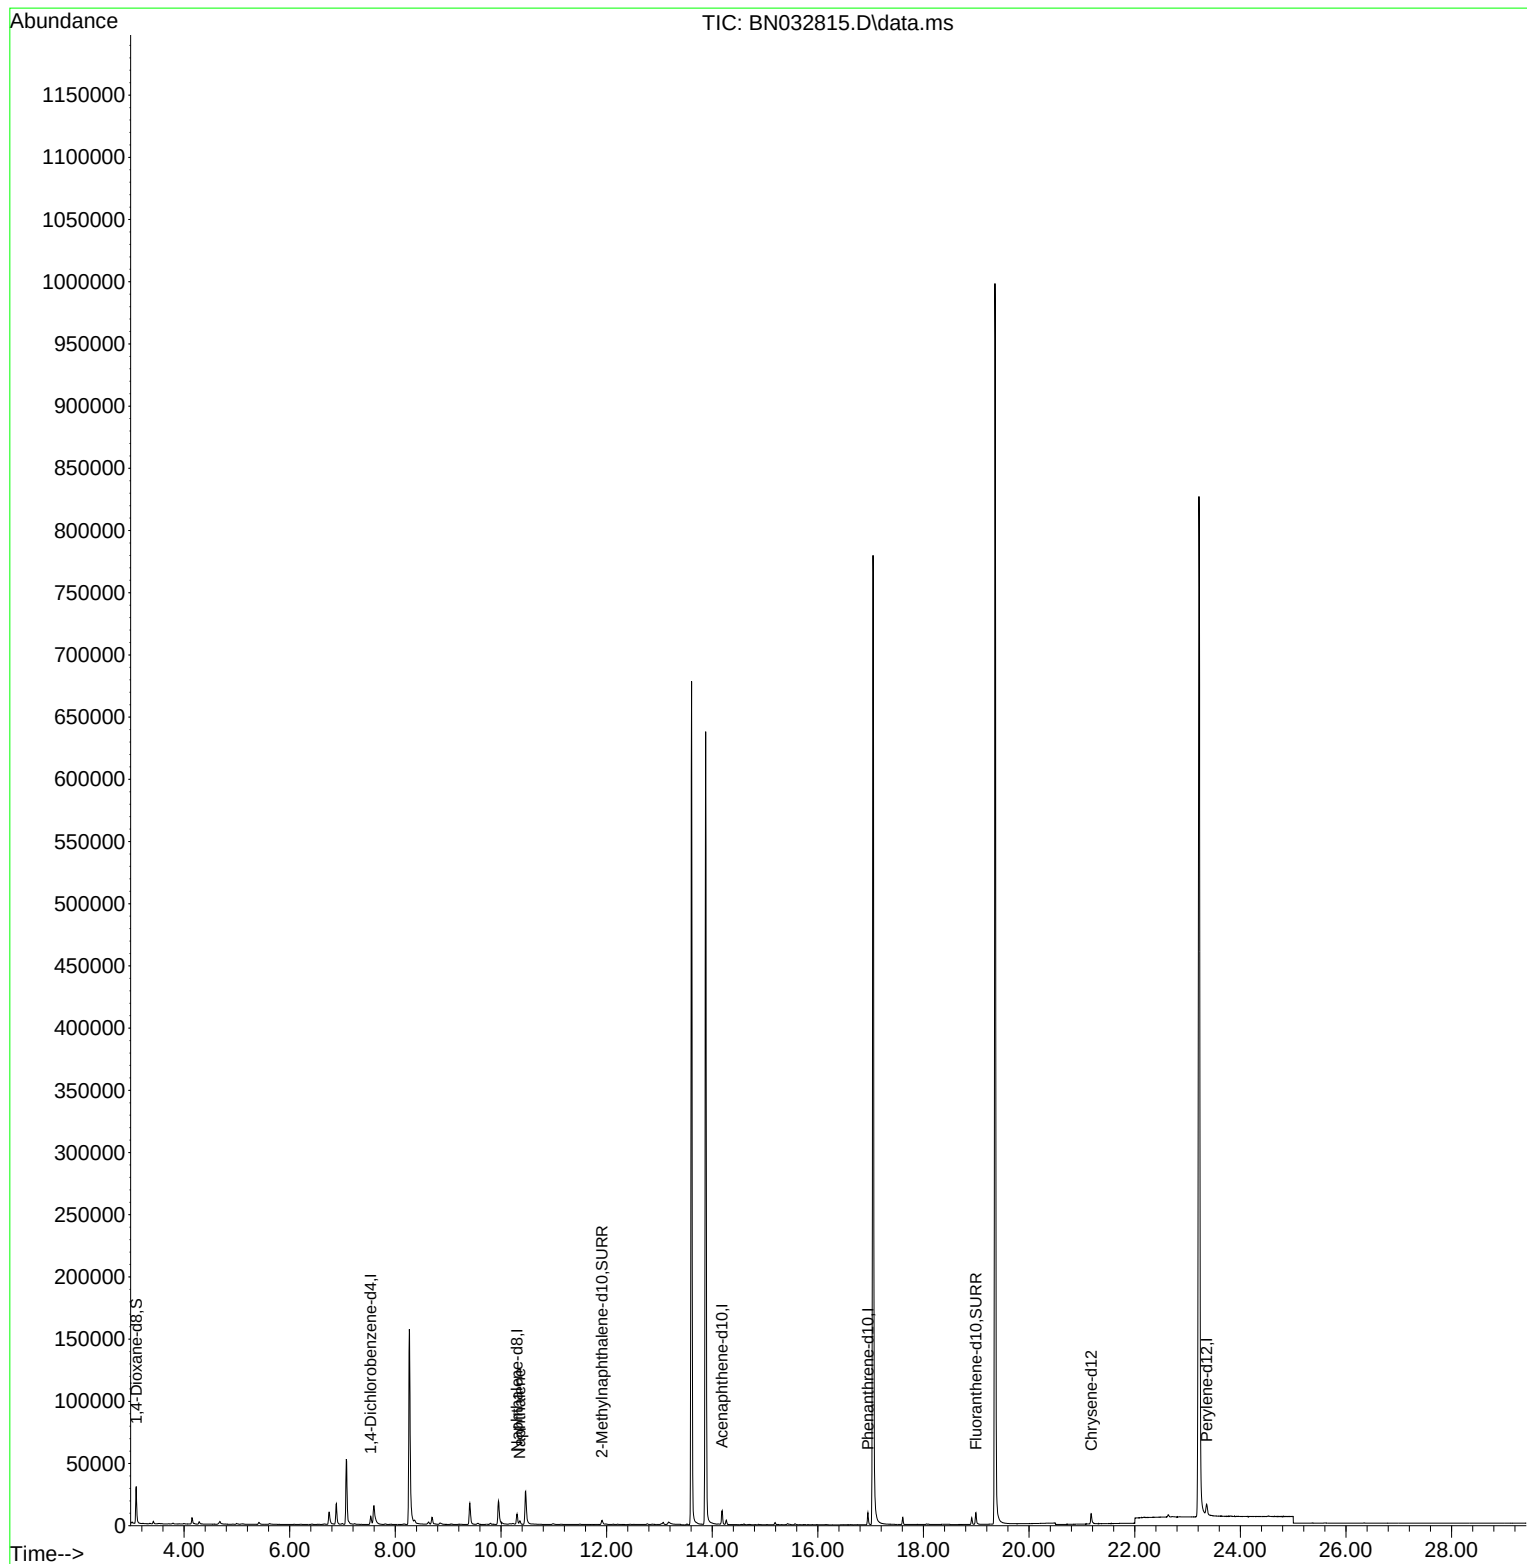

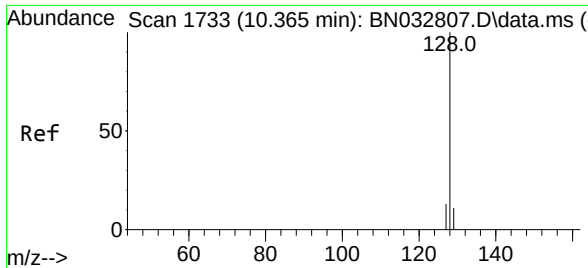

#5
Naphthalene
Concen: 0.038 ng/ul
RT: 10.353 min Scan# 1170
Delta R.T. -0.018 min
Lab File: BN032815.D
Acq: 18 Jul 2024 13:47

Instrument :
BNA_N
ClientSampleId :
E1GD0

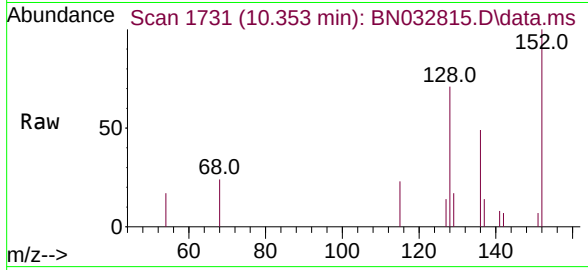

Tgt Ion:128 Resp: 1170

Ion	Ratio	Lower	Upper
128	100		
129	24.1	10.0	15.0
127	20.2	11.6	17.4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/18/2024
Supervised By :mohammad ahmed 07/19/2024

