


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071625\
Data File : BN037509.D
Acq On : 16 Jul 2025 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 10 02:20:59 2025

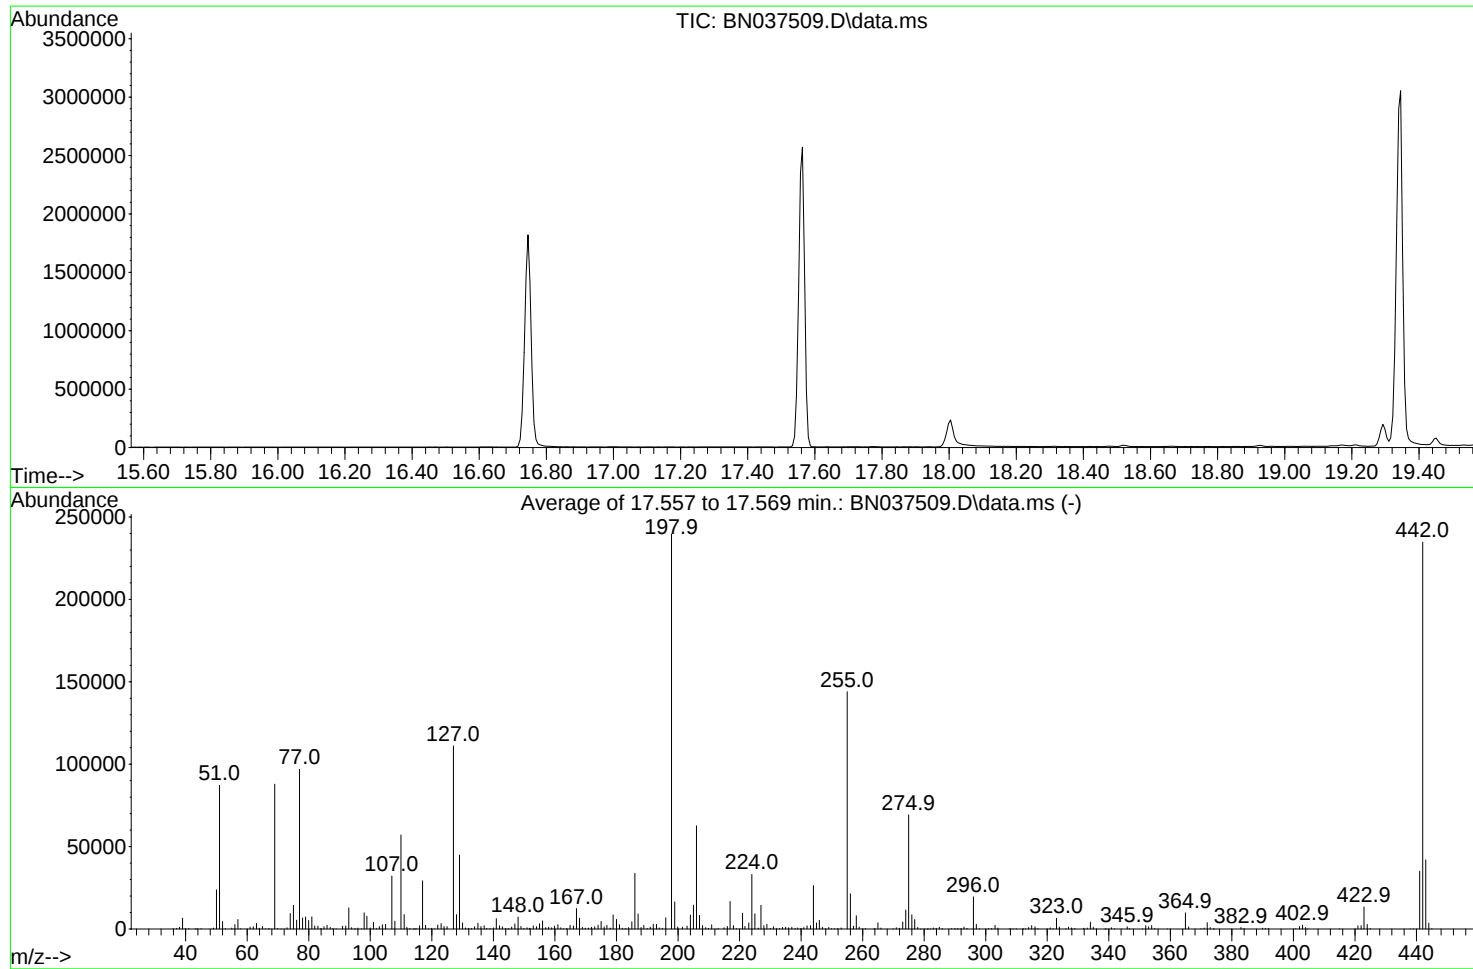




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	87885	PASS
70	69	0.00	2	0.5	431	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	239552	PASS
199	198	5	9	6.8	16396	PASS
365	198	1	100	4.1	9795	PASS
441	443	0.01	150	83.6	35077	PASS
442	442	100	100	100.0	234773	PASS
443	442	15	24	17.9	41957	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071625\
Data File : BN037509.D
Acq On : 16 Jul 2025 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 16 12:56:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

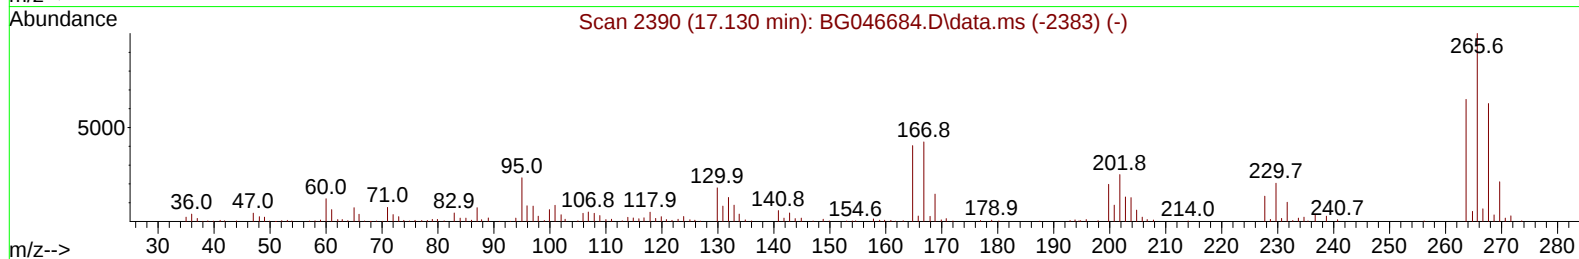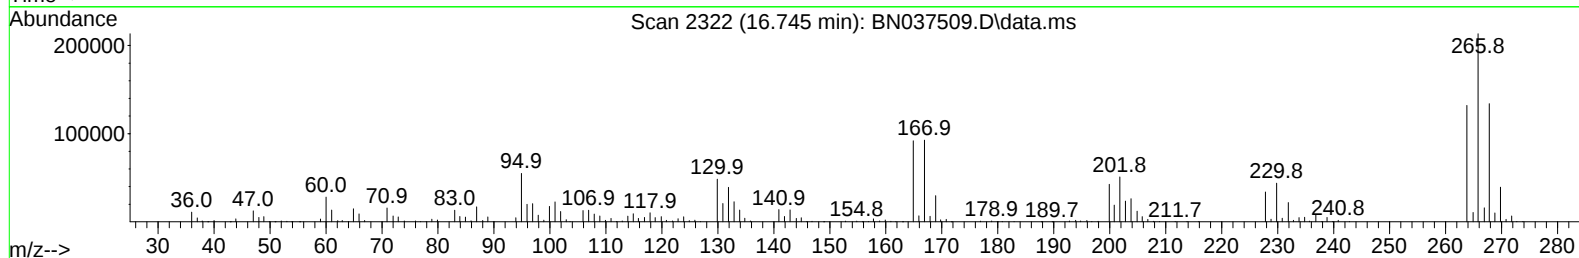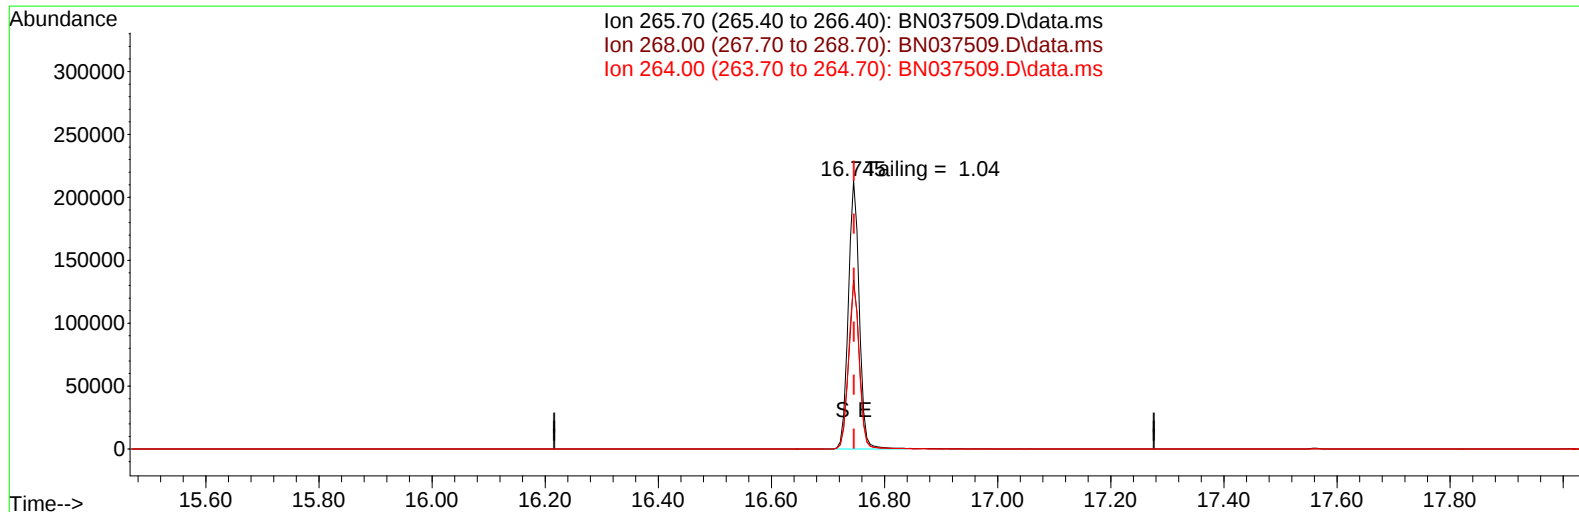

TIC: BN037509.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.001) 27368.56 ng




response 287163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.86
264.00	61.60	61.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071625\
Data File : BN037509.D
Acq On : 16 Jul 2025 09:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 16 12:56:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

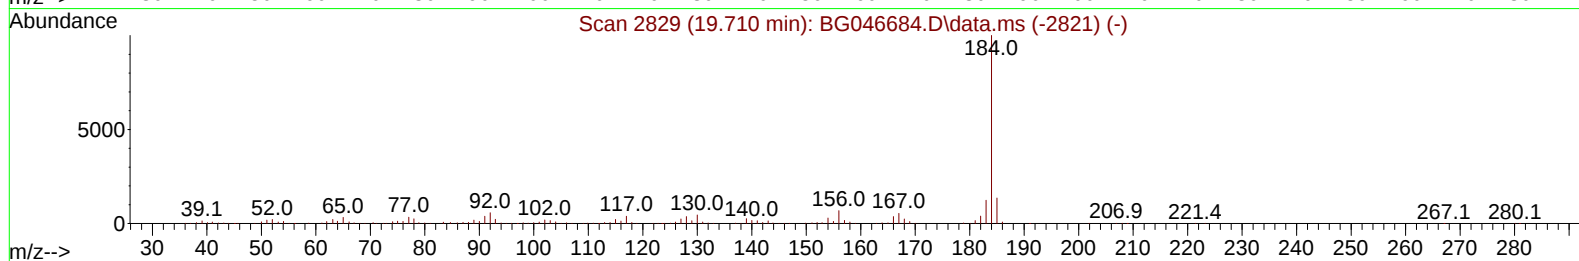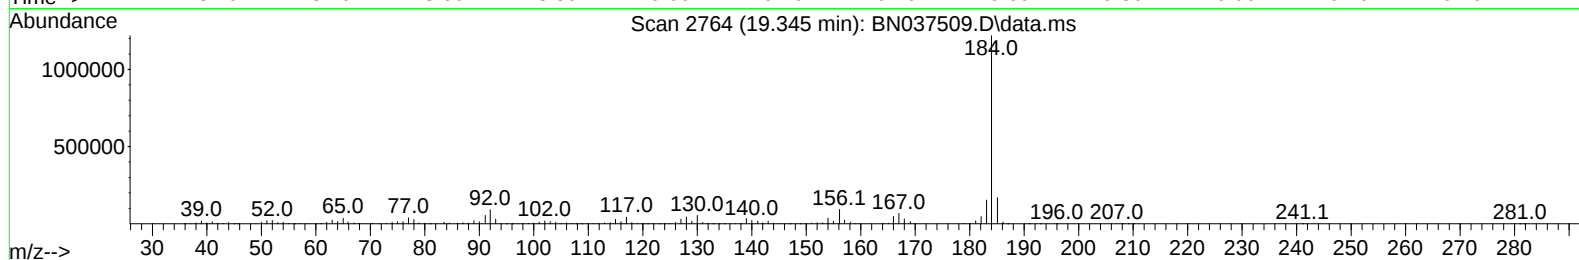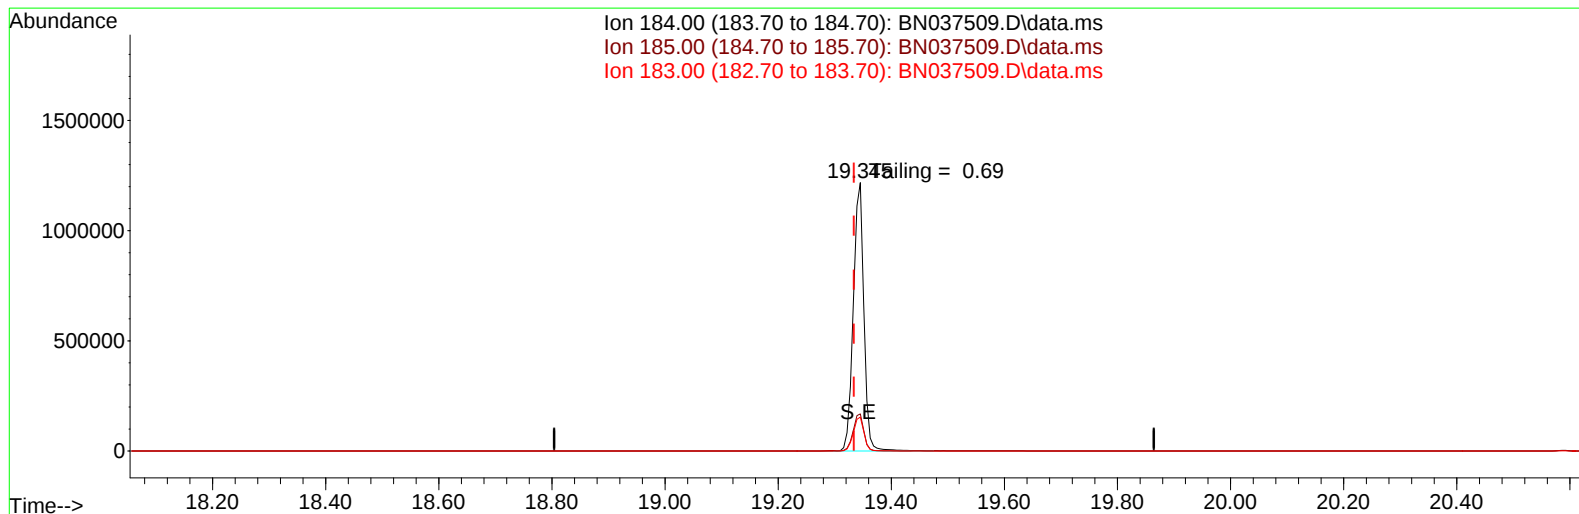

TIC: BN037509.D\data.ms

(77) Benzidine

19.345min (+ 0.011) 0.00 ng

response 1586462

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.85
183.00	13.20	12.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/16/2025	BNA_N	<u>BN037509.D</u>
Compound Name	Response	Retention Time
DDT	767819	20.592
DDD	7966	20.198
DDE	70	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8036	775855	1.04

Instrument :
BNA_N
ClientSampleId :
DFTPP