


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071721\
Data File : BN015607.D
Acq On : 16 Jul 2021 21:50
Operator : CG/JU
Sample : M2914-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK41

Manual Integrations
APPROVED

mohammad
7/19/2021 11:56:26 AM

Quant Time: Jul 17 00:40:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 16 15:41:51 2021
Response via : Initial Calibration

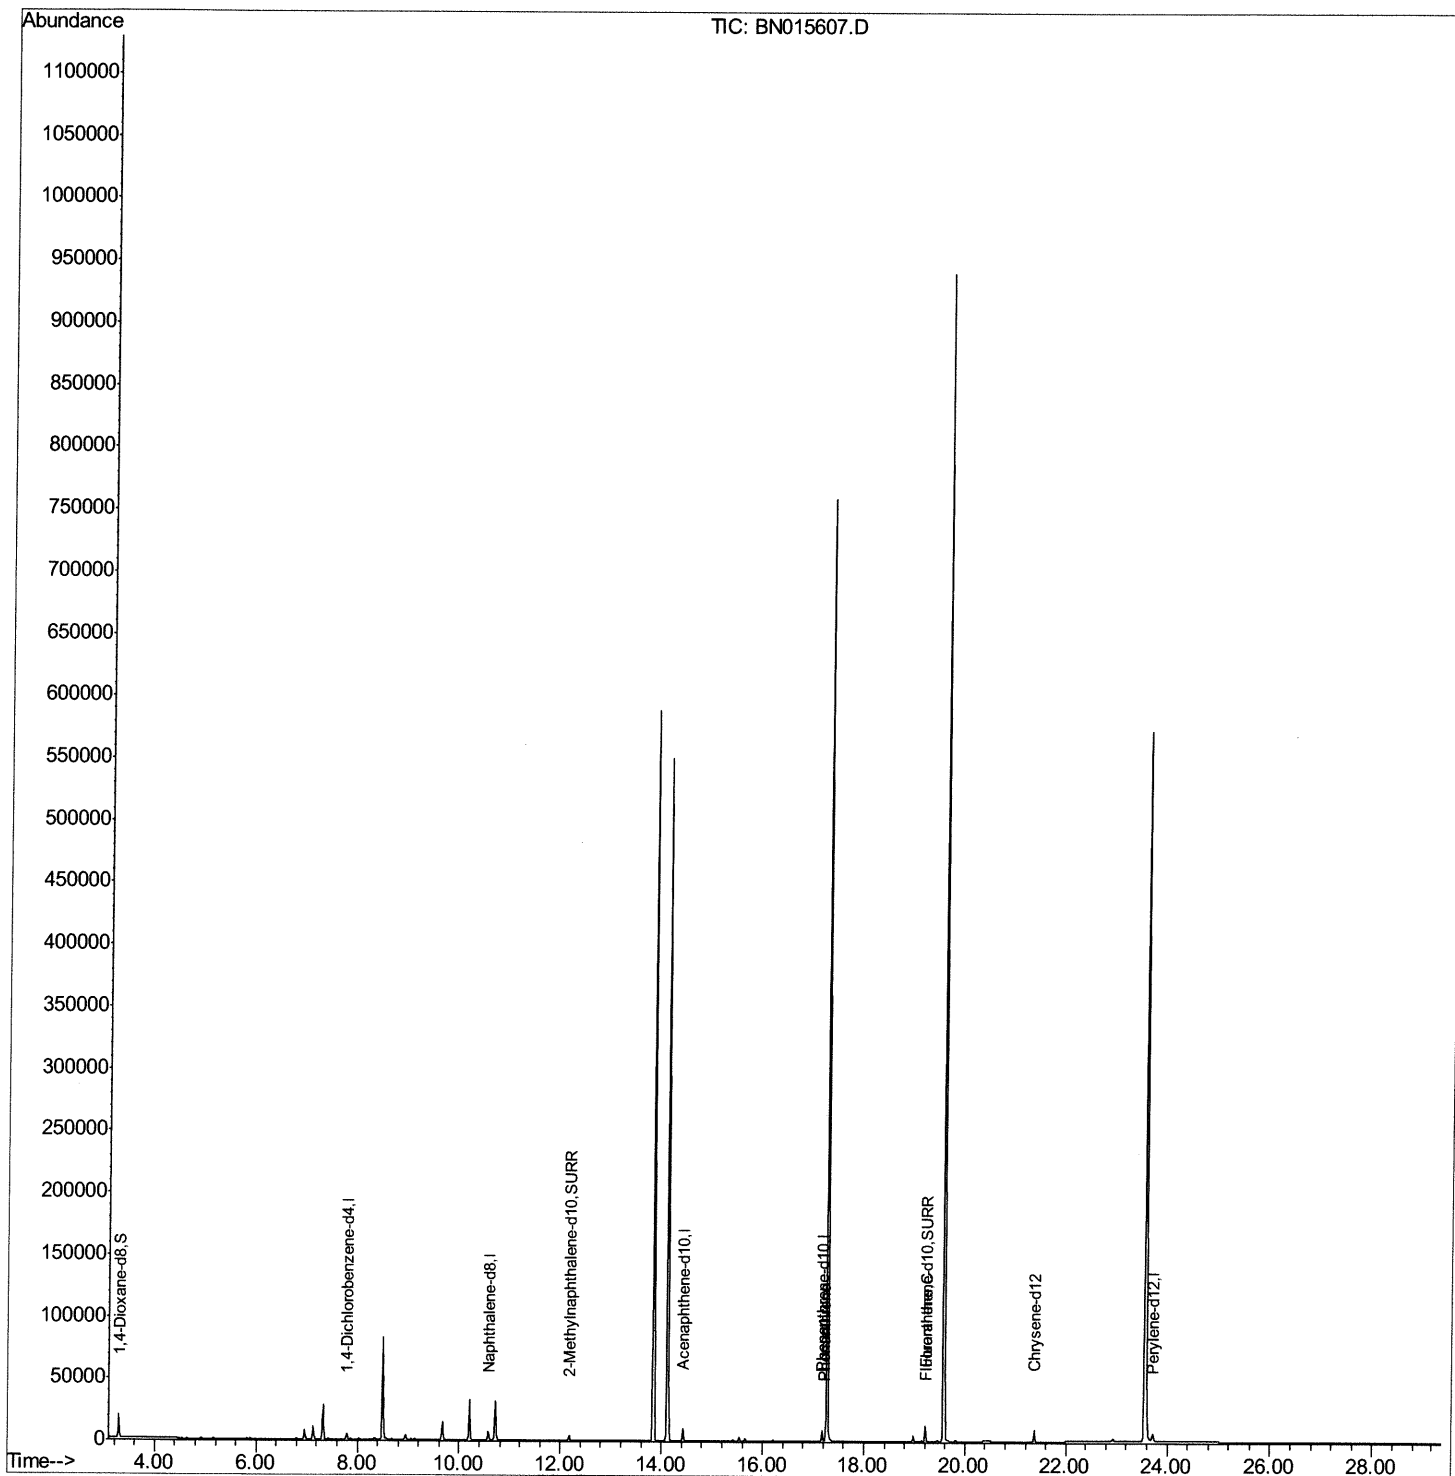

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071721\
 Data File : BN015607.D
 Acq On : 16 Jul 2021 21:50
 Operator : CG/JU
 Sample : M2914-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK41

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:56:26 AM

Quant Time: Jul 17 00:19:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 15:41:51 2021
 Response via : Initial Calibration

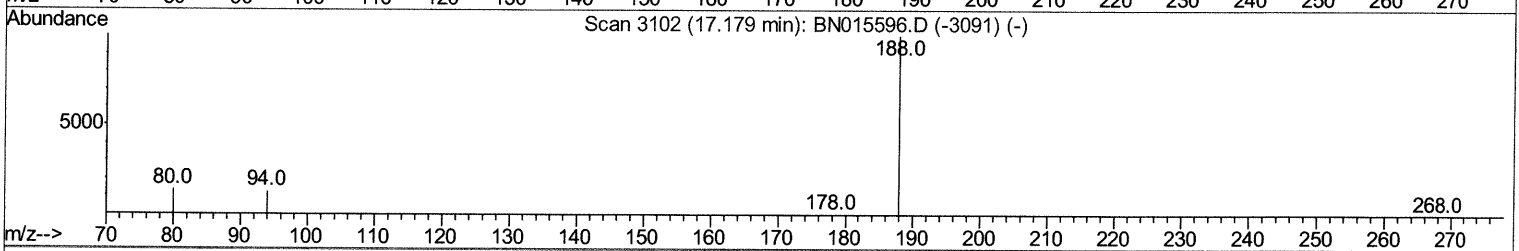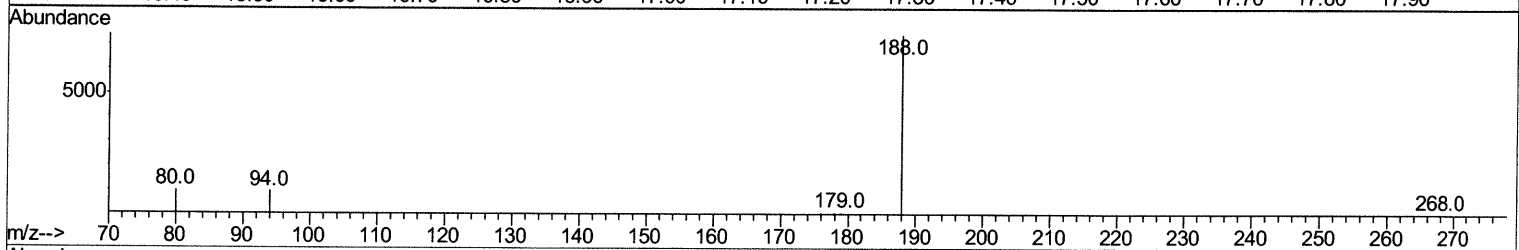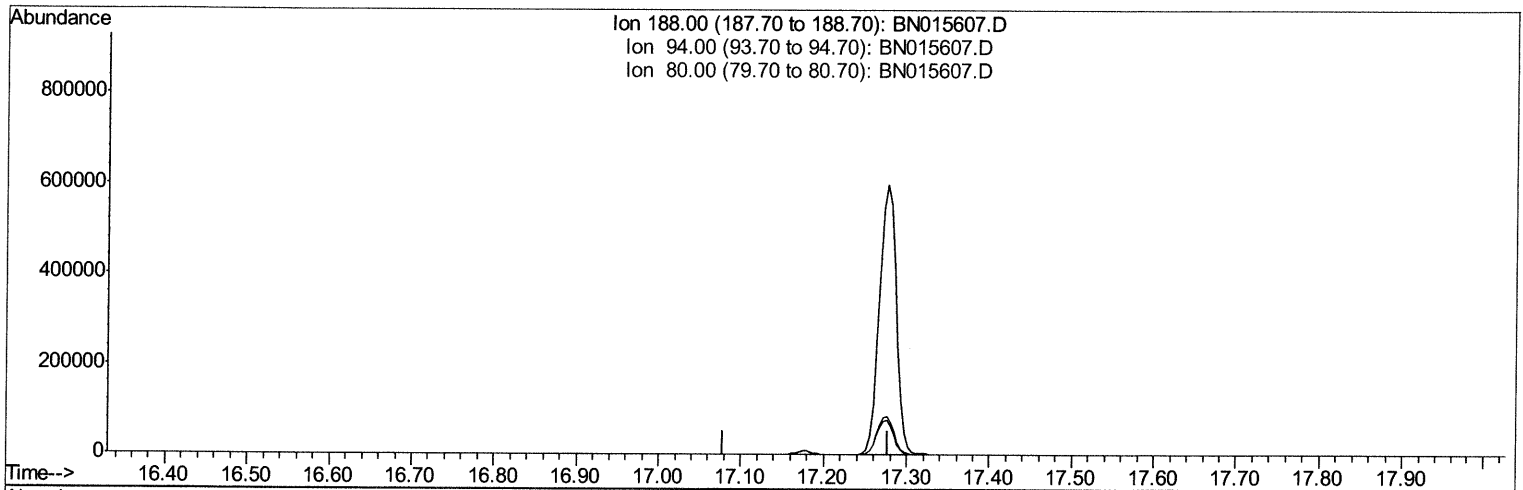

TIC: BN015607.D

(13) Phenanthrene-d10 (I)

17.179min (-17.179) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071721\
Data File : BN015607.D
Acq On : 16 Jul 2021 21:50
Operator : CG/JU
Sample : M2914-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK41

Manual Integrations
APPROVED

mohammad
7/19/2021 11:56:26 AM

Quant Time: Jul 17 00:19:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 16 15:41:51 2021
Response via : Initial Calibration

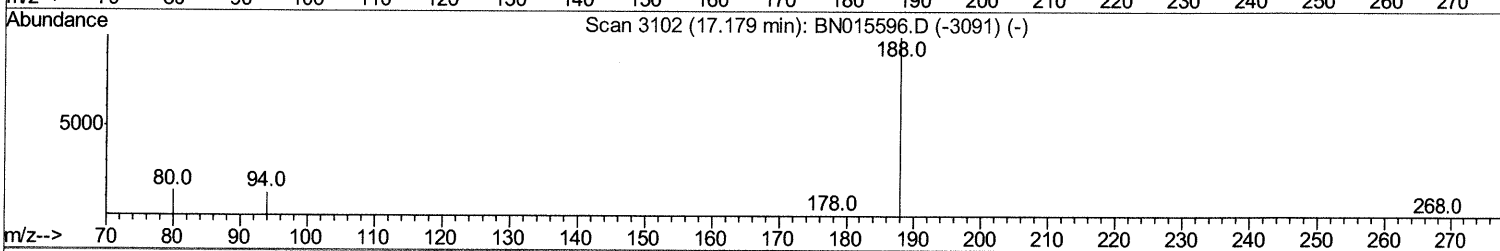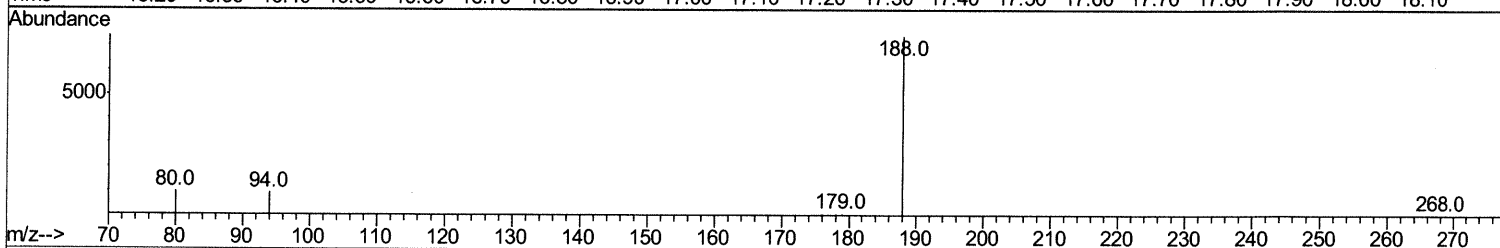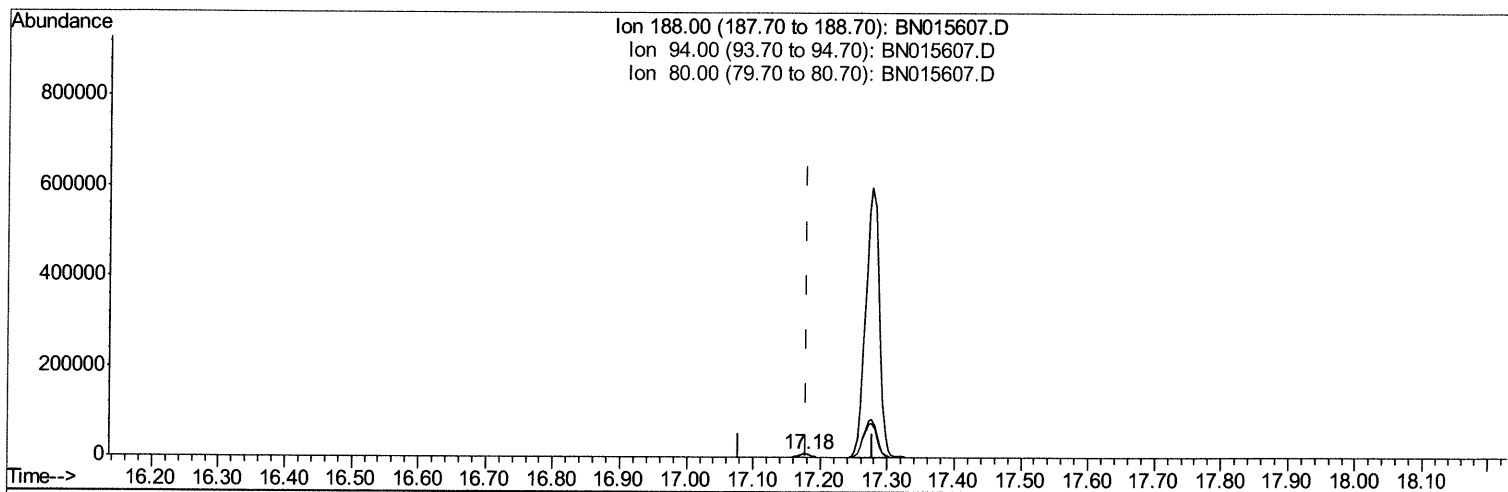

TIC: BN015607.D

(13) Phenanthrene-d10 (I)

17.179min (+0.000) 0.40ng/ul m 07/22/21 JU

response 10483

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	12.61
80.00	12.50	13.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071721\
 Data File : BN015607.D
 Acq On : 16 Jul 2021 21:50
 Operator : CG/JU
 Sample : M2914-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK41

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:56:26 AM

Quant Time: Jul 17 00:40:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 15:41:51 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	2399	0.40	ng/ul	0.00
4) Naphthalene-d8	10.58	136	8802	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.43	164	5191	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.18	188	10483m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.37	240	8720	0.40	ng/ul	0.00
23) Perylene-d12	23.72	264	8715	0.40	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.29	96	11775	4.35	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.17	152	4803	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.21	212	12538	0.44	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.22	178	1243	0.033	ng/ul#	87
19) Fluoranthene	19.24	202	872	0.022	ng/ul#	60

(#) = qualifier out of range (m) = manual integration (+) = signals summed