


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071721\
Data File : BN015608.D
Acq On : 16 Jul 2021 22:27
Operator : CG/JU
Sample : M2914-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK42

Manual Integrations
APPROVED

mohammad
7/19/2021 11:56:30 AM

Quant Time: Jul 17 00:43:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 16 15:41:51 2021
Response via : Initial Calibration

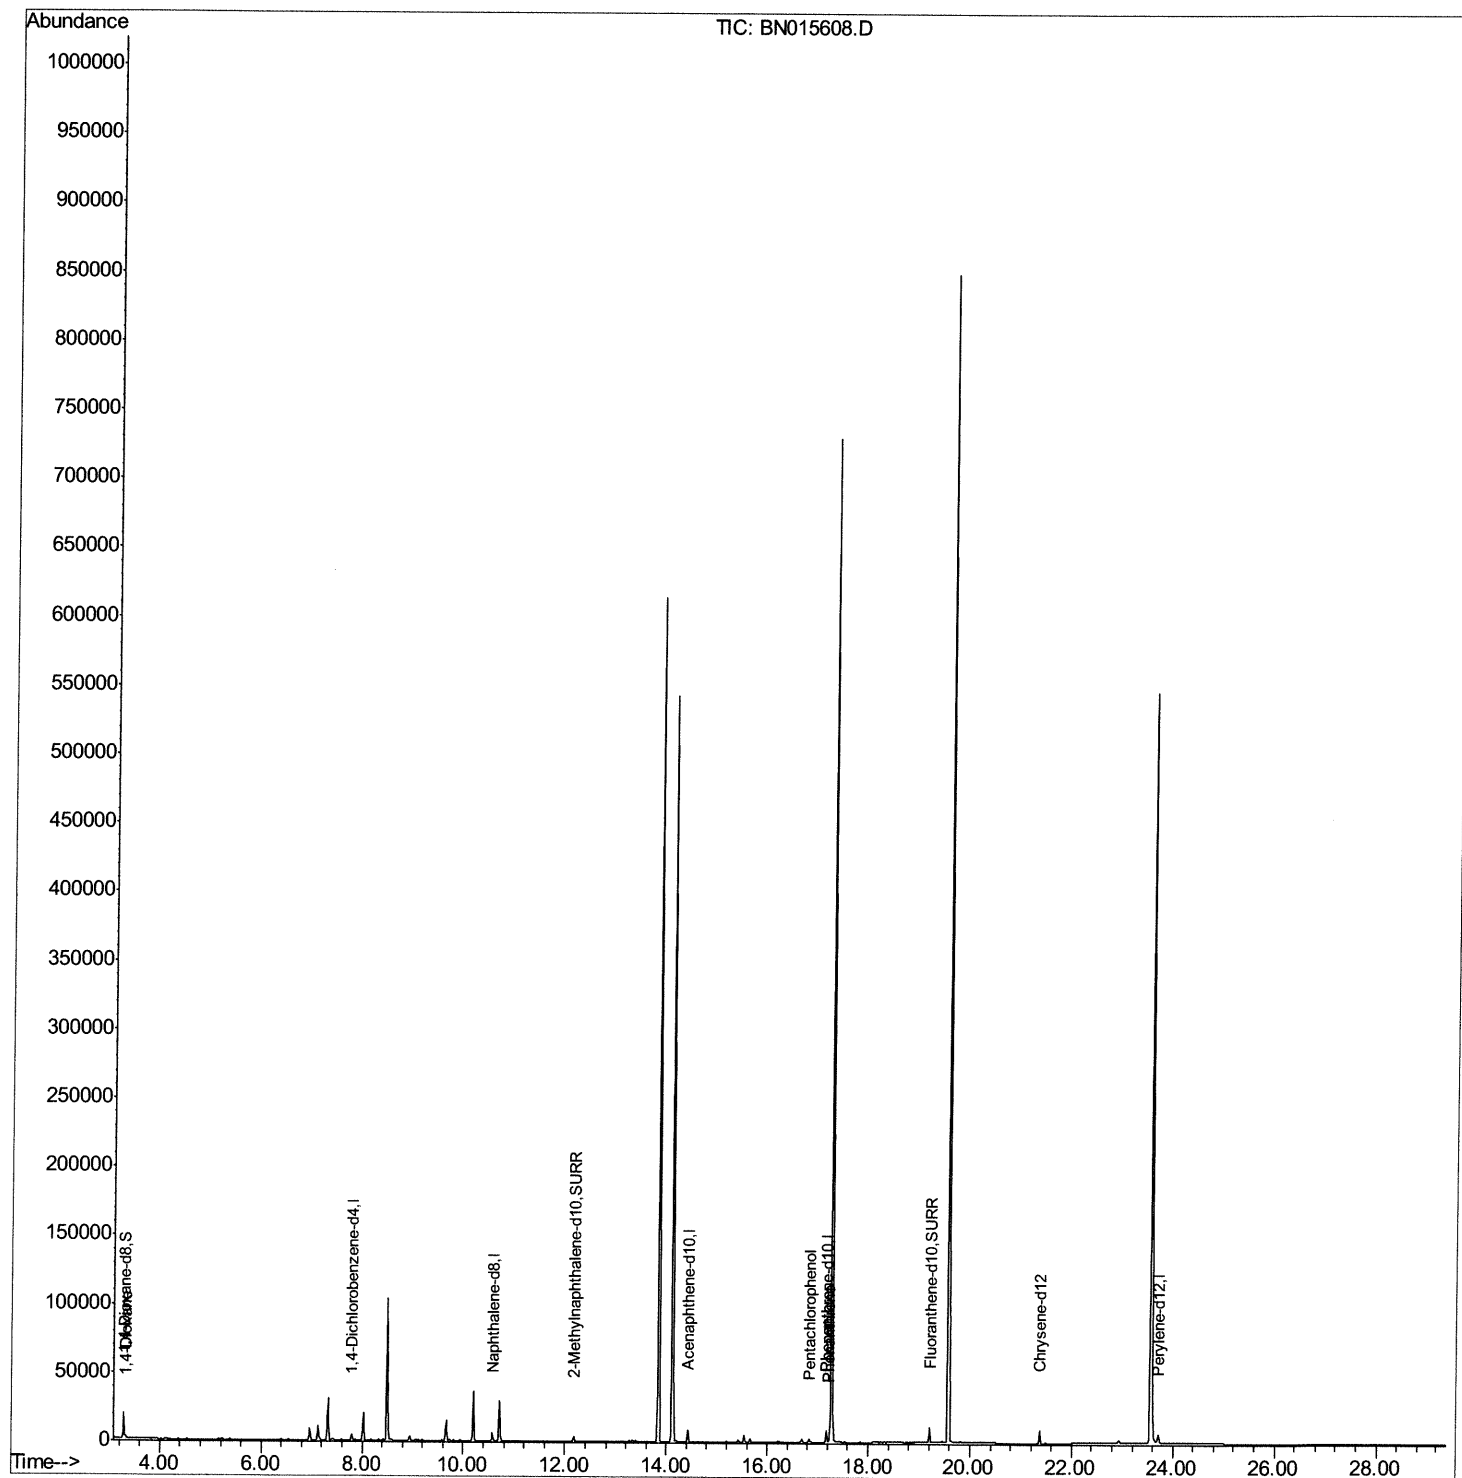

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071721\
Data File : BN015608.D
Acq On : 16 Jul 2021 22:27
Operator : CG/JU
Sample : M2914-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK42

Manual Integrations
APPROVED

mohammad
7/19/2021 11:56:30 AM

Quant Time: Jul 17 00:20:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 16 15:41:51 2021
Response via : Initial Calibration

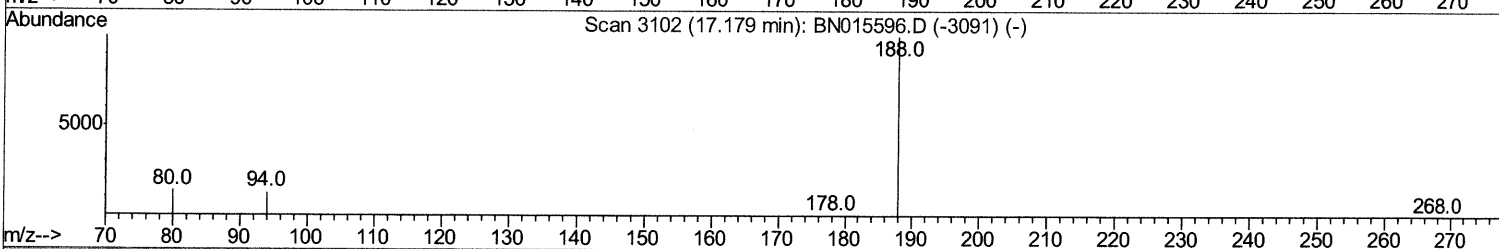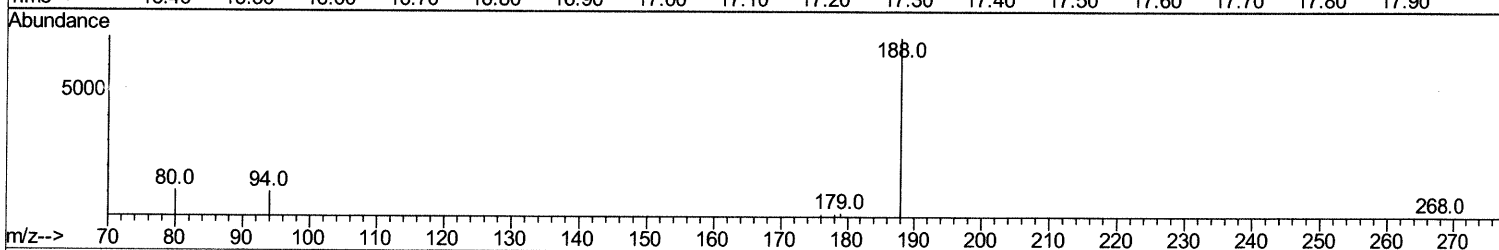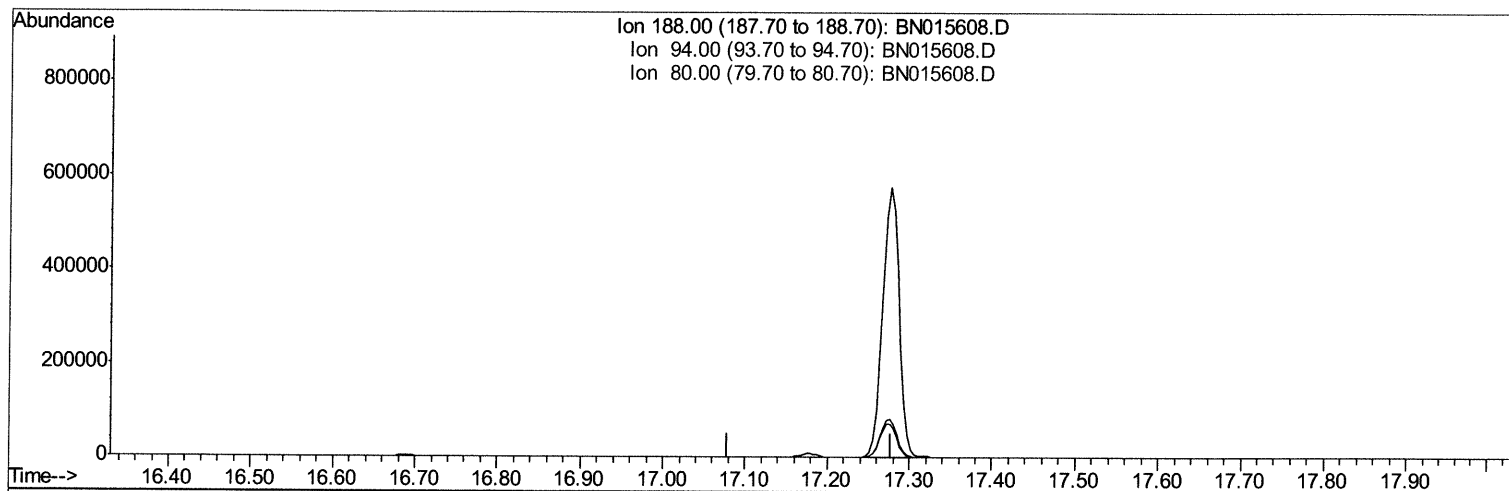

TIC: BN015608.D

(13) Phenanthrene-d10 (I)

17.179min (-17.179) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071721\
 Data File : BN015608.D
 Acq On : 16 Jul 2021 22:27
 Operator : CG/JU
 Sample : M2914-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK42

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:56:30 AM

Quant Time: Jul 17 00:20:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 15:41:51 2021
 Response via : Initial Calibration

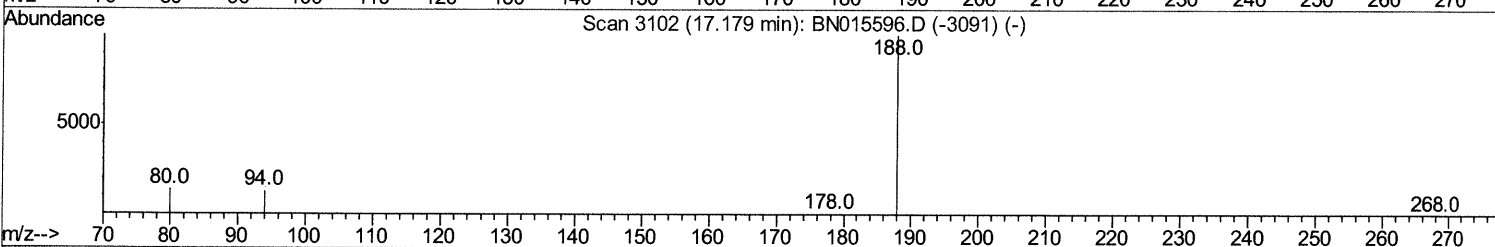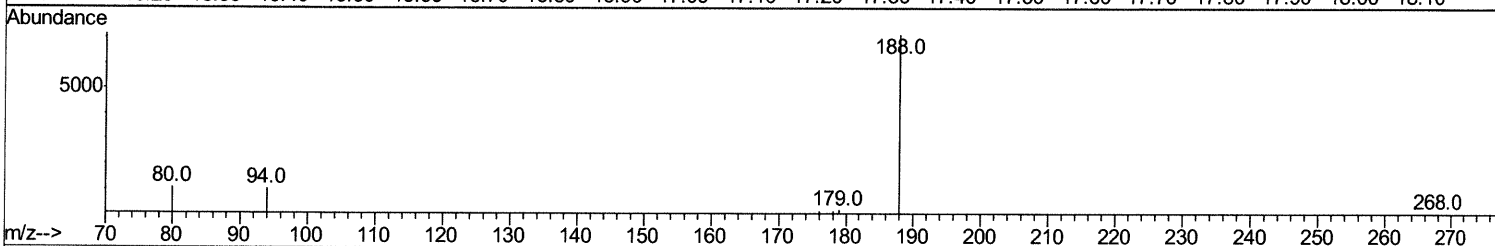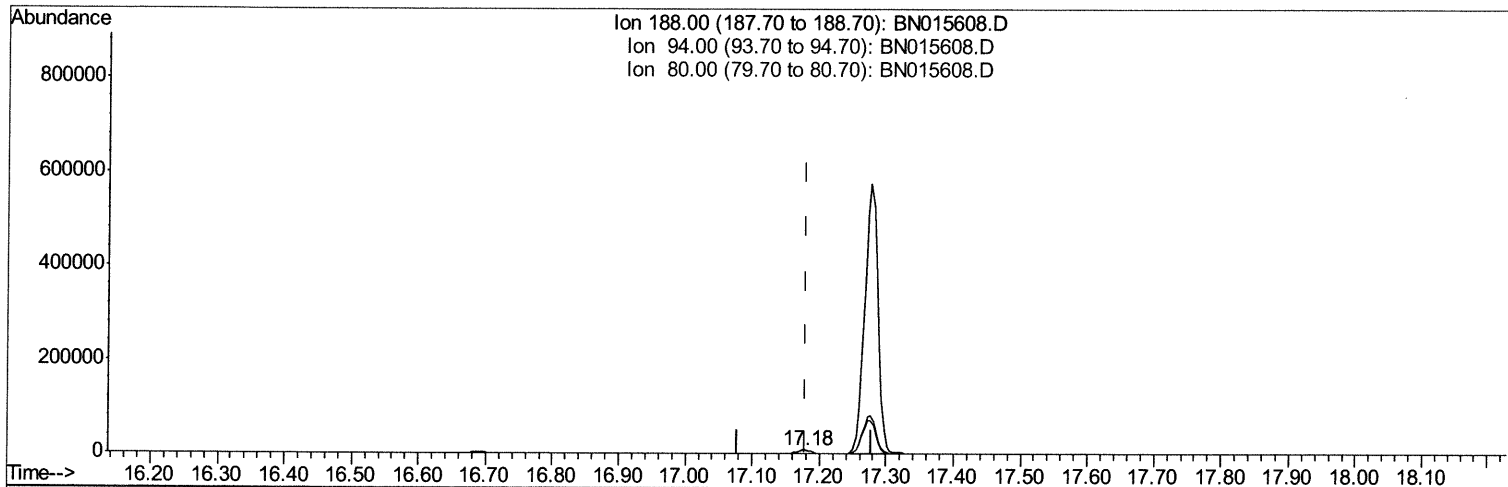

TIC: BN015608.D

(13) Phenanthrene-d10 (I)

17.179min (+0.000) 0.40ng/ul m 07/22/21 JU

response 9875

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	14.26#
80.00	12.50	14.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071721\
 Data File : BN015608.D
 Acq On : 16 Jul 2021 22:27
 Operator : CG/JU
 Sample : M2914-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK42

Manual Integrations
 APPROVED

mohammad
 7/19/2021 11:56:30 AM

Quant Time: Jul 17 00:43:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 16 15:41:51 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	2233	0.40	ng/ul	0.00
4) Naphthalene-d8	10.58	136	8260	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.43	164	4961	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.18	188	9875m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.37	240	8042	0.40	ng/ul	0.00
23) Perylene-d12	23.72	264	7935	0.40	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.29	96	11540	4.58	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.17	152	4533	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.21	212	11257	0.43	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.32	88	1305	0.480	ng/ul#	55
14) Pentachlorophenol	16.83	266	1495	0.684	ng/ul	90
15) Phenanthrene	17.22	178	926	0.026	ng/ul#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed