


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071921\
Data File : BN015612.D
Acq On : 19 Jul 2021 13:42
Operator : CG/JU
Sample : PB137577BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK577

Quant Time: Jul 19 14:23:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 19 13:54:50 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
7/20/2021 11:38:47 AM

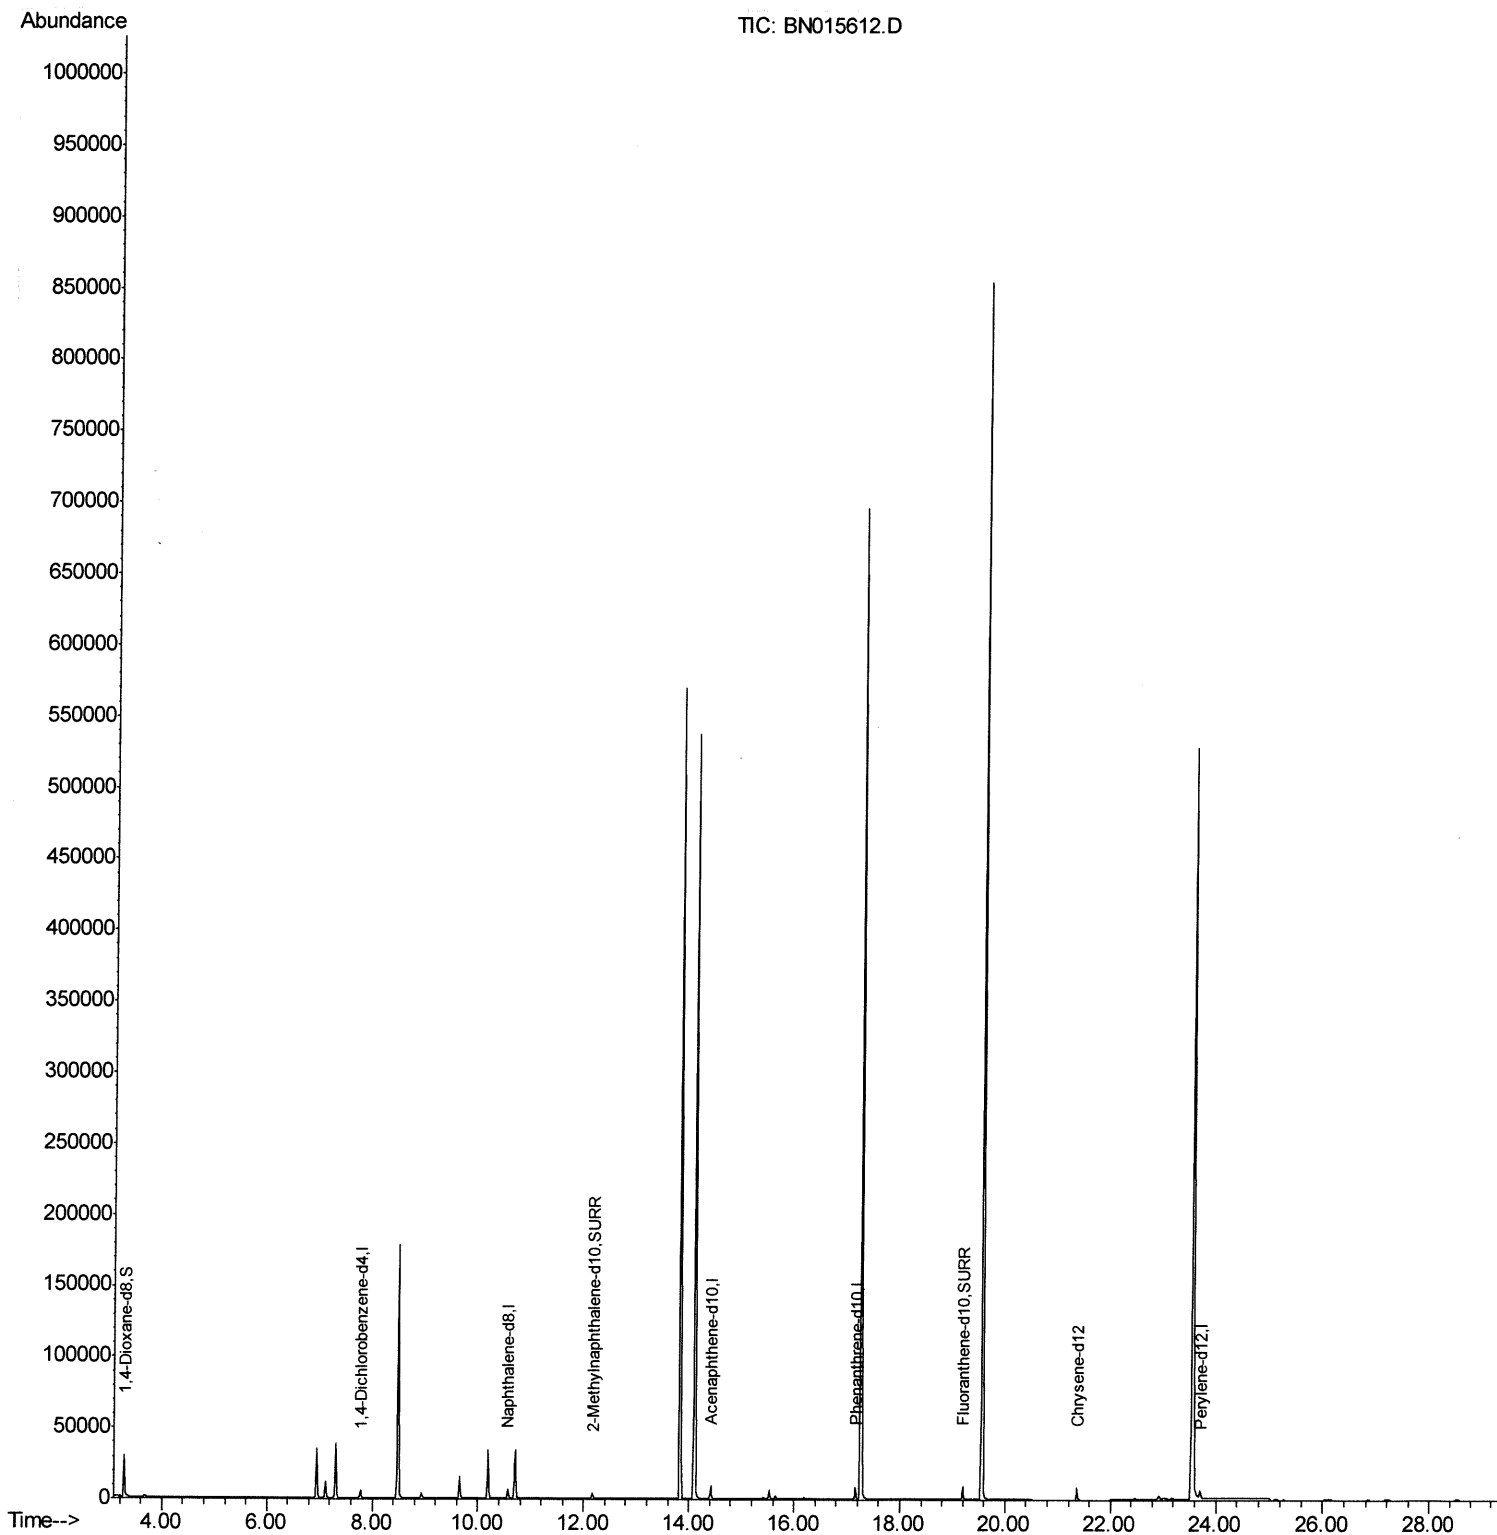




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071921\
 Data File : BN015612.D
 Acq On : 19 Jul 2021 13:42
 Operator : CG/JU
 Sample : PB137577BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK577

Manual Integrations
 APPROVED

mohammad
 7/20/2021 11:38:47 AM

Quant Time: Jul 19 14:22:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 19 13:54:50 2021
 Response via : Initial Calibration

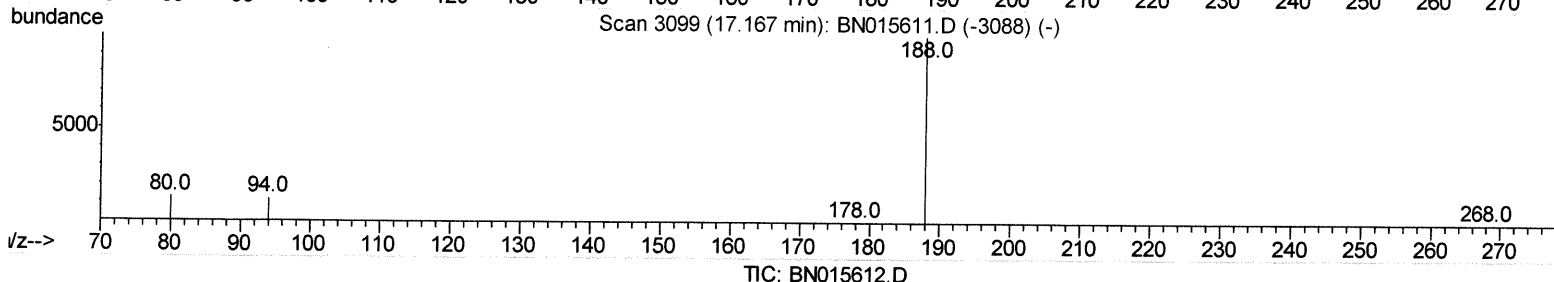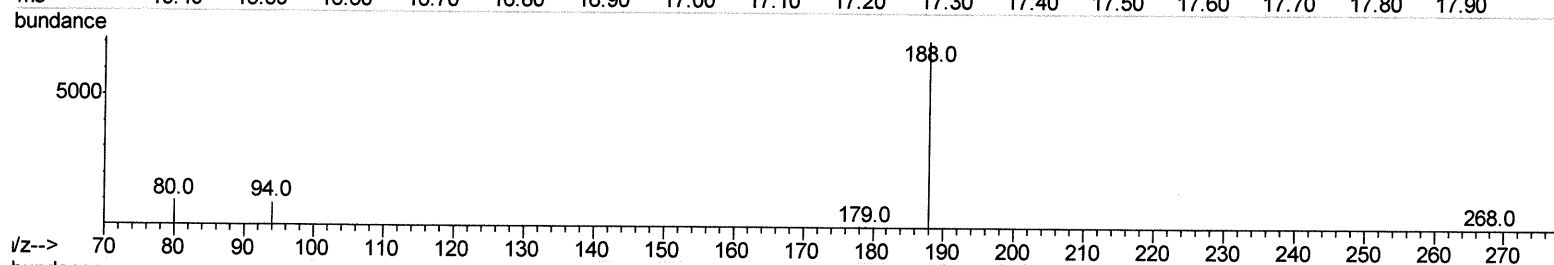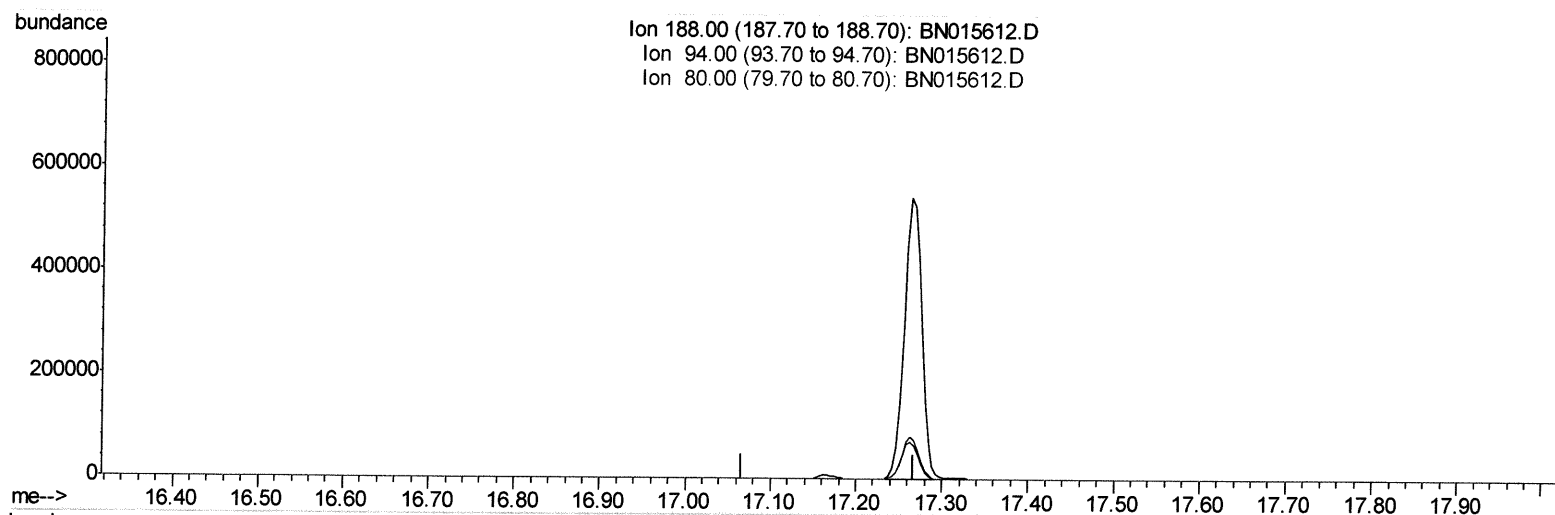

(13) Phenanthrene-d10 (I)

17.167min (-17.167) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071921\
Data File : BN015612.D
Acq On : 19 Jul 2021 13:42
Operator : CG/JU
Sample : PB137577BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK577

Manual Integrations
APPROVED

mohammad
7/20/2021 11:38:47 AM

Quant Time: Jul 19 14:22:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 19 13:54:50 2021
Response via : Initial Calibration

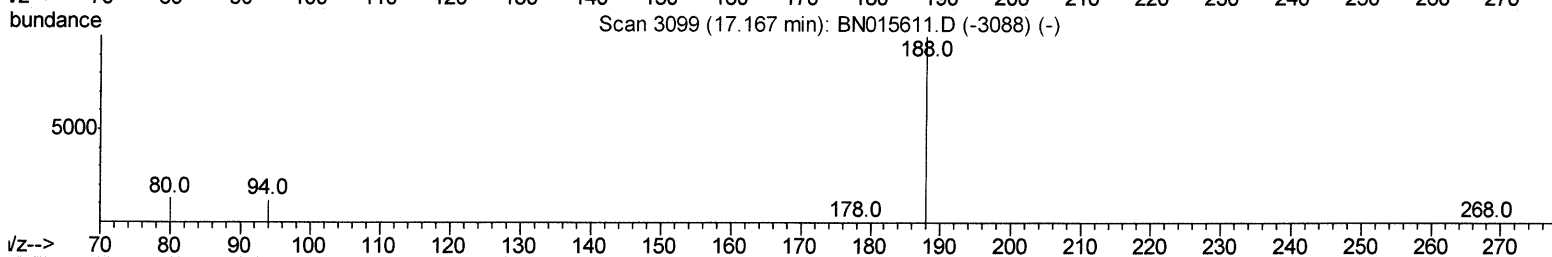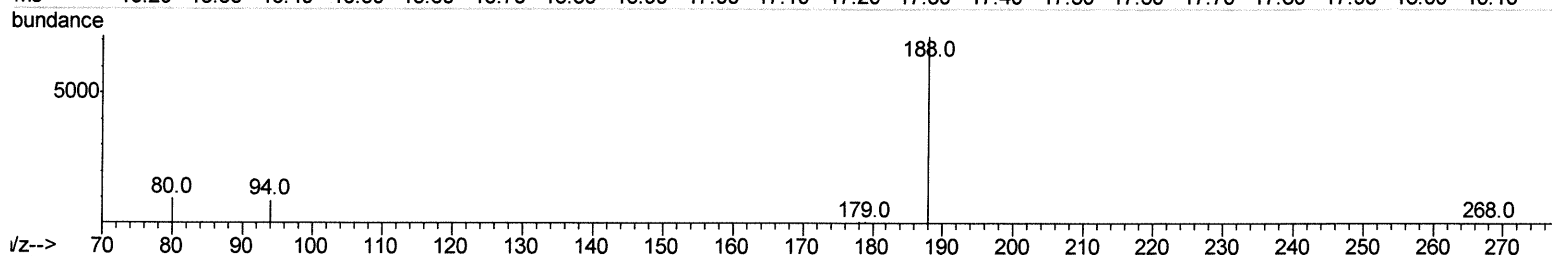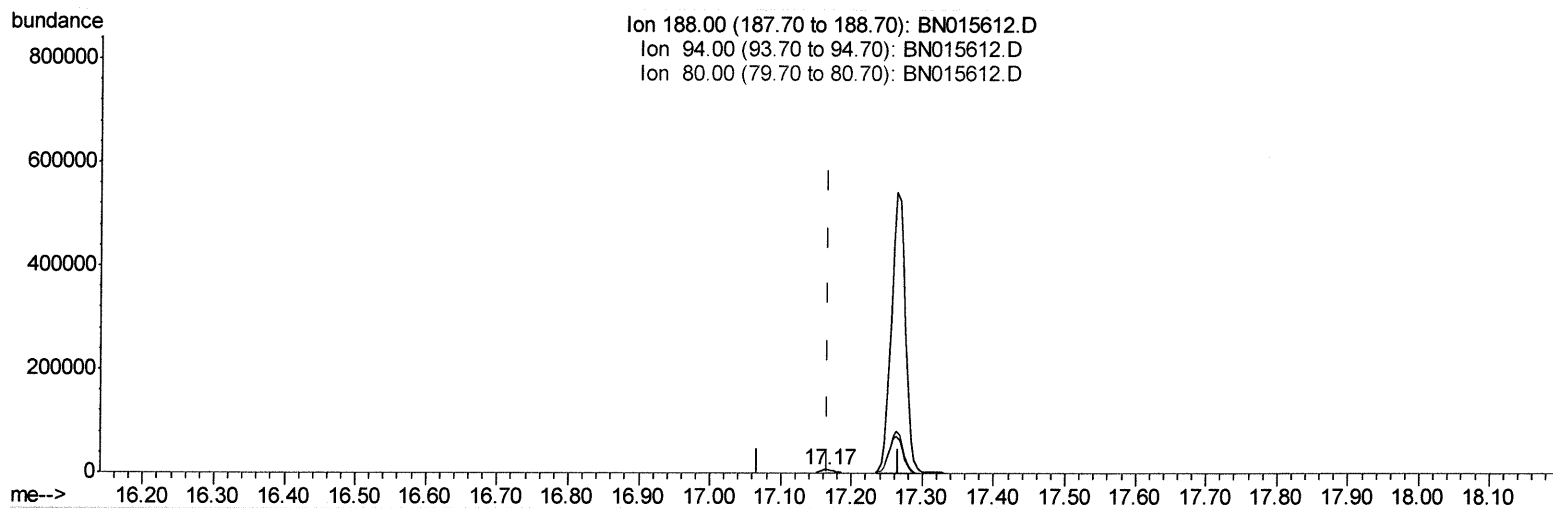

TIC: BN015612.D

(13) Phenanthrene-d10 (I)

17.166min (-0.001) 0.40ng/ul m

response 9684

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	12.55
80.00	12.50	13.44
0.00	0.00	0.00

JU 7/21/21

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071921\
 Data File : BN015612.D
 Acq On : 19 Jul 2021 13:42
 Operator : CG/JU
 Sample : PB137577BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK577

Manual Integrations
 APPROVED

mohammad
 7/20/2021 11:38:47 AM

Quant Time: Jul 19 14:23:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 19 13:54:50 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	2384	0.40	ng/ul	0.00
4) Naphthalene-d8	10.57	136	8447	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.42	164	4894	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.17	188	9684m	0.40	ng/ul	0.00
17) Chrysene-d12	21.36	240	7529	0.40	ng/ul	0.00
23) Perylene-d12	23.70	264	7636	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	18981	7.06	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.16	152	4624	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.20	212	9495	0.38	ng/ul	0.00

7/21/21

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed