


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071921\
Data File : BN015615.D
Acq On : 19 Jul 2021 19:23
Operator : CG/JU
Sample : SP5623
Misc : SFAM SURROGATE
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SP5623

Manual Integrations
APPROVED

mohammad
7/20/2021 11:38:53 AM

Quant Time: Jul 20 01:13:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 19 13:54:50 2021
Response via : Initial Calibration

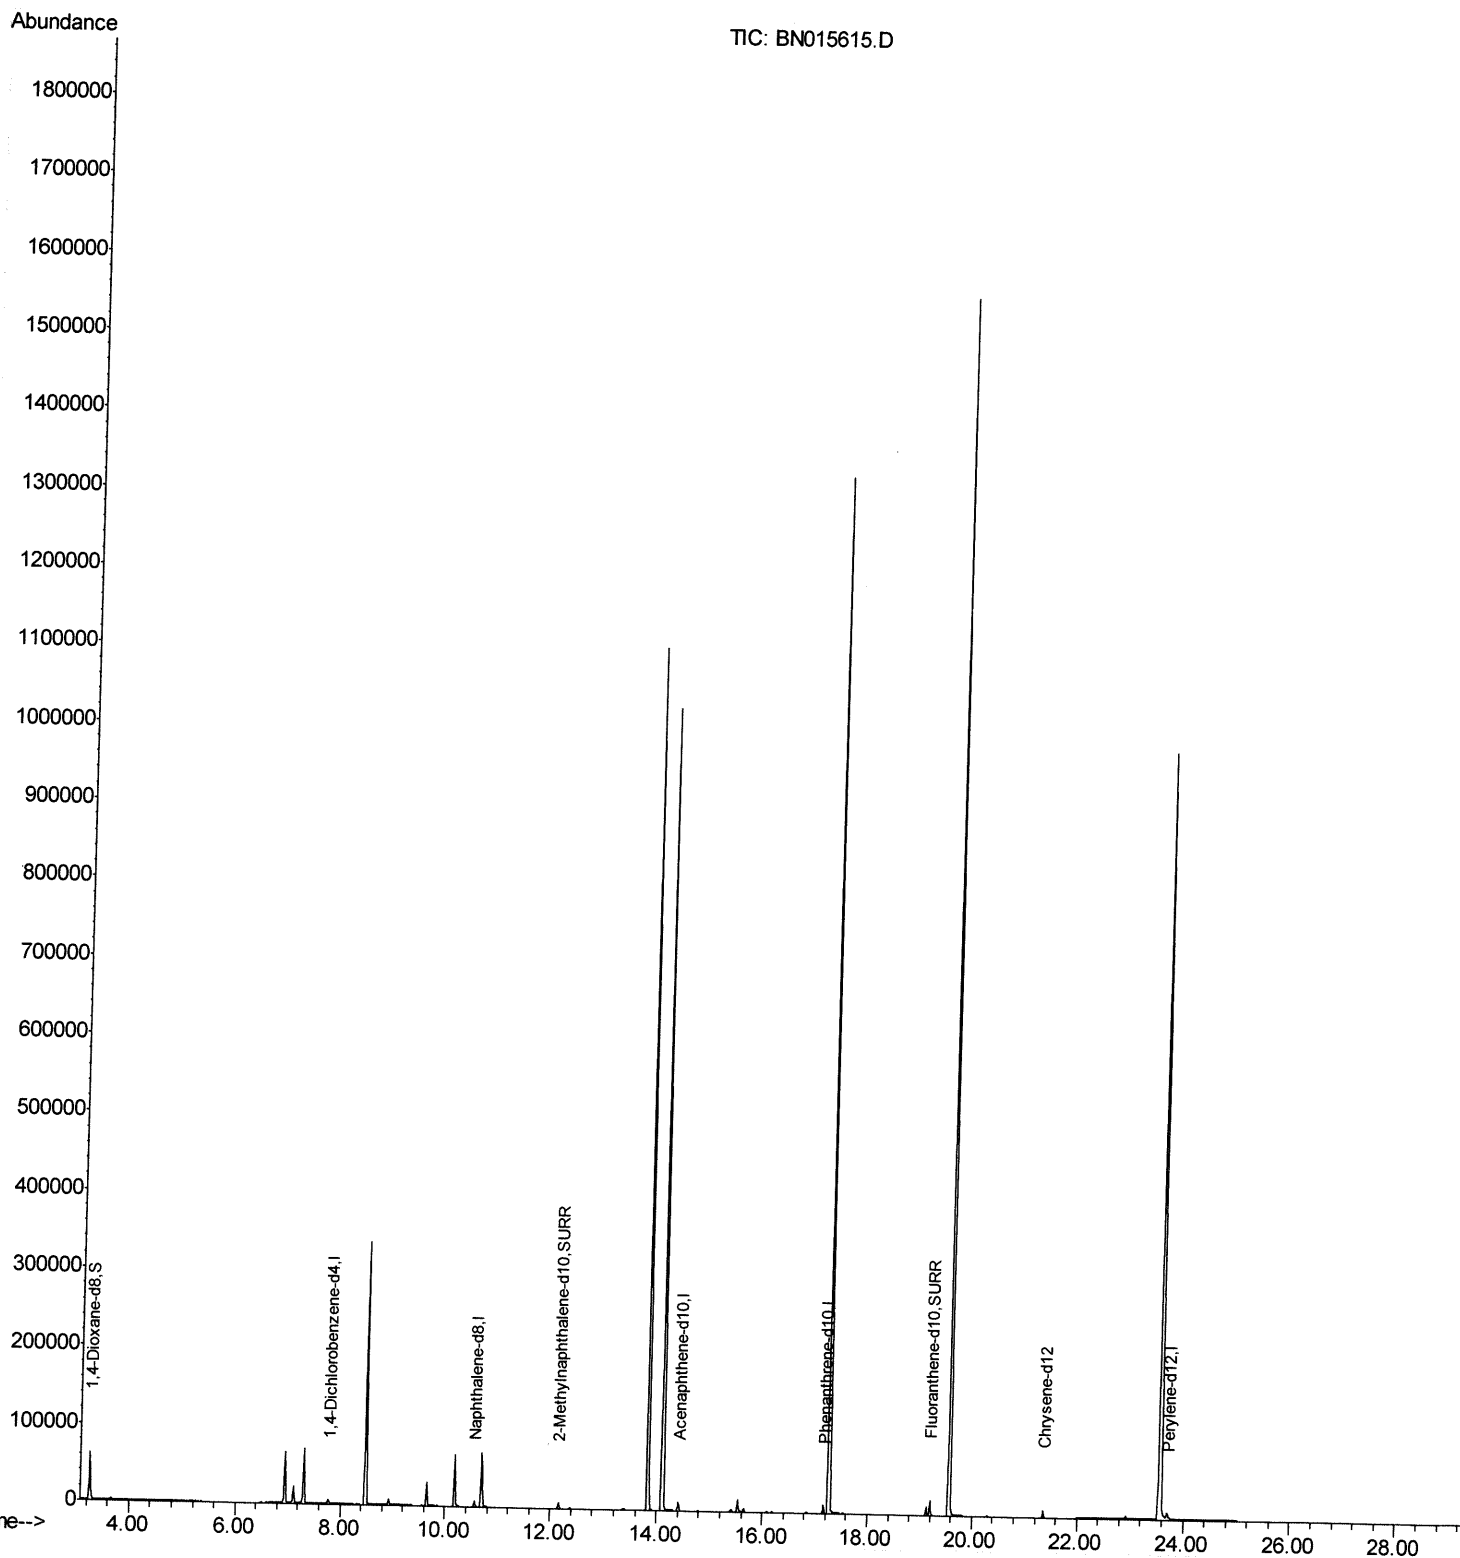


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071921\
 Data File : BN015615.D
 Acq On : 19 Jul 2021 19:23
 Operator : CG/JU
 Sample : SP5623
 Misc : SFAM SURROGATE
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP5623

Quant Time: Jul 20 01:10:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 19 13:54:50 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 7/20/2021 11:38:53 AM

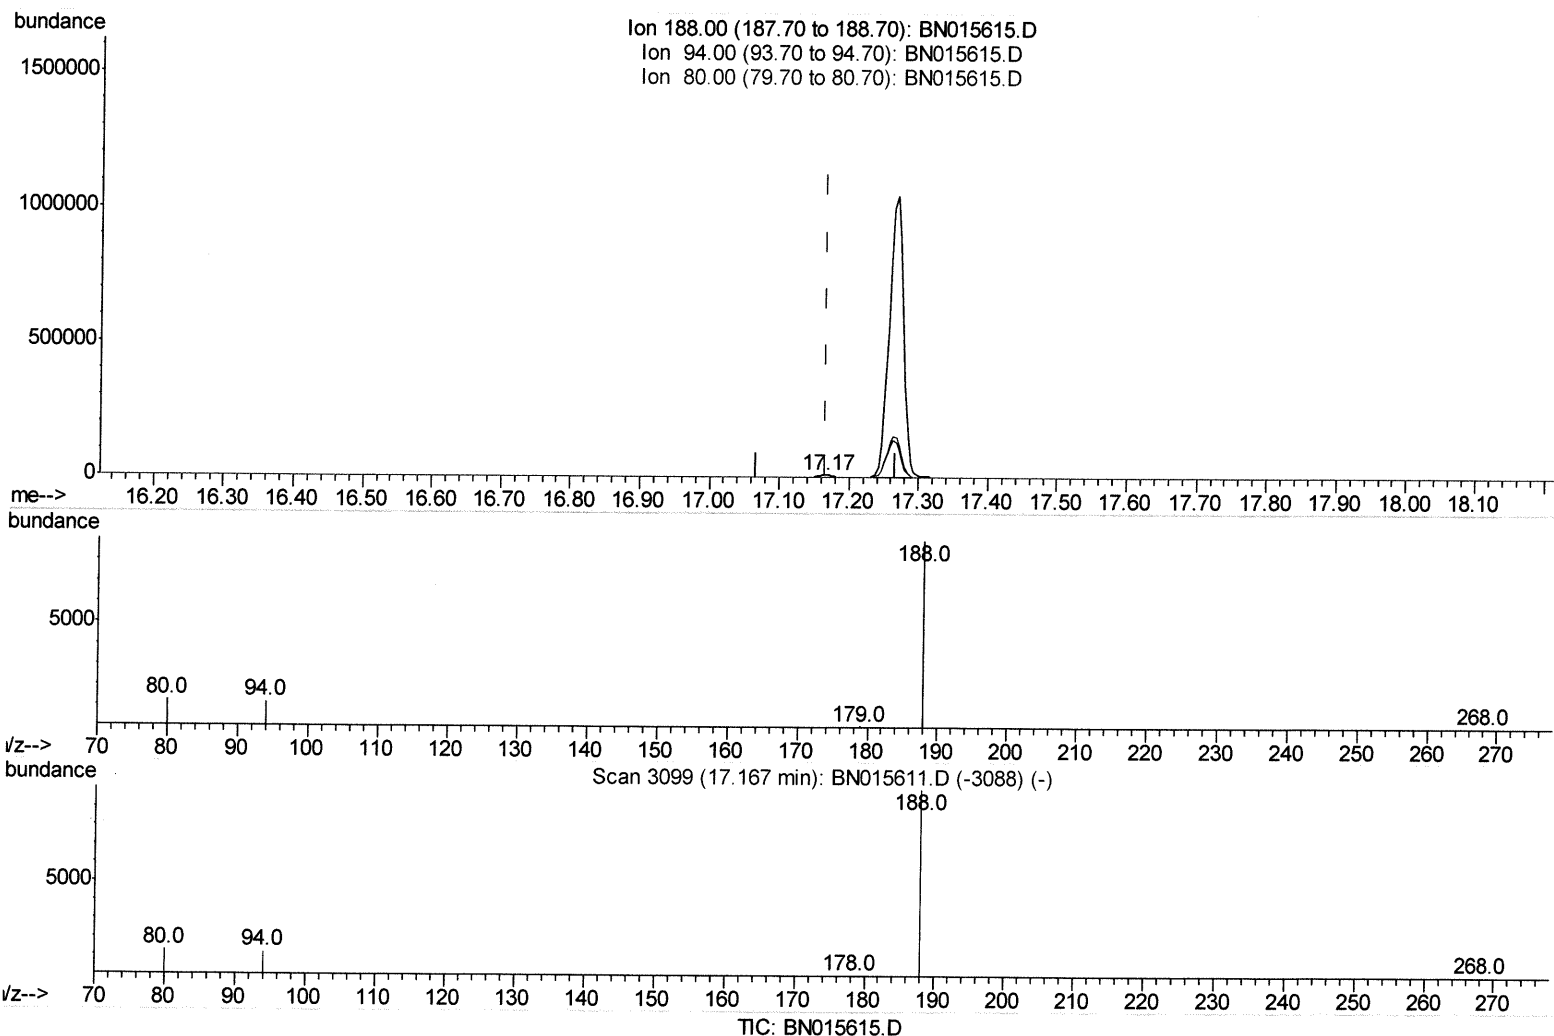

(13) Phenanthrene-d10 (I)

17.166min (-0.001) 0.40ng/ul m

response 12526

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	12.80
80.00	12.50	13.94
0.00	0.00	0.00

547/21/21


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071921\
 Data File : BN015615.D
 Acq On : 19 Jul 2021 19:23
 Operator : CG/JU
 Sample : SP5623
 Misc : SFAM SURROGATE
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP5623

Quant Time: Jul 20 01:10:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 19 13:54:50 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 7/20/2021 11:38:53 AM

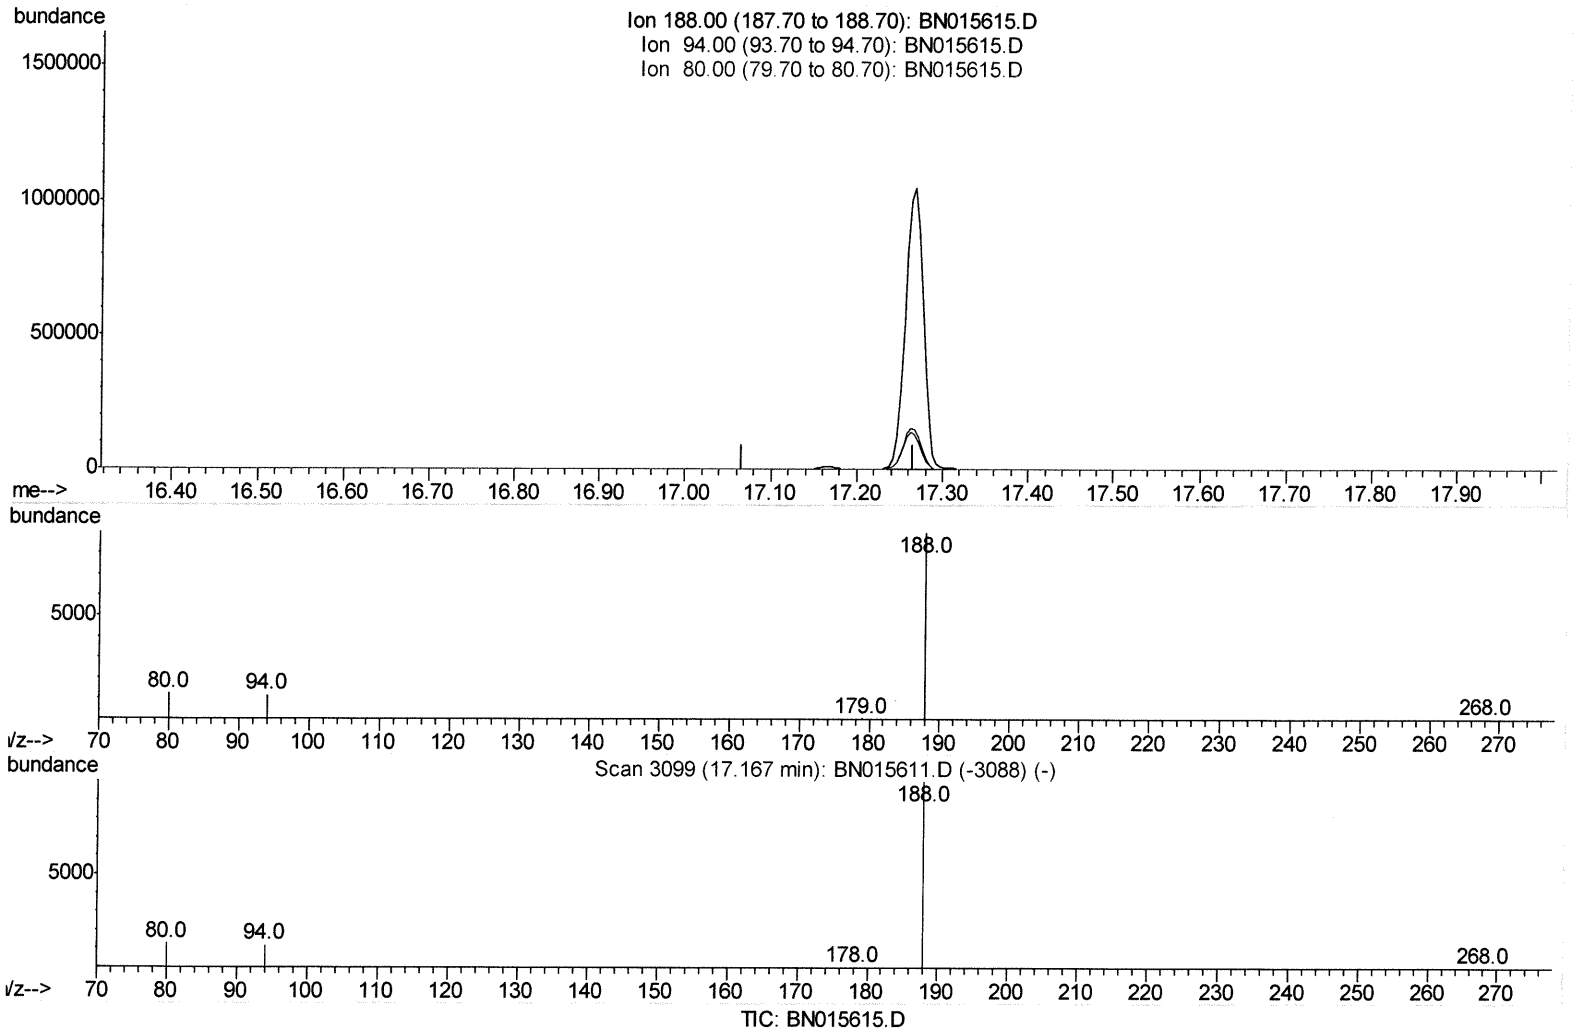

(13) Phenanthrene-d10 (I)

17.167min (-17.167) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071921\
 Data File : BN015615.D
 Acq On : 19 Jul 2021 19:23
 Operator : CG/JU
 Sample : SP5623
 Misc : SFAM SURROGATE
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SP5623

Quant Time: Jul 20 01:13:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 19 13:54:50 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 7/20/2021 11:38:53 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	2550	0.40	ng/ul	0.00
4) Naphthalene-d8	10.56	136	9239	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.42	164	6166	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.17	188	12526m	0.40	ng/ul	0.00
17) Chrysene-d12	21.37	240	9405	0.40	ng/ul	0.00
23) Perylene-d12	23.70	264	9952	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	37765	13.14	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	12.16	152	9112	0.63	ng/ul	0.00
18) Fluoranthene-d10	19.20	212	20273	0.66	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7/20/21/21