

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
 Data File : BN020770.D
 Acq On : 19 Jul 2022 12:11
 Operator : CG/JU
 Sample : N3753-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBHP4

Quant Time: Jul 20 01:04:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 01:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.821	152	2121	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	8532	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.469	164	5371	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.221	188	9528	0.400	ng/ul	0.00
17) Chrysene-d12	21.433	240	9596	0.400	ng/ul	0.00
23) Perylene-d12	23.772	264	11648	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	12971	5.279	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	4268	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.257	212	13252	0.419	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.620	202	1807	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.623	252	4026	0.082	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
Data File : BN020770.D
Acq On : 19 Jul 2022 12:11
Operator : CG/JU
Sample : N3753-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBHP4

Quant Time: Jul 20 01:04:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 01:02:30 2022
Response via : Initial Calibration




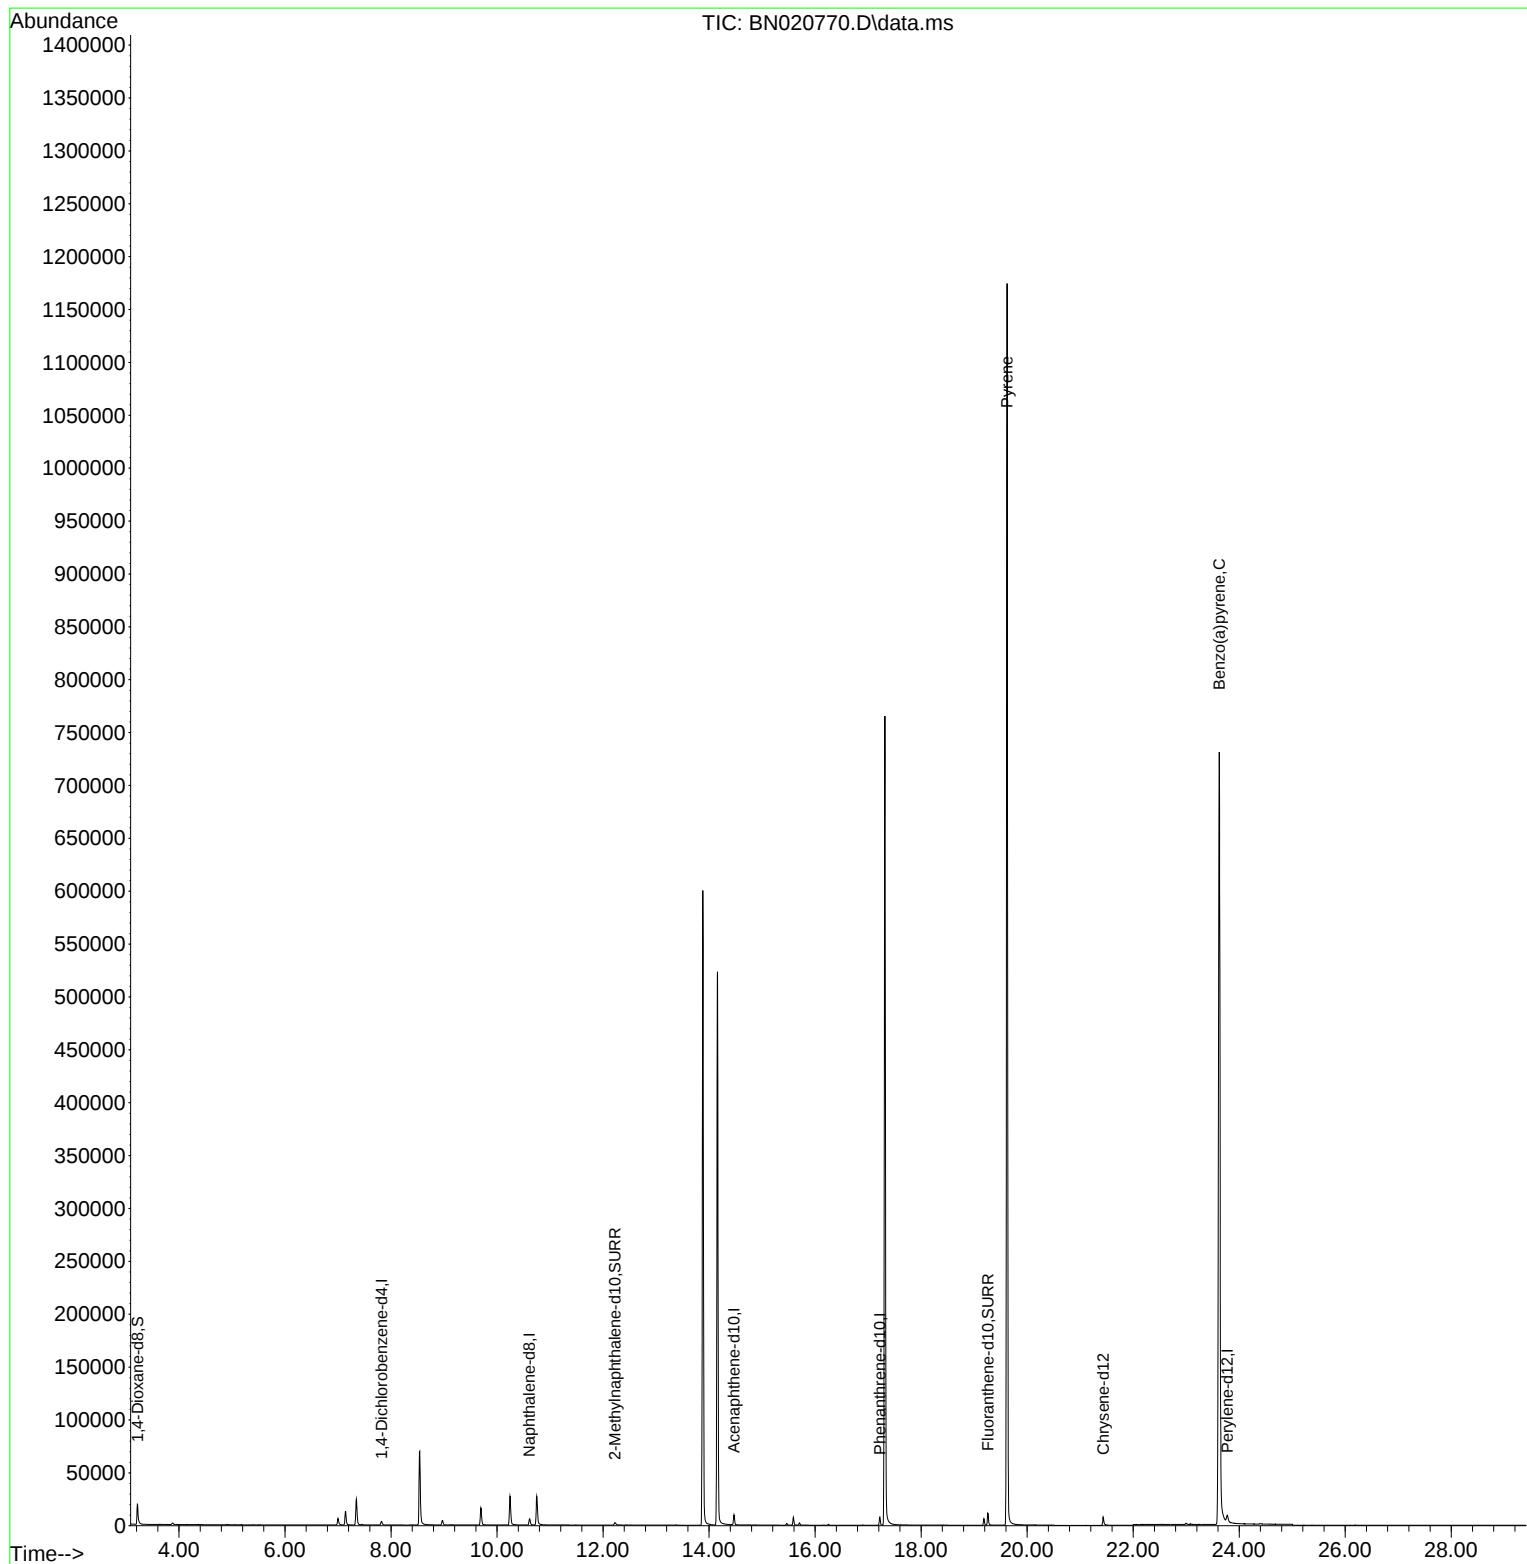


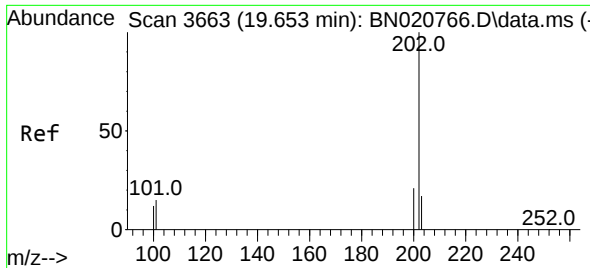

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.620 min Scan# 3656
Delta R.T. -0.033 min
Lab File: BN020770.D
Acq: 19 Jul 2022 12:11

Instrument :
BNA_N
ClientSampleId :
GBHP4

Tgt Ion:202 Resp: 1807
Ion Ratio Lower Upper
202 100
101 185.6 11.6 17.4#
100 1357.9 9.2 13.8#

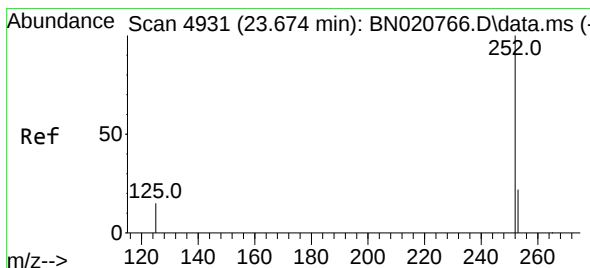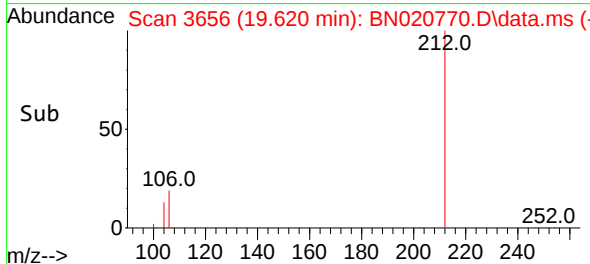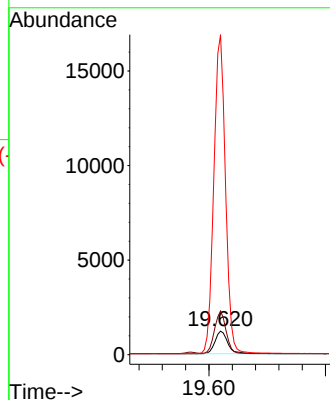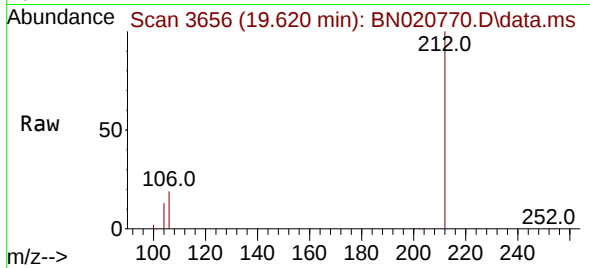

#26
Benzo(a)pyrene
Concen: 0.082 ng/ul
RT: 23.623 min Scan# 4913
Delta R.T. -0.052 min
Lab File: BN020770.D
Acq: 19 Jul 2022 12:11

Tgt Ion:252 Resp: 4026
Ion Ratio Lower Upper
252 100
253 42.6 21.0 31.4#
125 33.2 18.8 28.2#

