

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
 Data File : BN020774.D
 Acq On : 19 Jul 2022 14:39
 Operator : CG/JU
 Sample : N3704-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ5

Quant Time: Jul 20 01:05:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 01:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.821	152	2286	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	7913	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.469	164	4921	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.221	188	10566	0.400	ng/ul	0.00
17) Chrysene-d12	21.434	240	9456	0.400	ng/ul	0.00
23) Perylene-d12	23.778	264	10523	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	15856	5.987	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.218	152	4750	0.366	ng/ul	0.00
18) Fluoranthene-d10	19.258	212	13886	0.445	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.667	128	495	0.020	ng/ul#	48
20) Pyrene	19.625	202	1874	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.626	252	3769	0.085	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
Data File : BN020774.D
Acq On : 19 Jul 2022 14:39
Operator : CG/JU
Sample : N3704-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ5


Quant Time: Jul 20 01:05:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 01:02:30 2022
Response via : Initial Calibration

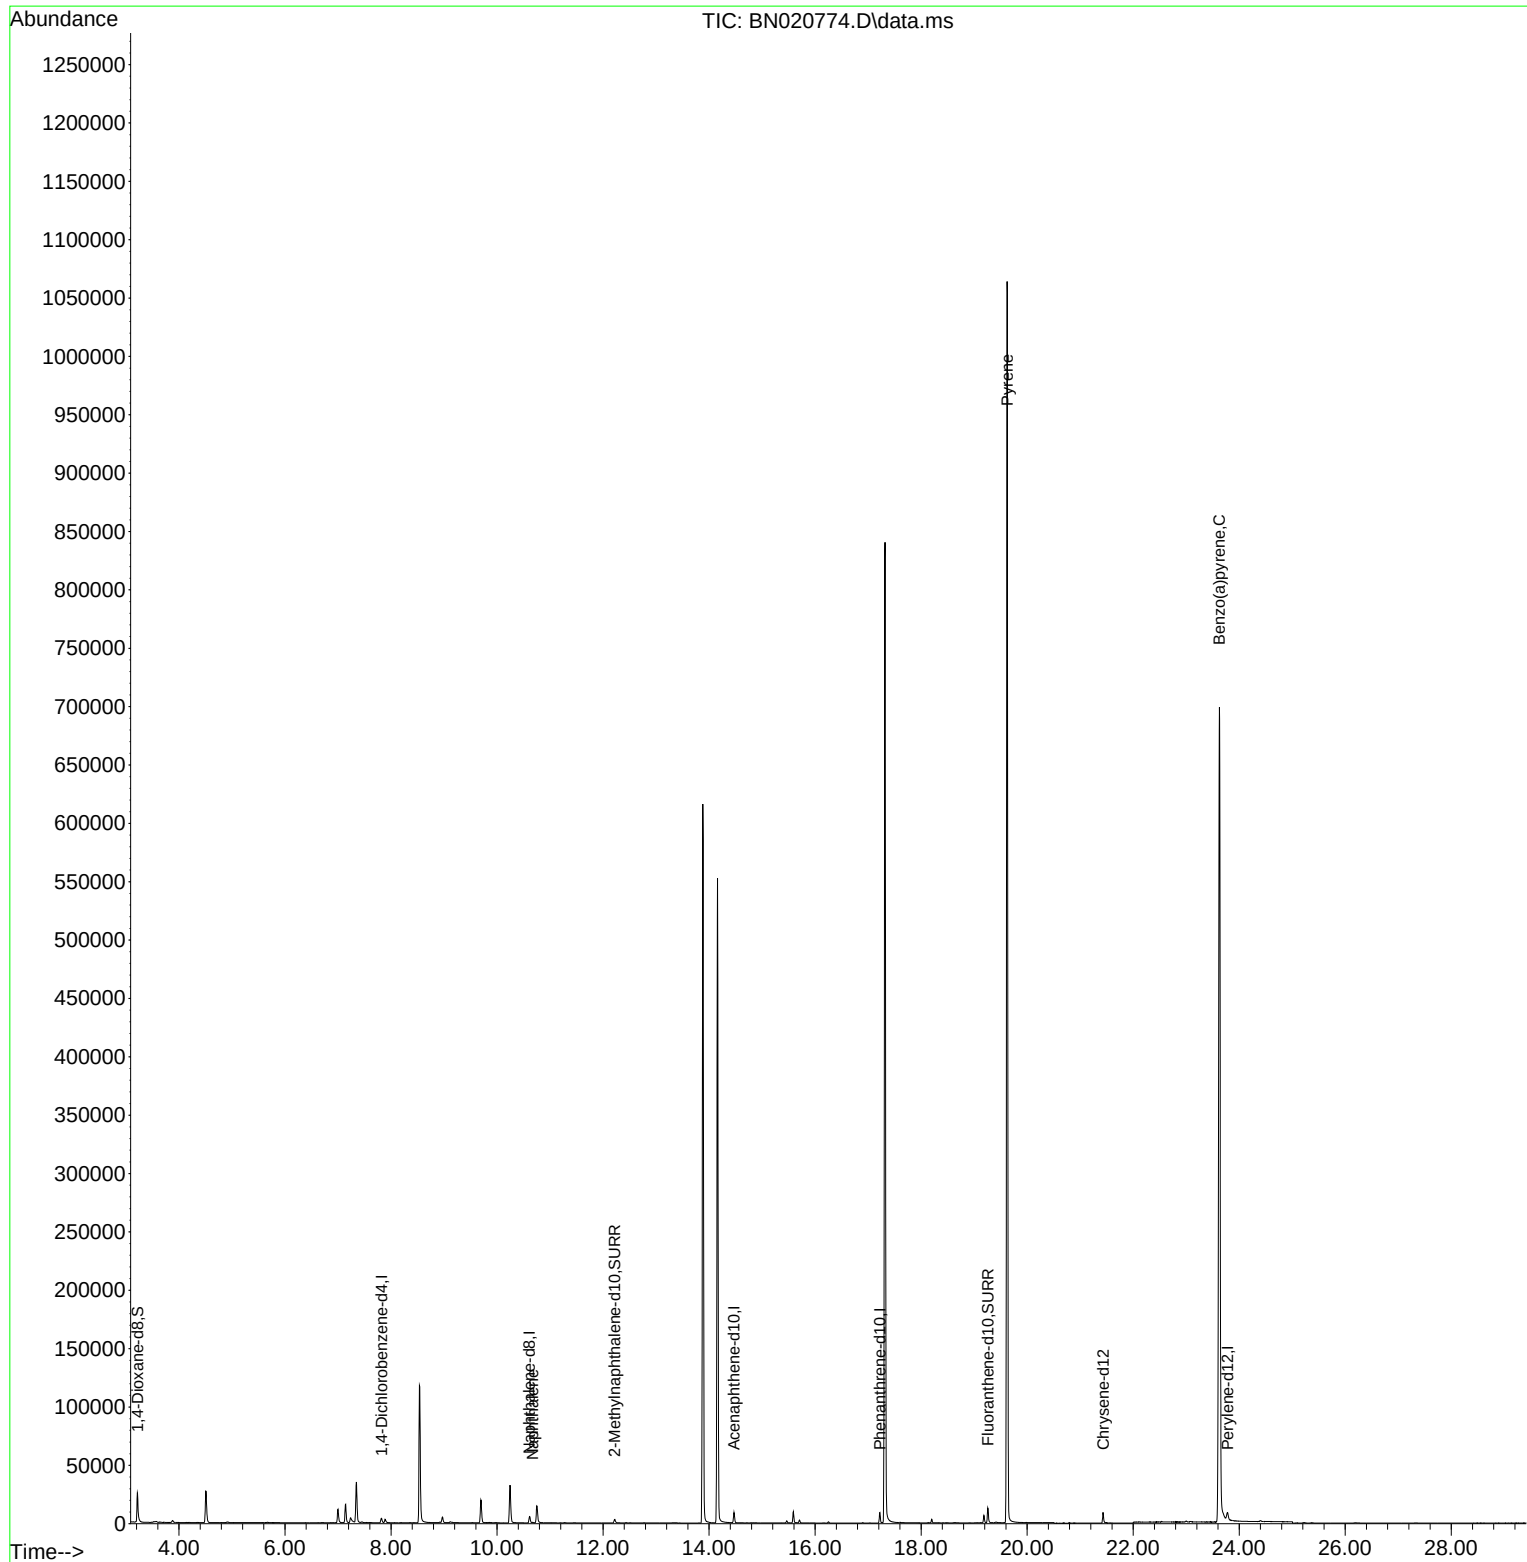



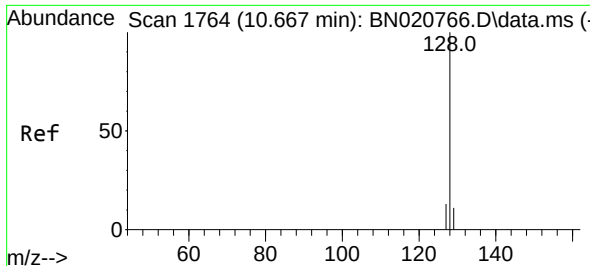


#5
Naphthalene
Concen: 0.020 ng/ul
RT: 10.667 min Scan# 1764
Delta R.T. 0.000 min
Lab File: BN020774.D
Acq: 19 Jul 2022 14:39

Instrument :
BNA_N
ClientSampleId :
C0AJ5



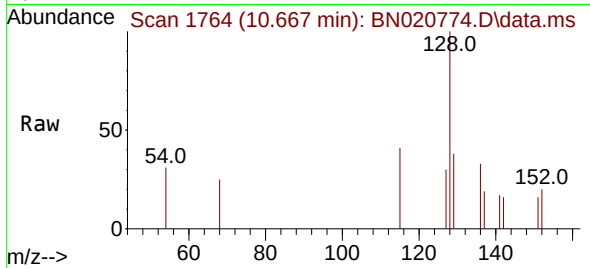



Tgt Ion:128 Resp: 495
Ion Ratio Lower Upper
128 100
129 37.9 9.5 14.3#
127 30.0 11.3 16.9#

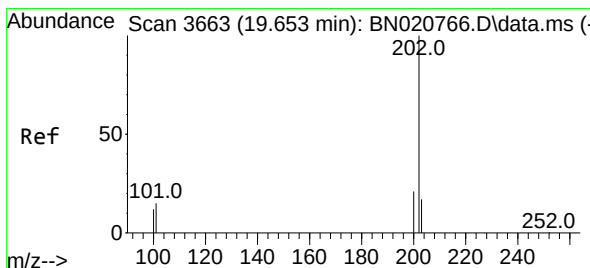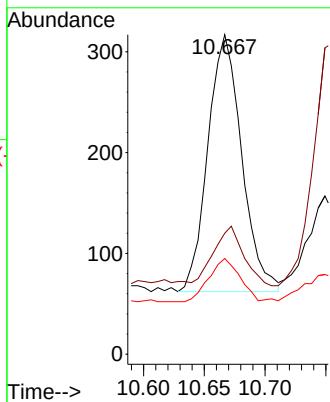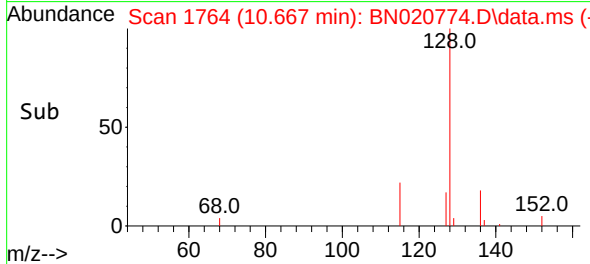

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.625 min Scan# 3657
Delta R.T. -0.029 min
Lab File: BN020774.D
Acq: 19 Jul 2022 14:39


Tgt Ion:202 Resp: 1874
Ion Ratio Lower Upper
202 100
101 170.1 11.6 17.4#
100 1199.5 9.2 13.8#

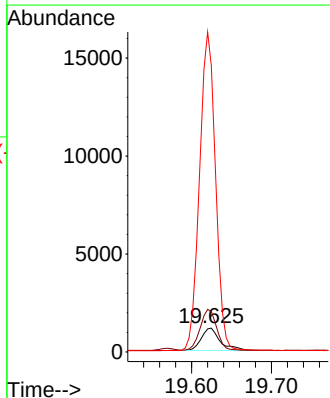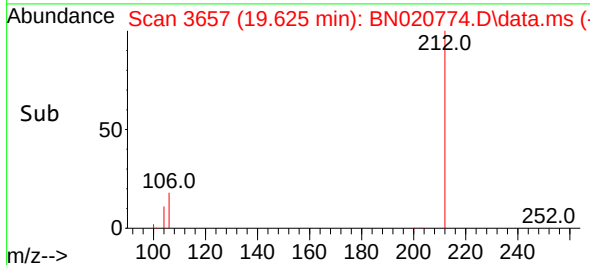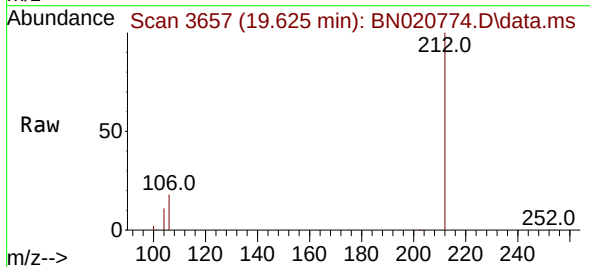

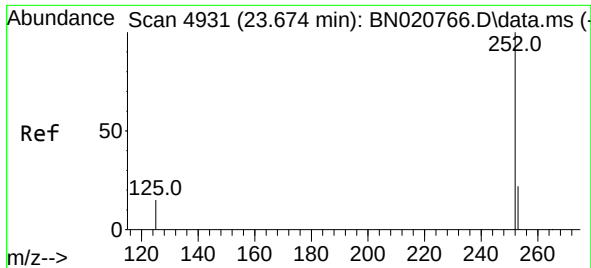

#26
 Benzo(a)pyrene
 Concen: 0.085 ng/ul
 RT: 23.626 min Scan# 4914
 Delta R.T. -0.049 min
 Lab File: BN020774.D
 Acq: 19 Jul 2022 14:39

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ5

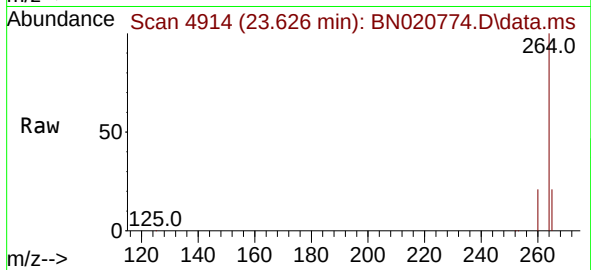

Tgt Ion:252 Resp: 3769
 Ion Ratio Lower Upper
 252 100
 253 44.5 21.0 31.4#
 125 41.2 18.8 28.2#

