

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
 Data File : BN020779.D
 Acq On : 19 Jul 2022 17:46
 Operator : CG/JU
 Sample : N3753-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBHQ4

Quant Time: Jul 20 01:05:26 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 01:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.821	152	2648	0.400	ng/ul	0.00
4) Naphthalene-d8	10.616	136	8073	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.473	164	5964	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.220	188	12579	0.400	ng/ul	0.00
17) Chrysene-d12	21.435	240	10324	0.400	ng/ul	0.00
23) Perylene-d12	23.777	264	12405	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	14332	4.672	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.222	152	5157	0.389	ng/ul	0.00
18) Fluoranthene-d10	19.261	212	15305	0.450	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.623	202	2008	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.625	252	4315	0.083	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
Data File : BN020779.D
Acq On : 19 Jul 2022 17:46
Operator : CG/JU
Sample : N3753-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBHQ4

Quant Time: Jul 20 01:05:26 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 01:02:30 2022
Response via : Initial Calibration




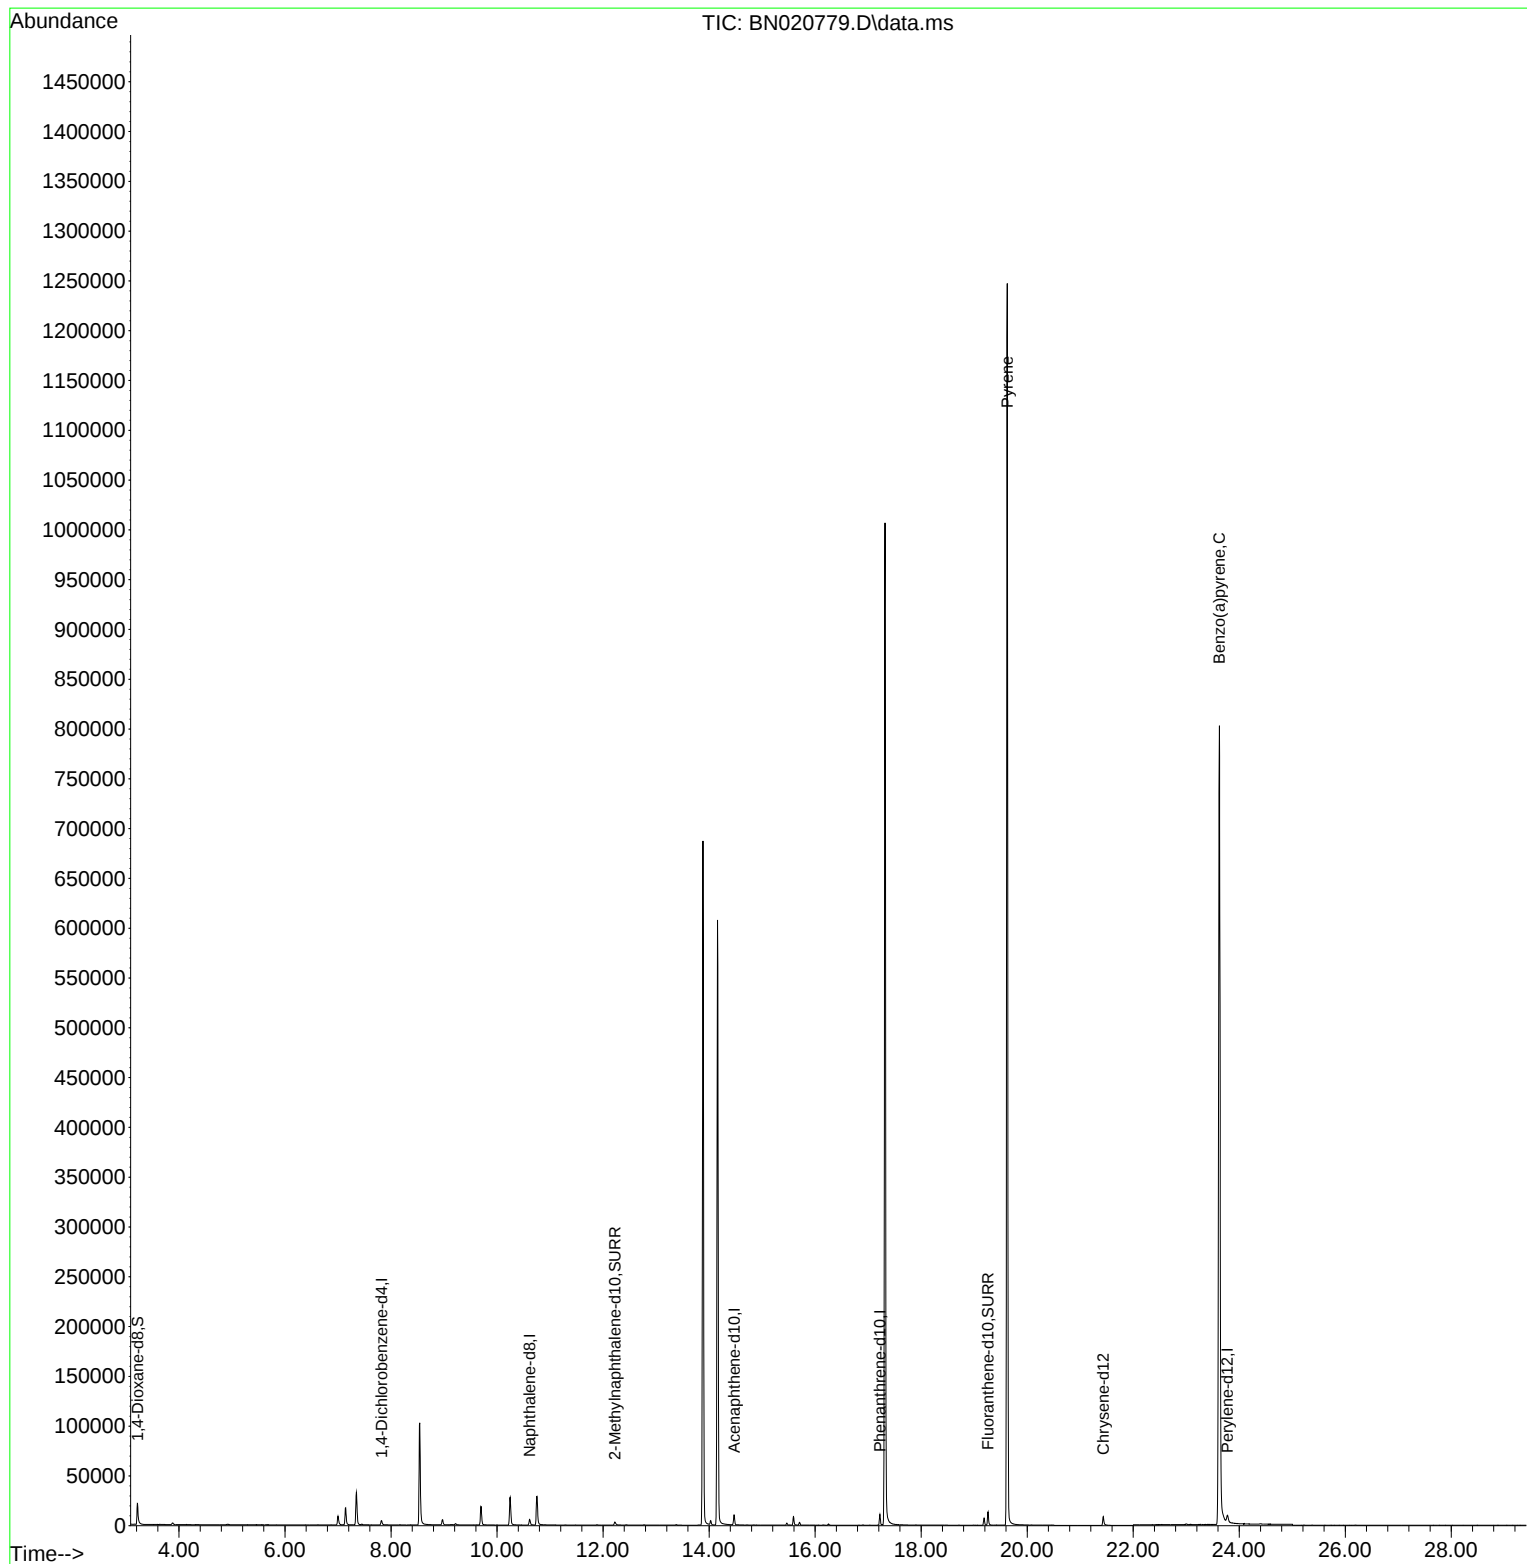


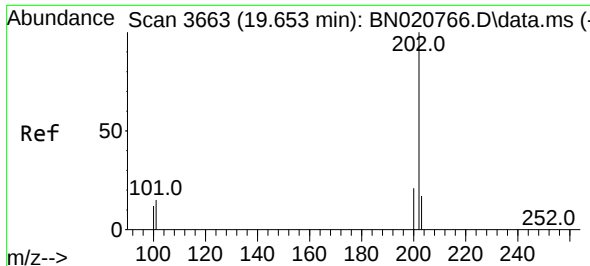

#20
Pyrene
Concen: 0.041 ng/ul
RT: 19.623 min Scan# 30
Delta R.T. -0.030 min
Lab File: BN020779.D
Acq: 19 Jul 2022 17:46

Instrument :
BNA_N
ClientSampleId :
GBHQ4

Tgt Ion:202 Resp: 2008
Ion Ratio Lower Upper
202 100
101 177.7 11.6 17.4#
100 1276.7 9.2 13.8#

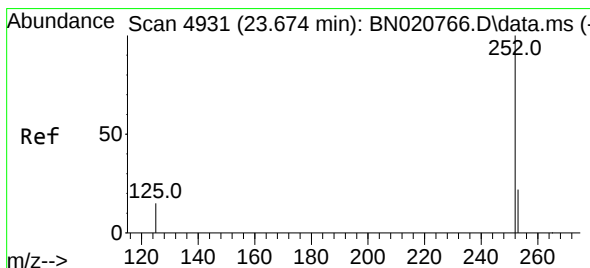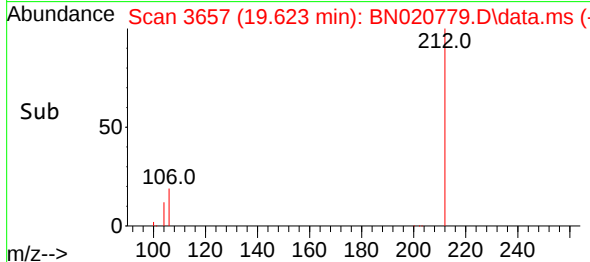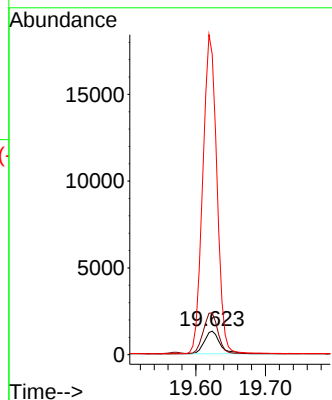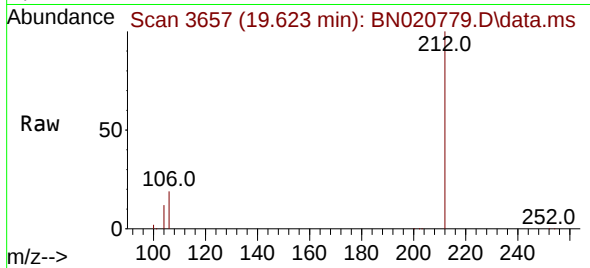

#26
Benzo(a)pyrene
Concen: 0.083 ng/ul
RT: 23.625 min Scan# 4914
Delta R.T. -0.050 min
Lab File: BN020779.D
Acq: 19 Jul 2022 17:46

Tgt Ion:252 Resp: 4315
Ion Ratio Lower Upper
252 100
253 40.6 21.0 31.4#
125 33.0 18.8 28.2#

