

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
 Data File : BN020783.D
 Acq On : 19 Jul 2022 20:53
 Operator : CG/JU
 Sample : PB146297BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK297

Quant Time: Jul 20 01:05:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 01:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	2782	0.400	ng/ul	0.00
4) Naphthalene-d8	10.617	136	8108	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.469	164	5904	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.221	188	12380	0.400	ng/ul	0.00
17) Chrysene-d12	21.432	240	9126	0.400	ng/ul	0.00
23) Perylene-d12	23.770	264	12030	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	18135	5.627	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.228	152	4694	0.353	ng/ul	0.01
18) Fluoranthene-d10	19.262	212	10924	0.363	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.464	166	1613	0.061	ng/ul#	15
20) Pyrene	19.620	202	1383	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.618	252	3592	0.071	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
Data File : BN020783.D
Acq On : 19 Jul 2022 20:53
Operator : CG/JU
Sample : PB146297BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK297

Quant Time: Jul 20 01:05:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 01:02:30 2022
Response via : Initial Calibration




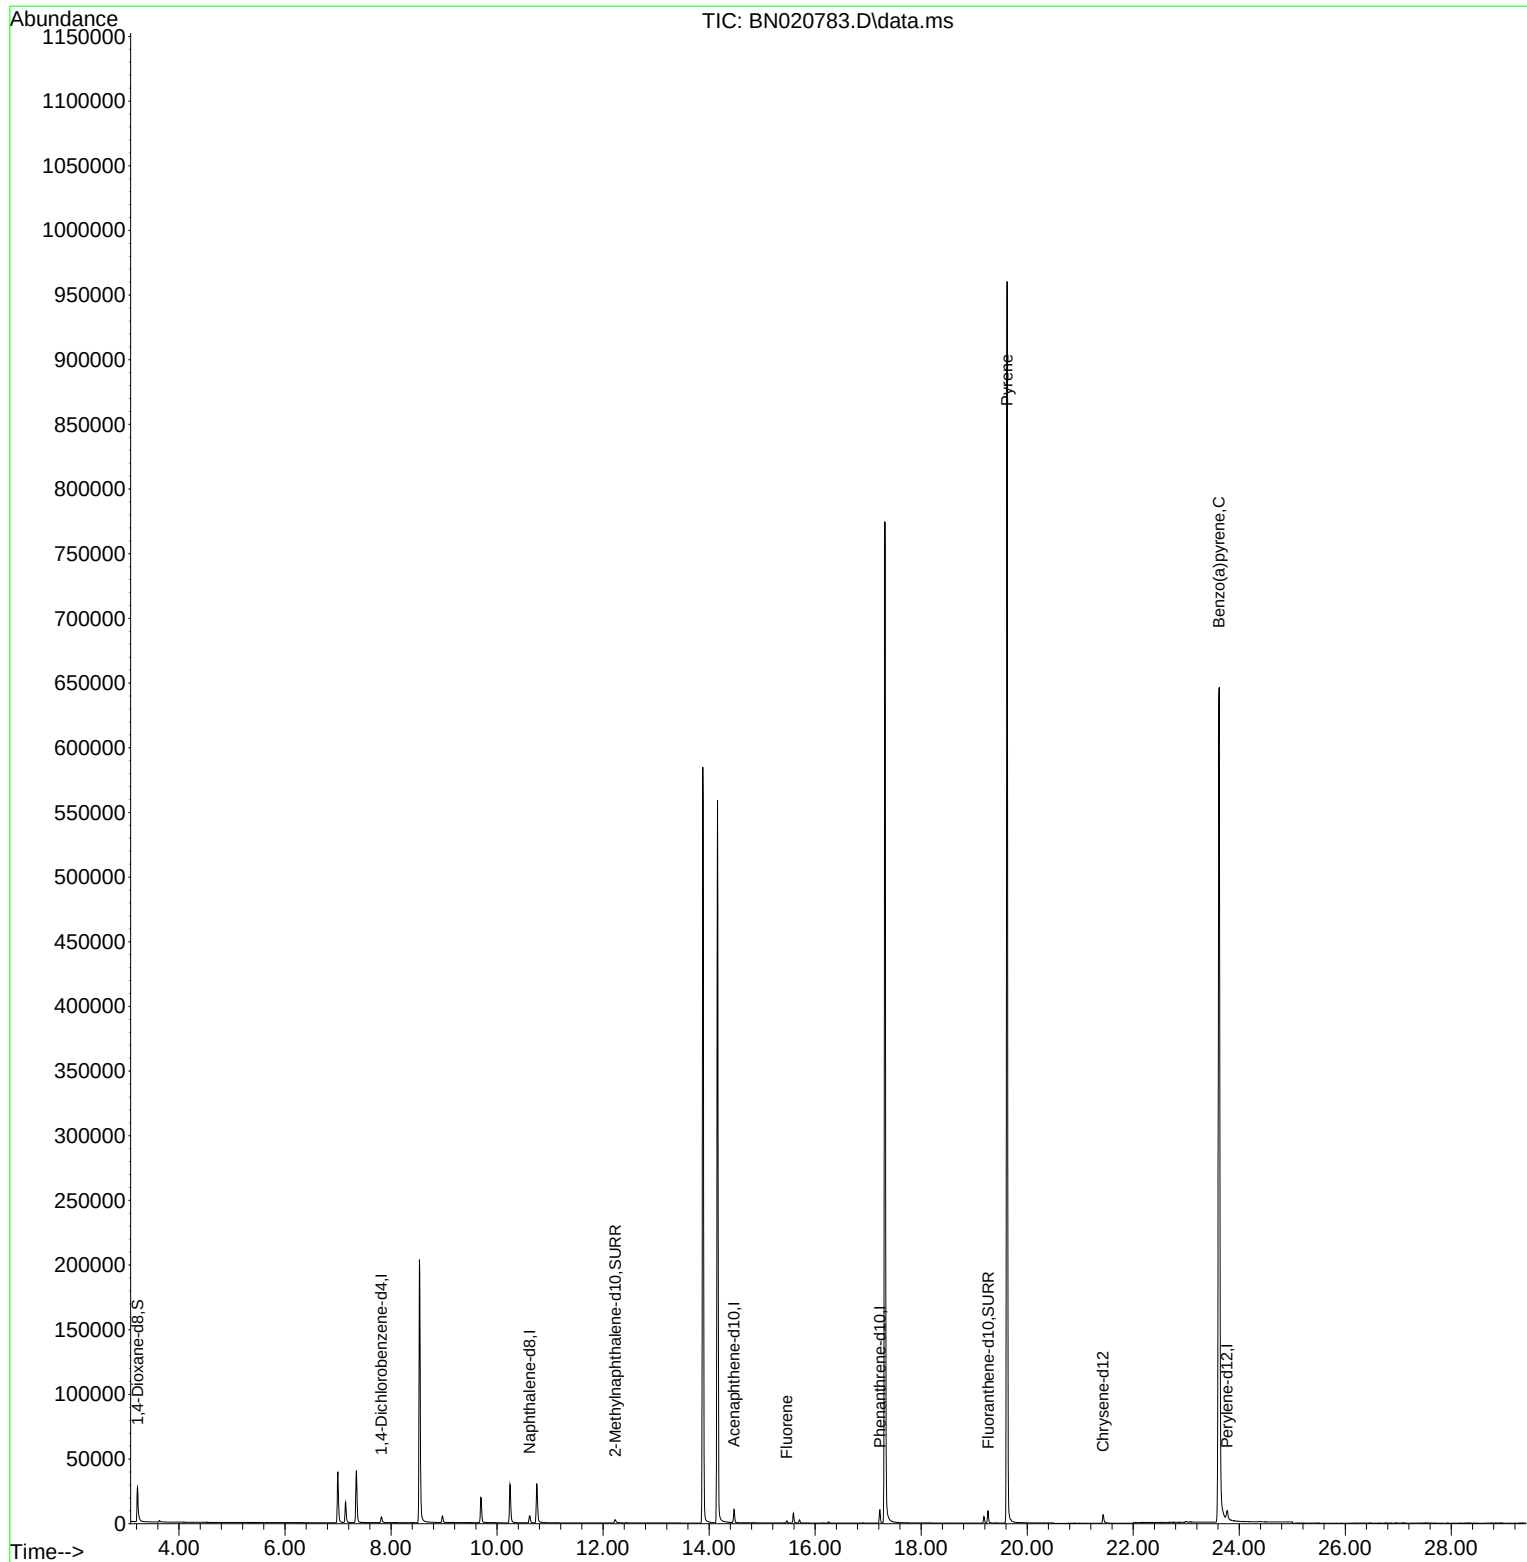


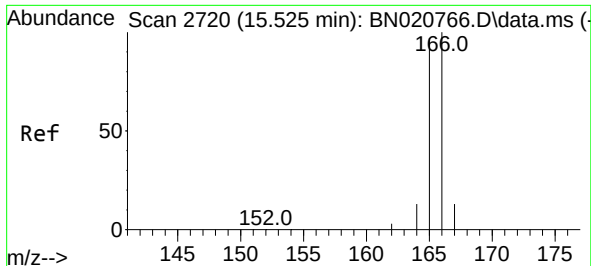

#12
Fluorene
Concen: 0.061 ng/ul
RT: 15.464 min Scan# 21
Delta R.T. -0.061 min
Lab File: BN020783.D
Acq: 19 Jul 2022 20:53




Instrument :
BNA_N
ClientSampleId :
SBLK297


Tgt Ion:166 Resp: 1613
Ion Ratio Lower Upper
166 100
165 8.5 78.2 117.2#
167 34.7 11.3 16.9#

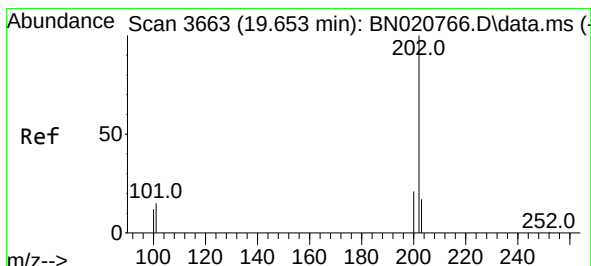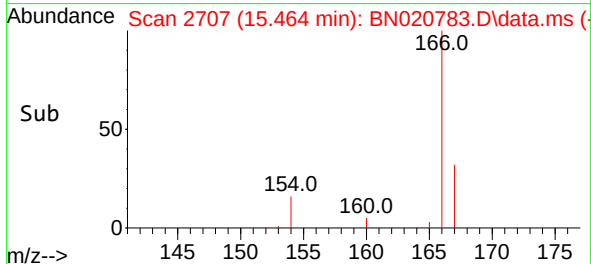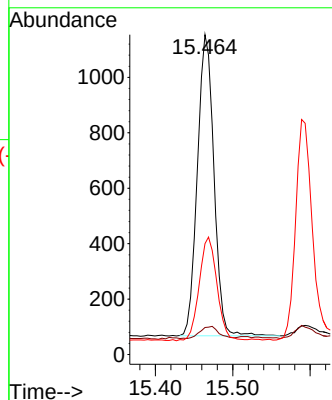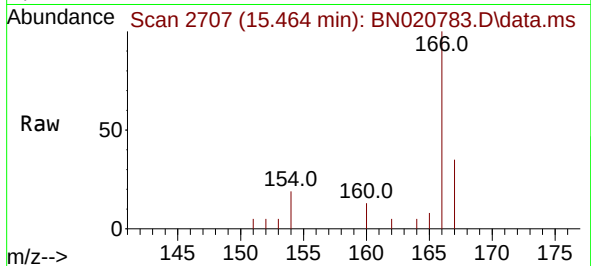

#20
Pyrene
Concen: 0.032 ng/ul
RT: 19.620 min Scan# 3656
Delta R.T. -0.033 min
Lab File: BN020783.D
Acq: 19 Jul 2022 20:53

Tgt Ion:202 Resp: 1383
Ion Ratio Lower Upper
202 100
101 180.5 11.6 17.4#
100 1343.4 9.2 13.8#

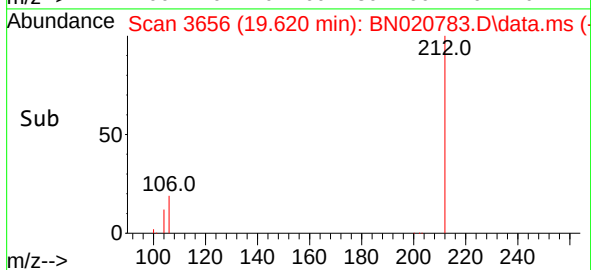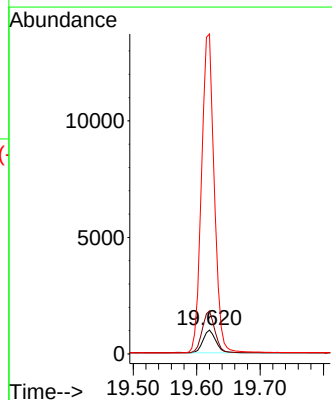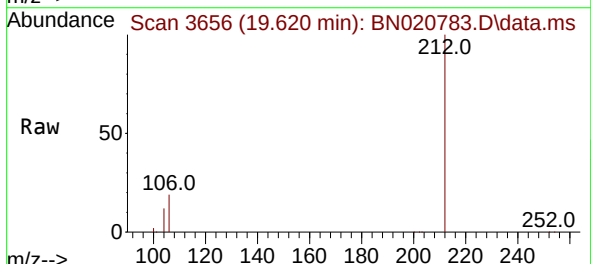

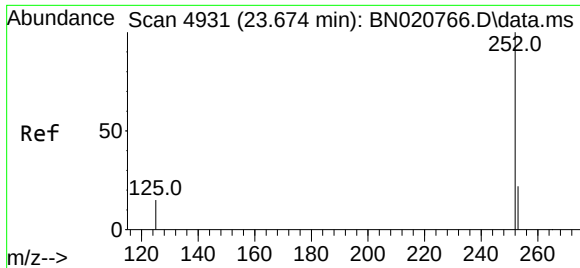

#26

Benzo(a)pyrene

Concen: 0.071 ng/ul

RT: 23.618 min Scan# 4912

Delta R.T. -0.056 min

Lab File: BN020783.D


Acq: 19 Jul 2022 20:53

Instrument :

BNA_N

ClientSampleId :

SBLK297

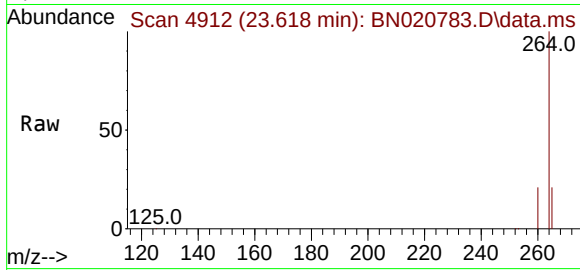

Tgt Ion:252 Resp: 3592

Ion Ratio Lower Upper

252 100

253 43.1 21.0 31.4#

125 34.0 18.8 28.2#

