

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
 Data File : BN020786.D
 Acq On : 19 Jul 2022 22:45
 Operator : CG/JU
 Sample : N3753-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBHP8

Quant Time: Jul 20 01:05:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 01:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	2627	0.400	ng/ul	0.00
4) Naphthalene-d8	10.617	136	9109	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.469	164	5029	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.221	188	9918	0.400	ng/ul	0.00
17) Chrysene-d12	21.427	240	10805	0.400	ng/ul	0.00
23) Perylene-d12	23.768	264	12106	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	10320	3.391	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	5067	0.339	ng/ul	0.00
18) Fluoranthene-d10	19.257	212	14390	0.404	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.251	88	73	0.023	ng/ul#	66
20) Pyrene	19.619	202	2081	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.613	252	4433	0.087	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
Data File : BN020786.D
Acq On : 19 Jul 2022 22:45
Operator : CG/JU
Sample : N3753-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBHP8


Quant Time: Jul 20 01:05:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 01:02:30 2022
Response via : Initial Calibration

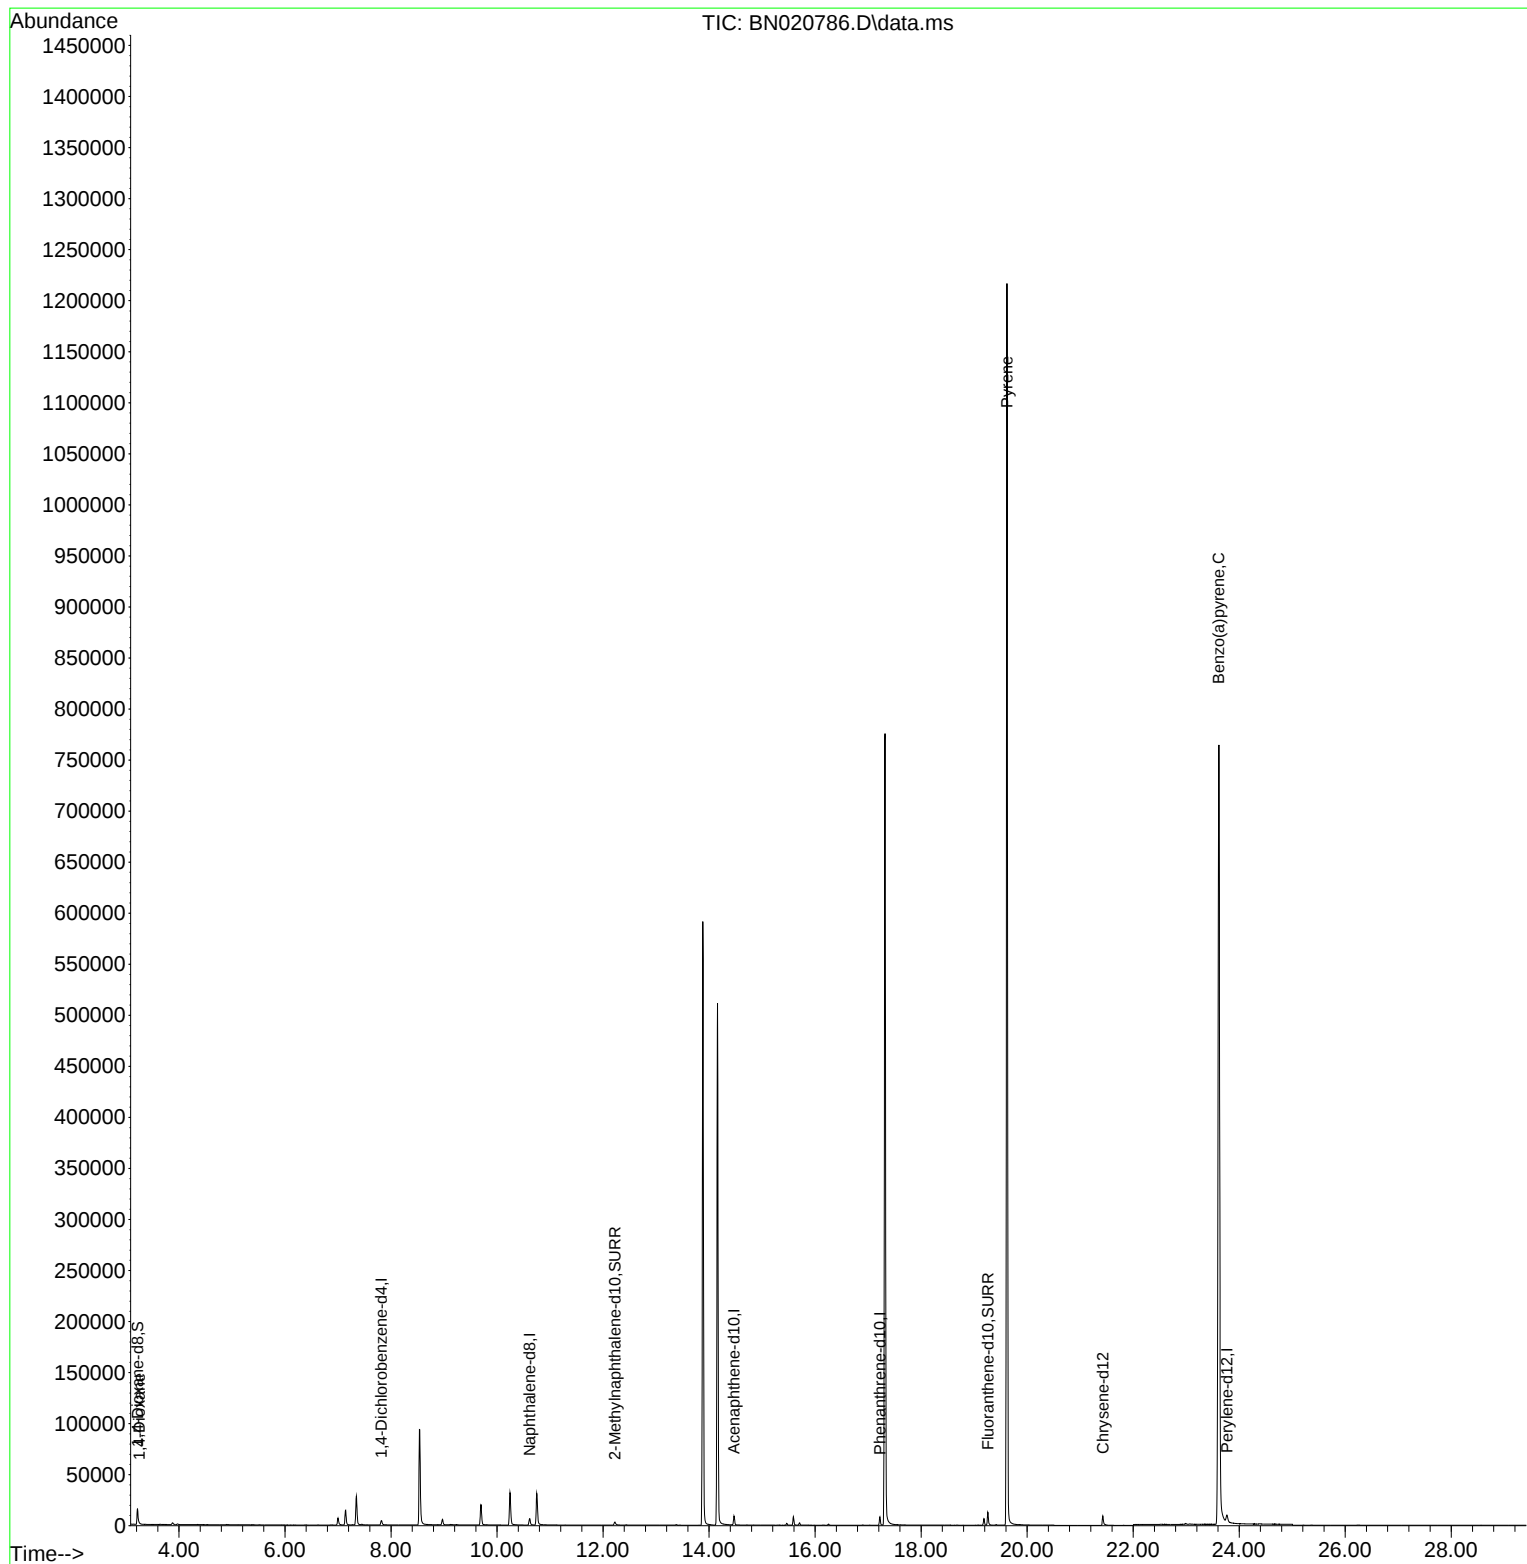

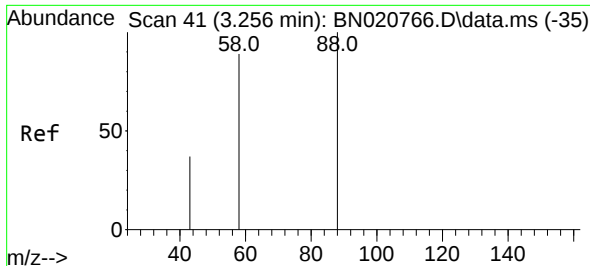




#2
 1,4-Dioxane
 Concen: 0.023 ng/ul
 RT: 3.251 min Scan# 40
 Delta R.T. -0.004 min
 Lab File: BN020786.D
 Acq: 19 Jul 2022 22:45

Instrument :
 BNA_N
 ClientSampleId :
 GBHP8

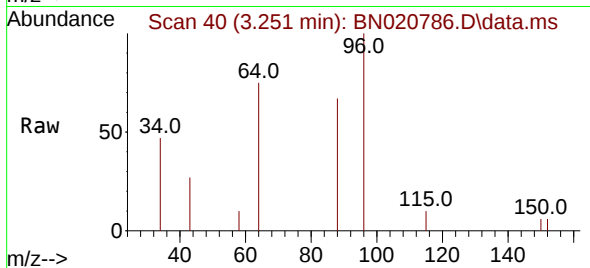


Tgt Ion: 88 Resp: 73

Ion	Ratio	Lower	Upper
88	100		
43	40.8	32.5	48.7
58	14.7	46.2	69.2#

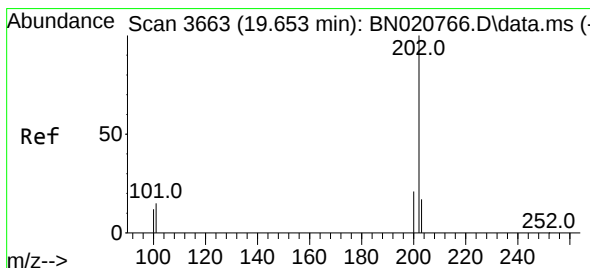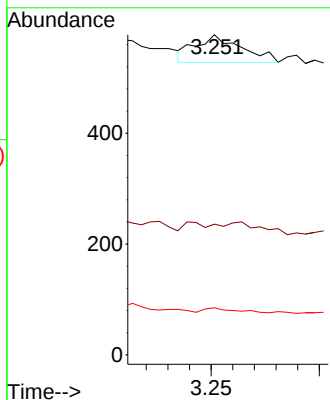
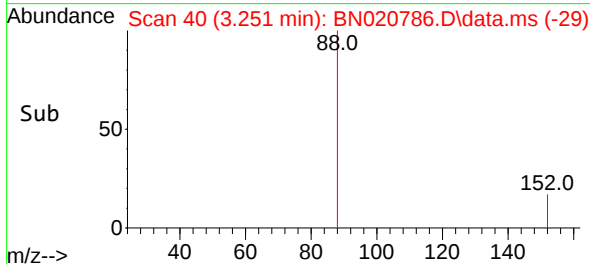



#20
 Pyrene
 Concen: 0.041 ng/ul
 RT: 19.619 min Scan# 3656
 Delta R.T. -0.034 min
 Lab File: BN020786.D
 Acq: 19 Jul 2022 22:45

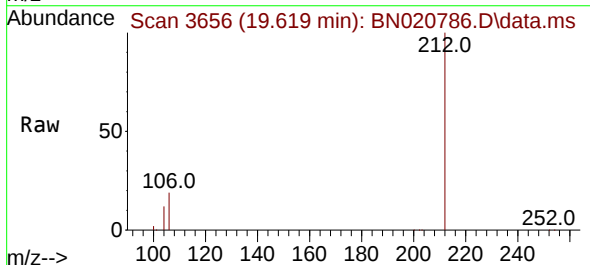

Tgt Ion: 202 Resp: 2081

Ion	Ratio	Lower	Upper
202	100		
101	179.3	11.6	17.4#
100	1305.1	9.2	13.8#

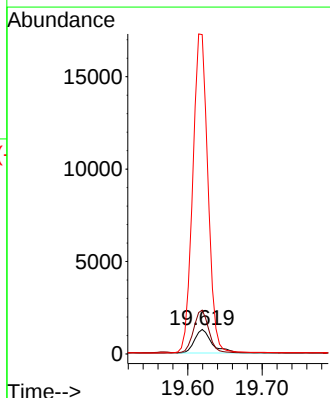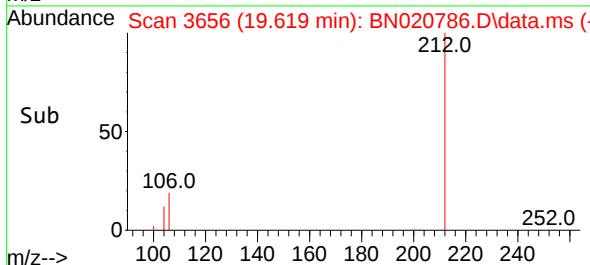

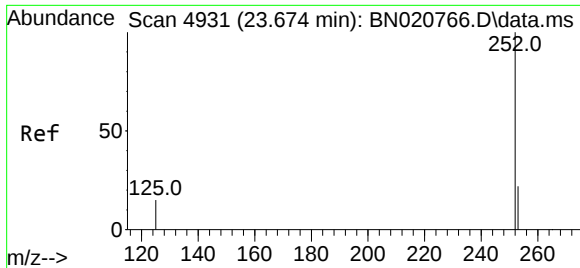

#26

Benzo(a)pyrene

Concen: 0.087 ng/ul

RT: 23.613 min Scan# 4910

Delta R.T. -0.061 min

Lab File: BN020786.D


Acq: 19 Jul 2022 22:45

Instrument :

BNA_N

ClientSampleId :

GBHP8

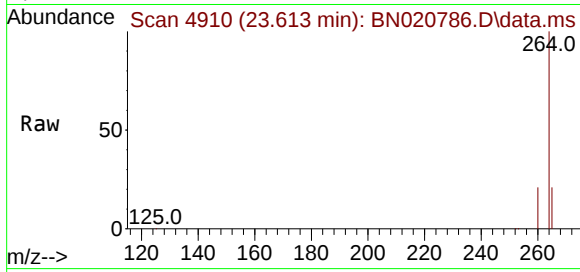

Tgt Ion:252 Resp: 4433

Ion Ratio Lower Upper

252 100

253 41.4 21.0 31.4#

125 34.4 18.8 28.2#

