

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
 Data File : BN020788.D
 Acq On : 19 Jul 2022 23:59
 Operator : CG/JU
 Sample : N3753-08
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBHP9

Quant Time: Jul 20 01:05:56 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 01:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	2328	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	9894	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.483	164	21932	0.400	ng/ul	# 0.01
13) Phenanthrene-d10	17.221	188	13245	0.400	ng/ul	0.00
17) Chrysene-d12	21.423	240	13143	0.400	ng/ul	0.00
23) Perylene-d12	23.767	264	13418	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	12599	4.671	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.218	152	5258	0.324	ng/ul	0.00
18) Fluoranthene-d10	19.258	212	15725	0.363	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.661	128	917	0.030	ng/ul#	76
20) Pyrene	19.620	202	1882	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.618	252	4123	0.073	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071922\
Data File : BN020788.D
Acq On : 19 Jul 2022 23:59
Operator : CG/JU
Sample : N3753-08
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBHP9

Quant Time: Jul 20 01:05:56 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 01:02:30 2022
Response via : Initial Calibration




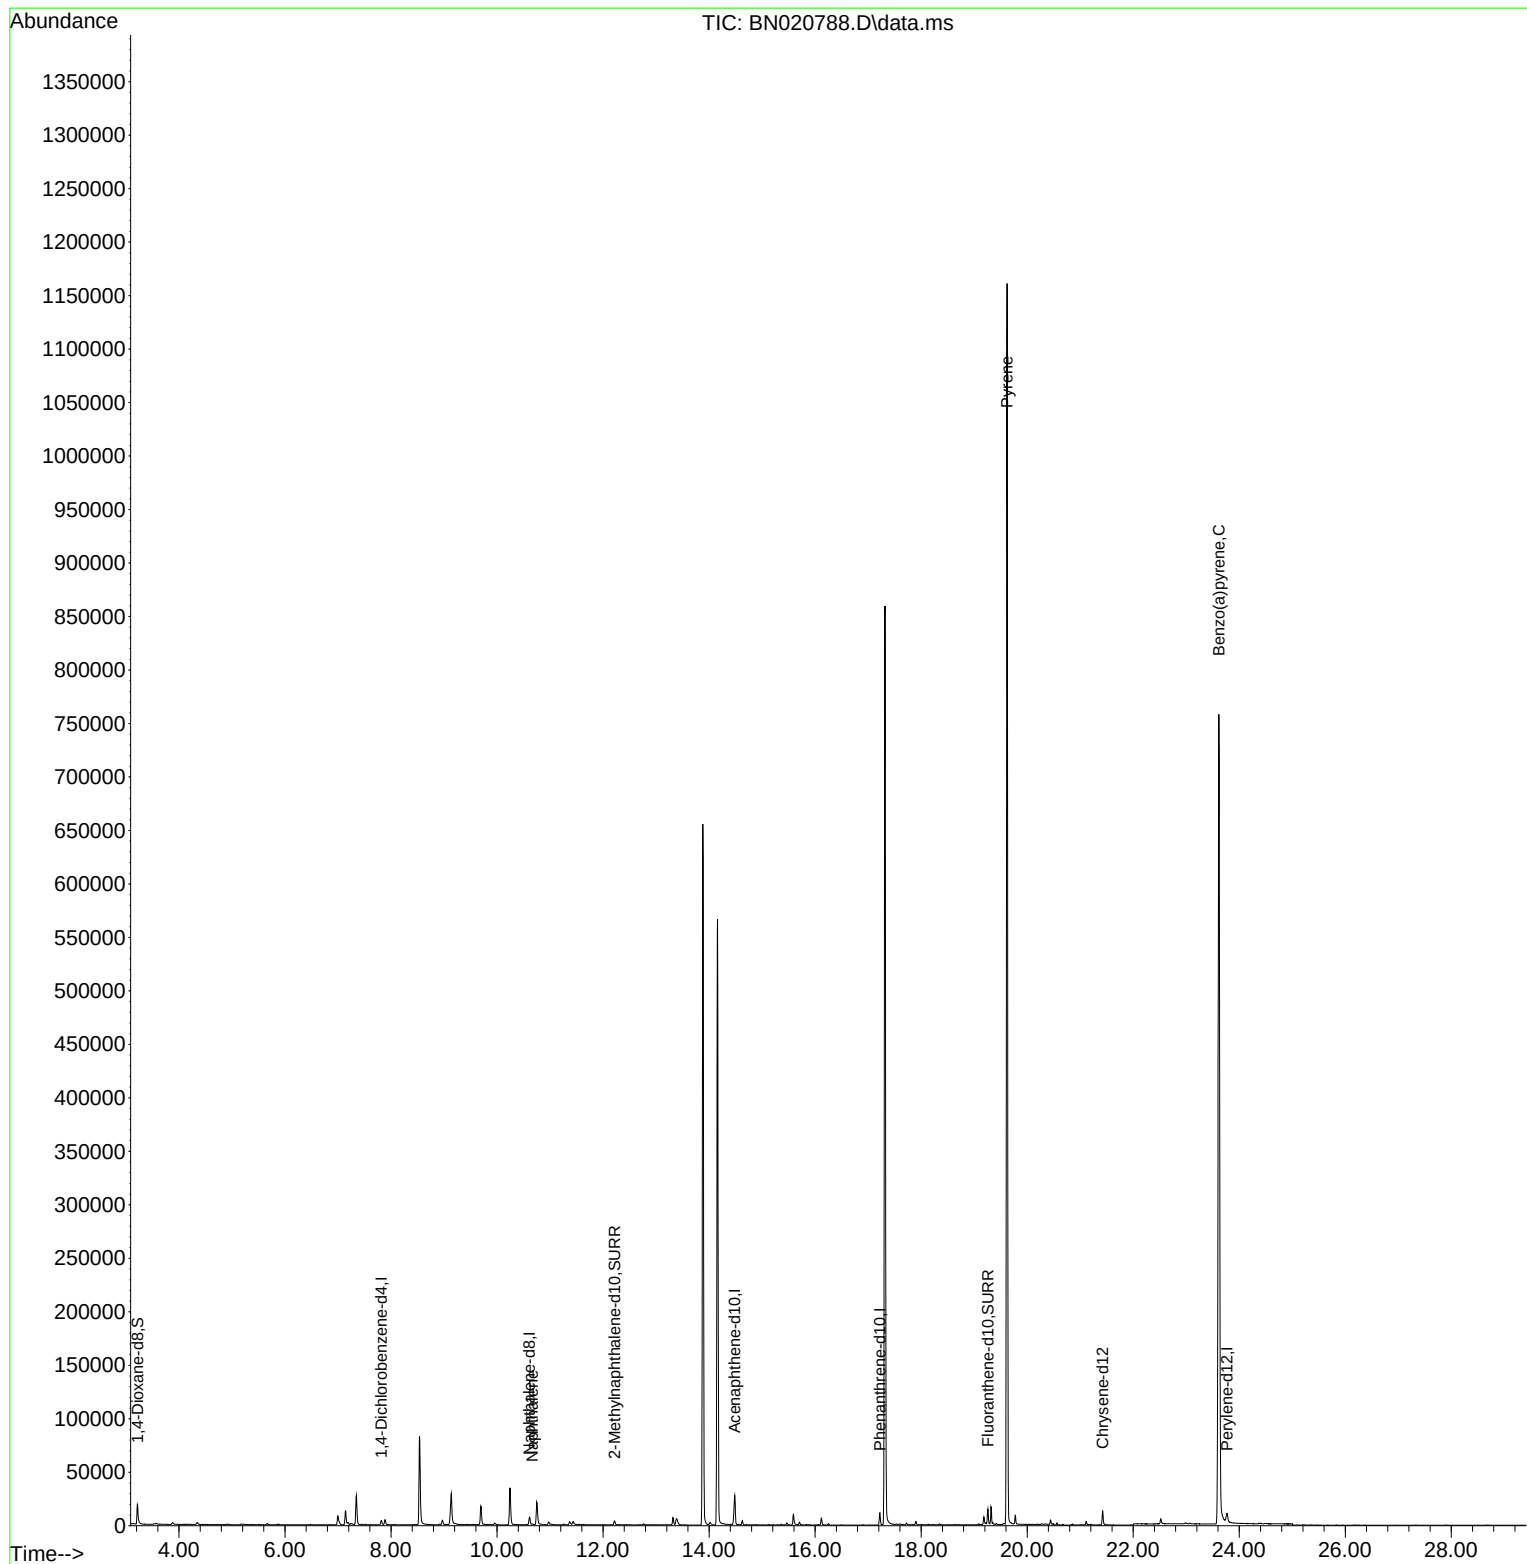


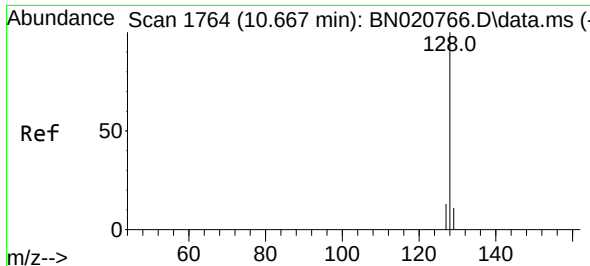

#5
Naphthalene
Concen: 0.030 ng/ul
RT: 10.661 min Scan# 1763
Delta R.T. -0.005 min
Lab File: BN020788.D
Acq: 19 Jul 2022 23:59




Instrument :
BNA_N
ClientSampleId :
GBHP9


Tgt Ion:128 Resp: 917
Ion Ratio Lower Upper
128 100
129 23.4 9.5 14.3#
127 21.8 11.3 16.9#

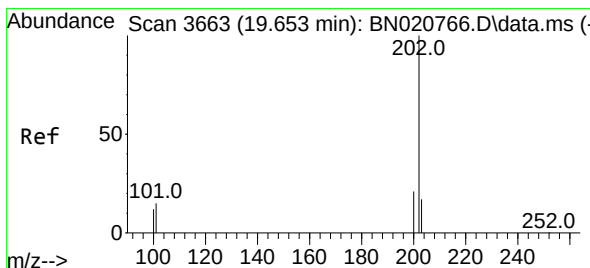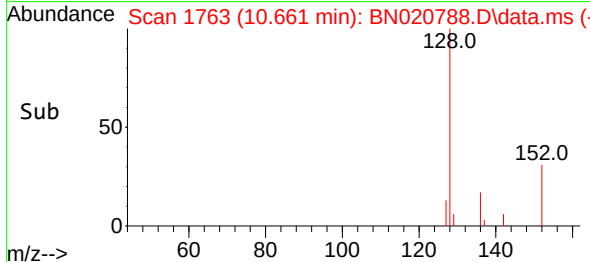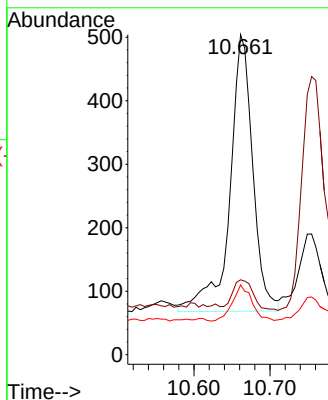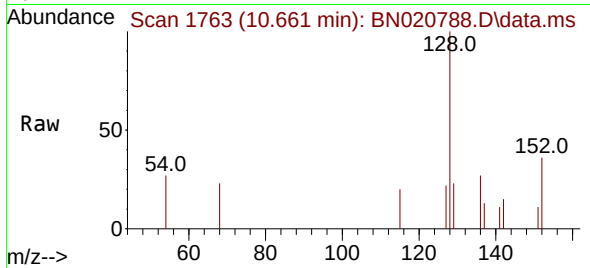

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.620 min Scan# 3656
Delta R.T. -0.033 min
Lab File: BN020788.D
Acq: 19 Jul 2022 23:59

Tgt Ion:202 Resp: 1882
Ion Ratio Lower Upper
202 100
101 177.3 11.6 17.4#
100 1248.9 9.2 13.8#

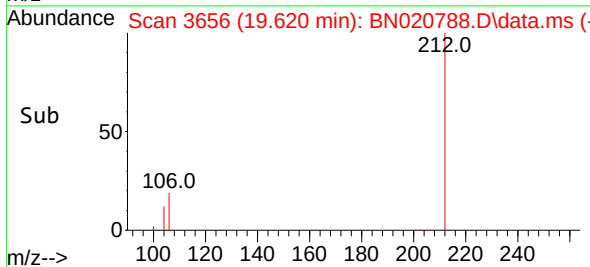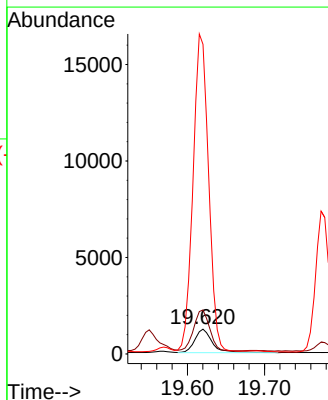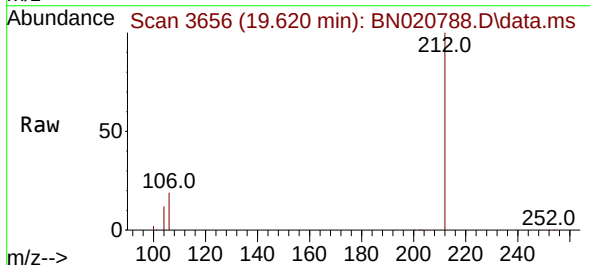

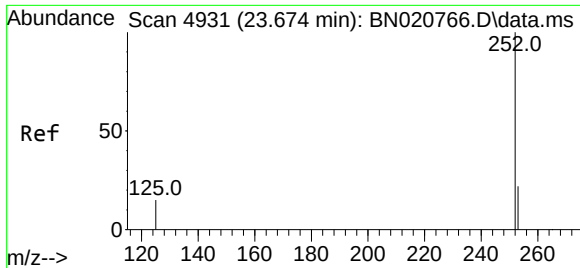

#26

Benzo(a)pyrene

Concen: 0.073 ng/ul

RT: 23.618 min Scan# 4912

Delta R.T. -0.056 min

Lab File: BN020788.D


Acq: 19 Jul 2022 23:59

Instrument :

BNA_N

ClientSampleId :

GBHP9

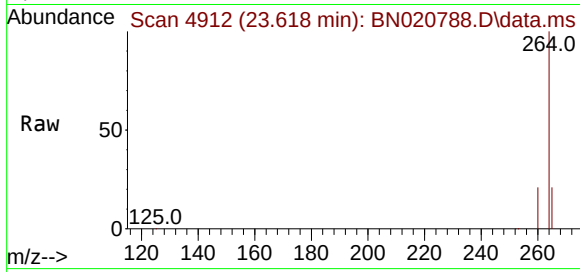

Tgt Ion:252 Resp: 4123

Ion Ratio Lower Upper

252 100

253 46.3 21.0 31.4#

125 38.2 18.8 28.2#

