
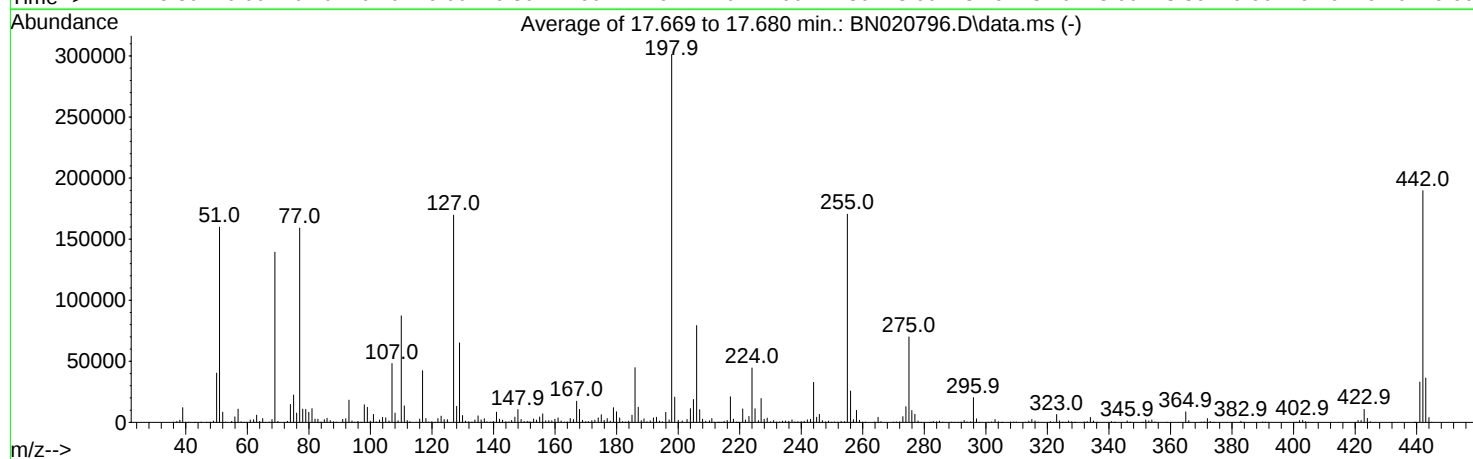


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072022\
 Data File : BN020796.D
 Acq On : 20 Jul 2022 08:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 16 03:21:59 2022

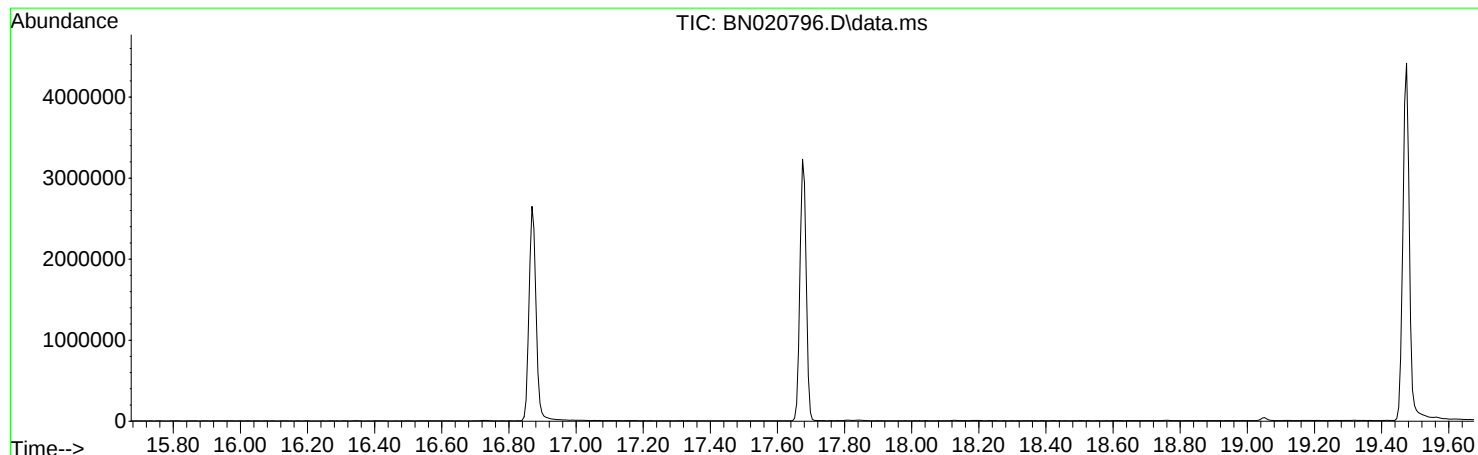




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.0	159779	PASS
68	69	0.00	2	1.7	2359	PASS
69	198	0.00	100	46.3	139461	PASS
70	69	0.00	2	0.5	750	PASS
127	198	10	80	56.3	169600	PASS
197	198	0.00	2	0.7	2041	PASS
198	198	100	100	100.0	301205	PASS
199	198	5	9	6.9	20753	PASS
275	198	10	60	23.2	69904	PASS
365	198	1	100	2.9	8593	PASS
441	198	0.01	100	11.0	33037	PASS
442	442	50	100	100.0	189744	PASS
443	442	15	24	19.2	36360	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072022\
 Data File : BN020796.D
 Acq On : 20 Jul 2022 08:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 20 10:52:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 10:52:33 2022
 Response via : Initial Calibration

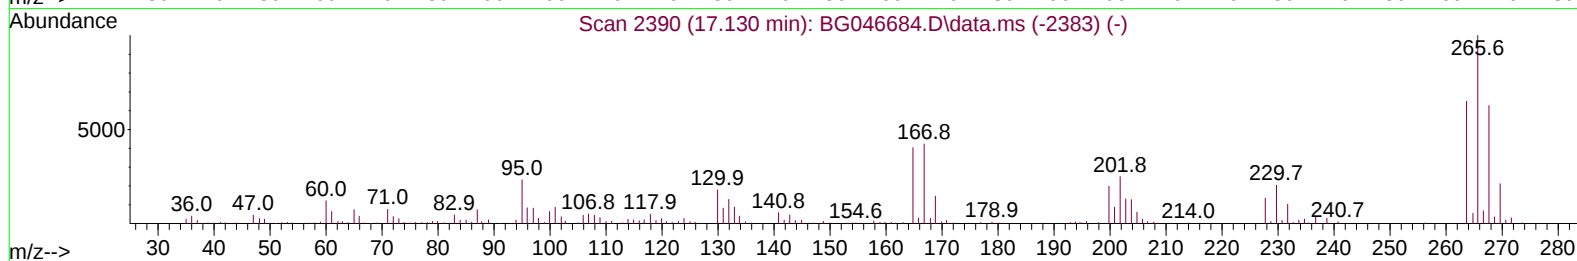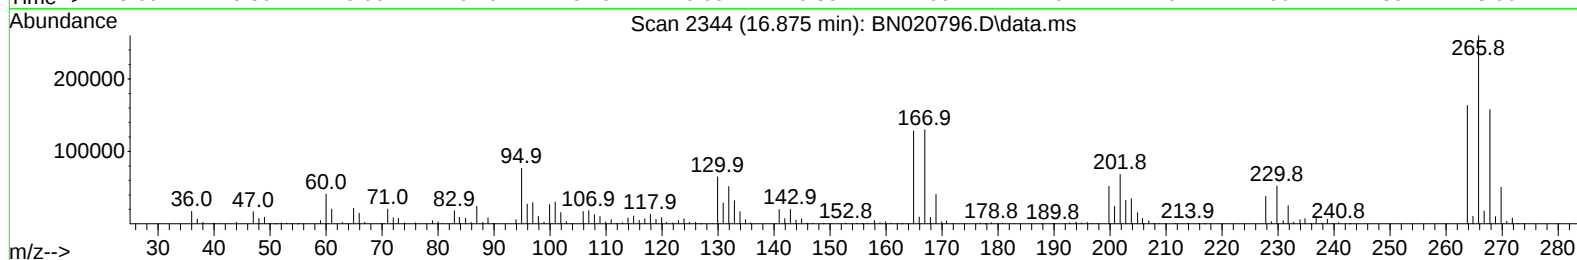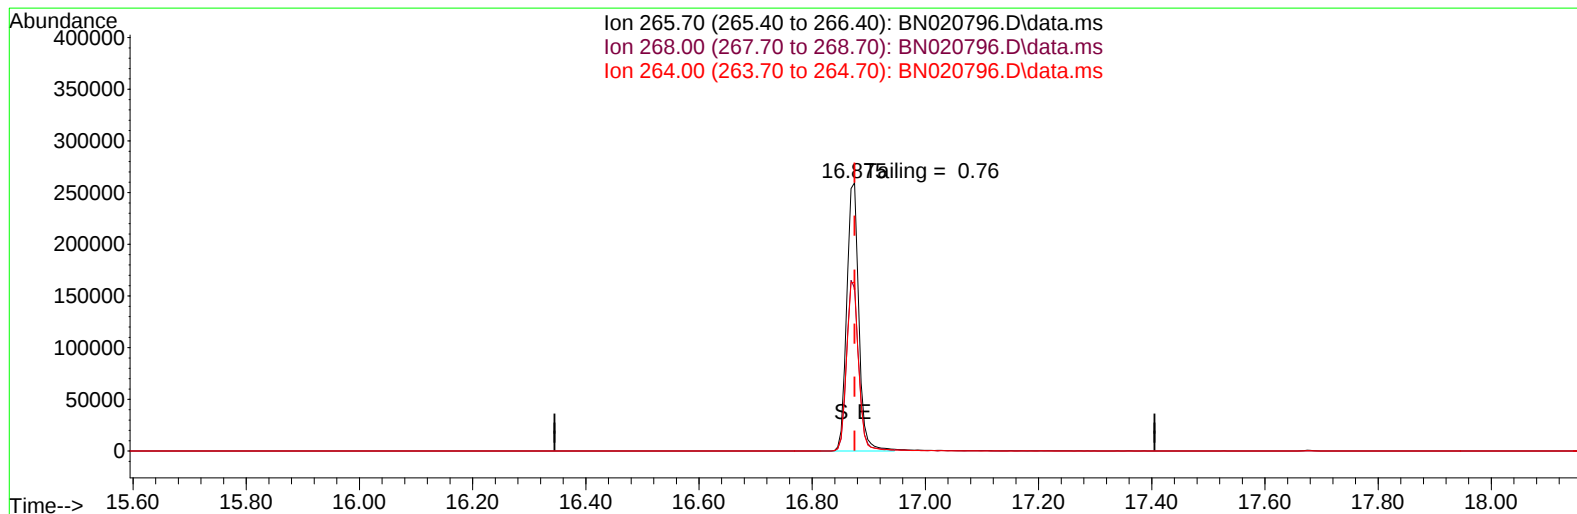

TIC: BN020796.D\data.ms

(70) Pentachlorophenol (C)

16.875min (0.000) 22241.57 ng




response 386969

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.78
264.00	61.60	62.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072022\
 Data File : BN020796.D
 Acq On : 20 Jul 2022 08:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jul 20 10:52:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 10:52:33 2022
 Response via : Initial Calibration

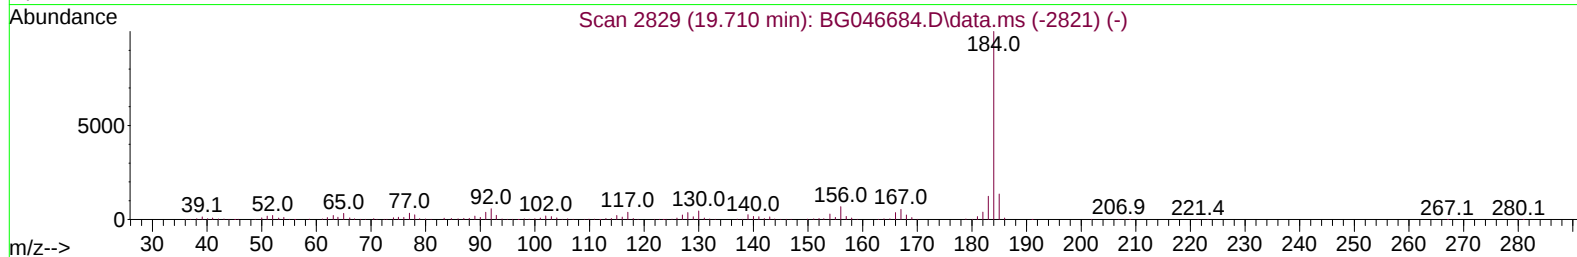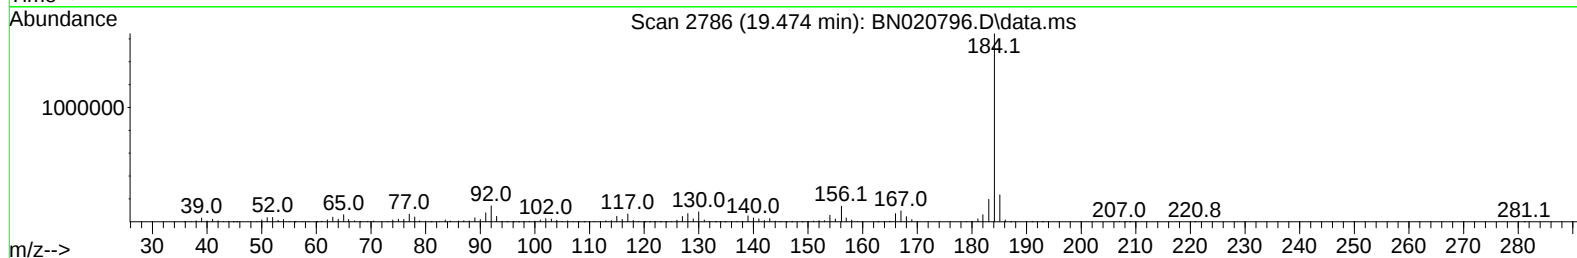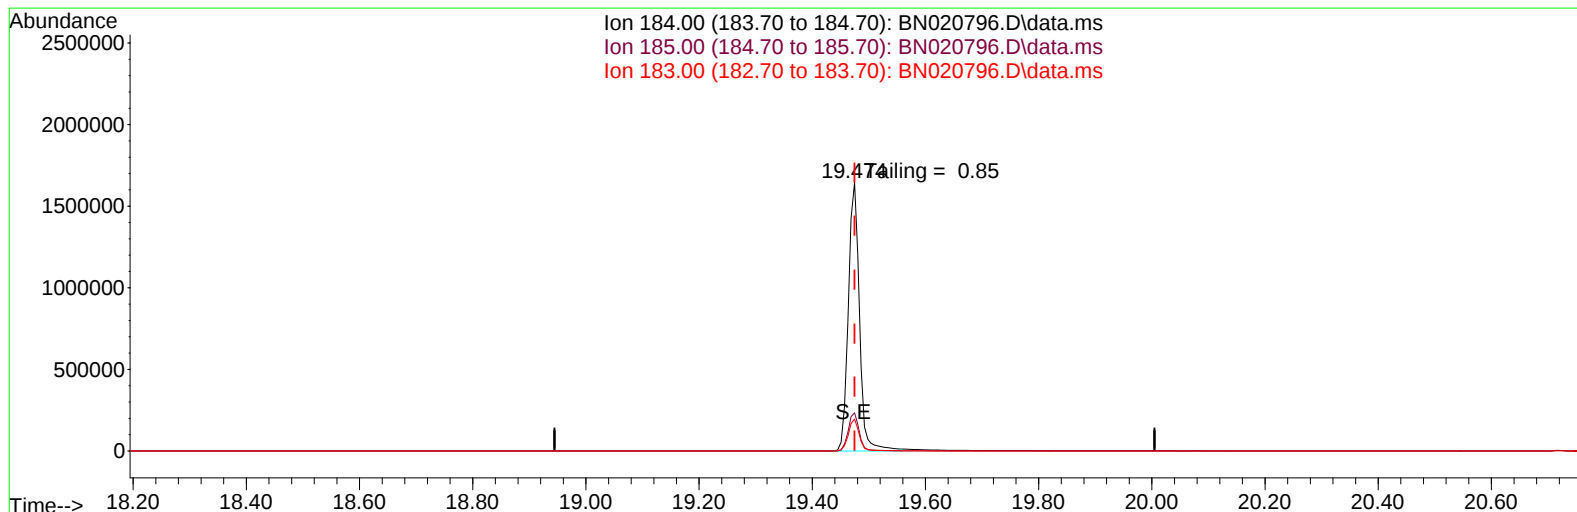

TIC: BN020796.D\data.ms

(77) Benzidine

19.474min (0.000) 0.00 ng

response 2303598

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.28
183.00	13.20	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/20/2022	BNA_N	<u>BN020796.D</u>
Compound Name	Response	Retention Time
DDT	1010253	20.72
DDD	23585	20.27
DDE	1789	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25374	1035627	2.45

Instrument :
BNA_N
ClientSampleId :
DFTPP