
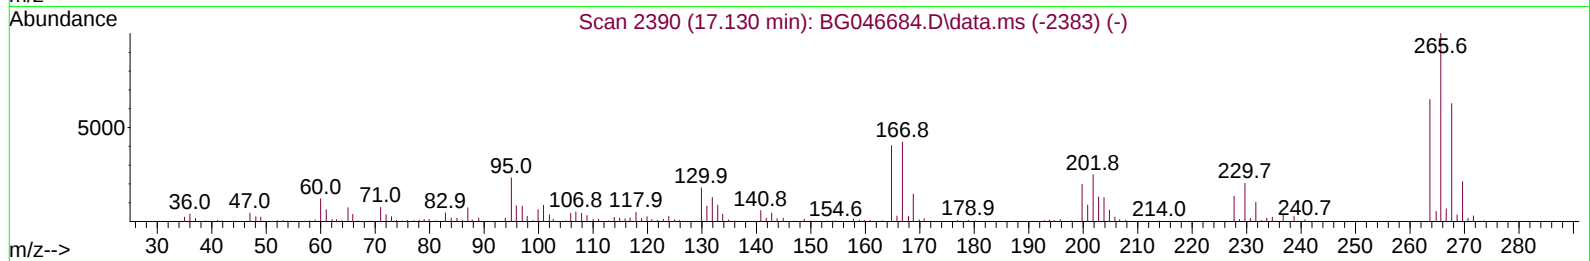
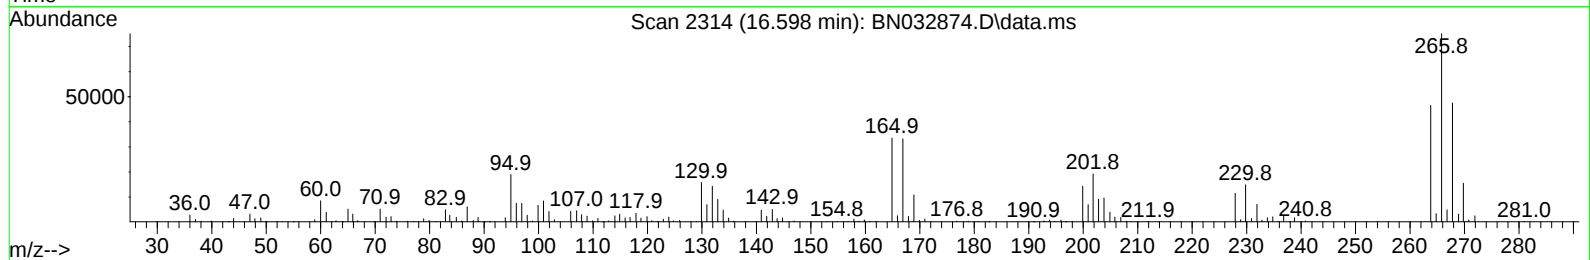


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072024\
Data File : BN032874.D
Acq On : 20 Jul 2024 12:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Jul 22 00:23:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

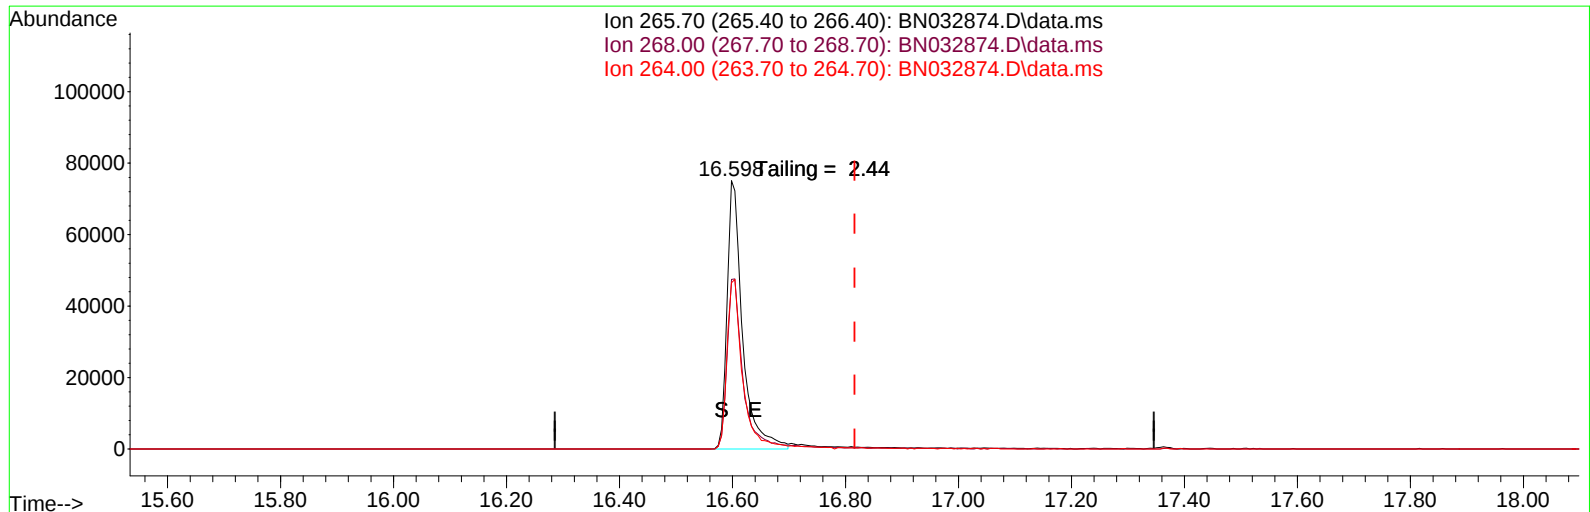

TIC: BN032874.D\data.ms

(70) Pentachlorophenol (C)




16.598min (-0.218) 17412.61 ng

response 148265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.23
264.00	61.60	61.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072024\
Data File : BN032874.D
Acq On : 20 Jul 2024 12:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Quant Time: Jul 22 00:23:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

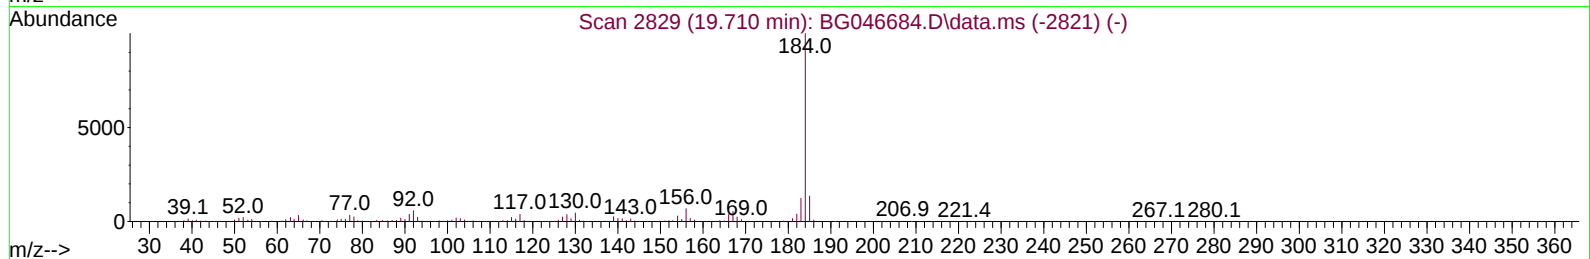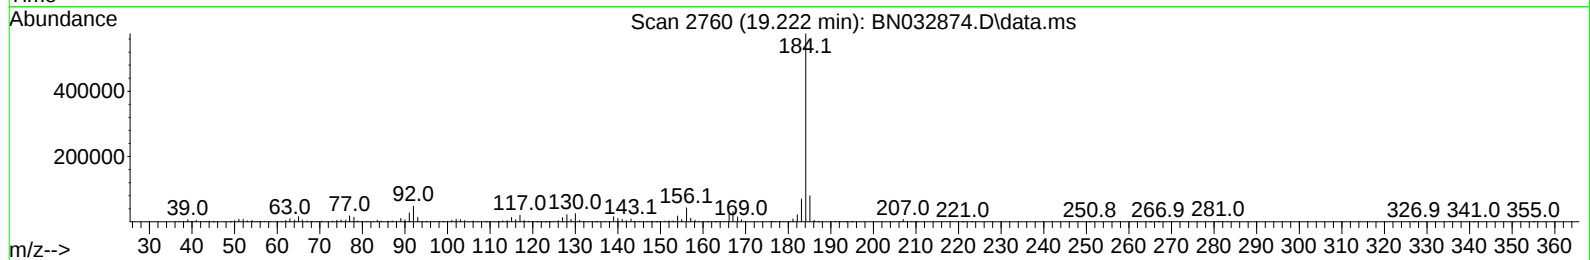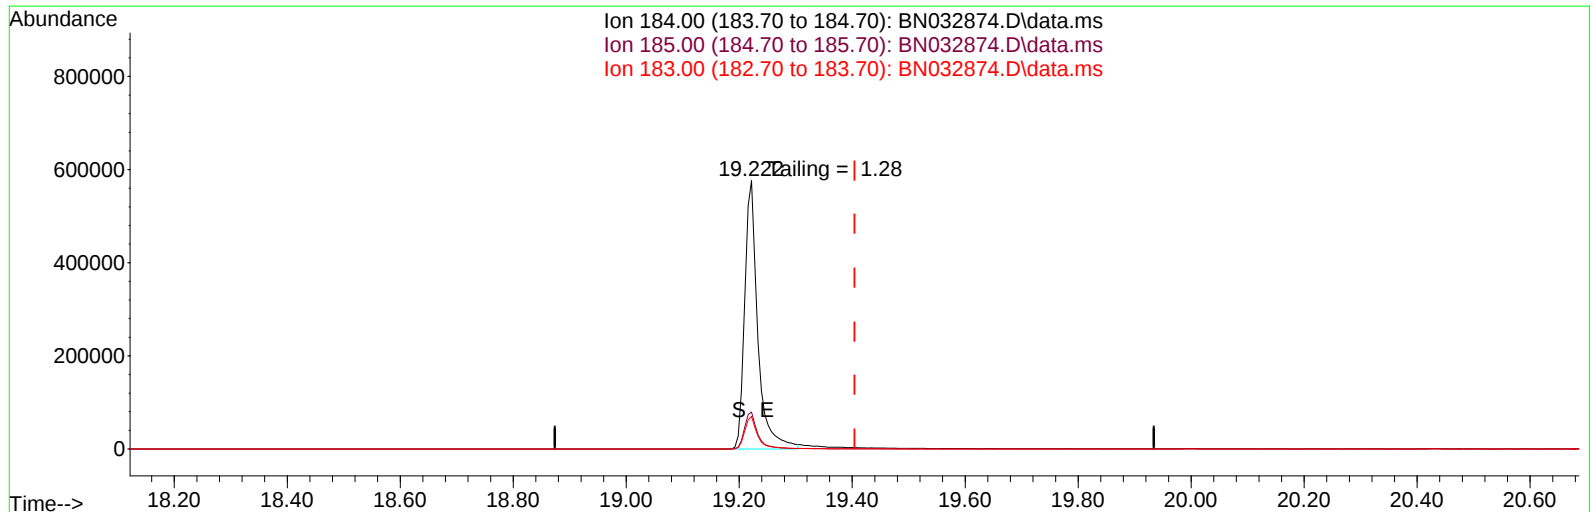

TIC: BN032874.D\data.ms

(77) Benzidine**19.222min (-0.182) 519042.84 ng****response 975981**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.78
183.00	13.20	12.15
0.00	0.00	0.00