
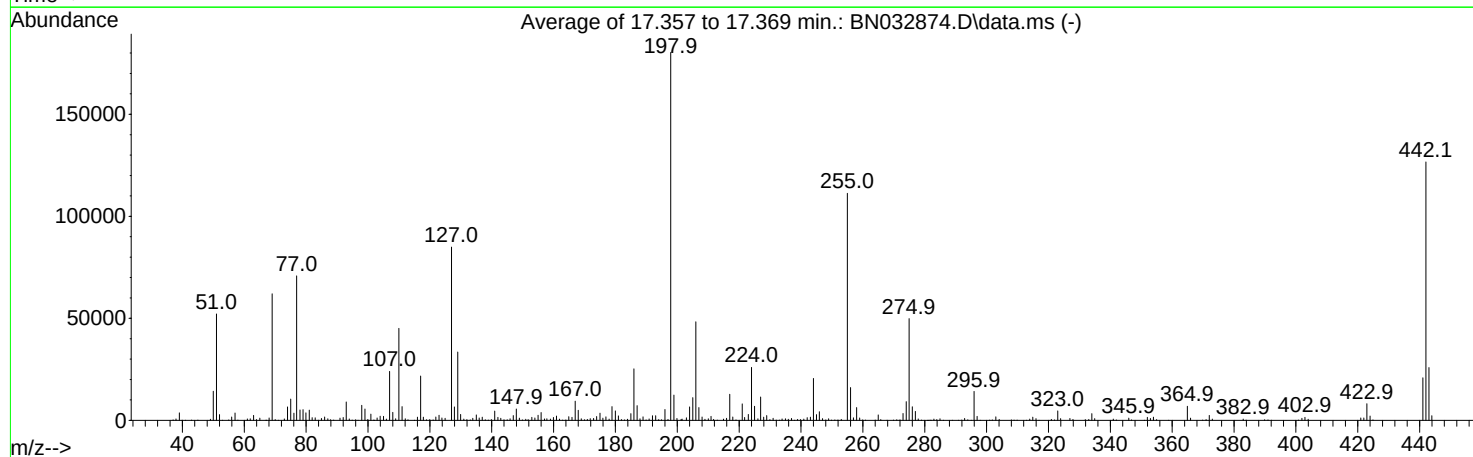


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072024\
Data File : BN032874.D
Acq On : 20 Jul 2024 12:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Jul 22 23:33:21 2024

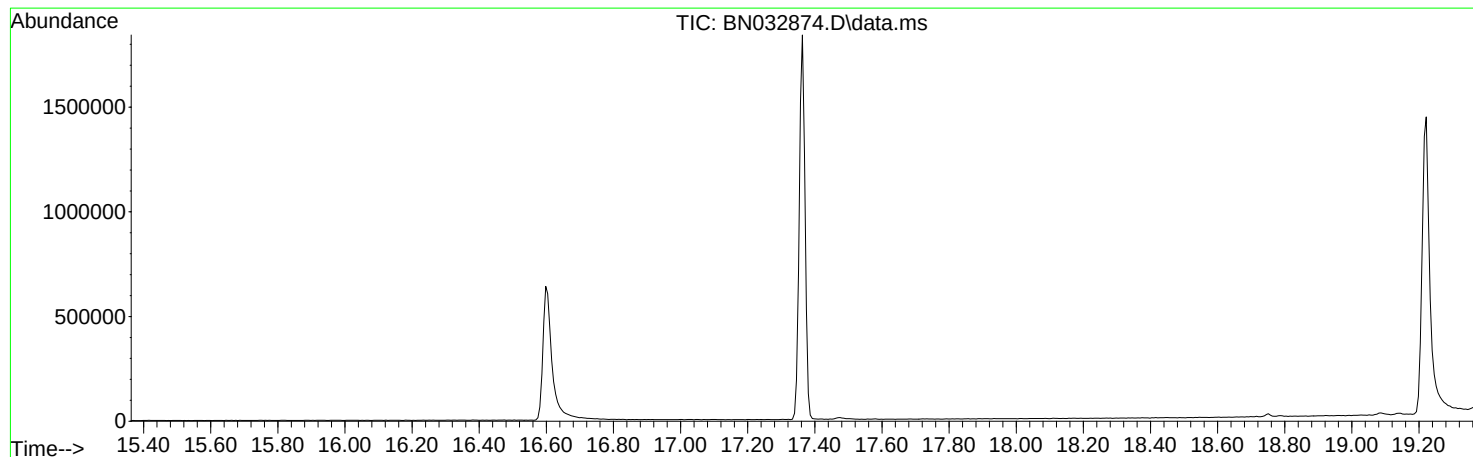

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	52179	PASS
68	69	0.00	2	1.9	1159	PASS
69	198	0.00	100	34.4	62000	PASS
70	69	0.00	2	0.7	408	PASS
127	198	10	80	47.1	84909	PASS
197	198	0.00	2	0.2	440	PASS
198	198	100	100	100.0	180267	PASS
199	198	5	9	6.9	12360	PASS
275	198	10	60	27.7	49880	PASS
365	198	1	100	3.8	6940	PASS
441	198	0.01	100	11.6	20871	PASS
442	442	50	100	100.0	126643	PASS
443	442	15	24	20.4	25888	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/20/2024	BNA_N	<u>BN032874.D</u>
Compound Name	Response	Retention Time
DDT	157944	20.433
DDD	245781	19.998
DDE	1502	19.48
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
247283	405227	61.02

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072024\
Data File : BN032874.D
Acq On : 20 Jul 2024 12:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 22 00:23:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

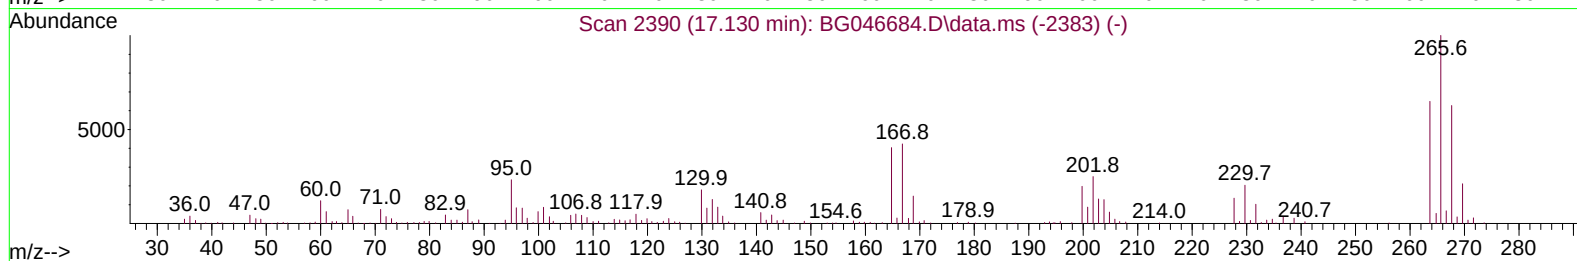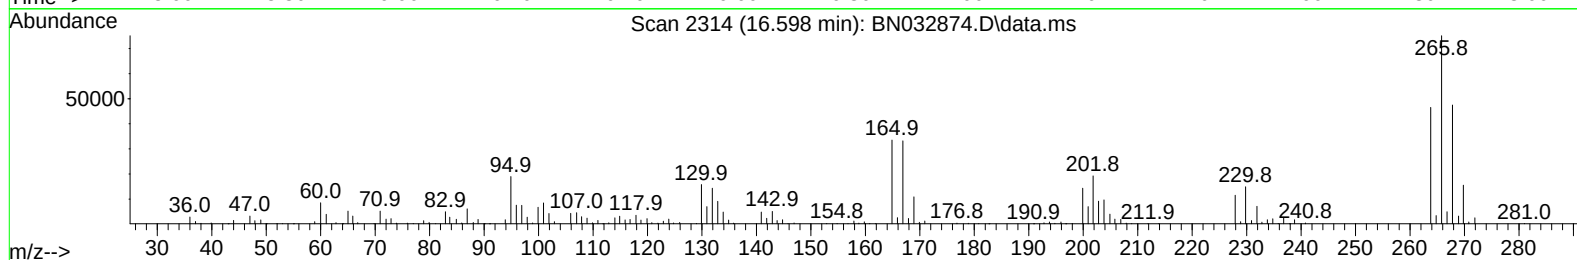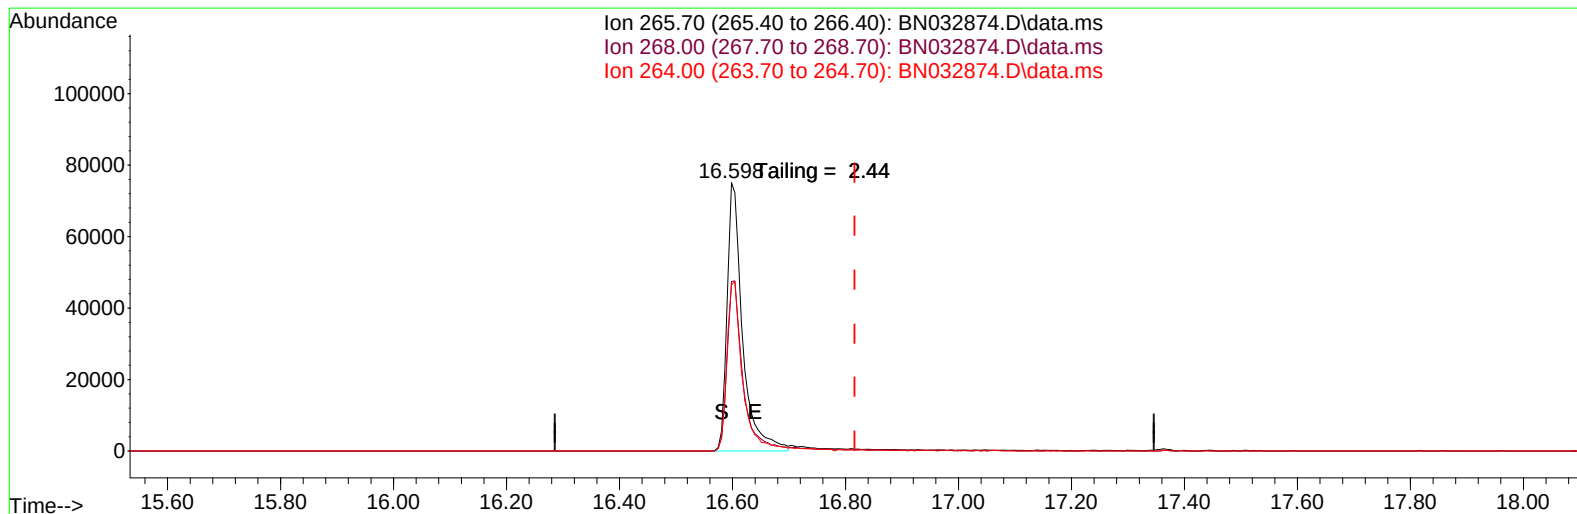

TIC: BN032874.D\data.ms

(70) Pentachlorophenol (C)

16.598min (-0.218) 17412.61 ng




response 148265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.23
264.00	61.60	61.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072024\
Data File : BN032874.D
Acq On : 20 Jul 2024 12:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 22 00:23:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 03:07:33 2024
Response via : Initial Calibration

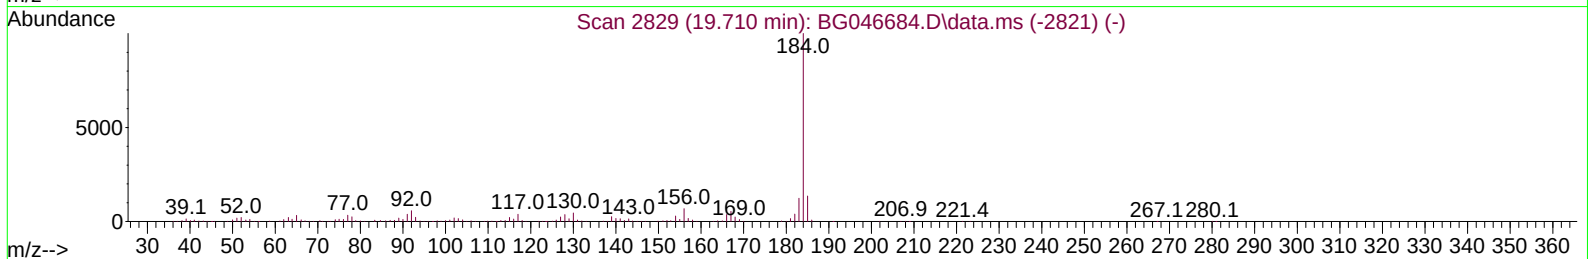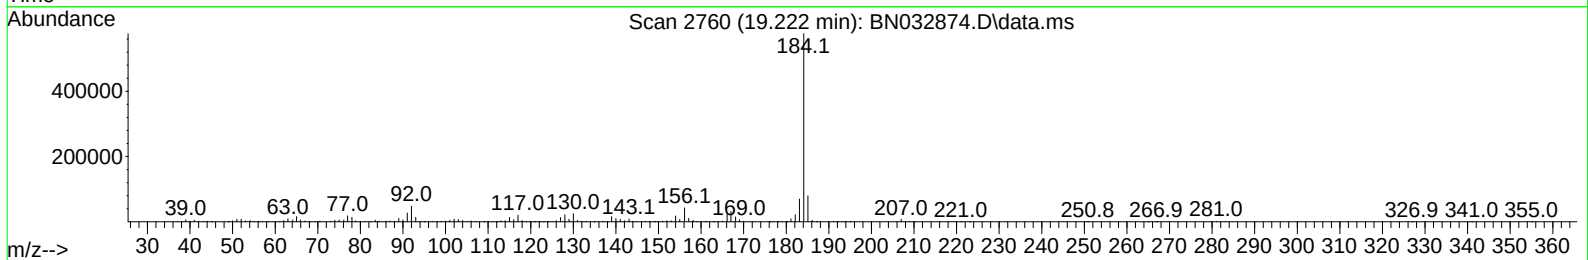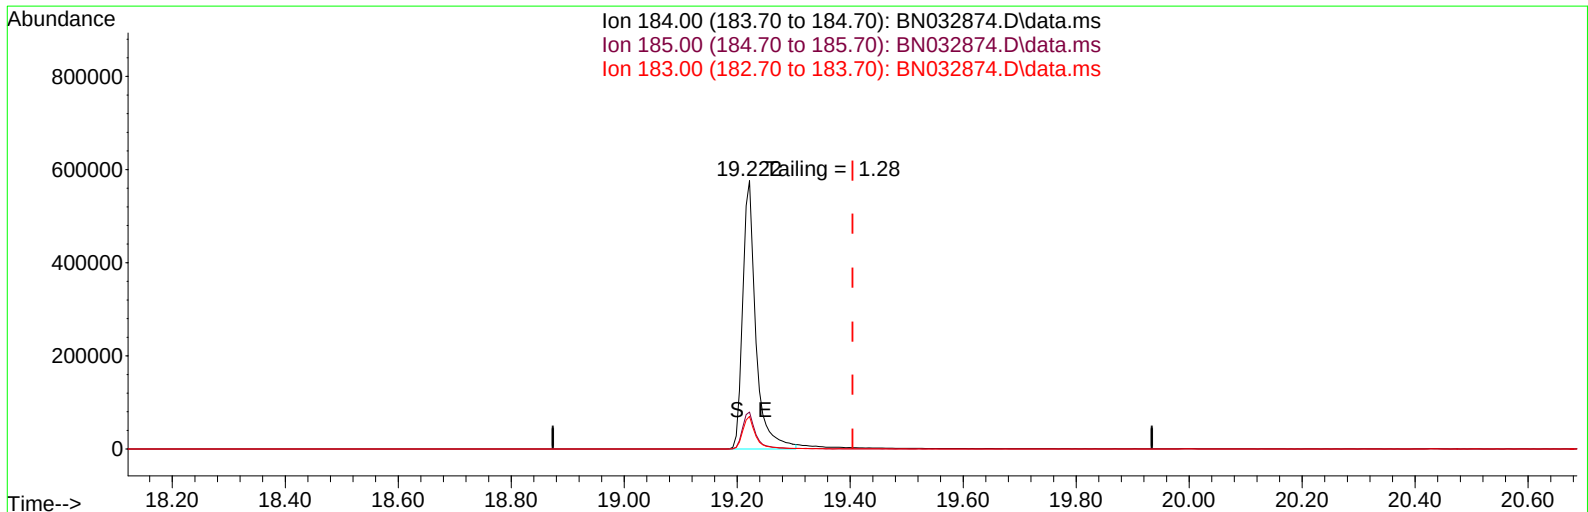

TIC: BN032874.D\data.ms

(77) Benzidine

19.222min (-0.182) 519042.84 ng

response 975981

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.78
183.00	13.20	12.15
0.00	0.00	0.00