


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072121\
Data File : BN015628.D
Acq On : 20 Jul 2021 18:58
Operator : CG/JU
Sample : PB137497BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK497

Manual Integrations
APPROVED

mohammad
7/21/2021 3:57:29 PM

Quant Time: Jul 20 19:29:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 18:52:28 2021
Response via : Initial Calibration

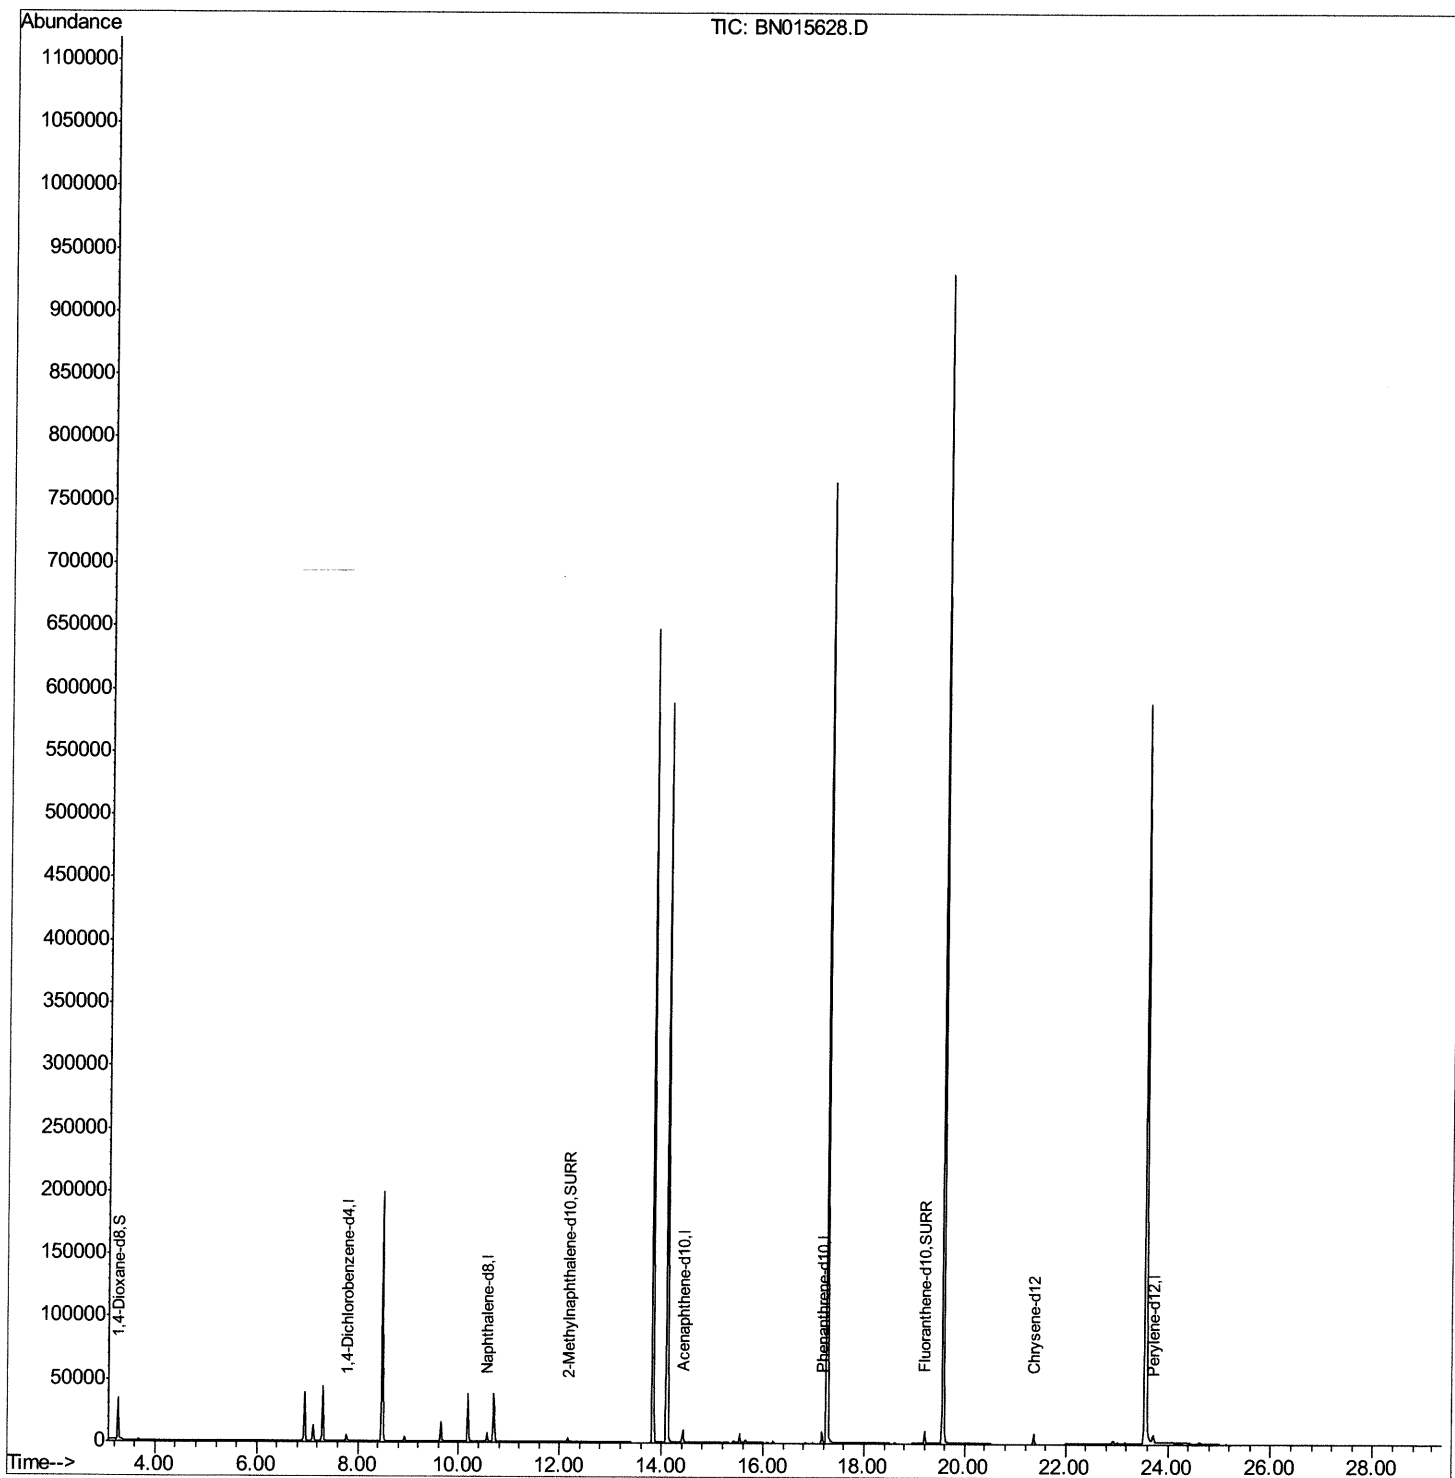

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072121\
 Data File : BN015628.D
 Acq On : 20 Jul 2021 18:58
 Operator : CG/JU
 Sample : PB137497BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK497

Manual Integrations
 APPROVED

mohammad
 7/21/2021 3:57:29 PM

Quant Time: Jul 20 19:27:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 18:52:28 2021
 Response via : Initial Calibration

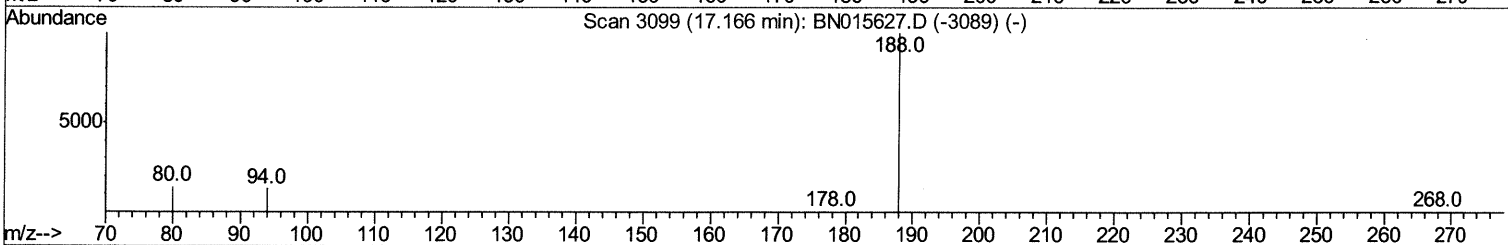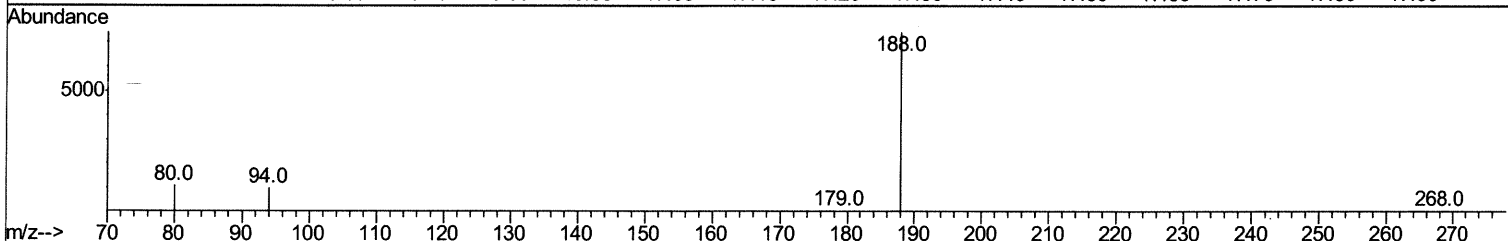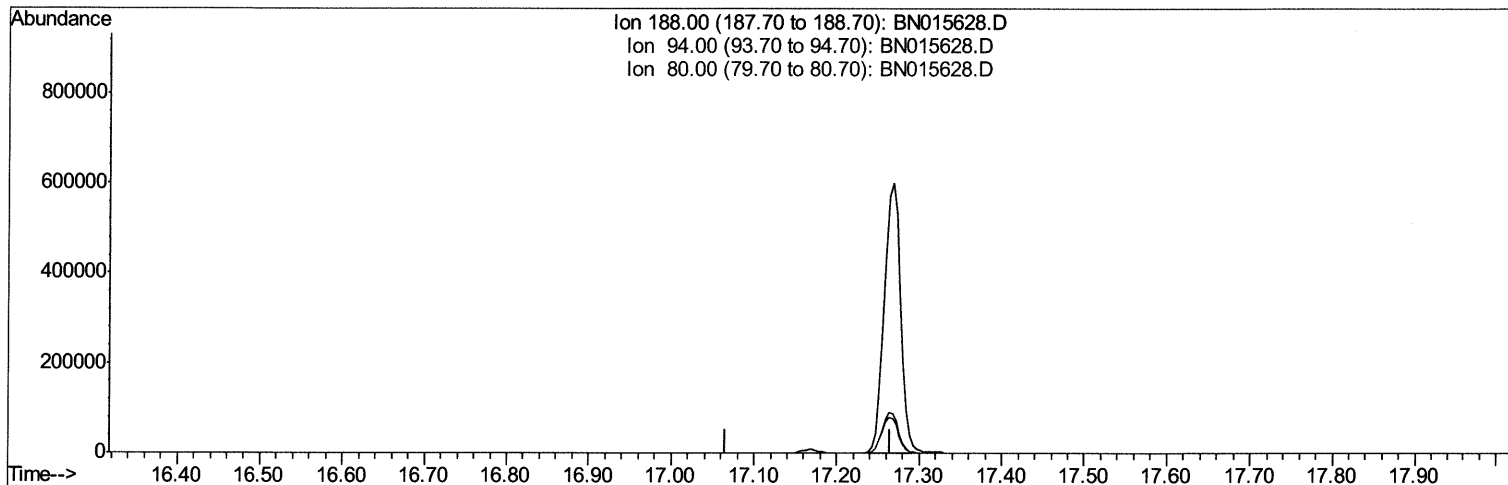

TIC: BN015628.D

(13) Phenanthrene-d10 (I)

17.166min (-17.166) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072121\
 Data File : BN015628.D
 Acq On : 20 Jul 2021 18:58
 Operator : CG/JU
 Sample : PB137497BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 SBLK497

Manual Integrations
APPROVED

mohammad
 7/21/2021 3:57:29 PM

Quant Time: Jul 20 19:27:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 18:52:28 2021
 Response via : Initial Calibration

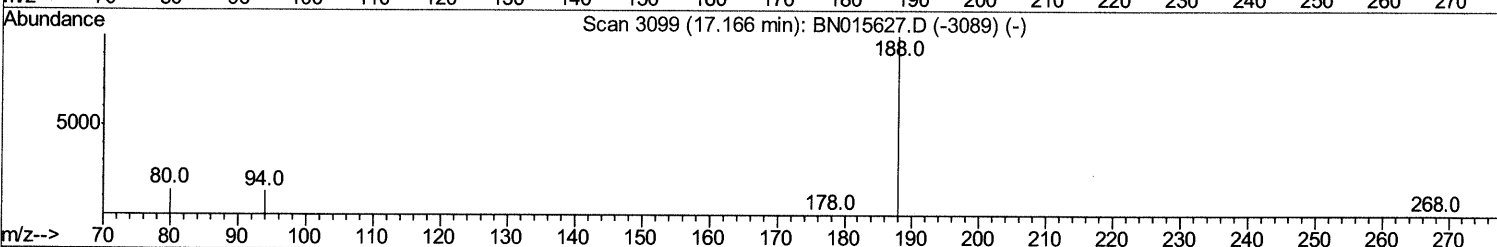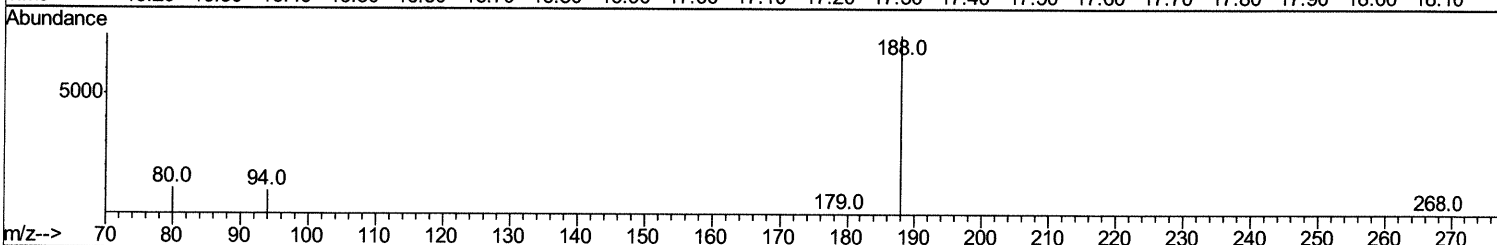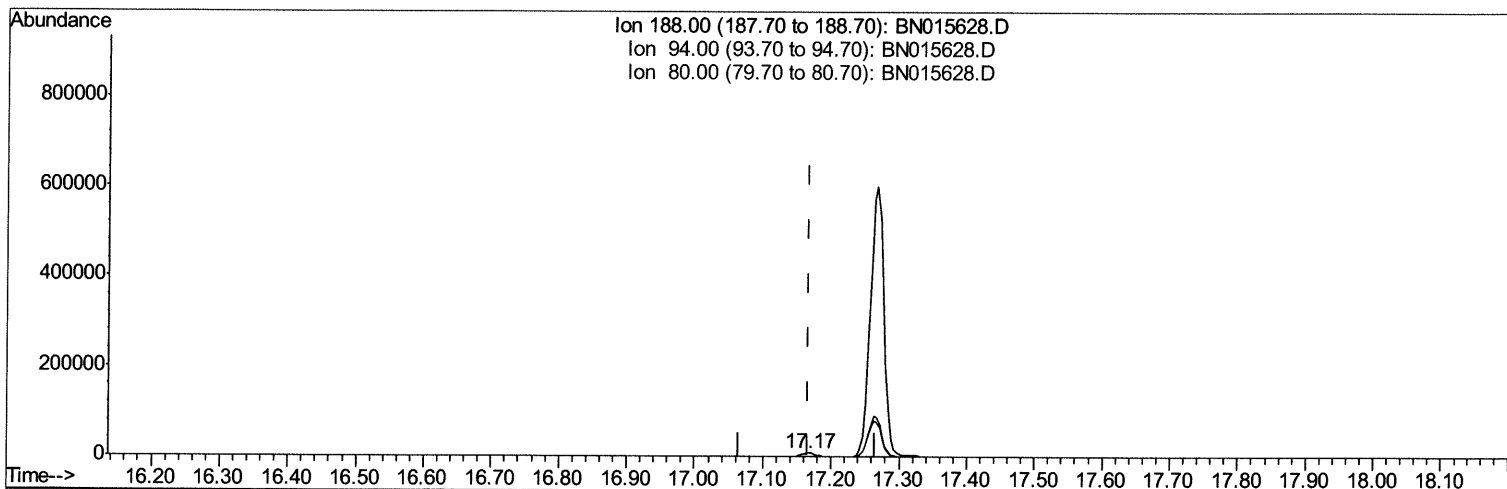

TIC: BN015628.D

(13) Phenanthrene-d10 (I)

17.166min (-0.000) 0.40ng/ul m

response 10565

JU 7/22/21

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	13.45#
80.00	12.50	14.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN072121\
Data File : BN015628.D
Acq On : 20 Jul 2021 18:58
Operator : CG/JU
Sample : PB137497BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK497

Manual Integrations
APPROVED

mohammad
7/21/2021 3:57:29 PM

Quant Time: Jul 20 19:29:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 18:52:28 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.78	152	2741	0.40	ng/ul	0.00
4) Naphthalene-d8	10.57	136	9276	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.42	164	5275	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.17	188	10565m	0.40	ng/ul	0.00
17) Chrysene-d12	21.37	240	7901	0.40	ng/ul	0.00
23) Perylene-d12	23.71	264	7968	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.27	96	21767	7.05	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.16	152	4993	0.34	ng/ul	0.00
18) Fluoranthene-d10	19.20	212	10211	0.39	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7/21/22/21