

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072121\
 Data File : BN015632.D
 Acq On : 20 Jul 2021 21:25
 Operator : CG/JU
 Sample : M2905-22DL 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK40DL

Quant Time: Jul 21 01:06:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 18:52:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.779	152	2576	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.562	136	8679	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.418	164	4749	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.166	188	9739	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.369	240	7697	0.400	ng/ul	# 0.00
23) Perylene-d12	23.707	264	7162	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.277	96	1416	0.488	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.162	152	843	0.062	ng/ul	0.00
18) Fluoranthene-d10	19.206	212	2071	0.082	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.820	266	4139	1.921	ng/ul	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072121\
Data File : BN015632.D
Acq On : 20 Jul 2021 21:25
Operator : CG/JU
Sample : M2905-22DL 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBK40DL

Quant Time: Jul 21 01:06:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 20 18:52:28 2021
Response via : Initial Calibration

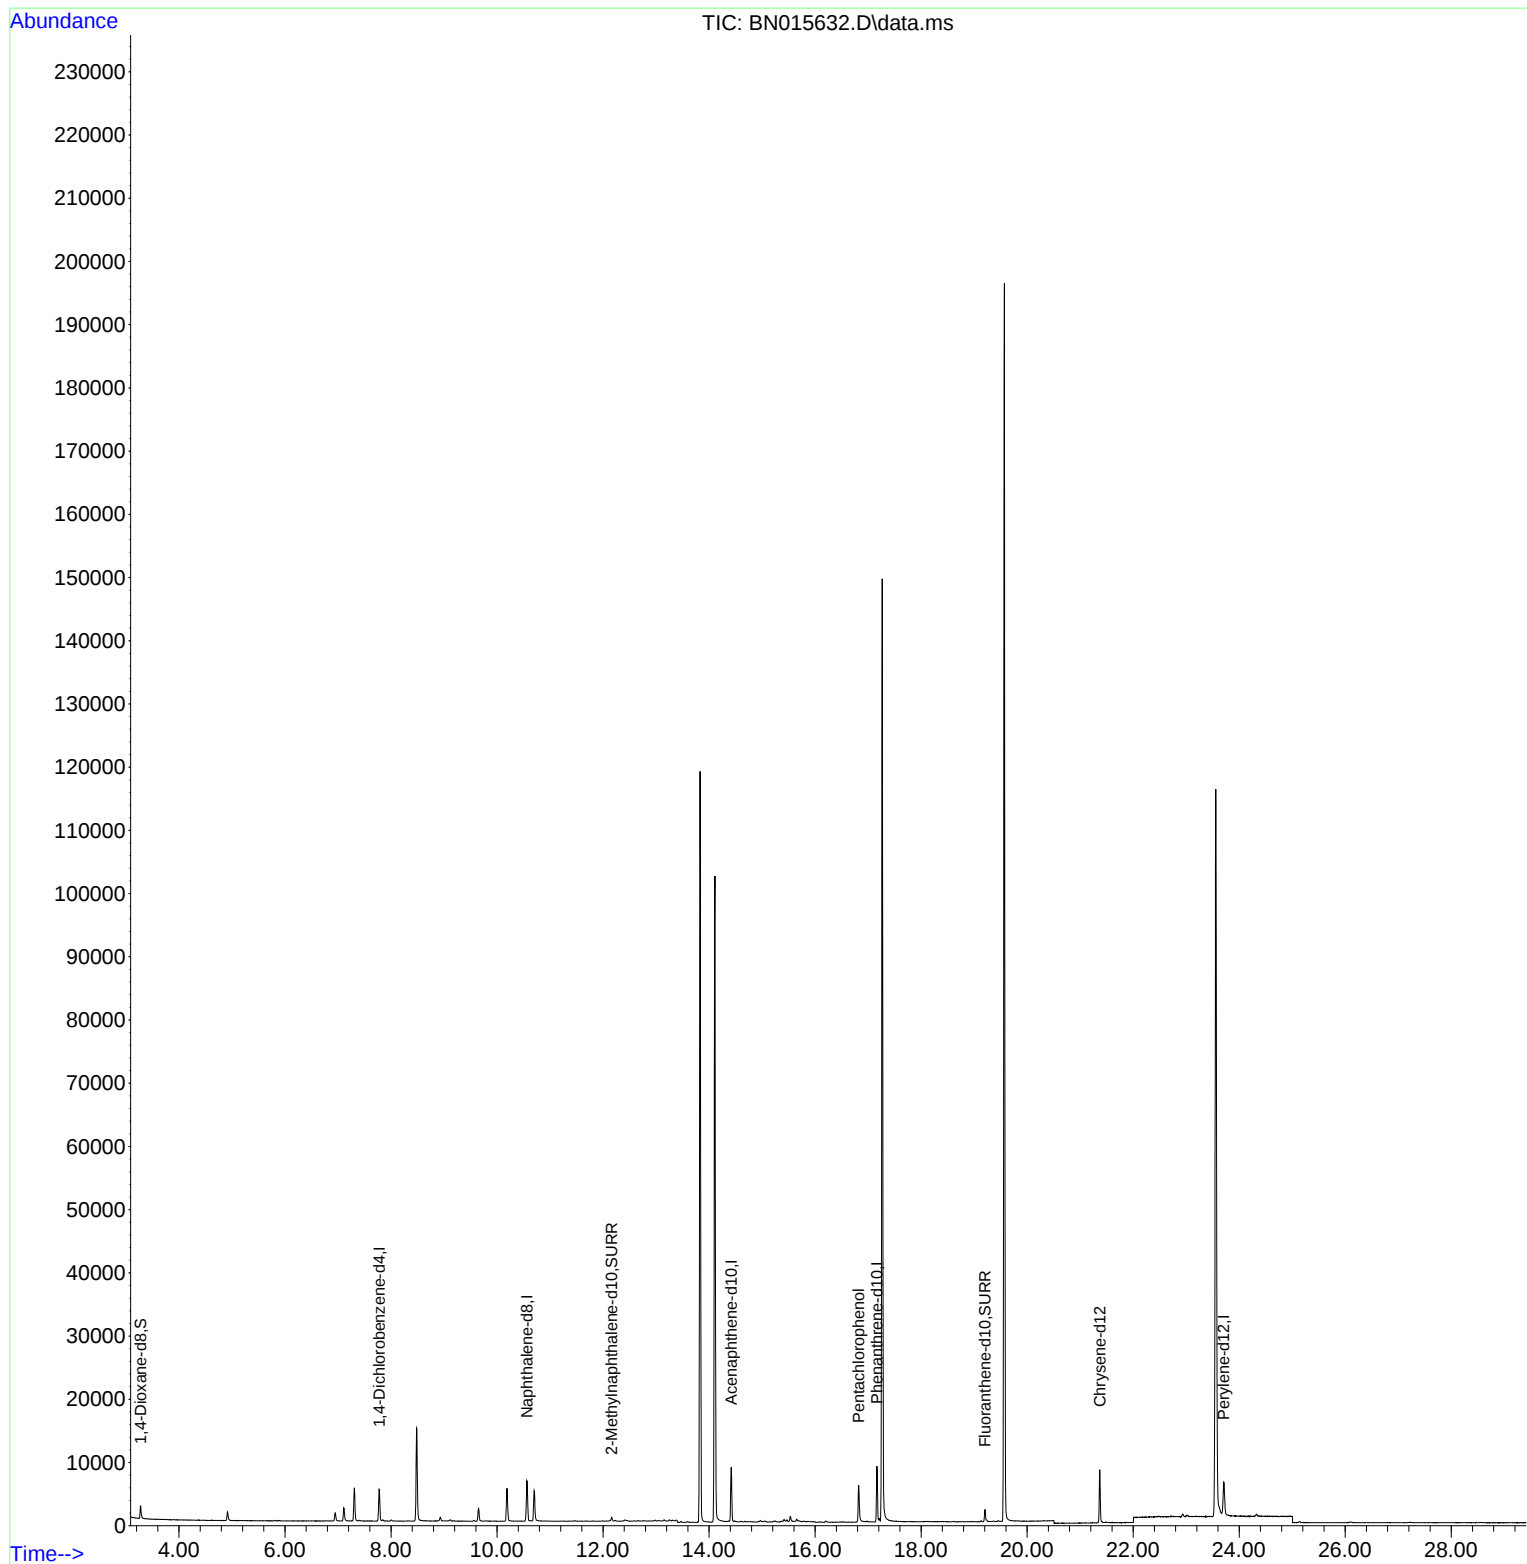

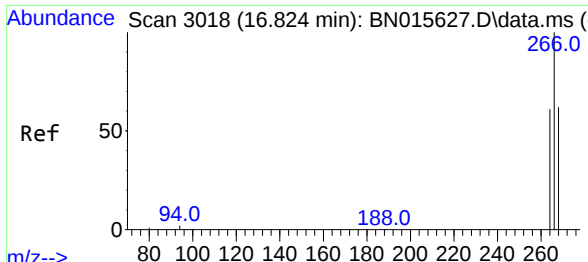

#14
Pentachlorophenol
Concen: 1.921 ng/ul
RT: 16.820 min Scan# 3017
Delta R.T. -0.004 min
Lab File: BN015632.D
Acq: 20 Jul 2021 21:25

Instrument :
BNA_N
ClientSampleId :
DBK40DL

Tgt Ion:	266	Resp:	4139
Ion	Ratio	Lower	Upper
266	100		
264	62.5	52.9	79.3
268	63.3	59.4	89.0

