

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
 Data File : BN006953.D
 Acq On : 22 Jul 2019 22:18
 Operator : HP/JU
 Sample : K3890-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 23 04:25:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 23 04:22:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2539	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.35	136	8730	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.23	164	4506	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	820954	0.40	ng/ul	0.07
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	736586	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	4359	0.32	ng/ul	-0.03
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.40	128	1128	0.045	ng/ul#	Ovalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
Data File : BN006953.D
Acq On : 22 Jul 2019 22:18
Operator : HP/JU
Sample : K3890-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 23 04:25:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 23 04:22:37 2019
Response via : Initial Calibration

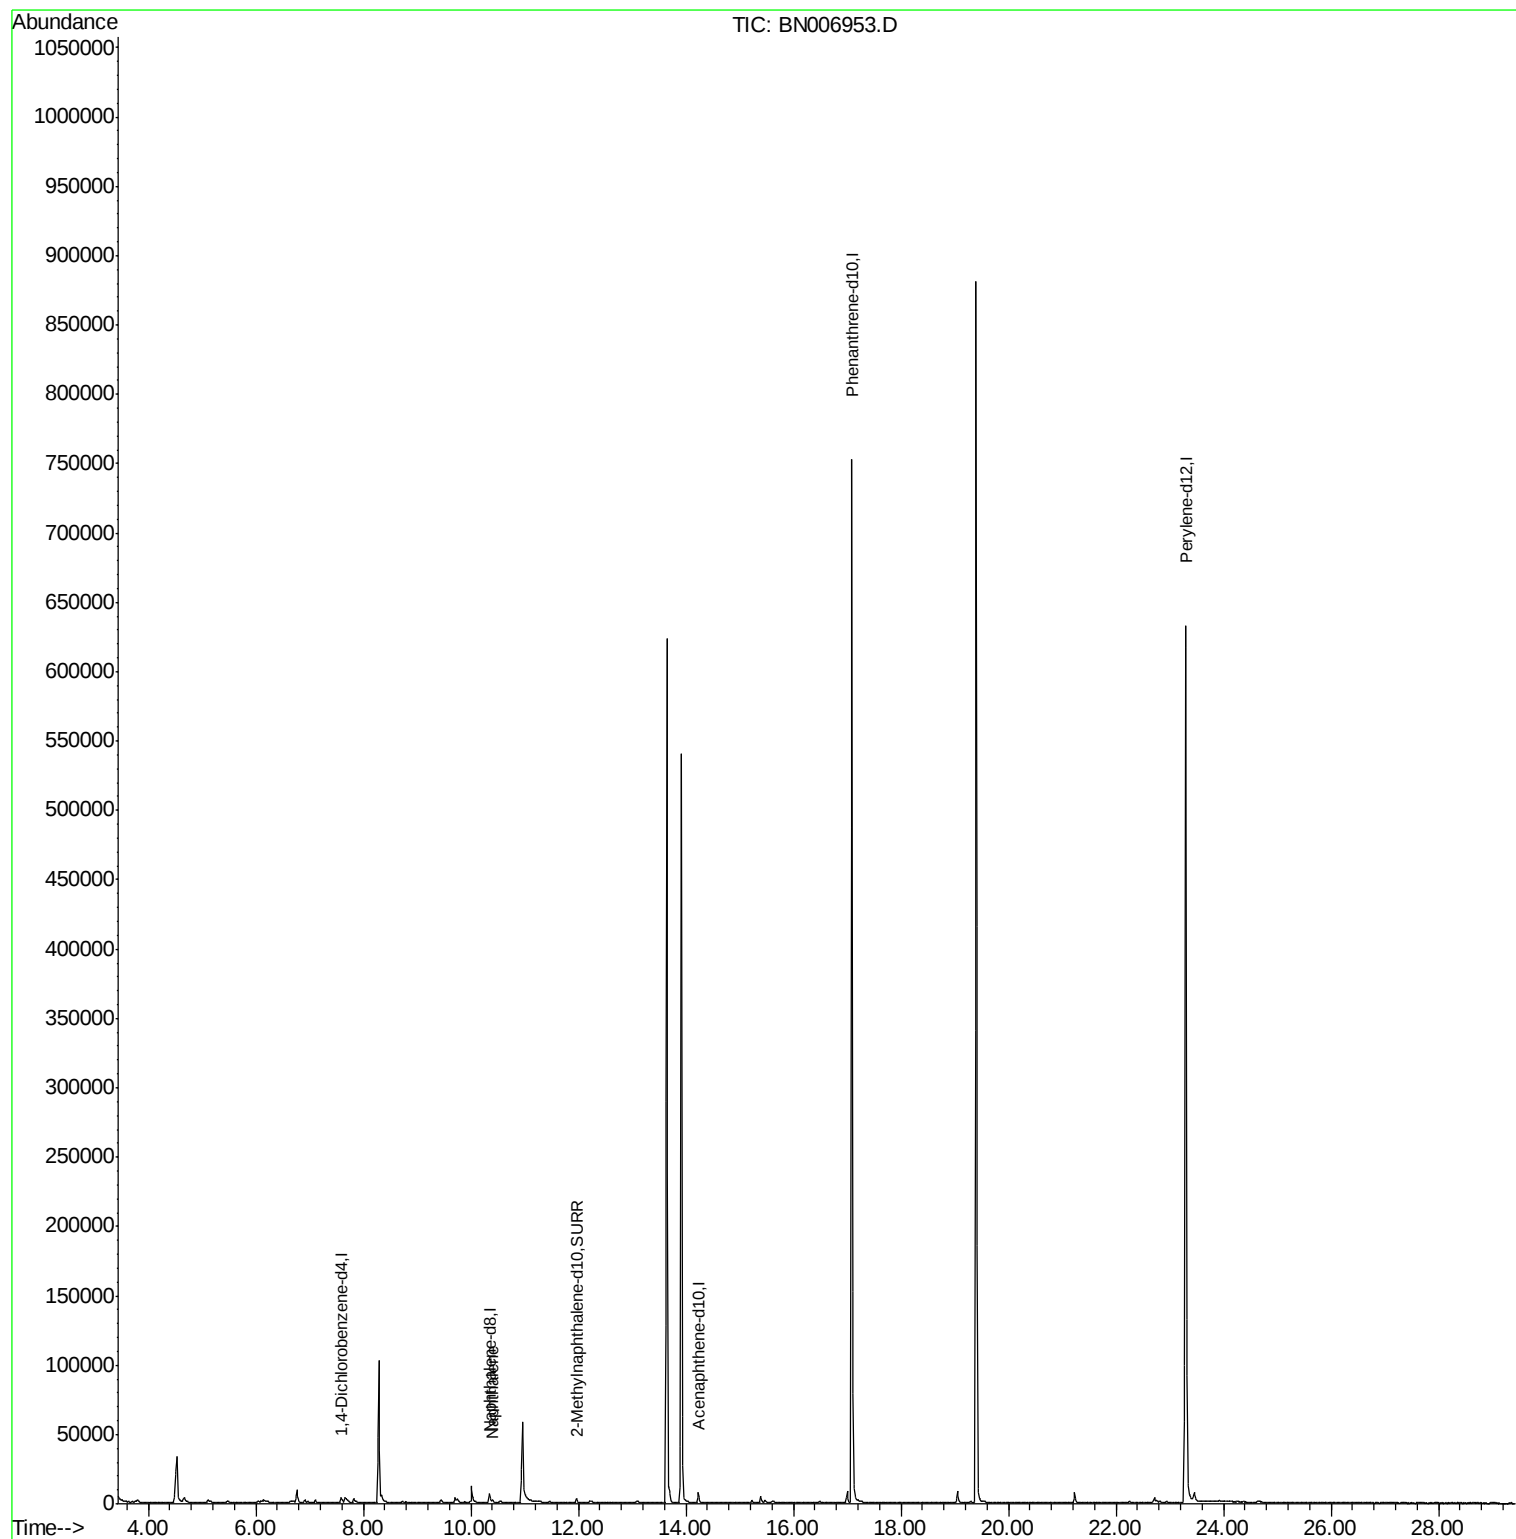

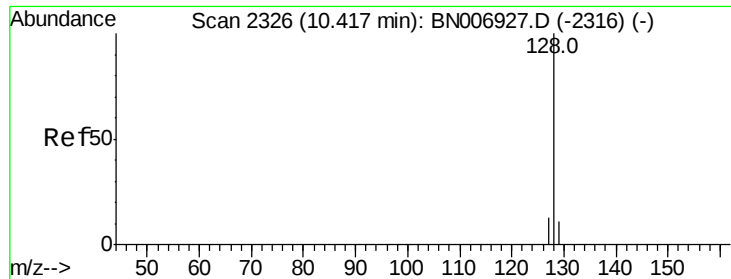

#3

Naphthalene

Concen: 0.045 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.02 min

Lab File: BN006953.D

Acq: 22 Jul 2019 22:18

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 1128

Ion Ratio Lower Upper

128 100

129 23.2 9.4 14.0#

127 20.9 10.6 16.0#

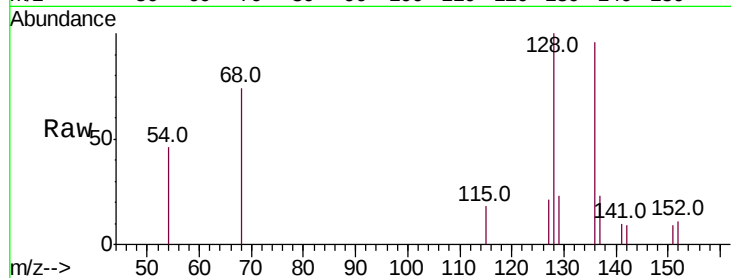

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

