

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
 Data File : BN006955.D
 Acq On : 22 Jul 2019 23:27
 Operator : HP/JU
 Sample : K3890-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 23 04:25:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 23 04:22:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	2532	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	9061	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4599	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	861667	0.40	ng/ul	0.07
16) Chrysene-d12	21.24	240	6087	0.40	ng/ul	0.00
20) Perylene-d12	23.29	264	742427	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	3404	0.24	ng/ul	0.02
14) Fluoranthene-d10	19.05	212	7370	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
9) Fluorene	15.23	166	1351	0.067	ng/ul#	15
17) Pyrene	19.40	202	1610	0.058	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
Data File : BN006955.D
Acq On : 22 Jul 2019 23:27
Operator : HP/JU
Sample : K3890-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 23 04:25:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 23 04:22:37 2019
Response via : Initial Calibration




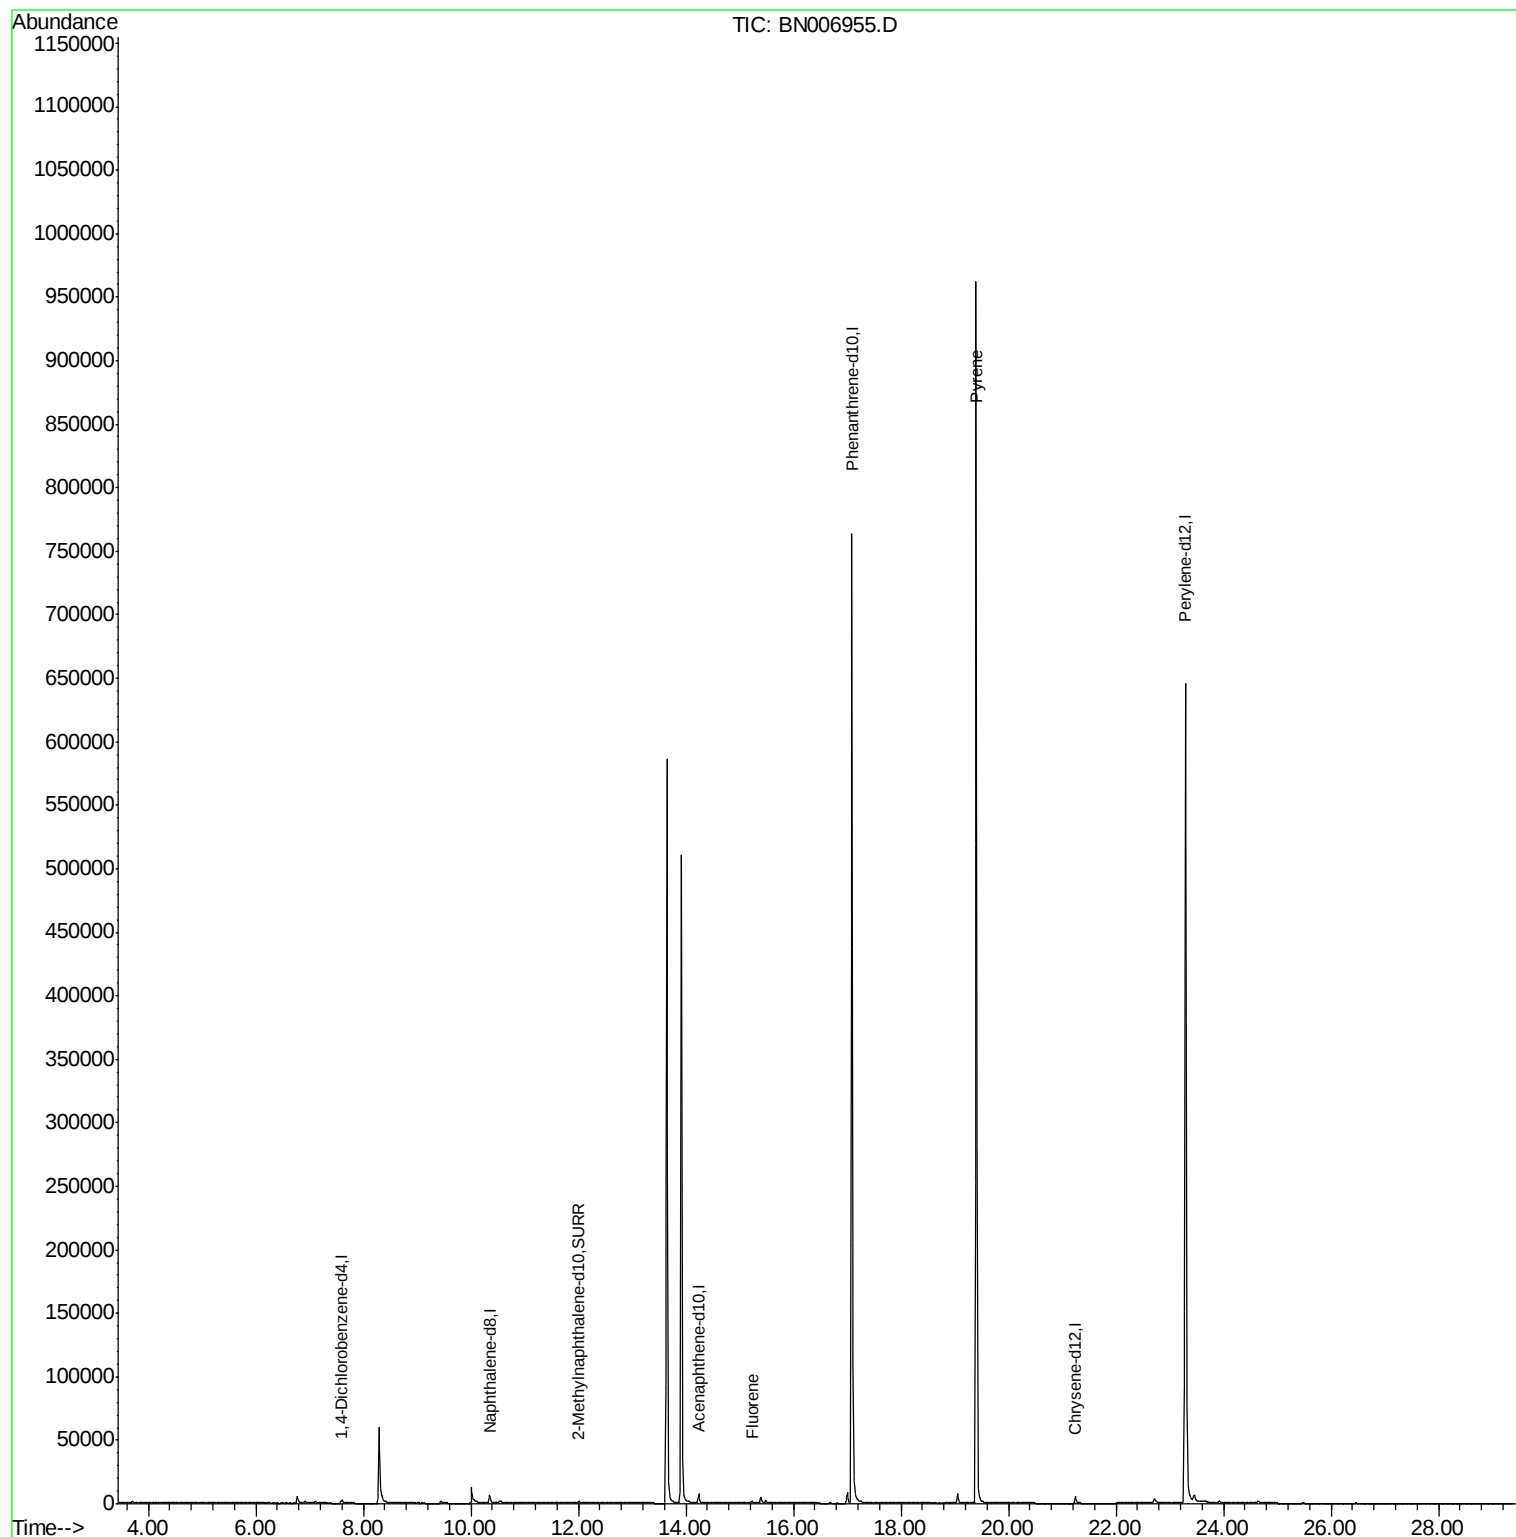


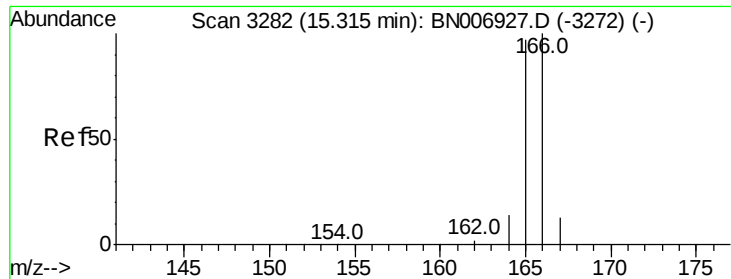

#9
Fluorene
Concen: 0.067 ng/ul
RT: 15.23 min Scan# 3264
Delta R.T. -0.08 min
Lab File: BN006955.D
Acq: 22 Jul 2019 23:27

Instrument :
BNA_N
ClientSampleId :

Tot Ion:166 Resp: 1351
Ion Ratio Lower Upper
166 100
165 9.5 78.2 117.4#
167 36.8 11.3 16.9#

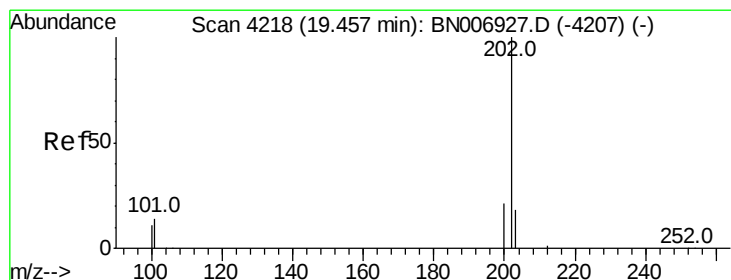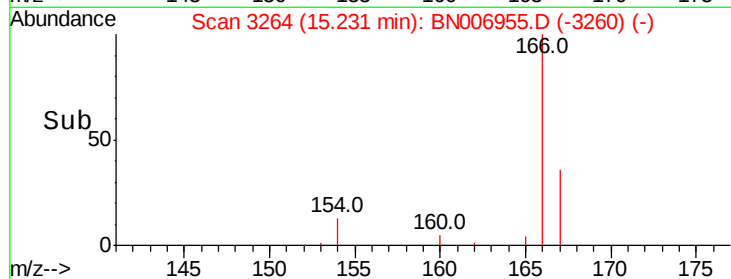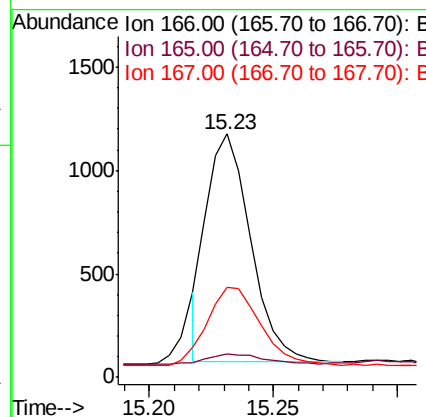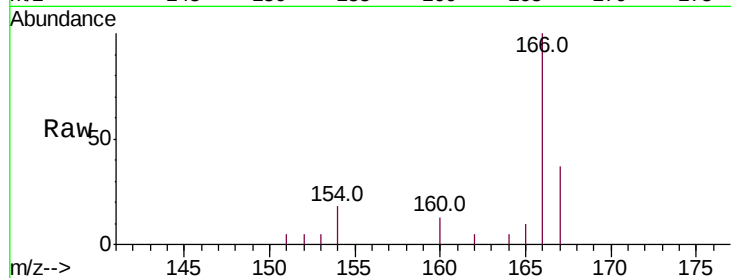

#17
Pyrene
Concen: 0.058 ng/ul
RT: 19.40 min Scan# 4206
Delta R.T. -0.05 min
Lab File: BN006955.D
Acq: 22 Jul 2019 23:27

Tgt Ion:202 Resp: 1610
Ion Ratio Lower Upper
202 100
101 182.3 12.2 18.2#
100 1269.7 9.8 14.8#

