

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
 Data File : BN006958.D
 Acq On : 23 Jul 2019 01:11
 Operator : HP/JU
 Sample : PB121592BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 23 04:25:57 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 23 04:22:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	2373	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	8455	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4222	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	820061	0.40	ng/ul	0.07
16) Chrysene-d12	21.25	240	5500	0.40	ng/ul	0.00
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.47
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	3684	0.28	ng/ul	0.03
14) Fluoranthene-d10	19.05	212	6751	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.23	166	1362	0.074	ng/ul#	14
17) Pyrene	19.40	202	1494	0.059	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
Data File : BN006958.D
Acq On : 23 Jul 2019 01:11
Operator : HP/JU
Sample : PB121592BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 23 04:25:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 23 04:22:37 2019
Response via : Initial Calibration




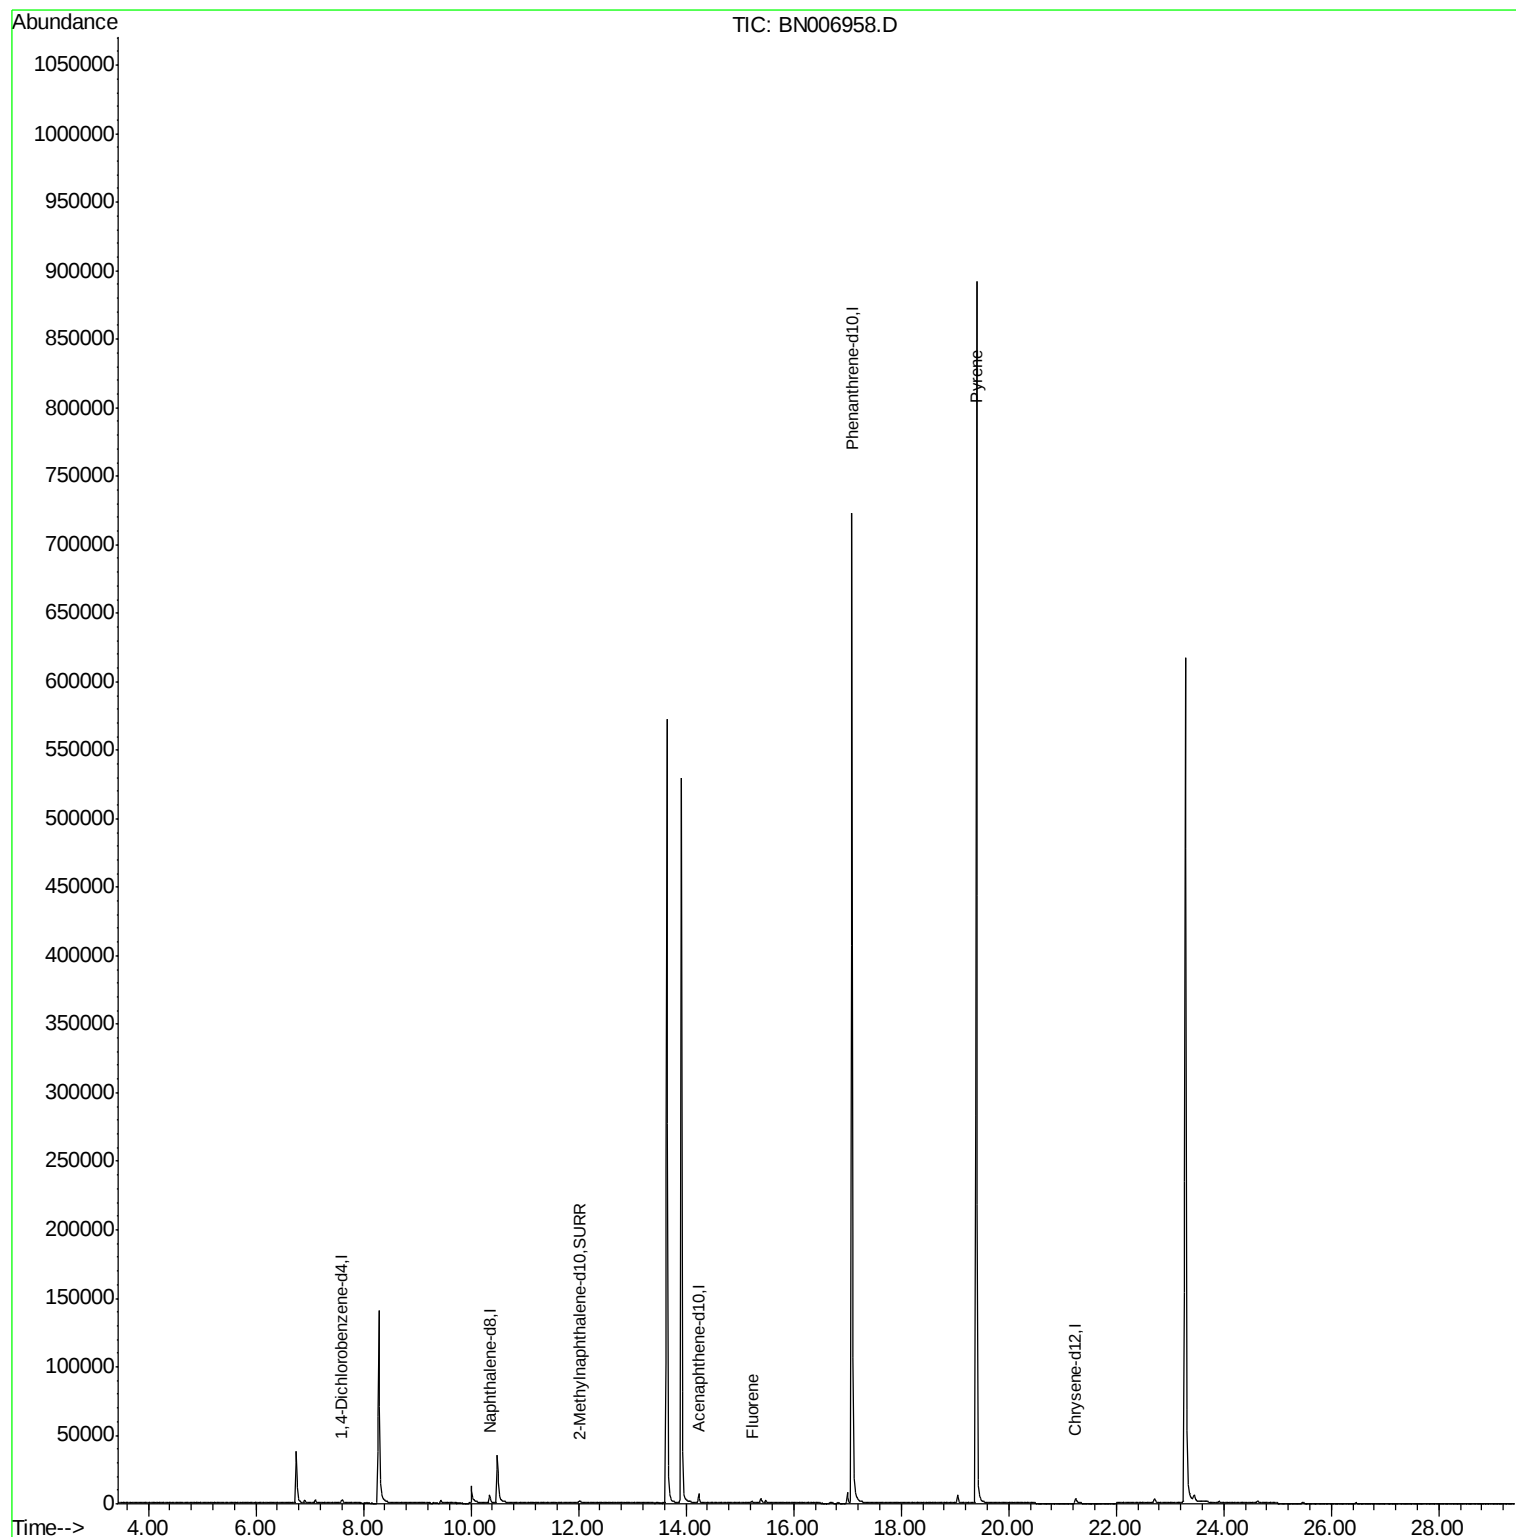


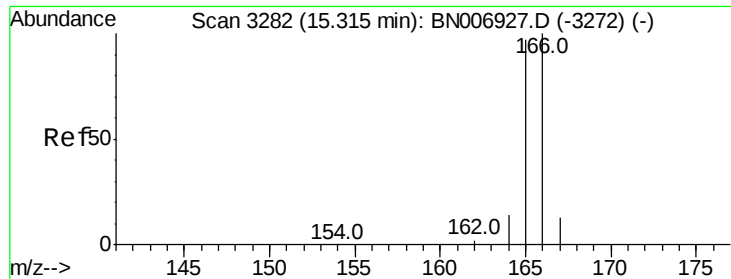

#9
Fluorene
 Concen: 0.074 ng/ul
 RT: 15.23 min Scan# 3264
 Delta R.T. -0.08 min
 Lab File: BN006958.D
 Acq: 23 Jul 2019 01:11

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion:166 Resp: 1362
 Ion Ratio Lower Upper
 166 100
 165 9.2 78.2 117.4#
 167 37.0 11.3 16.9#

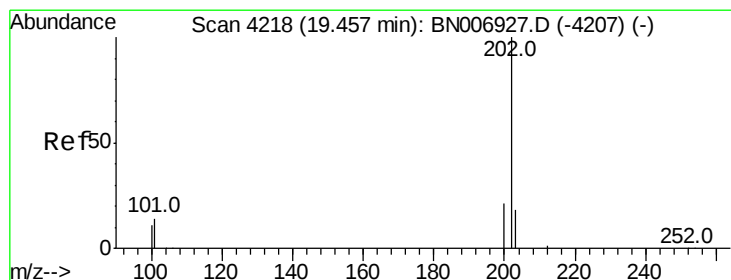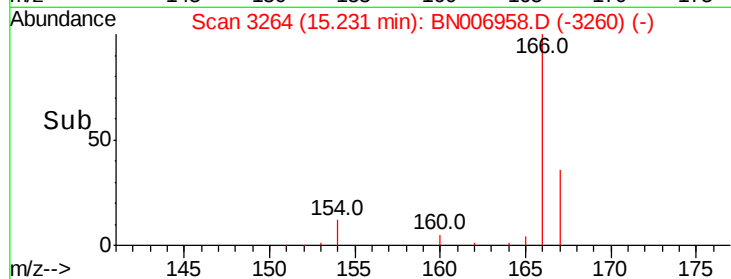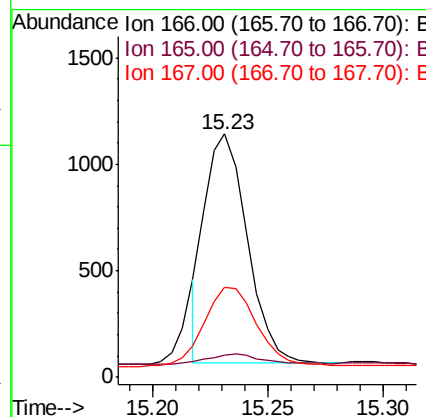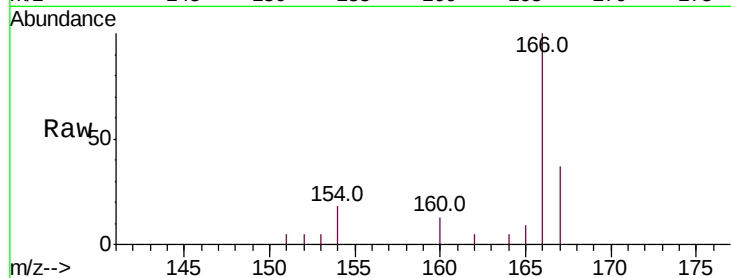

#17
Pyrene
 Concen: 0.059 ng/ul
 RT: 19.40 min Scan# 4206
 Delta R.T. -0.05 min
 Lab File: BN006958.D
 Acq: 23 Jul 2019 01:11

Tgt Ion:202 Resp: 1494
 Ion Ratio Lower Upper
 202 100
 101 179.9 12.2 18.2#
 100 1204.9 9.8 14.8#

