

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
 Data File : BN006961.D
 Acq On : 23 Jul 2019 04:40
 Operator : HP/JU
 Sample : K3890-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 23 06:30:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 23 04:26:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	2614	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	9312	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4659	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	861056	0.40	ng/ul	0.07
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.28	264	648233	0.40	ng/ul	-0.19
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	3660	0.26	ng/ul	0.01
14) Fluoranthene-d10	19.05	212	7211	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.40	128	1015	0.038	ng/ul#	Ovalue 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
Data File : BN006961.D
Acq On : 23 Jul 2019 04:40
Operator : HP/JU
Sample : K3890-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 23 06:30:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 23 04:26:14 2019
Response via : Initial Calibration

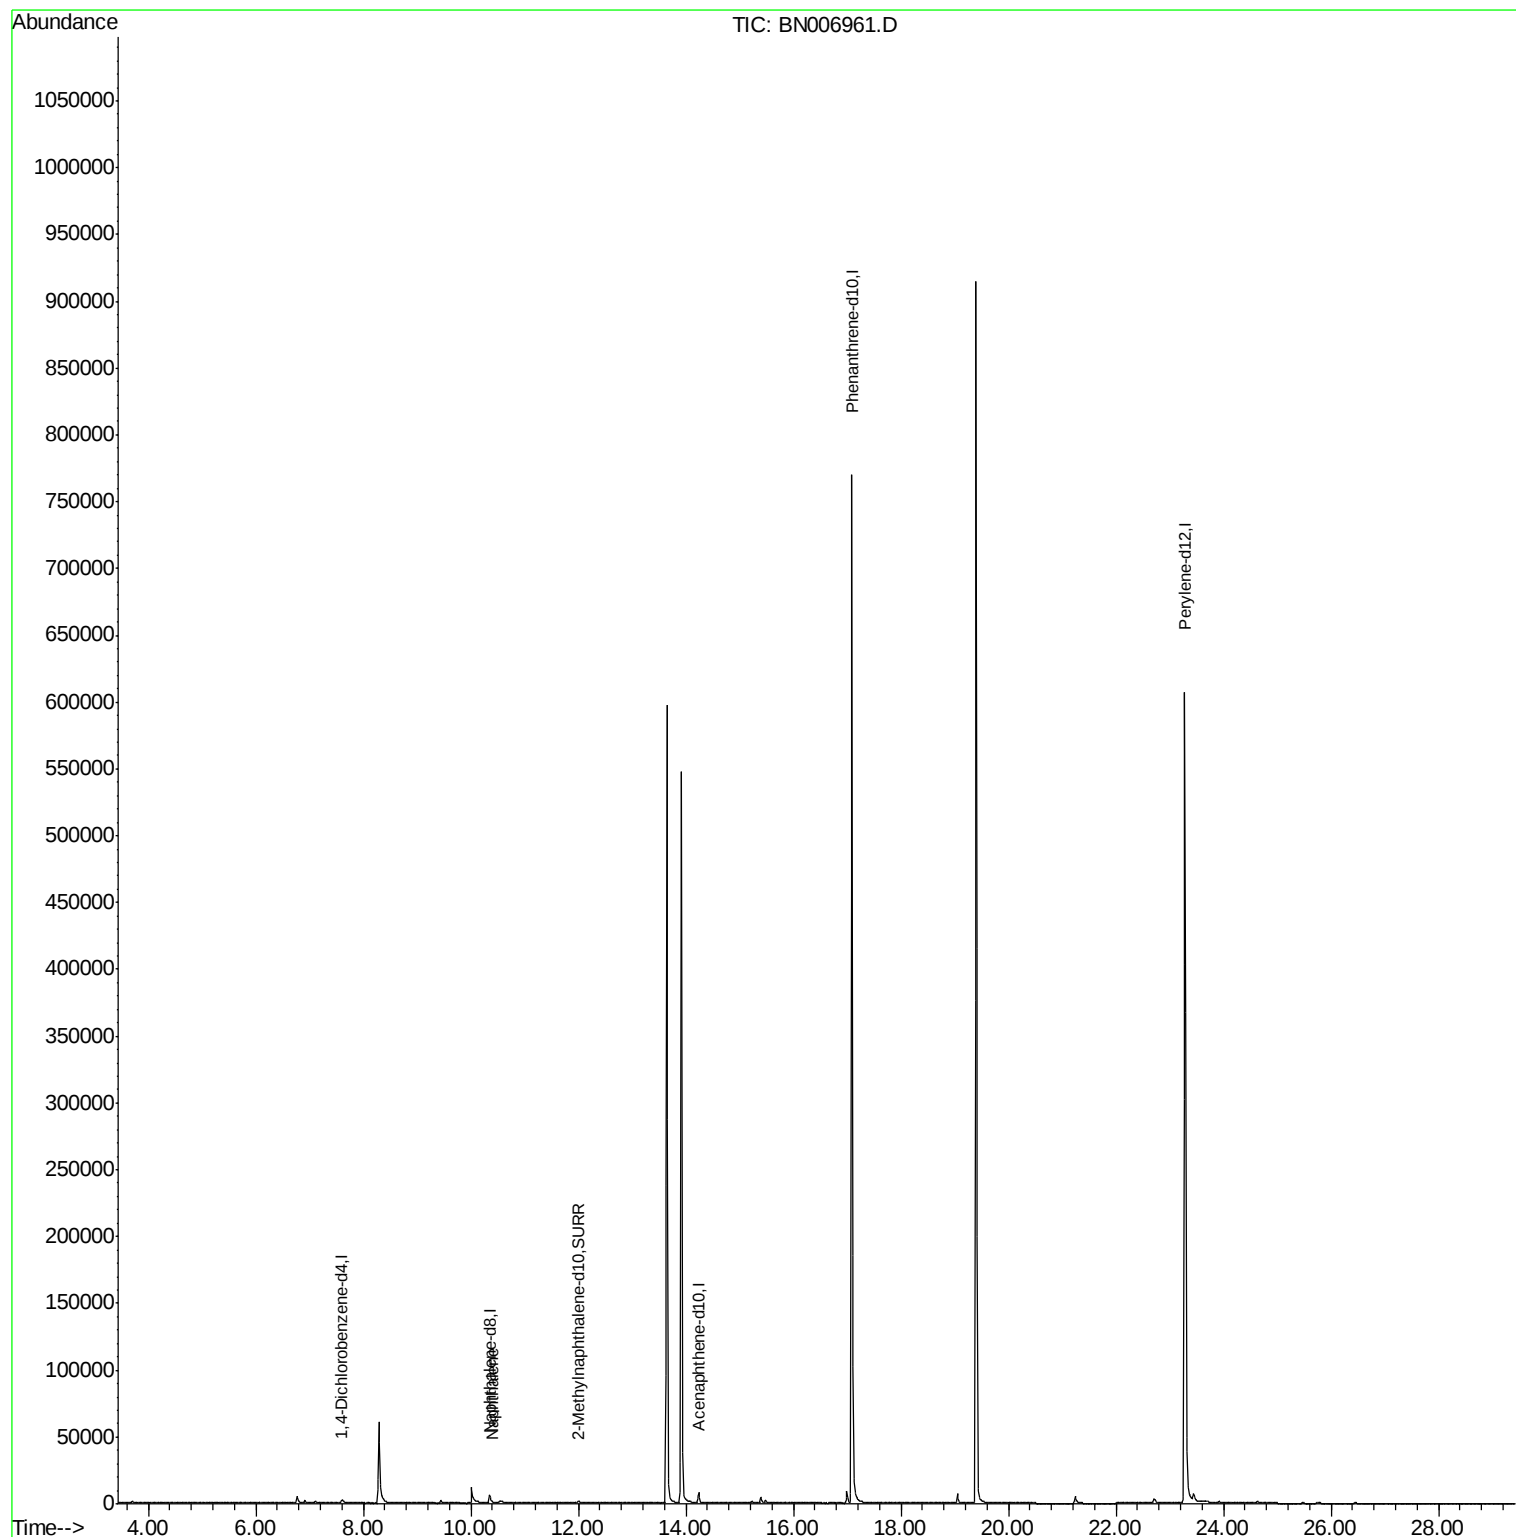

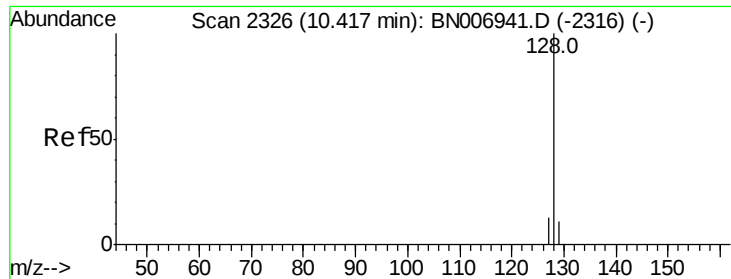

#3

Naphthalene

Concen: 0.038 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.02 min

Lab File: BN006961.D

Acq: 23 Jul 2019 04:40

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 1015

Ion Ratio Lower Upper

128 100

129 26.1 9.4 14.0#

127 21.4 10.6 16.0#

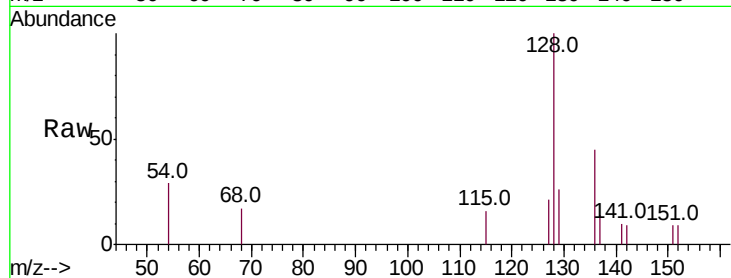

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

