

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
 Data File : BN006962.D
 Acq On : 23 Jul 2019 05:15
 Operator : HP/JU
 Sample : K3890-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 23 06:30:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 23 04:26:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	2392	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	8646	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4338	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	810545	0.40	ng/ul	0.07
16) Chrysene-d12	21.24	240	5590	0.40	ng/ul	0.00
20) Perylene-d12	23.29	264	627762	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	3189	0.24	ng/ul	0.02
14) Fluoranthene-d10	19.05	212	6623	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.40	128	1048	0.042	ng/ul#	73
17) Pyrene	19.43	202	1106	0.043	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
Data File : BN006962.D
Acq On : 23 Jul 2019 05:15
Operator : HP/JU
Sample : K3890-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 23 06:30:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 23 04:26:14 2019
Response via : Initial Calibration

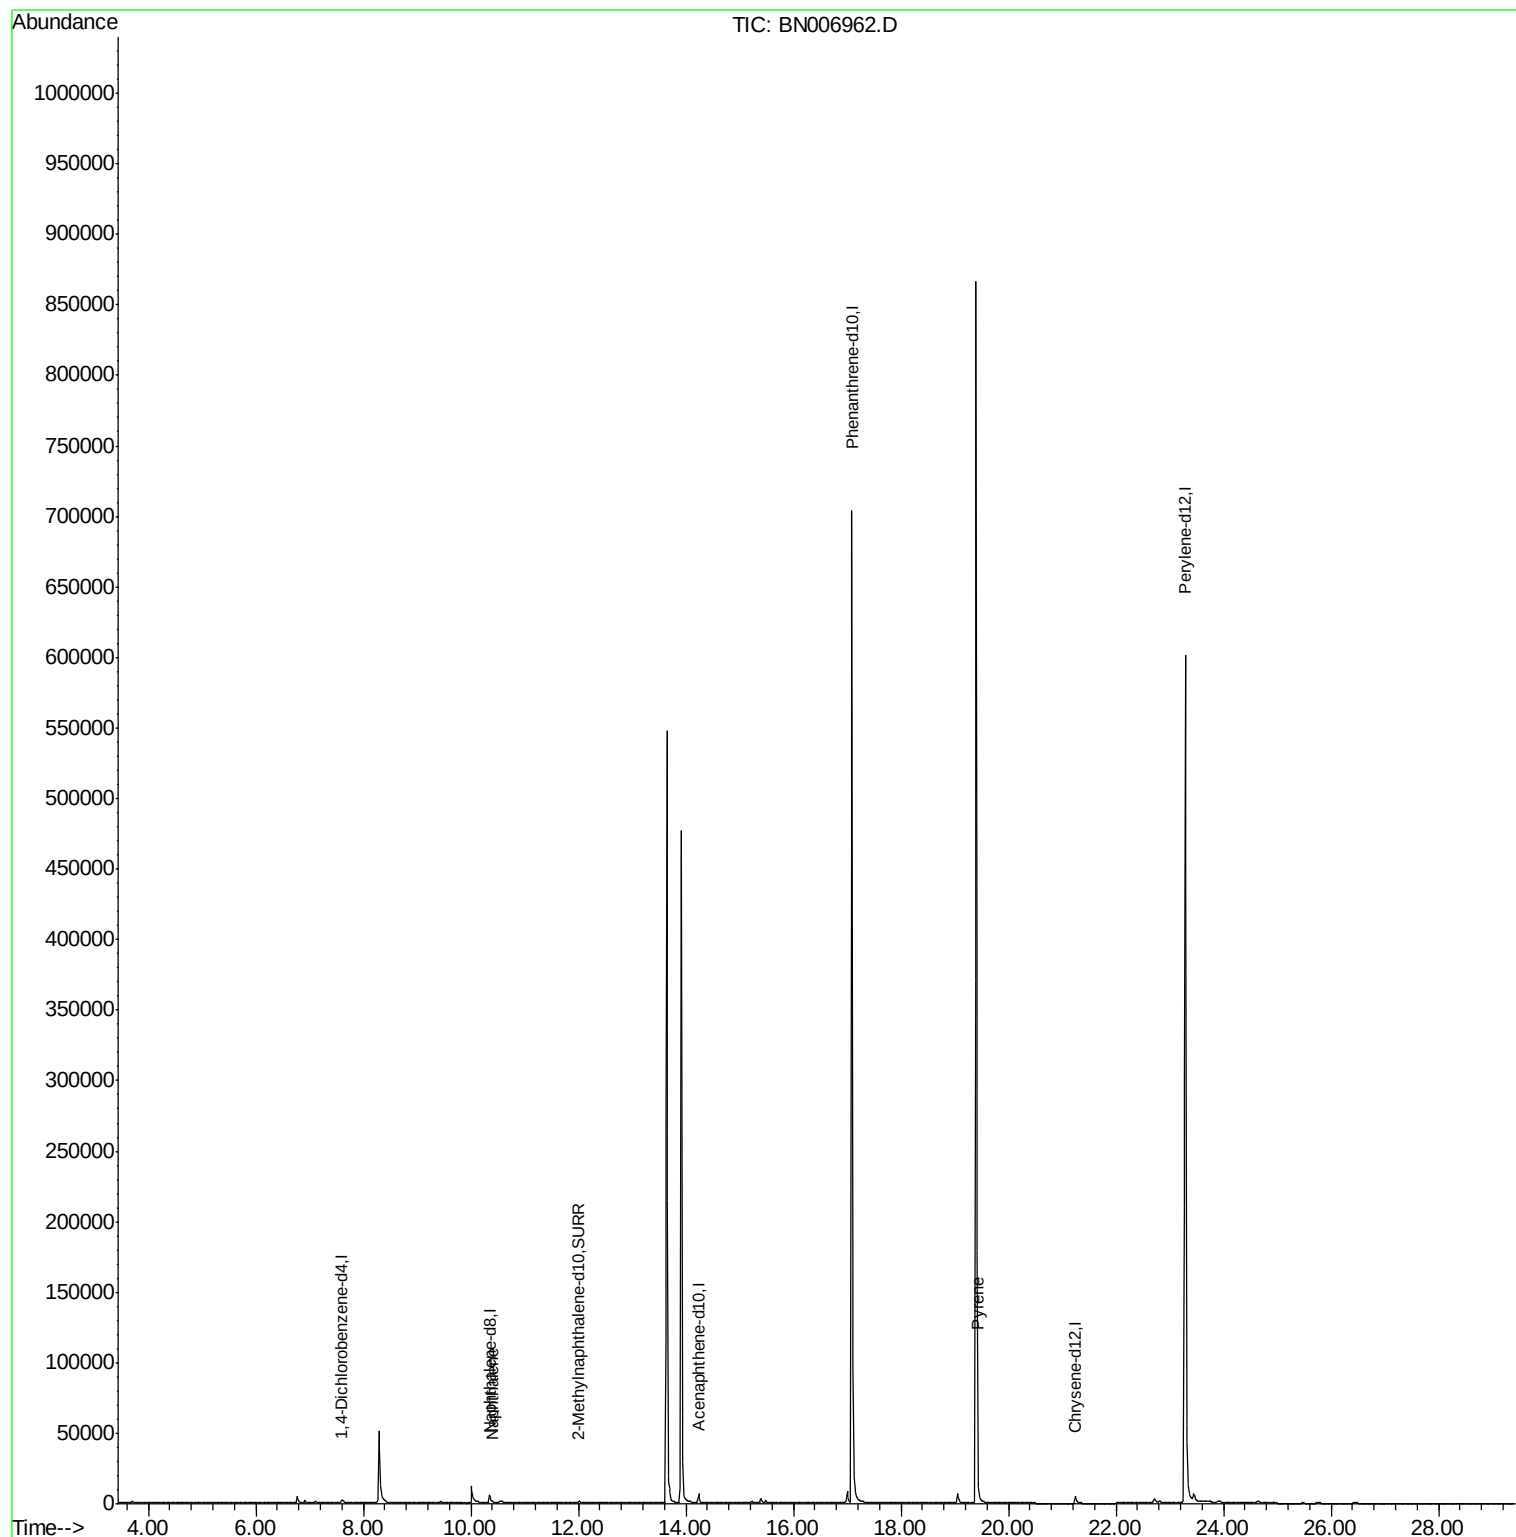

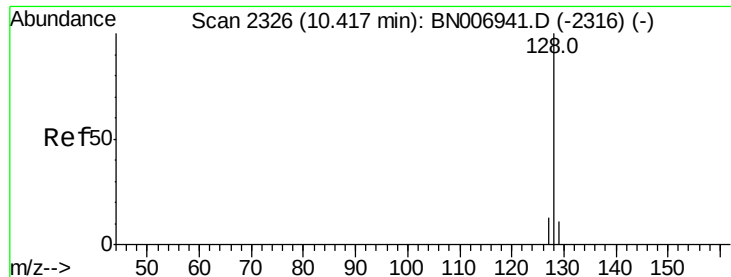

#3

Naphthalene

Concen: 0.042 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.02 min

Lab File: BN006962.D

Acq: 23 Jul 2019 05:15

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 1048

Ion Ratio Lower Upper

128 100

129 25.8 9.4 14.0#




127 21.0 10.6 16.0#

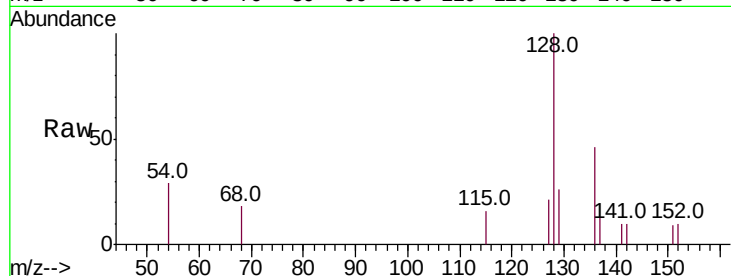

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

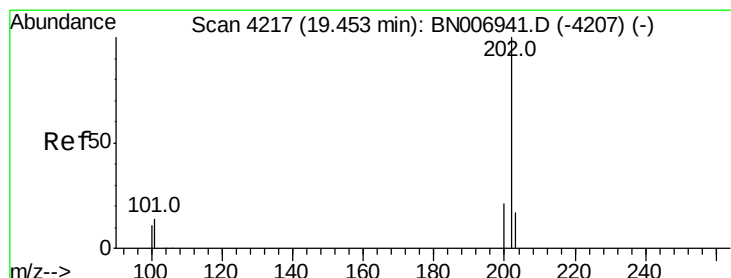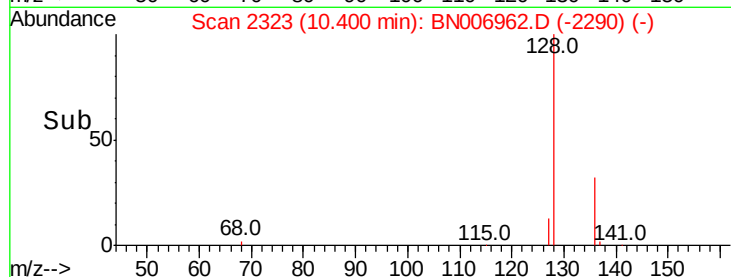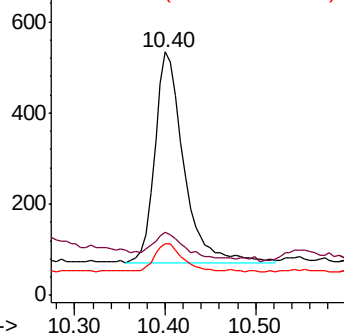

#17

Pyrene

Concen: 0.043 ng/ul

RT: 19.43 min Scan# 4212

Delta R.T. -0.02 min

Lab File: BN006962.D

Acq: 23 Jul 2019 05:15


Tgt Ion:202 Resp: 1106

Ion Ratio Lower Upper

202 100

101 28.3 12.2 18.2#

100 54.4 9.8 14.8#

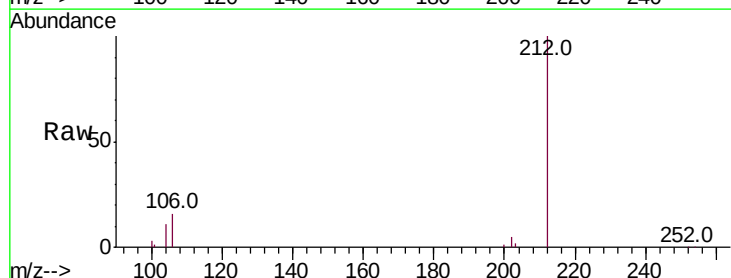

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

