

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
 Data File : BN006963.D
 Acq On : 23 Jul 2019 05:49
 Operator : HP/JU
 Sample : K3920-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 23 06:30:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 23 04:26:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2546	0.40	ng/ul	-0.02
2) Naphthalene-d8	10.35	136	8999	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.23	164	4515	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	843322	0.40	ng/ul	0.07
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.28	264	598358	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	3786	0.27	ng/ul	-0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.40	128	816	0.032	ng/ul#	Ovalue 42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072219\
Data File : BN006963.D
Acq On : 23 Jul 2019 05:49
Operator : HP/JU
Sample : K3920-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 23 06:30:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 23 04:26:14 2019
Response via : Initial Calibration

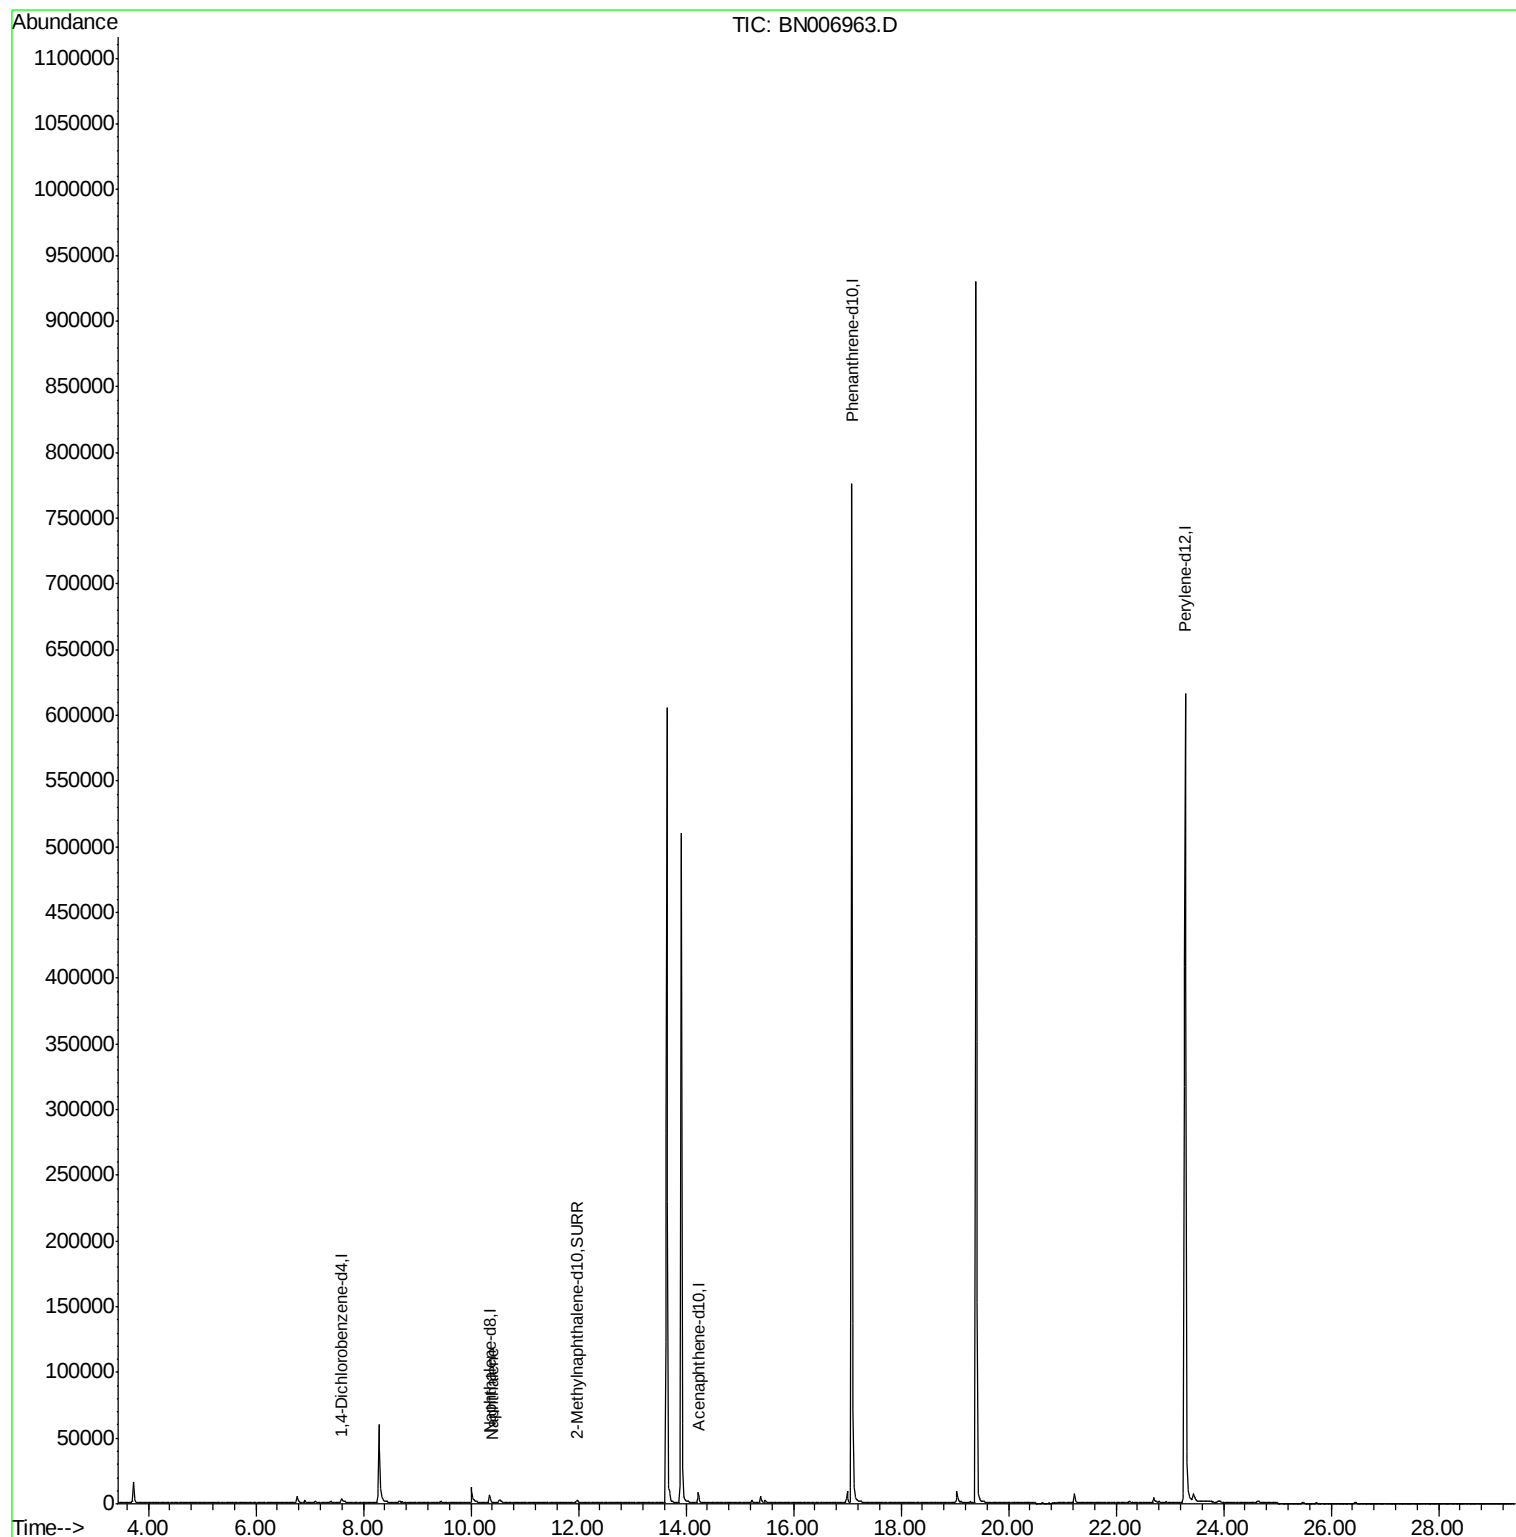

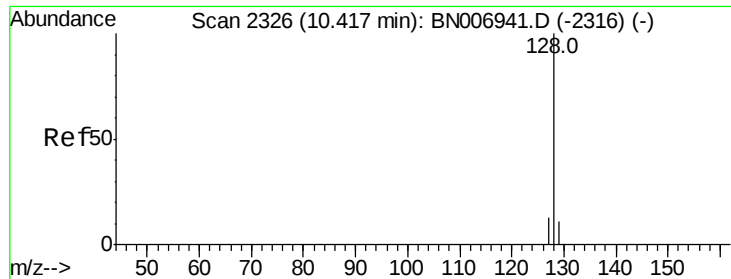

#3

Napthalene

Concen: 0.032 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.02 min

Lab File: BN006963.D

Acq: 23 Jul 2019 05:49

Instrument :

BNA_N

ClientSampleId :


Tot Ion:128 Resp: 816

Ion Ratio Lower Upper

128 100

129 39.8 9.4 14.0#

127 31.3 10.6 16.0#

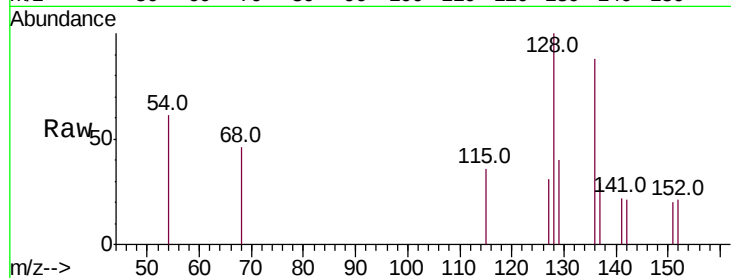

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

