
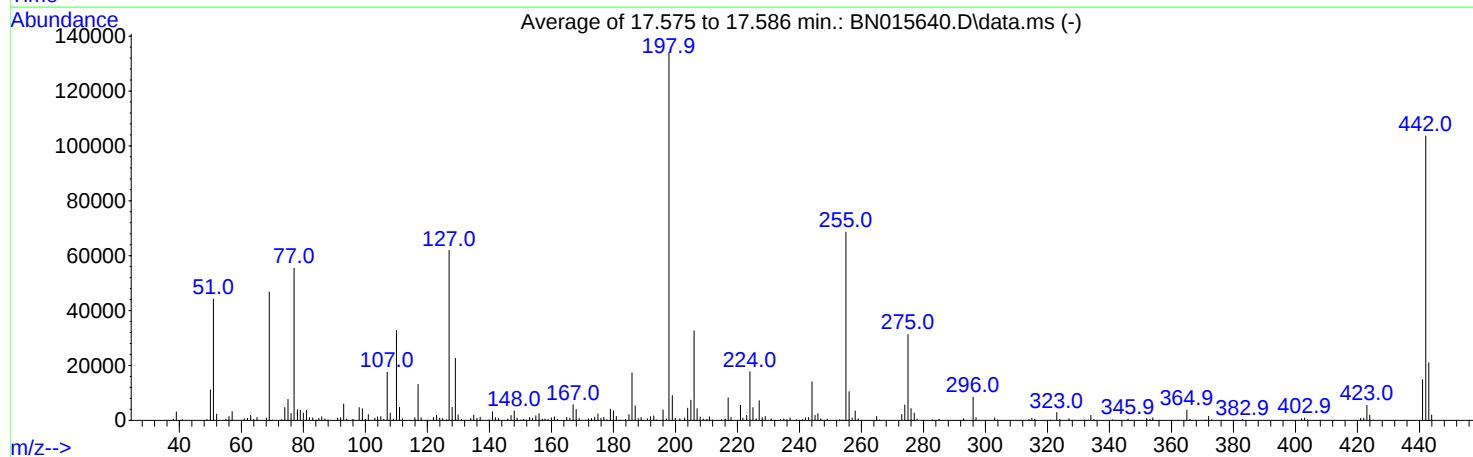


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072221\
 Data File : BN015640.D
 Acq On : 21 Jul 2021 11:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 21 16:45:21 2021

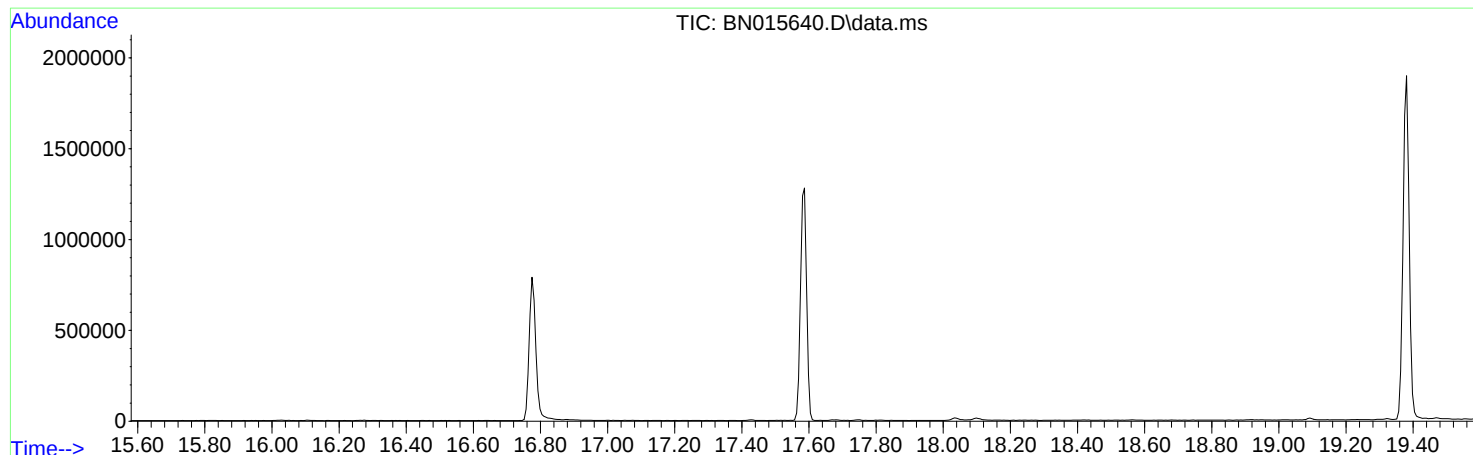




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	44211	PASS
68	69	0.00	2	1.8	857	PASS
69	198	0.00	100	34.9	46747	PASS
70	69	0.00	2	0.3	119	PASS
127	198	10	80	46.2	61899	PASS
197	198	0.00	2	0.4	541	PASS
198	198	100	100	100.0	134029	PASS
199	198	5	9	6.7	9022	PASS
275	198	10	60	23.4	31312	PASS
365	198	1	100	2.8	3723	PASS
441	198	0.01	100	11.1	14818	PASS
442	442	50	100	100.0	103619	PASS
443	442	15	24	20.3	21011	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072221\
Data File : BN015640.D
Acq On : 21 Jul 2021 11:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 21 12:25:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 05:41:44 2021
Response via : Initial Calibration

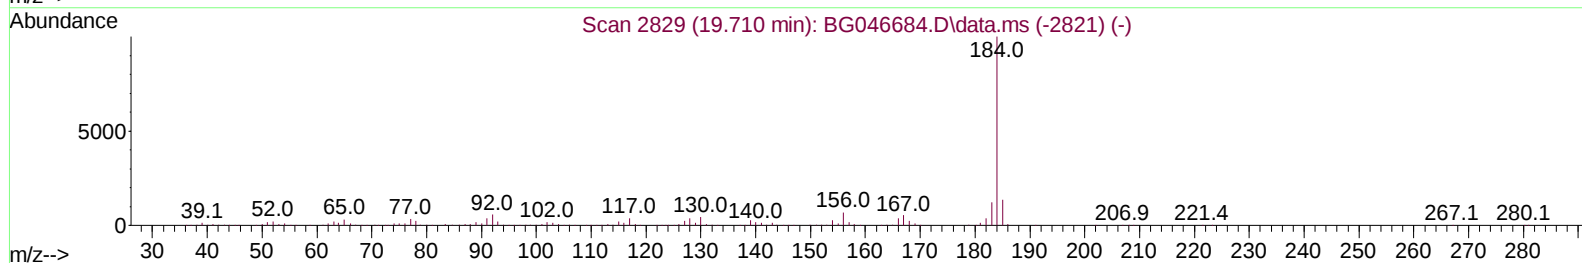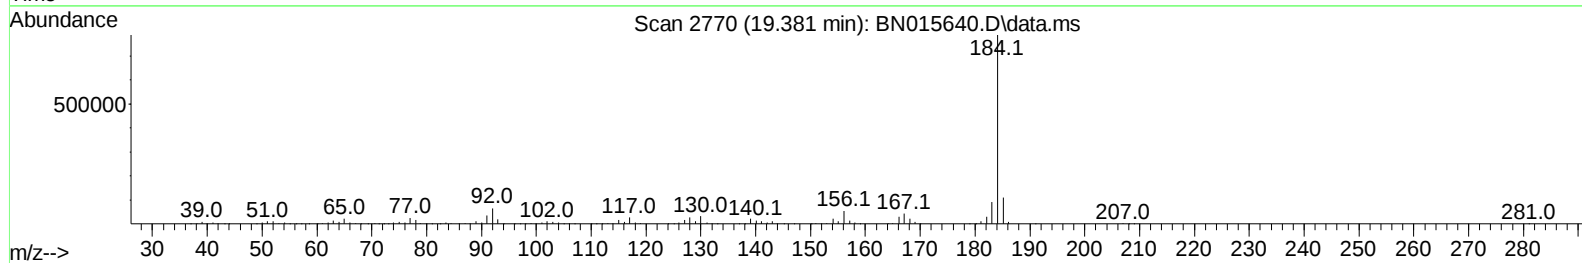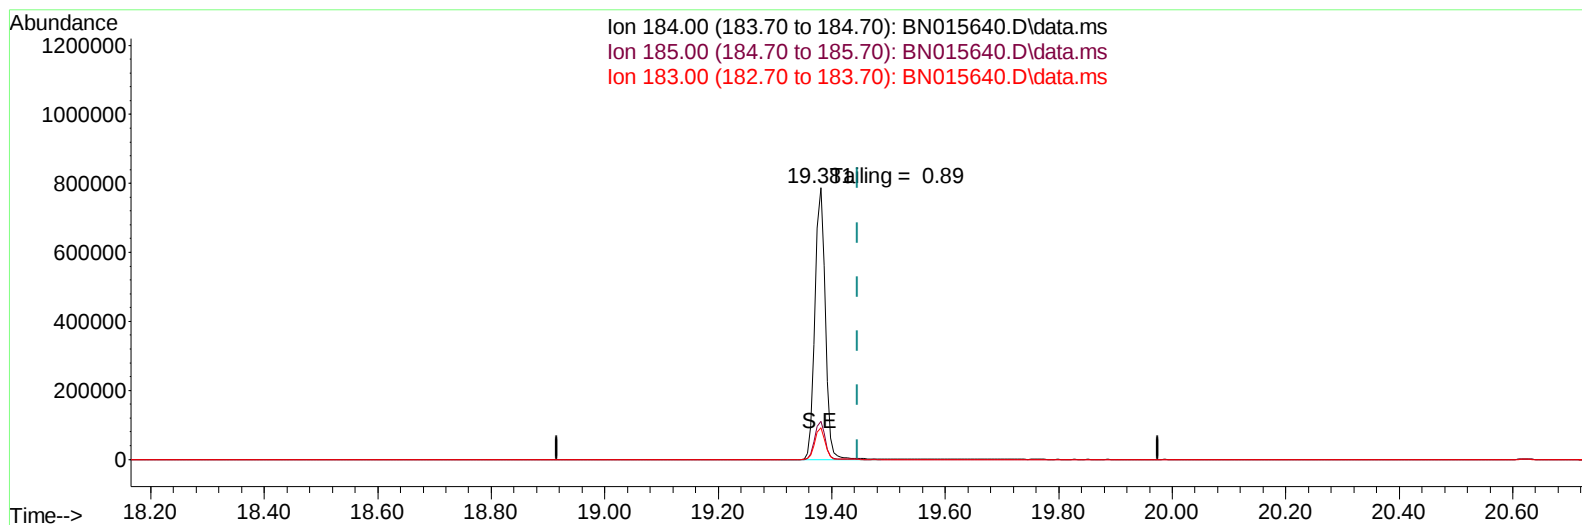

TIC: BN015640.D\data.ms

(77) Benzidine

19.381min (-0.065) 0.00 ng

response 998845

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.94
183.00	13.20	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/22/2021	BNA_N	<u>BN015640.D</u>
Compound Name	Response	Retention Time
DDT	479851	20.62
DDD	331	20.18
DDE	425	19.675
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
756	480607	0.16

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP