

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072222\
 Data File : BN020814.D
 Acq On : 22 Jul 2022 11:13
 Operator : CG/JU
 Sample : PB146344BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 22 23:35:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 01:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	2203	0.400	ng/ul	0.00
4) Naphthalene-d8	10.612	136	7658	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.470	164	4839	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.217	188	10066	0.400	ng/ul	0.00
17) Chrysene-d12	21.429	240	8180	0.400	ng/ul	0.00
23) Perylene-d12	23.767	264	9714	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	15129	5.928	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	3791	0.302	ng/ul	0.00
18) Fluoranthene-d10	19.258	212	9119	0.338	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.615	202	1272	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.615	252	2905	0.071	ng/ul#	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072222\
Data File : BN020814.D
Acq On : 22 Jul 2022 11:13
Operator : CG/JU
Sample : PB146344BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 22 23:35:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 01:02:30 2022
Response via : Initial Calibration




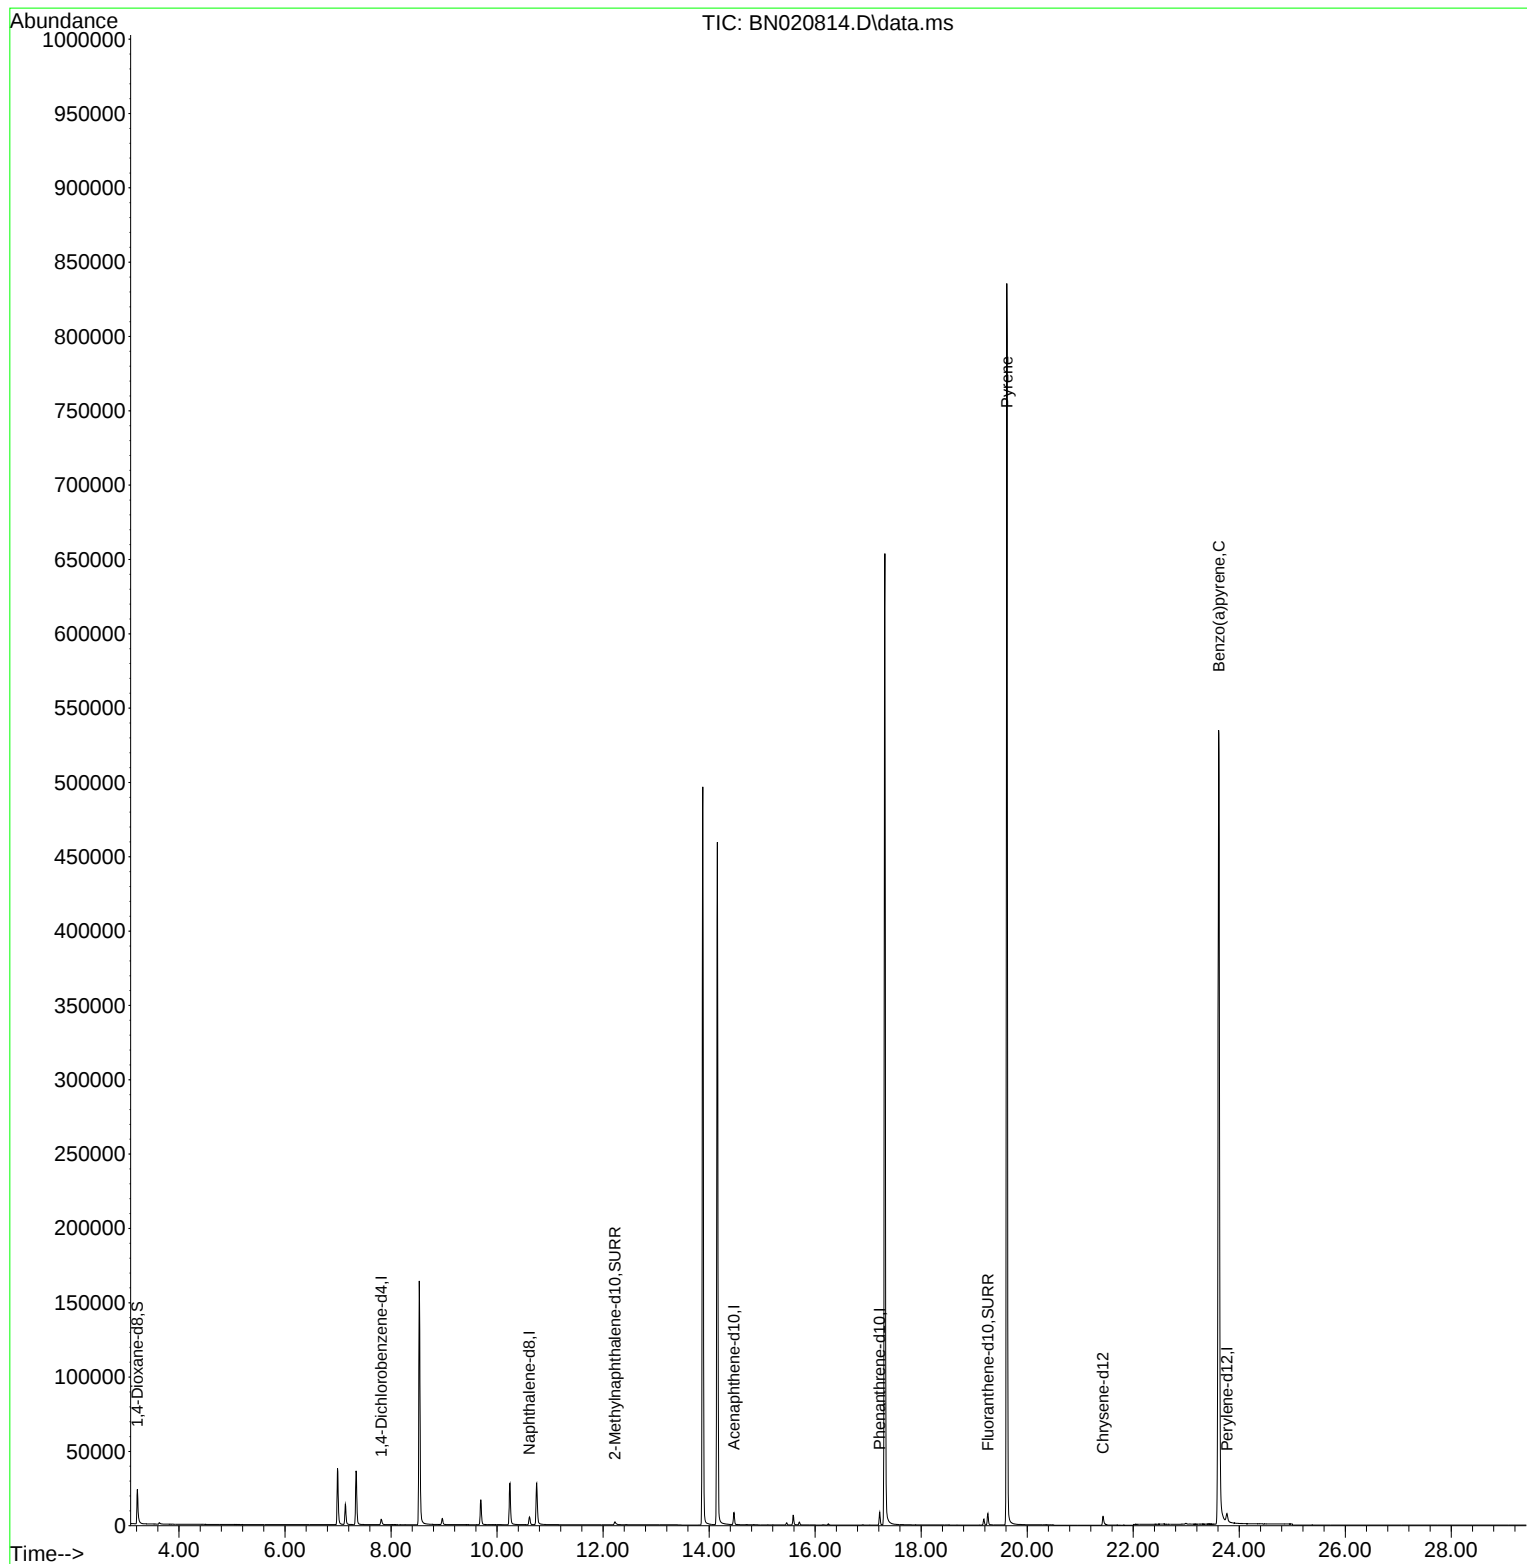


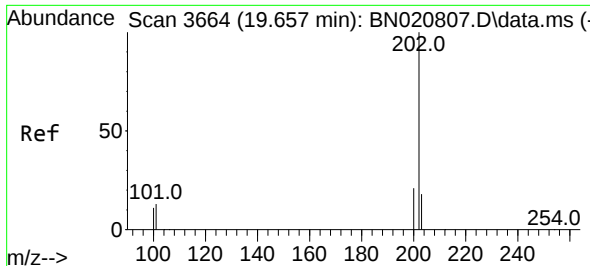

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.615 min Scan# 3655
Delta R.T. -0.038 min
Lab File: BN020814.D
Acq: 22 Jul 2022 11:13

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1272
Ion Ratio Lower Upper
202 100
101 182.4 11.6 17.4#
100 1372.0 9.2 13.8#

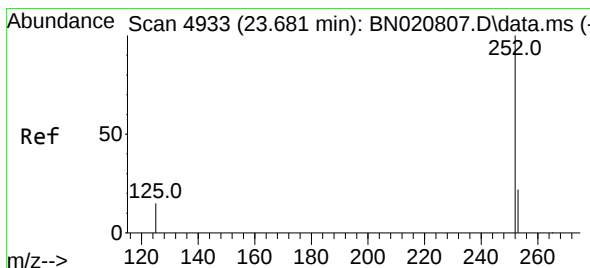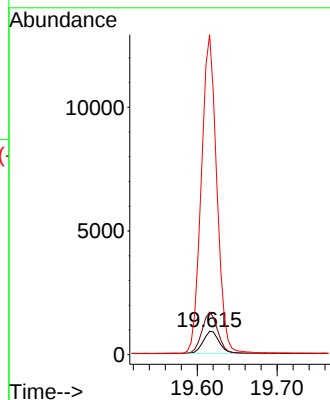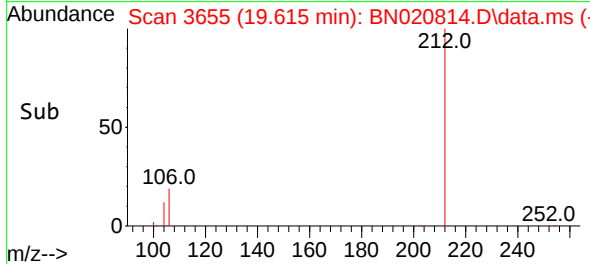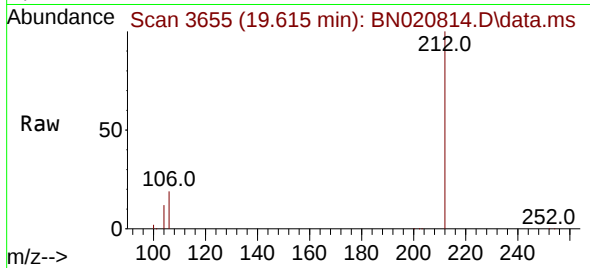

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.615 min Scan# 4911
Delta R.T. -0.059 min
Lab File: BN020814.D
Acq: 22 Jul 2022 11:13

Tgt Ion:252 Resp: 2905
Ion Ratio Lower Upper
252 100
253 44.3 21.0 31.4#
125 35.1 18.8 28.2#

