

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072222\
 Data File : BN020816.D
 Acq On : 22 Jul 2022 12:27
 Operator : CG/JU
 Sample : N3704-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 22 23:35:32 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 20 01:02:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	2928	0.400	ng/ul	0.00
4) Naphthalene-d8	10.611	136	11546	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.468	164	6093	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.216	188	15726	0.400	ng/ul	0.00
17) Chrysene-d12	21.429	240	14559	0.400	ng/ul	0.00
23) Perylene-d12	23.770	264	14863	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.214	96	25138	7.411	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.216	152	6259	0.330	ng/ul	0.00
18) Fluoranthene-d10	19.256	212	17170	0.358	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.463	166	1873	0.068	ng/ul#	14
20) Pyrene	19.618	202	2060	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.618	252	4308	0.069	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072222\
Data File : BN020816.D
Acq On : 22 Jul 2022 12:27
Operator : CG/JU
Sample : N3704-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jul 22 23:35:32 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 20 01:02:30 2022
Response via : Initial Calibration

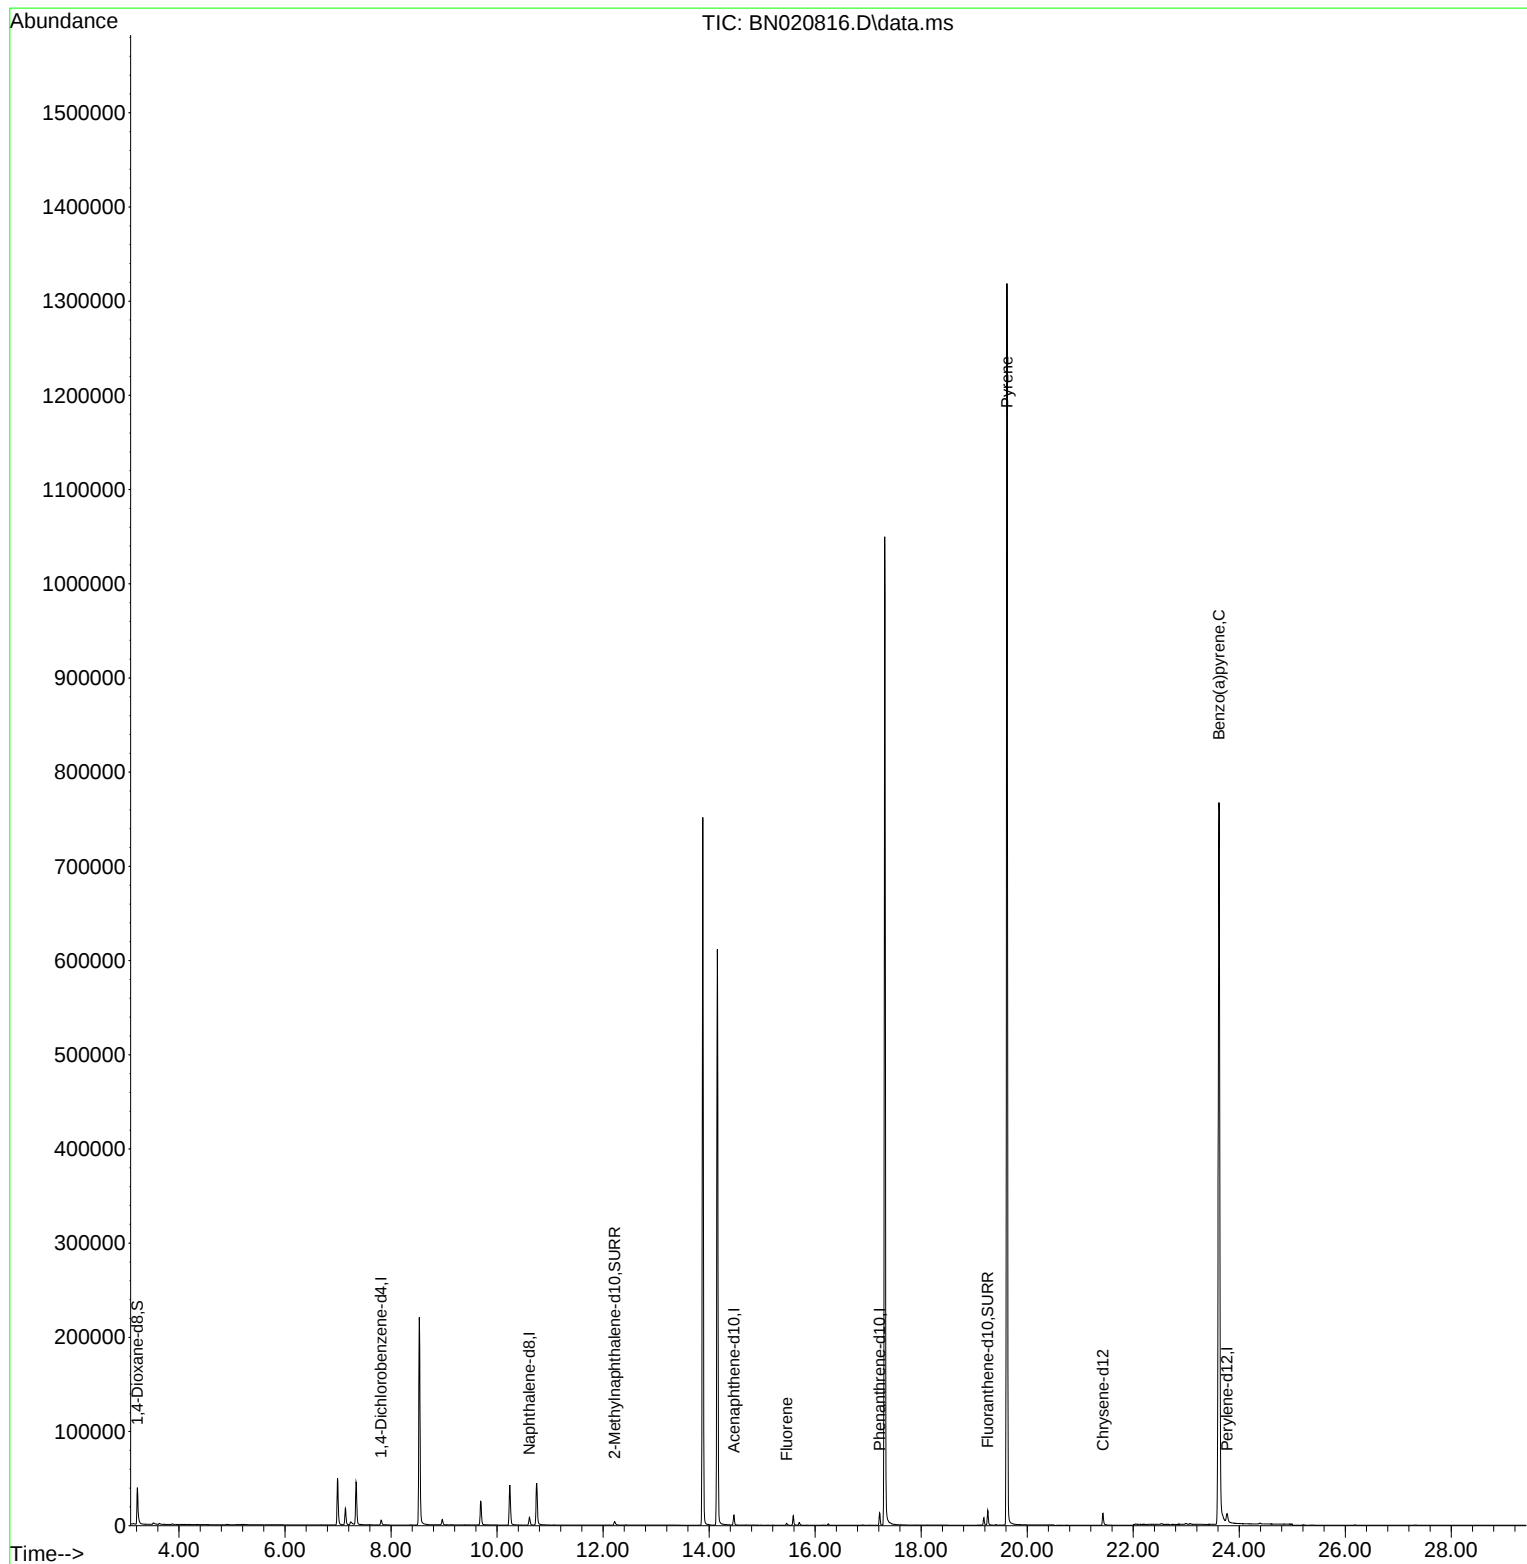



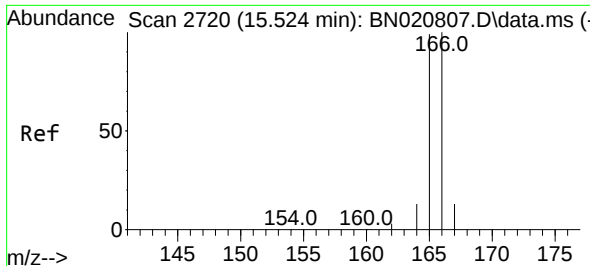


#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.463 min Scan# 21
Delta R.T. -0.062 min
Lab File: BN020816.D
Acq: 22 Jul 2022 12:27

Instrument :
BNA_N
ClientSampleId :



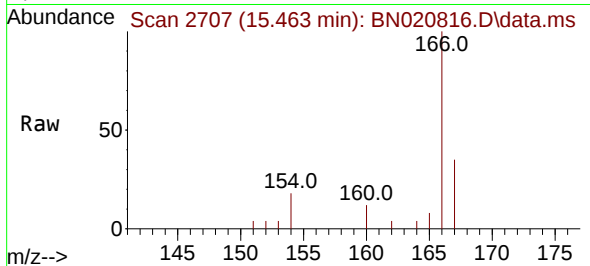



Tgt Ion:166 Resp: 1873
Ion Ratio Lower Upper
166 100
165 7.8 78.2 117.2#
167 35.1 11.3 16.9#

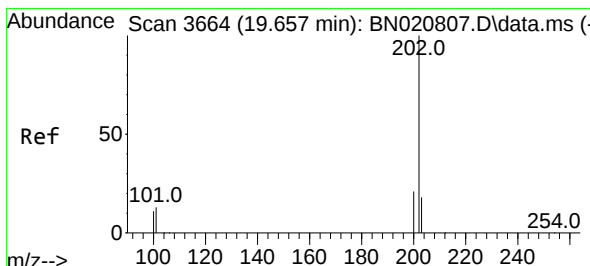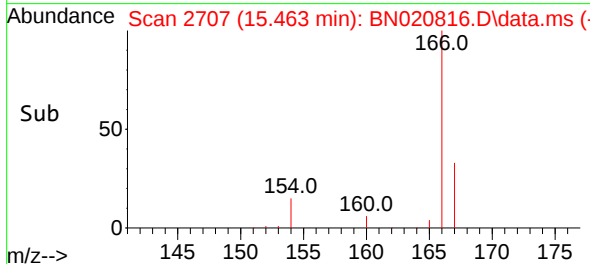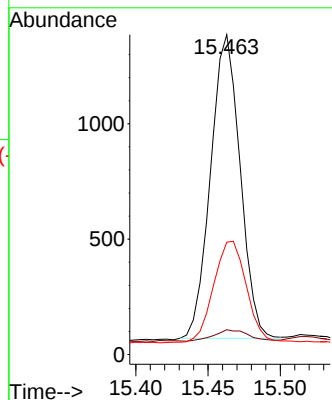

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.618 min Scan# 3656
Delta R.T. -0.035 min
Lab File: BN020816.D
Acq: 22 Jul 2022 12:27

Tgt Ion:202 Resp: 2060
Ion Ratio Lower Upper
202 100
101 183.3 11.6 17.4#
100 1344.4 9.2 13.8#

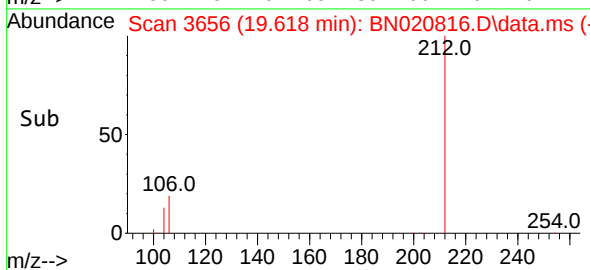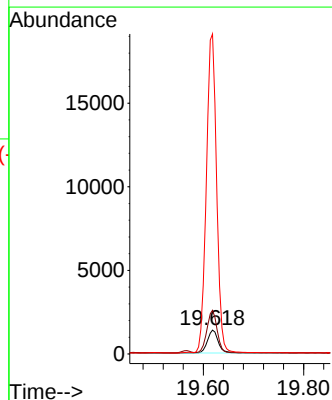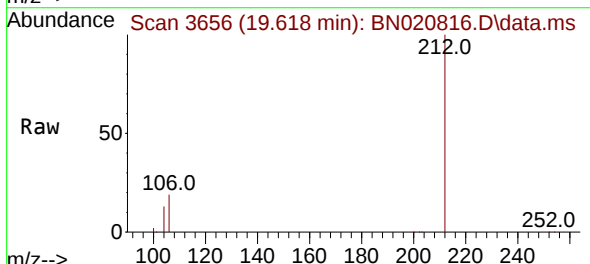

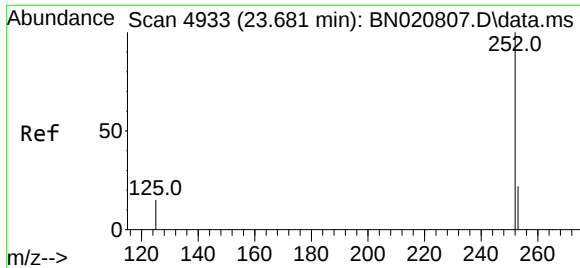

#26

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.618 min Scan# 49

Delta R.T. -0.056 min


Lab File: BN020816.D

Acq: 22 Jul 2022 12:27

Instrument :

BNA_N

ClientSampleId :

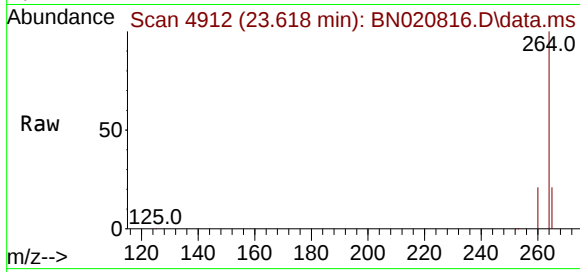

Tgt Ion:252 Resp: 4308

Ion Ratio Lower Upper

252 100

253 42.9 21.0 31.4#

125 42.6 18.8 28.2#

