
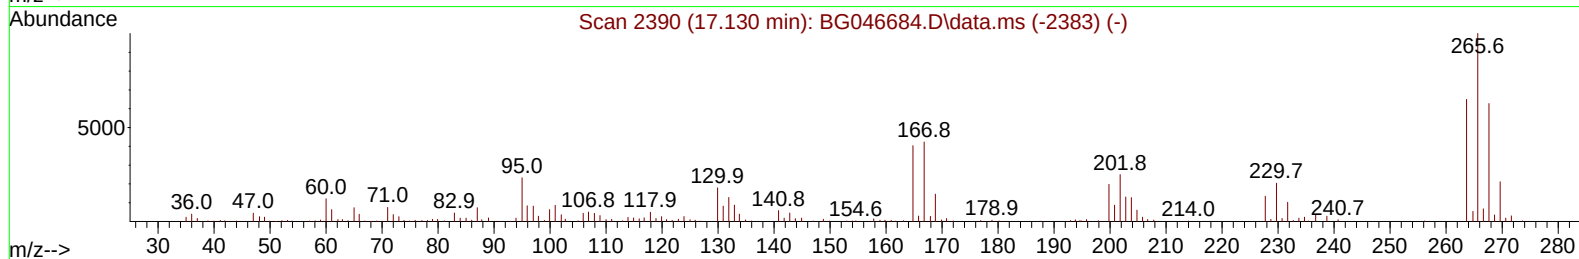
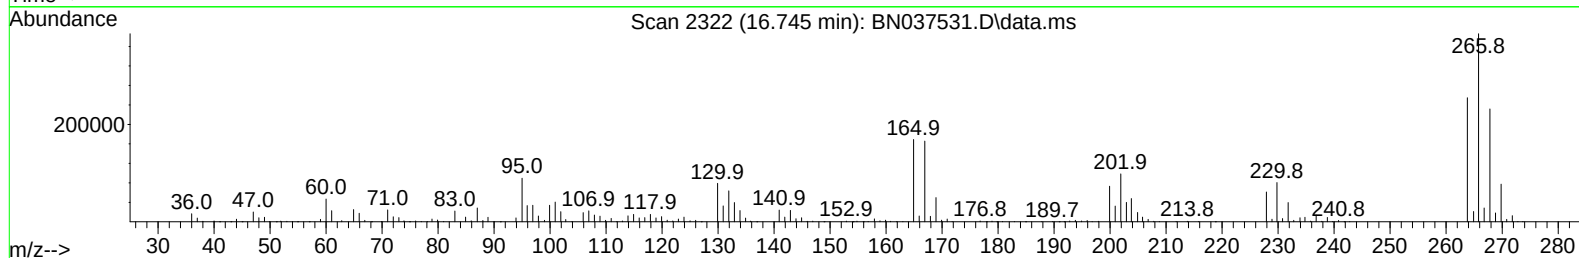


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072225\
Data File : BN037531.D
Acq On : 22 Jul 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 18:01:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

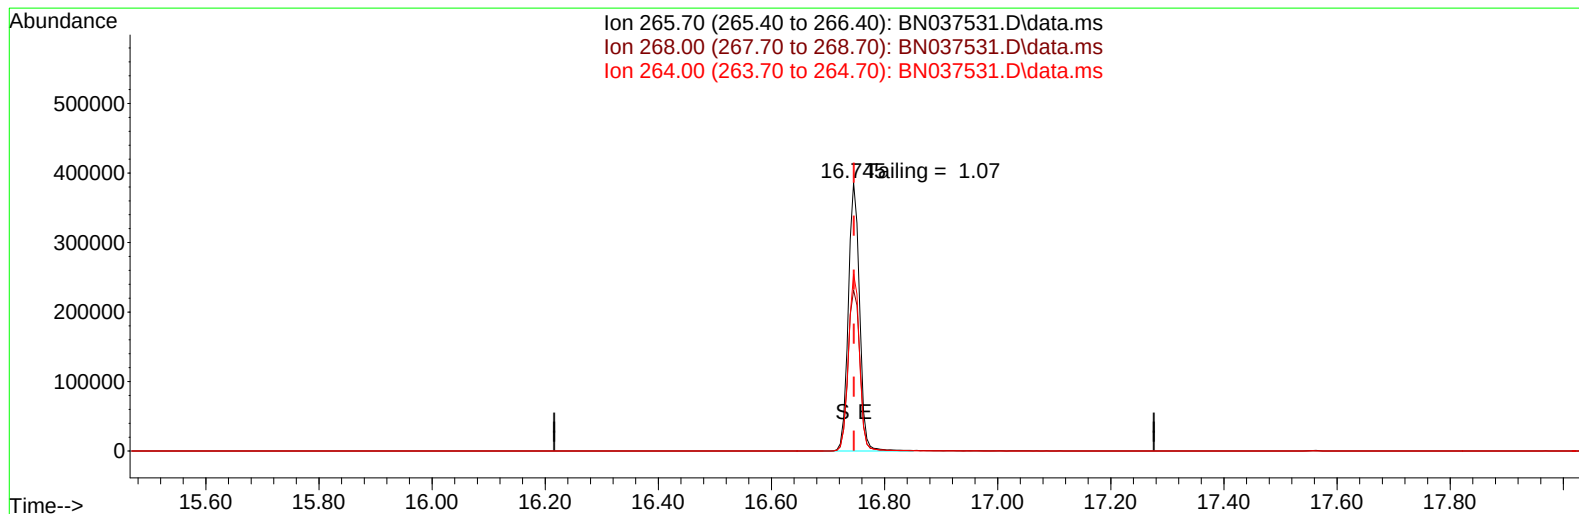

TIC: BN037531.D\data.ms

(70) Pentachlorophenol (C)




16.745min (-0.001) 26722.11 ng

response 535805

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.01
264.00	61.60	65.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072225\
Data File : BN037531.D
Acq On : 22 Jul 2025 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 18:01:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

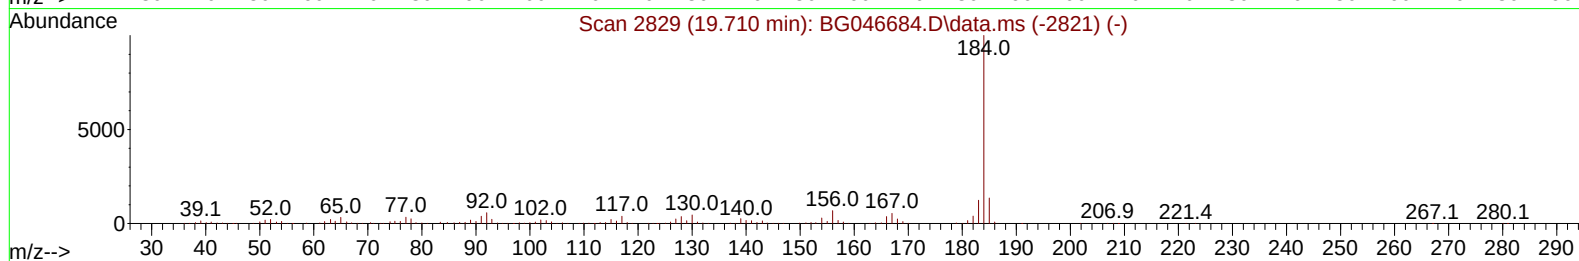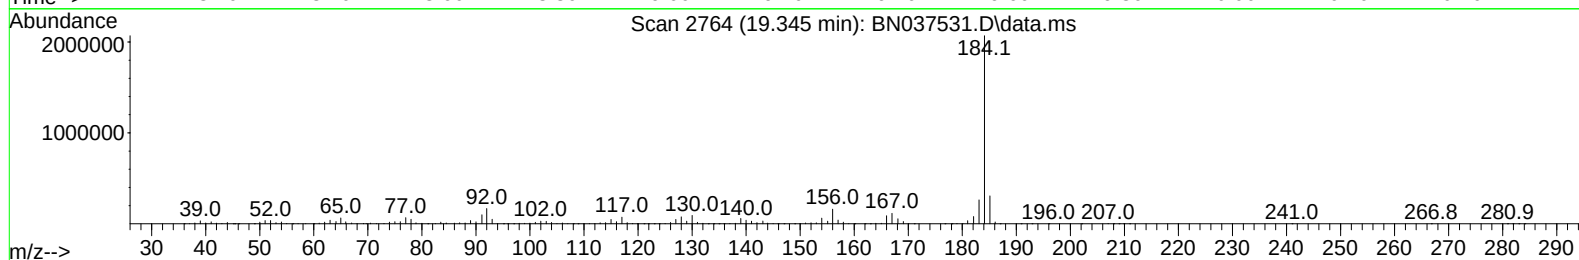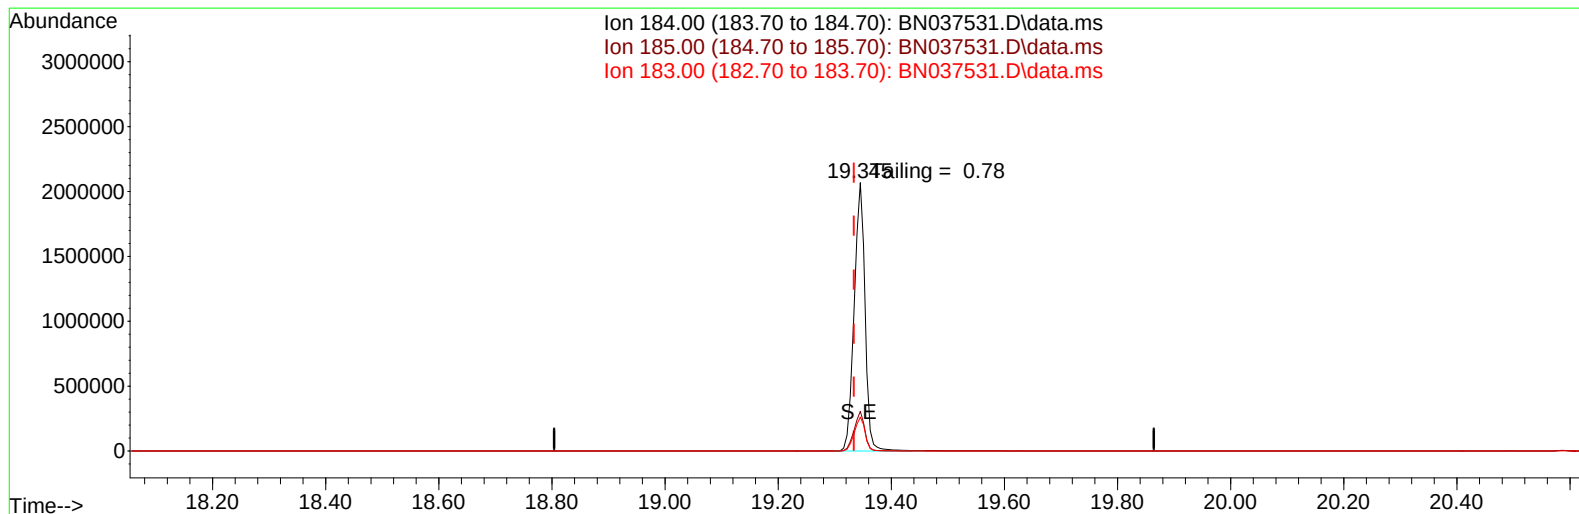

TIC: BN037531.D\data.ms

(77) Benzidine

19.345min (+ 0.011) 0.00 ng

response 2779976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.81
183.00	13.20	12.68
0.00	0.00	0.00