

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072420\
 Data File : BN011259.D
 Acq On : 25 Jul 2020 03:03
 Operator : CG/JU
 Sample : L3388-17
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 25 04:22:14 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 11:01:43 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	203518	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	859649	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	562219	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	1202868	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	1174316	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	949686	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	31234	5.86	ng/uL	0.00
5) Phenol-d5	6.68	99	602678	37.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	324825	37.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	498067	35.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	510869	38.28	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	249983	35.80	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	284814	38.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	507974	35.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	666040	43.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1614851	35.42	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	1975512	36.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.33	143	252432	30.99	ng/ul	0.00
58) Fluorene-d10	15.11	176	1421788	35.26	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	243283	33.14	ng/ul	0.00
71) Anthracene-d10	16.96	188	2120242	36.21	ng/ul	0.00
79) Pyrene-d10	19.27	212	2412488	41.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	1913654	37.19	ng/ul	-0.01
Target Compounds						
15) N-Nitroso-di-n-propylamine	8.19	70	14173	1.218	ng/ul#	1
45) Dimethylphthalate	13.58	163	358966	7.453	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072420\
Data File : BN011259.D
Acq On : 25 Jul 2020 03:03
Operator : CG/JU
Sample : L3388-17
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 25 04:22:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 11:01:43 2020
Response via : Initial Calibration

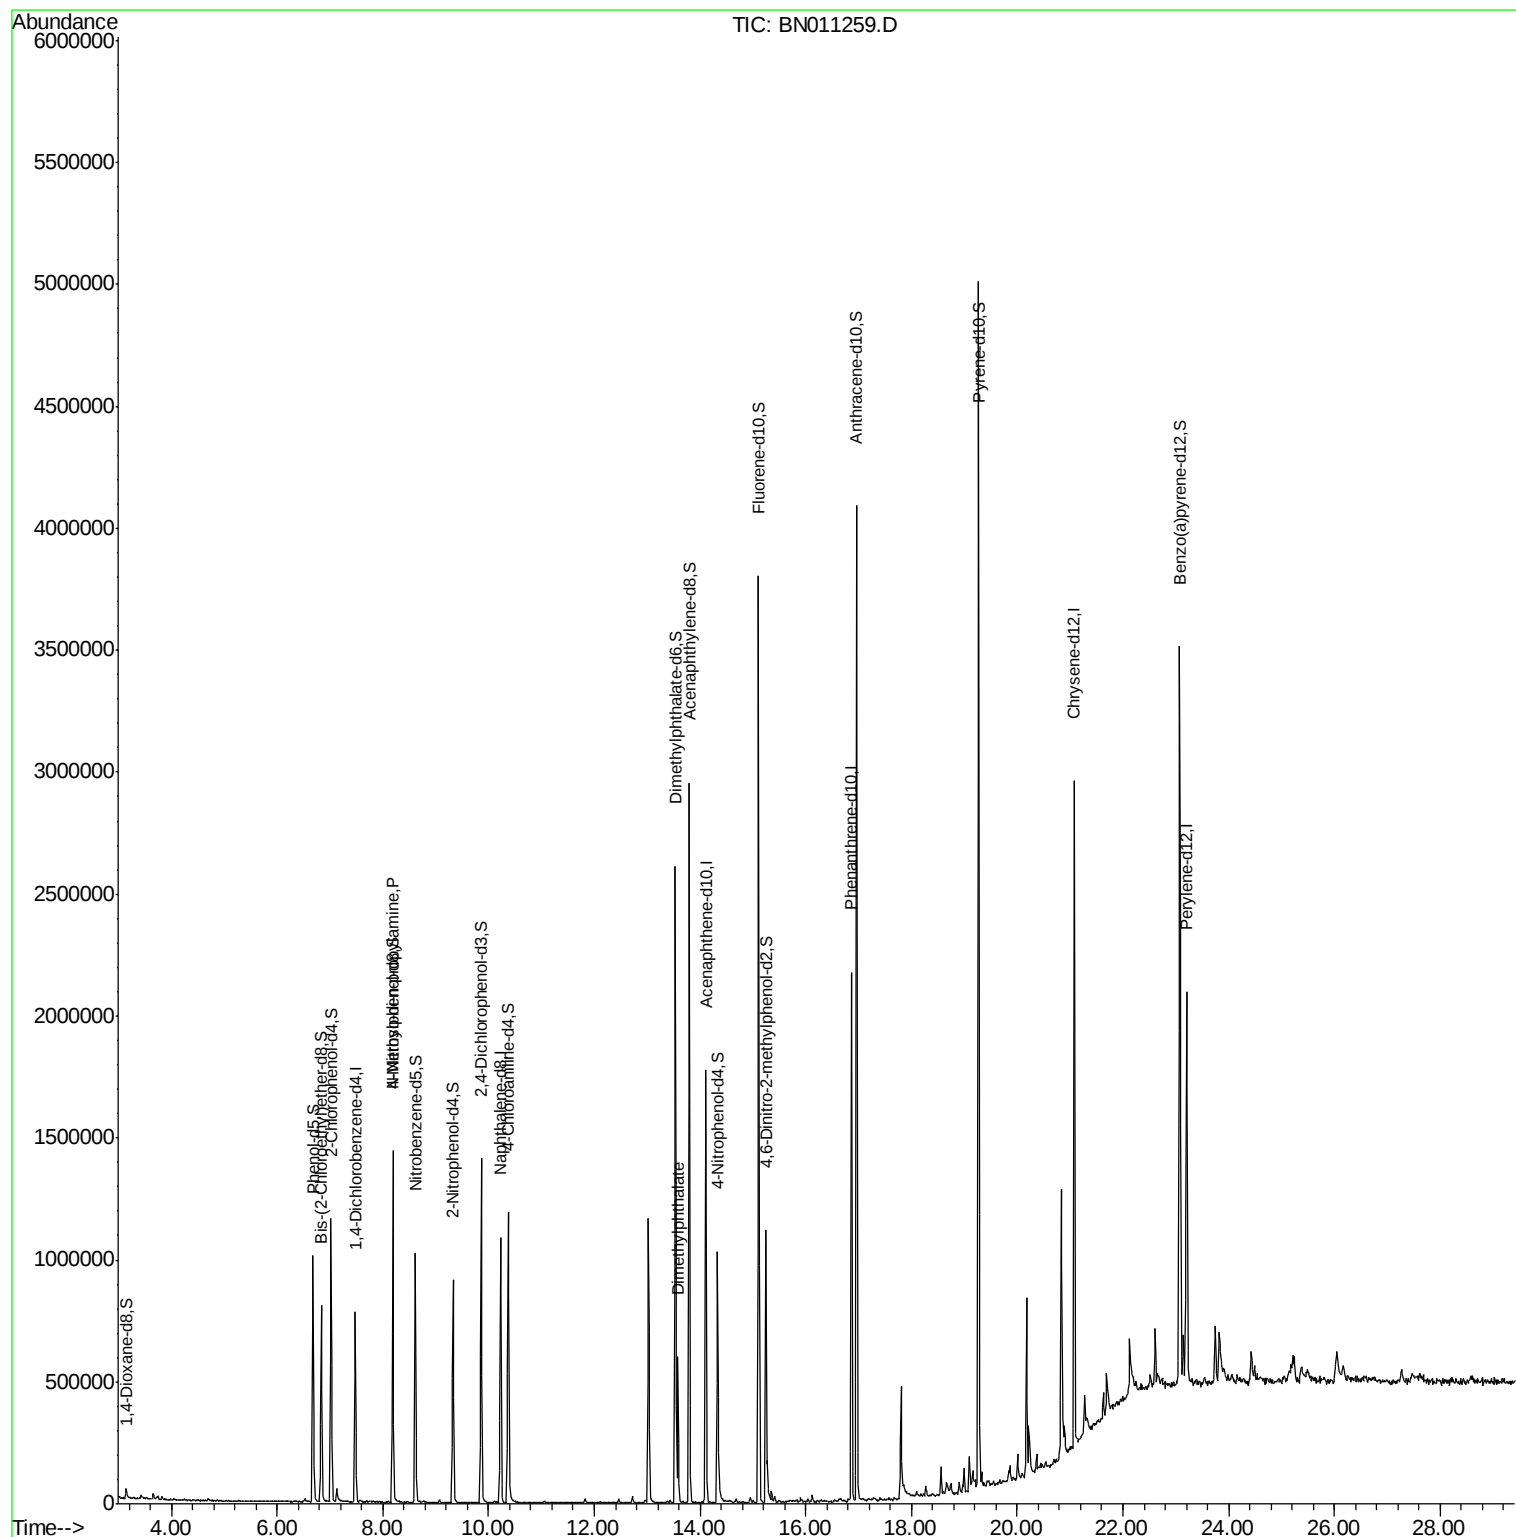

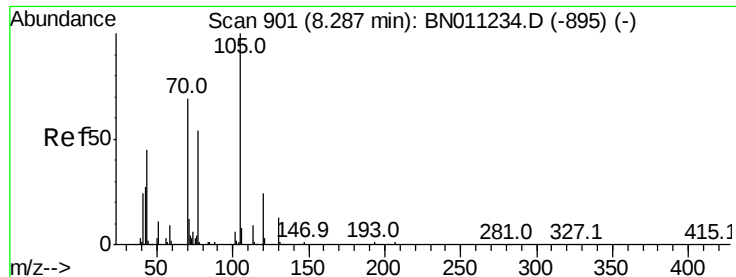

#15

N-Nitroso-di-n-propylamine

Concen: 1.218 ng/ul

RT: 8.19 min Scan# 884

Delta R.T. -0.10 min

Lab File: BN011259.D

Acq: 25 Jul 2020 03:03

Instrument :

BNA_N

ClientSampleId :

Tot Ion: 70 Resp: 14173





Ion Ratio Lower Upper

70 100

42 238.3 31.1 46.7#

101 0.0 8.0 12.0#

130 0.0 16.8 25.2#

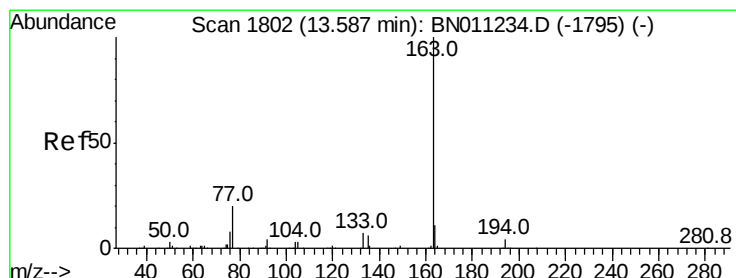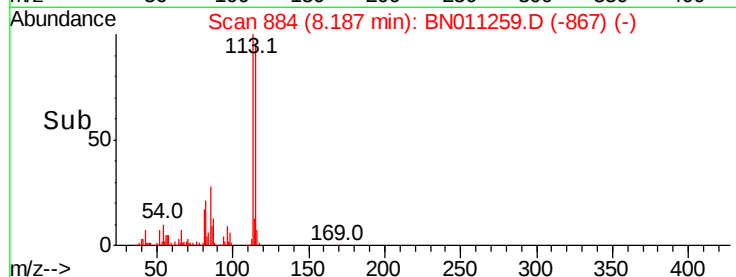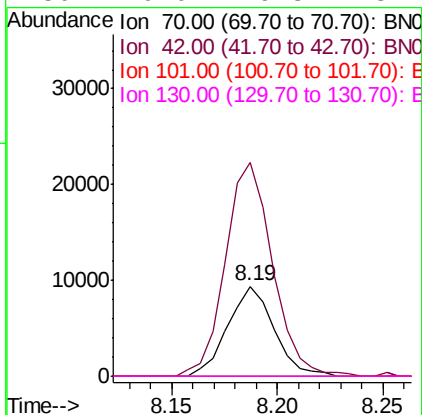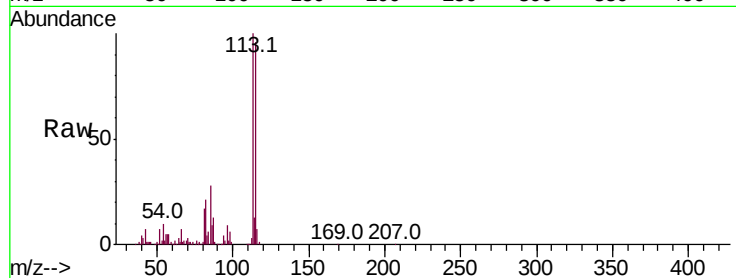

#45

Dimethylphthalate

Concen: 7.453 ng/ul

RT: 13.58 min Scan# 1801

Delta R.T. -0.01 min

Lab File: BN011259.D

Acq: 25 Jul 2020 03:03

Tgt Ion: 163 Resp: 358966

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 9.9 7.8 11.8

