

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
 Data File : BN011239.D
 Acq On : 24 Jul 2020 13:18
 Operator : CG/JU
 Sample : L3386-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0F88

Quant Time: Jul 24 14:15:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 11:01:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	239321	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	999062	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	639398	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	1440170	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1359573	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1126380	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	30798	4.92	ng/uL	0.00
5) Phenol-d5	6.68	99	127389	6.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	319392	31.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	388783	23.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	251975	16.06	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	240261	29.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	264680	30.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	450286	26.94	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	47458	2.69	ng/ul	0.00
44) Dimethylphthalate-d6	13.54	166	1679561	32.39	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	1918418	31.18	ng/ul	0.00
52) 4-Nitrophenol-d4	14.33	143	37700	4.07	ng/ul	0.00
58) Fluorene-d10	15.12	176	1534056	33.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	294806	33.55	ng/ul	0.00
71) Anthracene-d10	16.97	188	2691045	38.38	ng/ul	0.00
79) Pyrene-d10	19.27	212	3058787	45.12	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2475232	40.56	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.58	163	294002	5.367	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
Data File : BN011239.D
Acq On : 24 Jul 2020 13:18
Operator : CG/JU
Sample : L3386-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0F88

Quant Time: Jul 24 14:15:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 11:01:43 2020
Response via : Initial Calibration

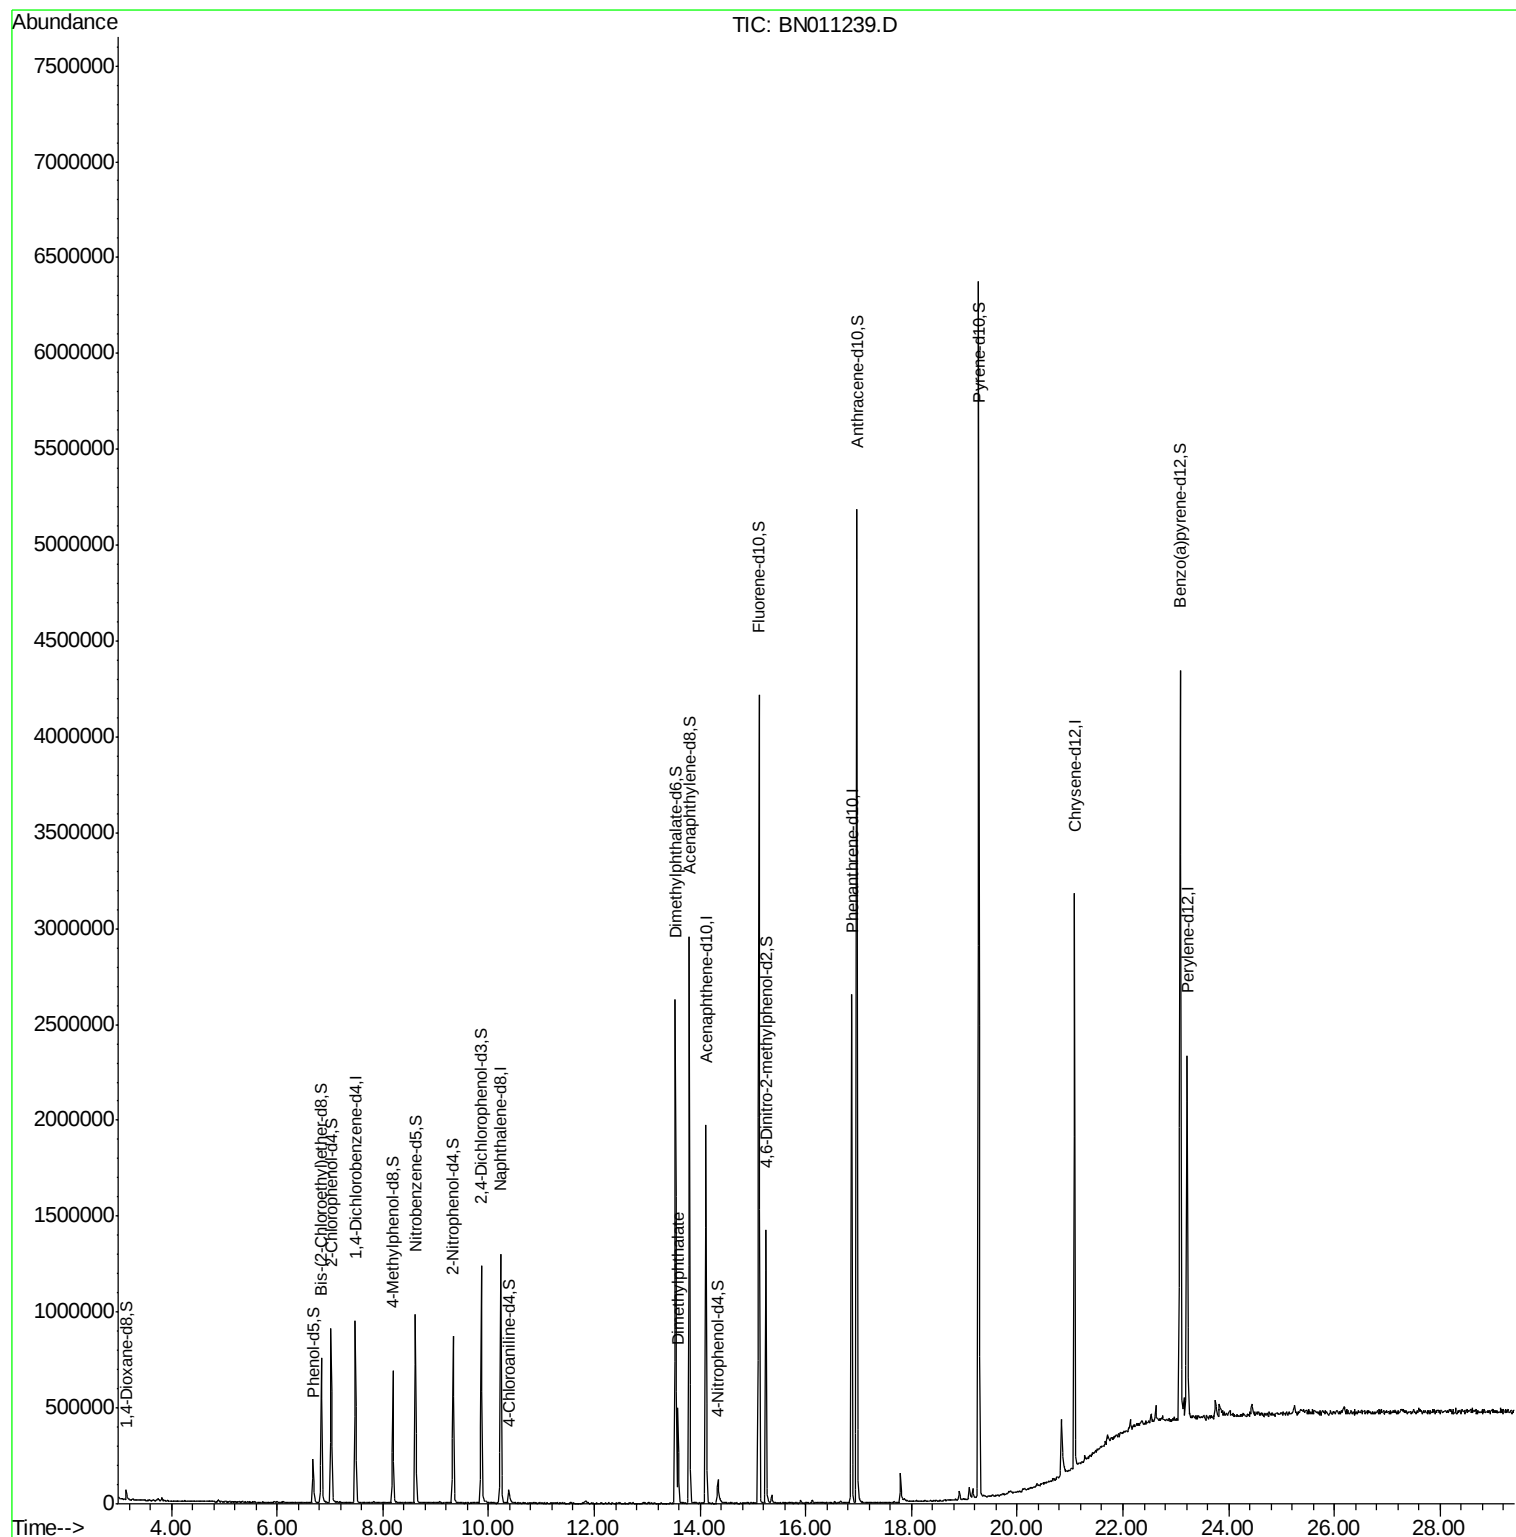

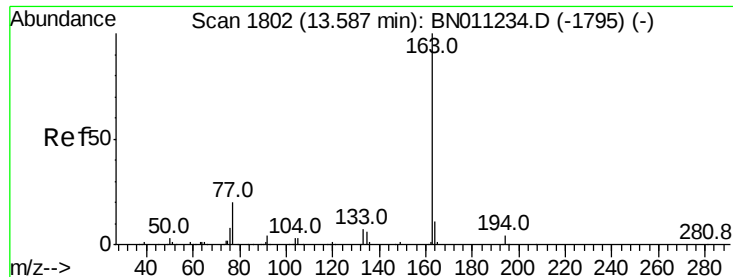

#45

Dimethylphthalate

Concen: 5.367 ng/ul

RT: 13.58 min Scan# 1801

Delta R.T. -0.01 min

Lab File: BN011239.D

Acq: 24 Jul 2020 13:18

Instrument :

BNA_N

ClientSampleId :

C0F88

Tot Ion:163 Resp: 294002

Ion Ratio Lower Upper

163 100

194 3.7 3.4 5.0

164 11.0 7.8 11.8

