

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
 Data File : BN011240.D
 Acq On : 24 Jul 2020 13:54
 Operator : CG/JU
 Sample : L3386-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0F86

Quant Time: Jul 24 14:24:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 11:01:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	214574	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	889431	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	577489	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	1304915	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1368696	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1161776	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	27033	4.81	ng/uL	0.00
5) Phenol-d5	6.68	99	130315	7.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	319829	35.08	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	382721	25.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	253063	17.99	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	243140	33.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	262273	34.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	444988	29.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	51596	3.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1594018	34.04	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	1895707	34.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	38915	4.65	ng/ul	0.00
58) Fluorene-d10	15.12	176	1465920	35.40	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	275420	34.59	ng/ul	0.00
71) Anthracene-d10	16.96	188	2438968	38.39	ng/ul	0.00
79) Pyrene-d10	19.27	212	2882583	42.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2458578	39.06	ng/ul	0.00


Target Compounds					Ovalue	
20) Nitrobenzene	8.66	77	71173	3.795	ng/ul	98
45) Dimethylphthalate	13.58	163	346787	7.009	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072420\
Data File : BN011240.D
Acq On : 24 Jul 2020 13:54
Operator : CG/JU
Sample : L3386-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0F86

Quant Time: Jul 24 14:24:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 11:01:43 2020
Response via : Initial Calibration




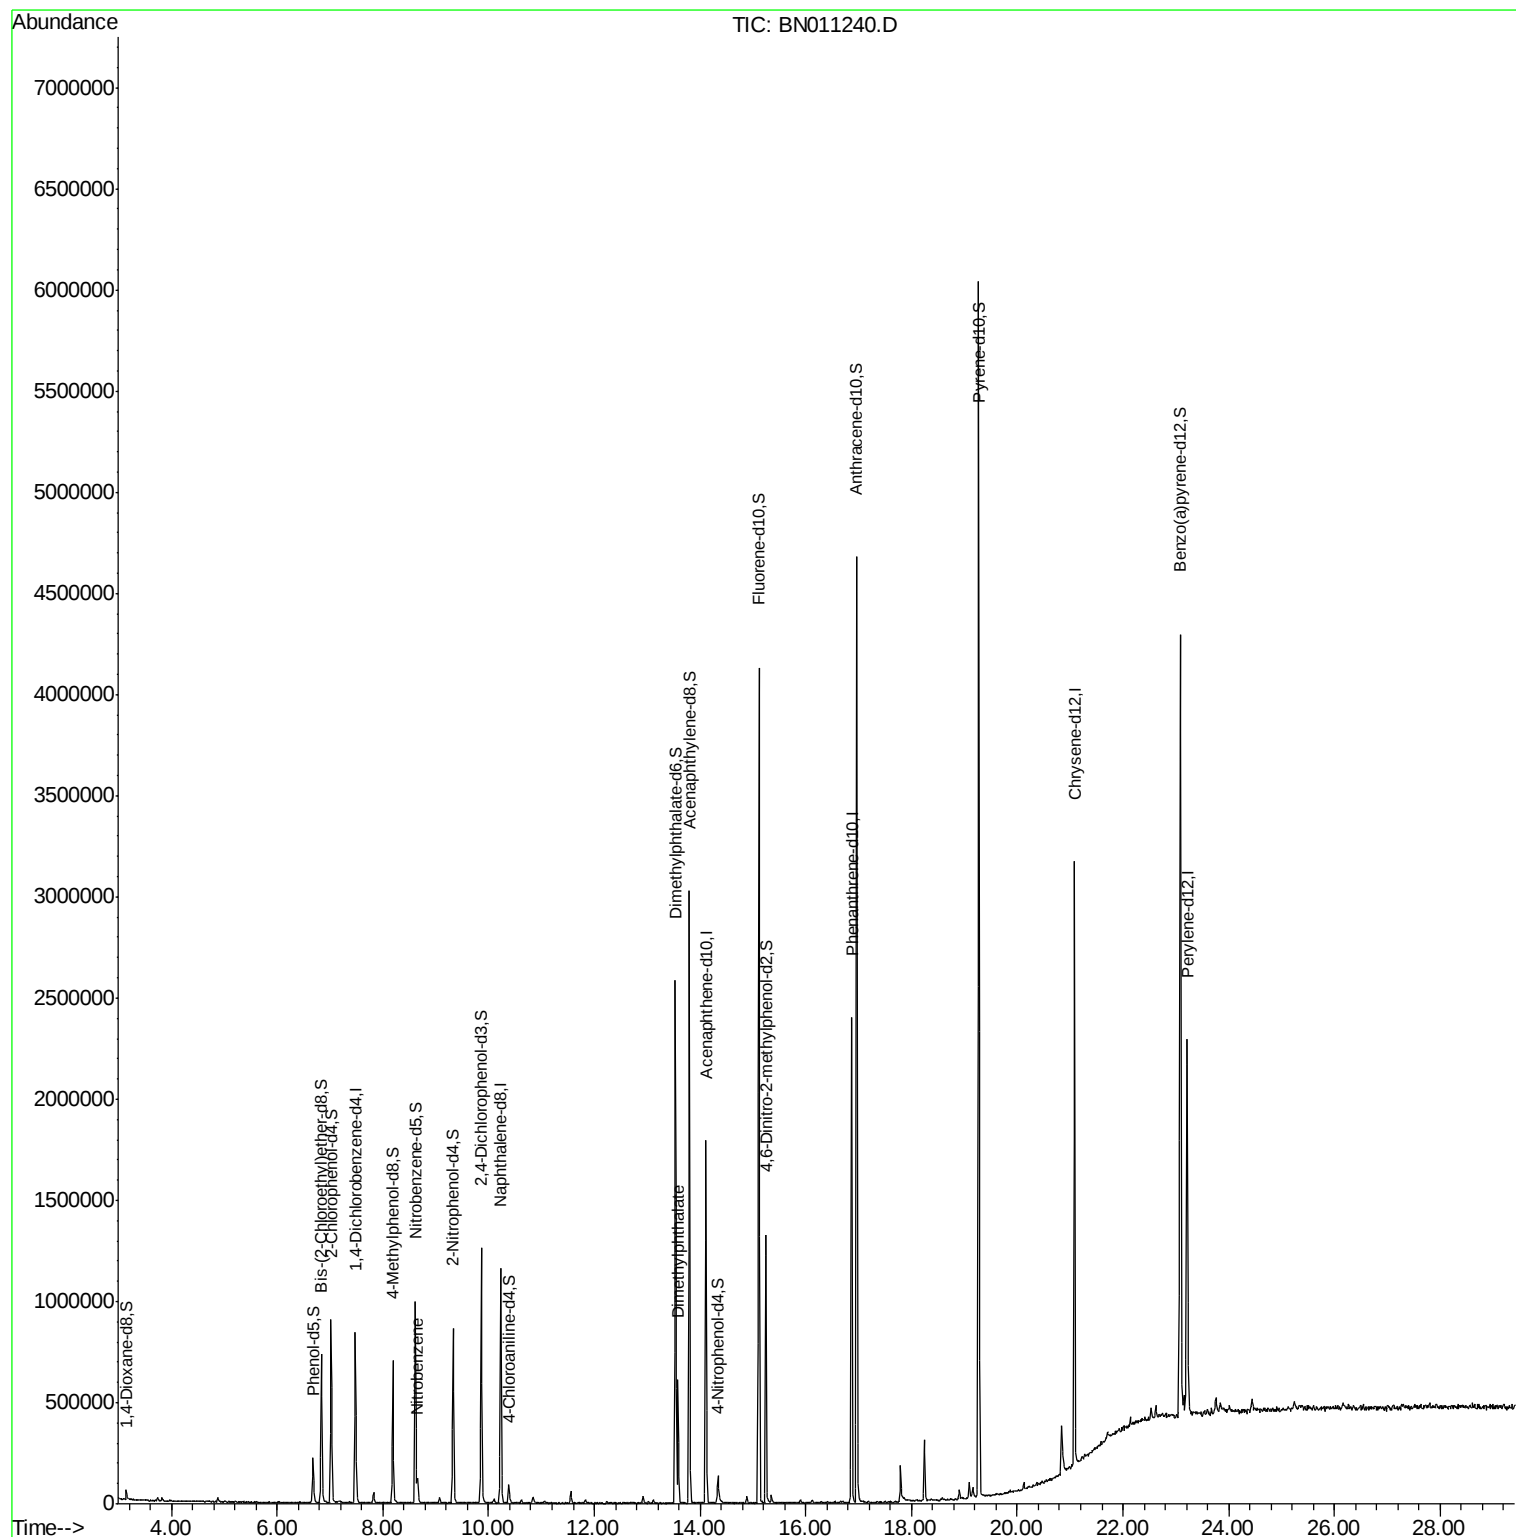


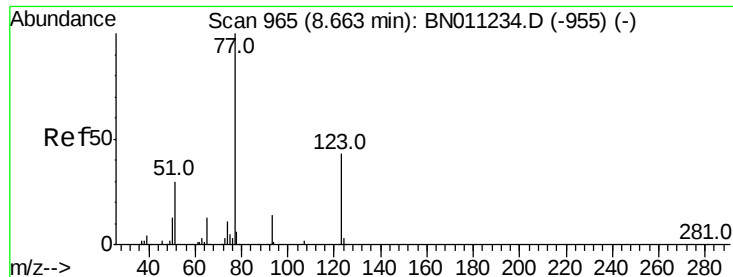

#20
Nitrobenzene
Concen: 3.795 ng/ul
RT: 8.66 min Scan# 964
Delta R.T. -0.01 min
Lab File: BN011240.D
Acq: 24 Jul 2020 13:54

Instrument :
BNA_N
ClientSampled :
C0F86

Tot Ion	Ratio	Lower	Upper
77	100		
123	41.1	33.7	50.5
65	11.8	10.0	15.0

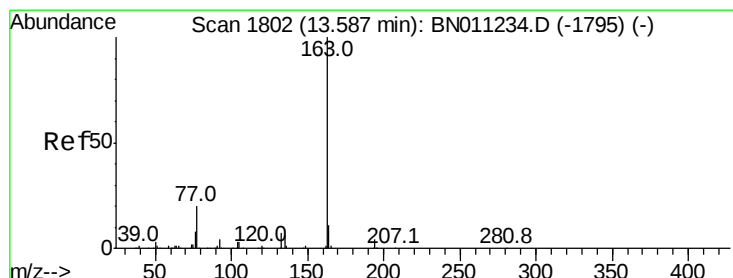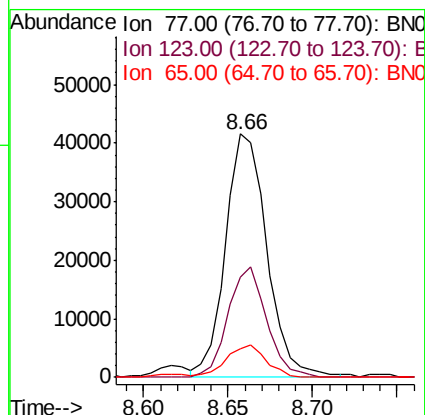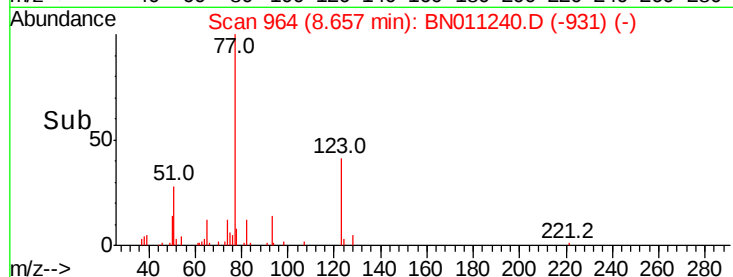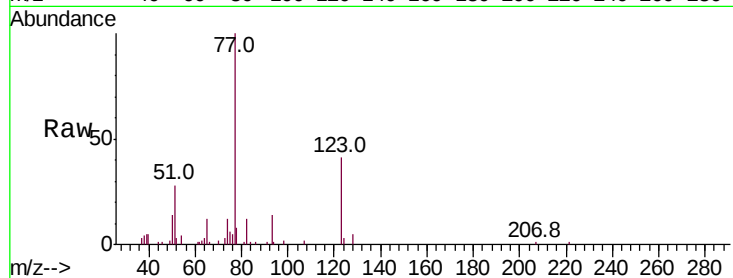

#45
Dimethylphthalate
Concen: 7.009 ng/ul
RT: 13.58 min Scan# 1801
Delta R.T. -0.01 min
Lab File: BN011240.D
Acq: 24 Jul 2020 13:54

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.0
164	10.5	7.8	11.8

