

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
 Data File : BN011247.D
 Acq On : 24 Jul 2020 18:05
 Operator : CG/JU
 Sample : L3388-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD3

Quant Time: Jul 24 18:36:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 11:01:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	169090	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	663232	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	426203	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	990230	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1058931	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	933272	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	8480	1.92	ng/uL	0.00
5) Phenol-d5	6.68	99	149159	11.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	87847	12.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	129588	11.03	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	115072	10.38	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	62276	11.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	61700	10.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	116181	10.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	156597	13.39	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	425783	12.32	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	470038	11.46	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	37229	6.03	ng/ul	0.00
58) Fluorene-d10	15.11	176	359193	11.75	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	44079	7.29	ng/ul	0.00
71) Anthracene-d10	16.96	188	579657	12.02	ng/ul	0.00
79) Pyrene-d10	19.27	212	643950	12.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.08	264	505290	9.99	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.59	163	143318	3.925	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072420\
Data File : BN011247.D
Acq On : 24 Jul 2020 18:05
Operator : CG/JU
Sample : L3388-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD3

Quant Time: Jul 24 18:36:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 11:01:43 2020
Response via : Initial Calibration

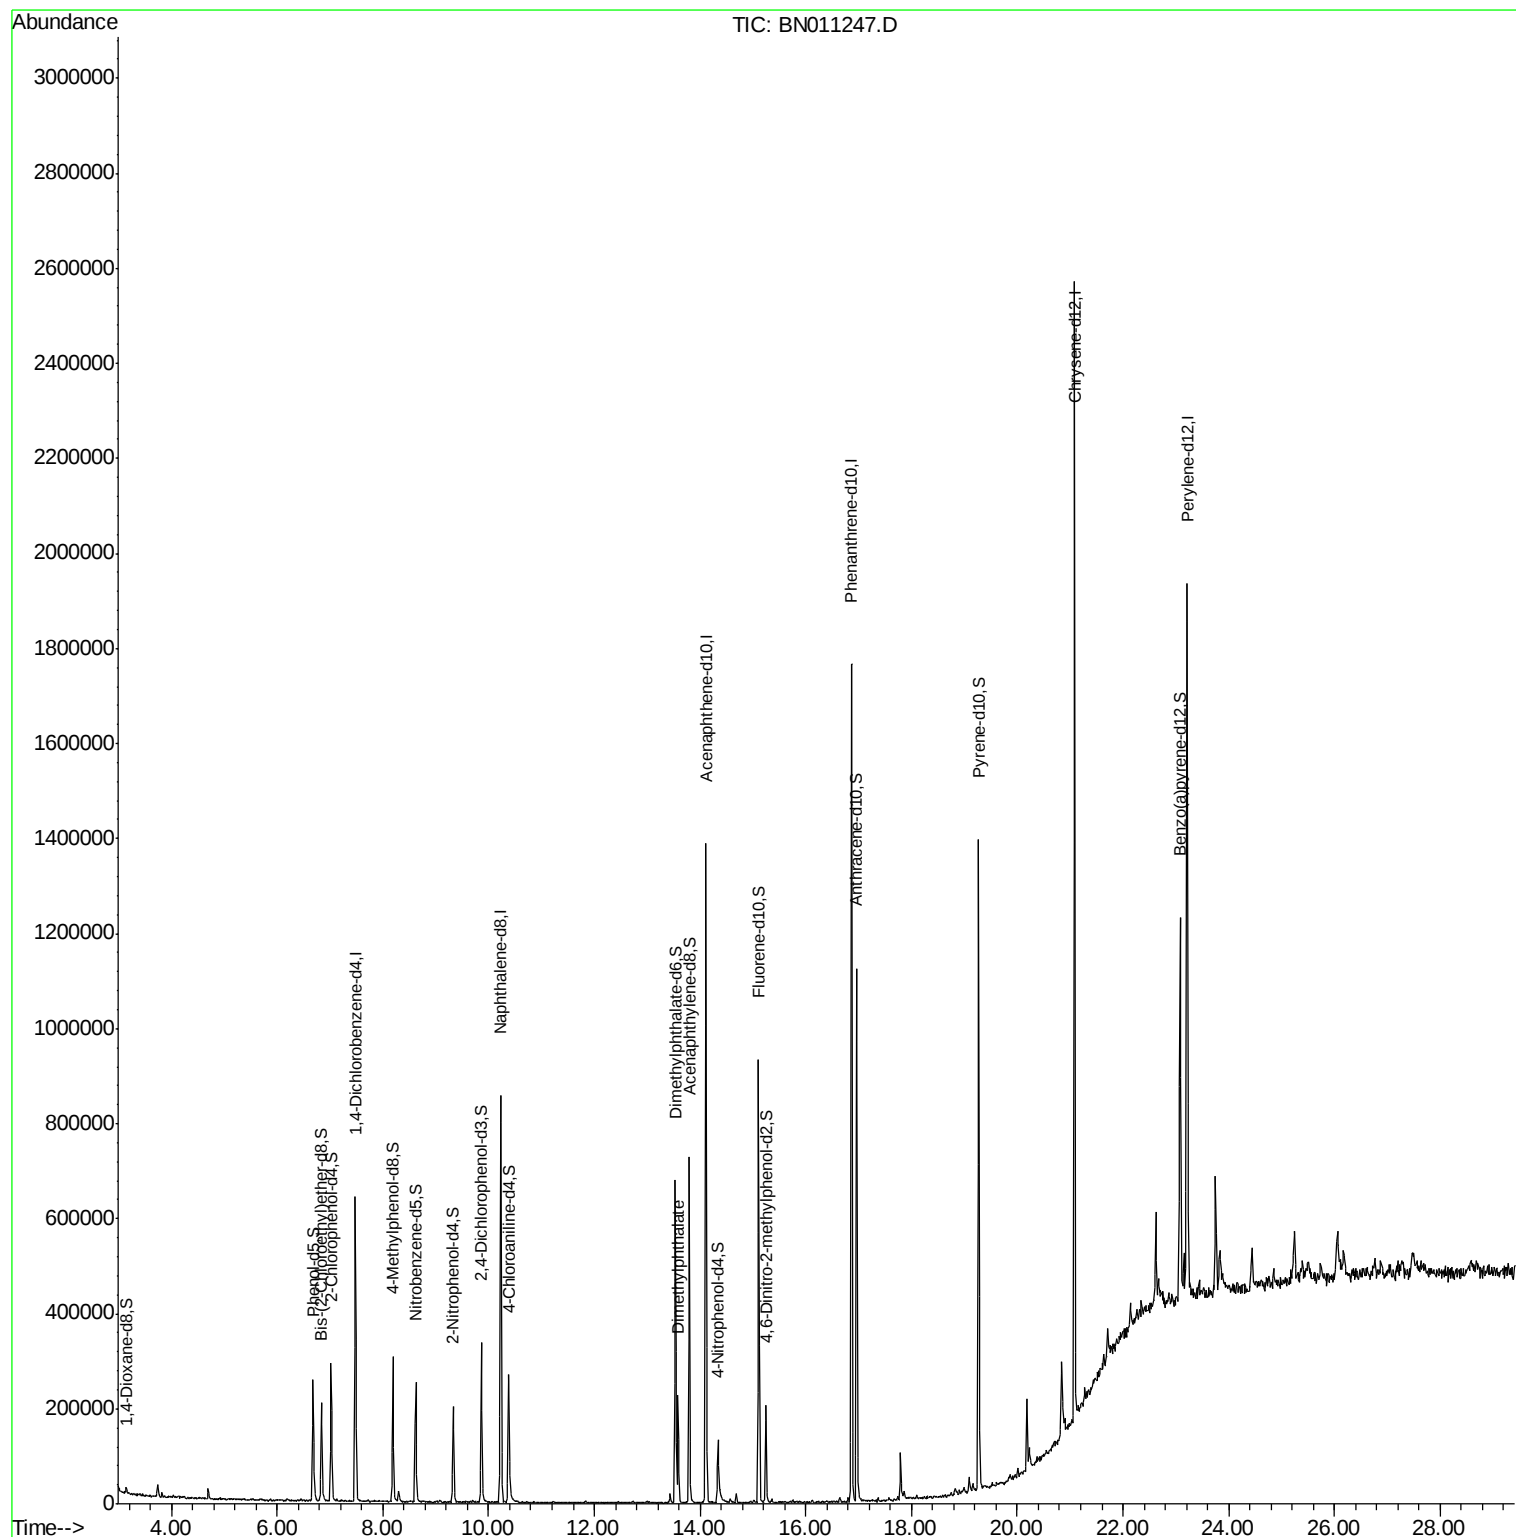

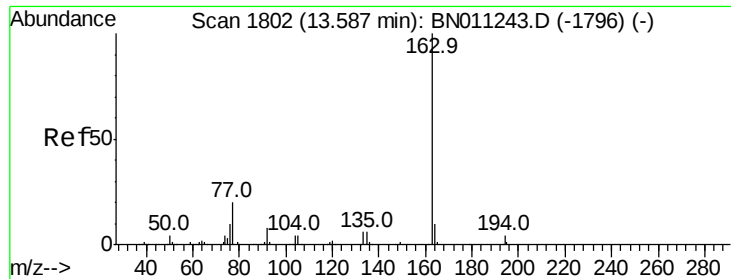

#45

Dimethylphthalate

Concen: 3.925 ng/ul

RT: 13.59 min Scan# 1802

Delta R.T. -0.00 min

Lab File: BN011247.D

Acq: 24 Jul 2020 18:05

Instrument :

BNA_N

ClientSampleId :

C0AD3


Tot Ion:163 Resp: 143318

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 8.7 7.8 11.8

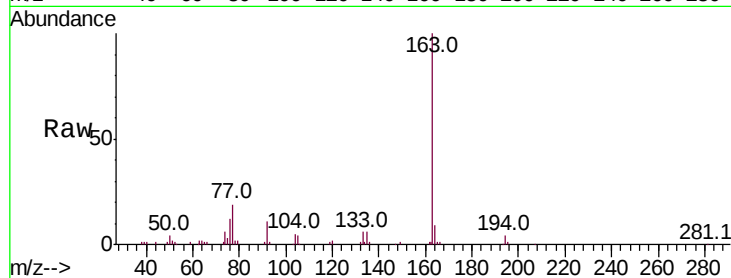

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

