

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072420\
 Data File : BN011251.D
 Acq On : 24 Jul 2020 20:28
 Operator : CG/JU
 Sample : L3388-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE7

Quant Time: Jul 25 00:21:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 11:01:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	264847	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	1099726	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	698089	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.87	188	1538689	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	1514618	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	1230657	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	31291	4.51	ng/uL	0.00
5) Phenol-d5	6.68	99	583415	27.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	341119	30.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	496062	26.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	491283	28.29	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	256336	28.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	258696	27.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	490833	26.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	589256	30.40	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	1510384	26.68	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	1928960	28.71	ng/ul	0.00
52) 4-Nitrophenol-d4	14.33	143	164820	16.30	ng/ul	0.00
58) Fluorene-d10	15.12	176	1398613	27.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	165116	17.59	ng/ul	0.00
71) Anthracene-d10	16.96	188	2175209	29.04	ng/ul	0.00
79) Pyrene-d10	19.27	212	2482777	32.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	2030226	30.45	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.58	163	349072	5.837	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
Data File : BN011251.D
Acq On : 24 Jul 2020 20:28
Operator : CG/JU
Sample : L3388-20
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE7

Quant Time: Jul 25 00:21:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 11:01:43 2020
Response via : Initial Calibration

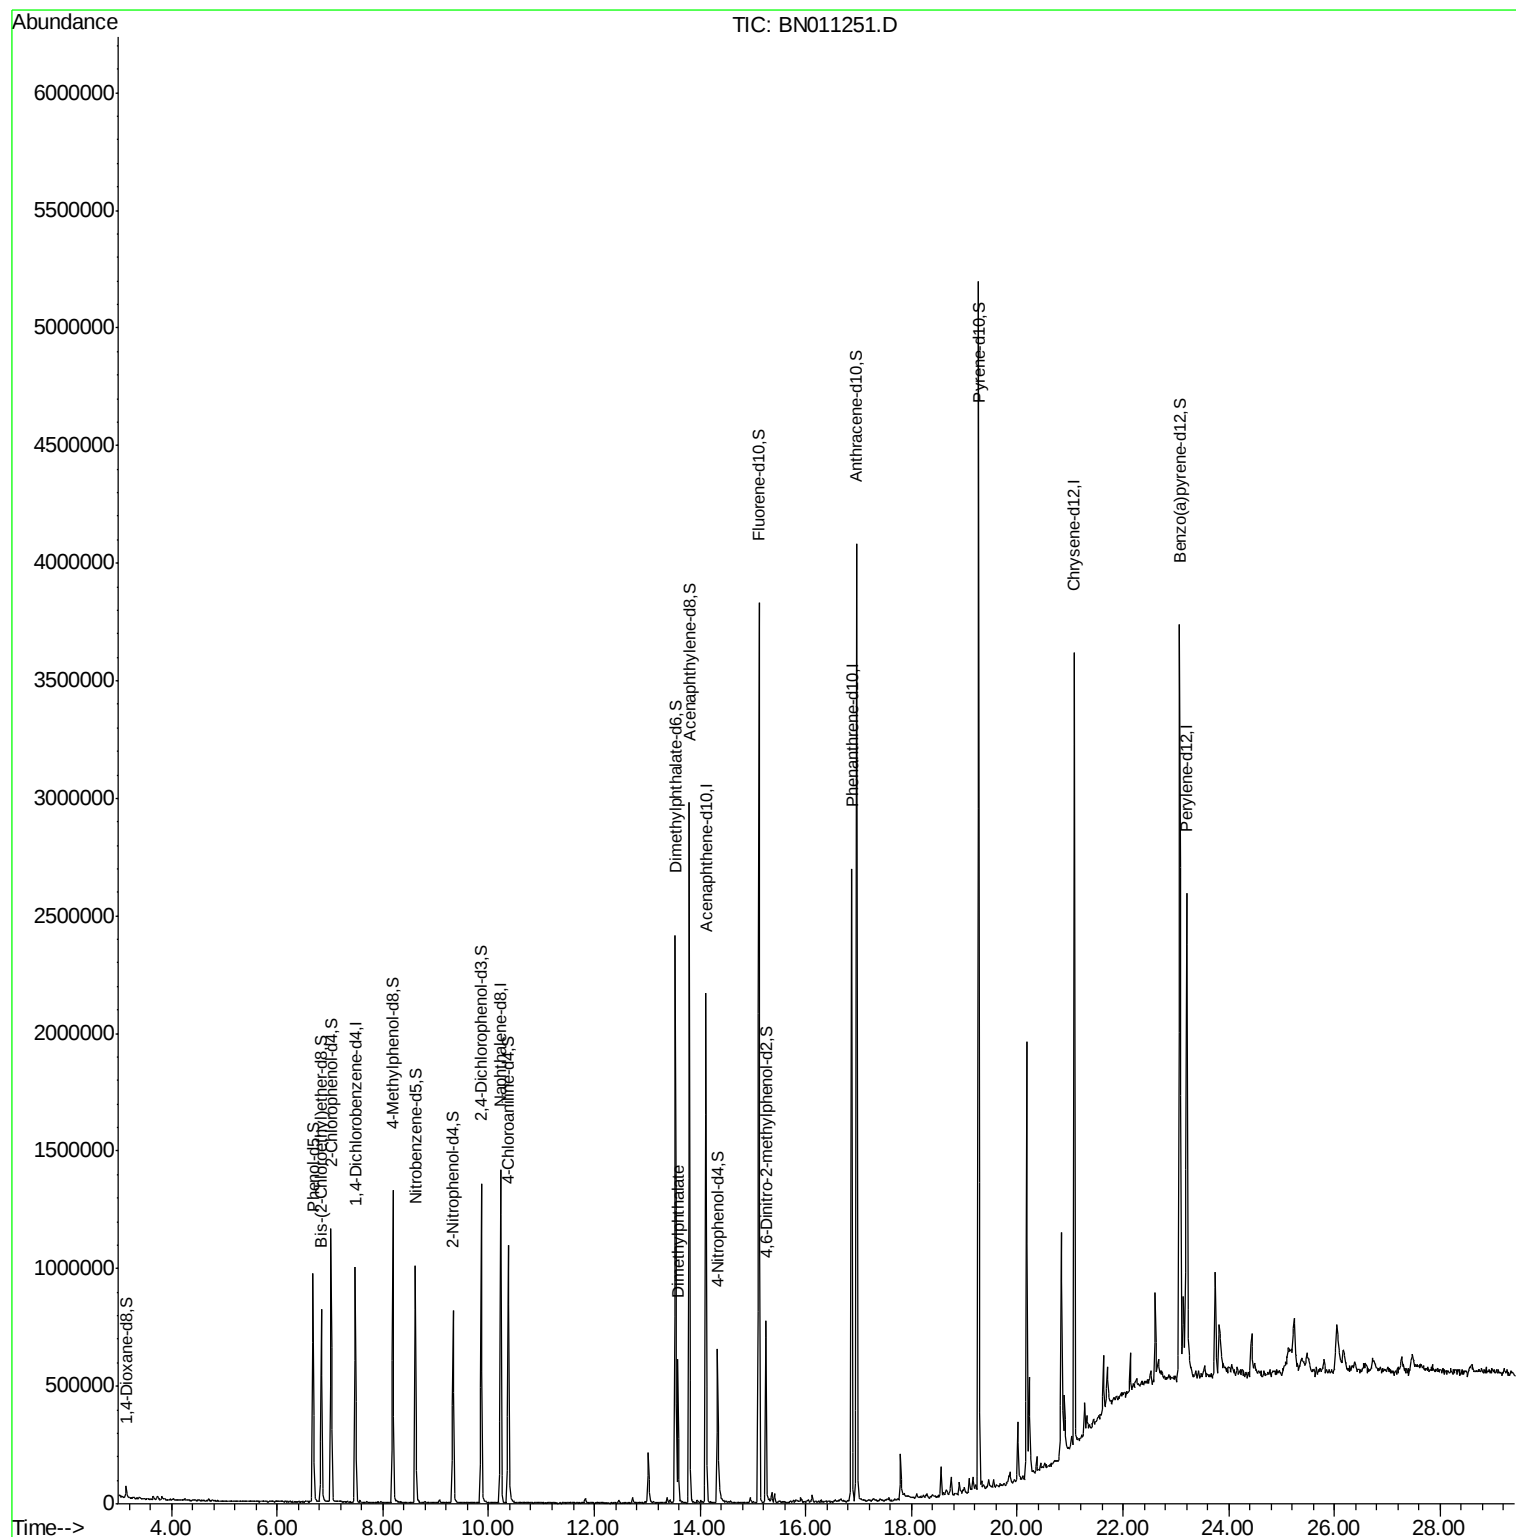

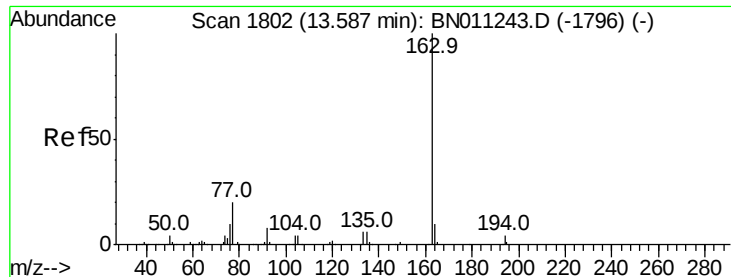

#45

Dimethylphthalate

Concen: 5.837 ng/ul

RT: 13.58 min Scan# 1801

Delta R.T. -0.01 min

Lab File: BN011251.D

Acq: 24 Jul 2020 20:28

Instrument :

BNA_N

ClientSampleId :

C0AE7


Tot Ion:163 Resp: 349072

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.7 7.8 11.8

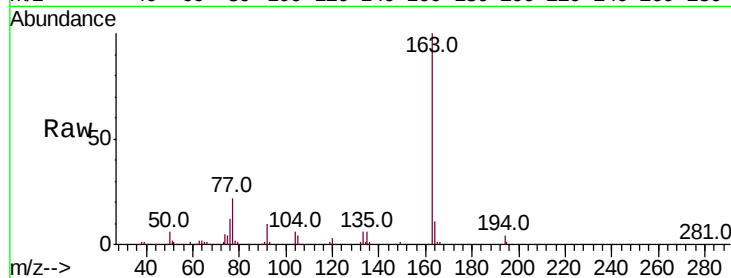

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

