

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072420\
 Data File : BN011258.D
 Acq On : 25 Jul 2020 02:27
 Operator : CG/JU
 Sample : L3388-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD9

Manual Integrations
 APPROVED

mohammad
 7/27/2020 12:21:42 PM

Quant Time: Jul 25 04:29:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 24 11:01:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	266158	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	1040051	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	691713	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	1587622	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	1443689	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	1224776	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.15	96	3973m	0.57	ng/uL	0.00
5) Phenol-d5	6.68	99	72847	3.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	50194	4.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	65132	3.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	66413	3.81	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	35745	4.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	35148	3.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.87	165	61861	3.55	ng/ul	0.00
29) 4-Chloroaniline-d4	10.38	131	68277	3.72	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	246736	4.40	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	237662	3.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	19889	1.98	ng/ul	0.00
58) Fluorene-d10	15.11	176	204675	4.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	25585	2.64	ng/ul	0.00
71) Anthracene-d10	16.96	188	301724	3.90	ng/ul	0.00
79) Pyrene-d10	19.27	212	294795	4.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	214166	3.23	ng/ul	-0.02

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.58	163	98523	1.663	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072420\
Data File : BN011258.D
Acq On : 25 Jul 2020 02:27
Operator : CG/JU
Sample : L3388-13
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AD9

Manual Integrations
APPROVED

mohammad
7/27/2020 12:21:42 PM

Quant Time: Jul 25 04:29:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 24 11:01:43 2020
Response via : Initial Calibration

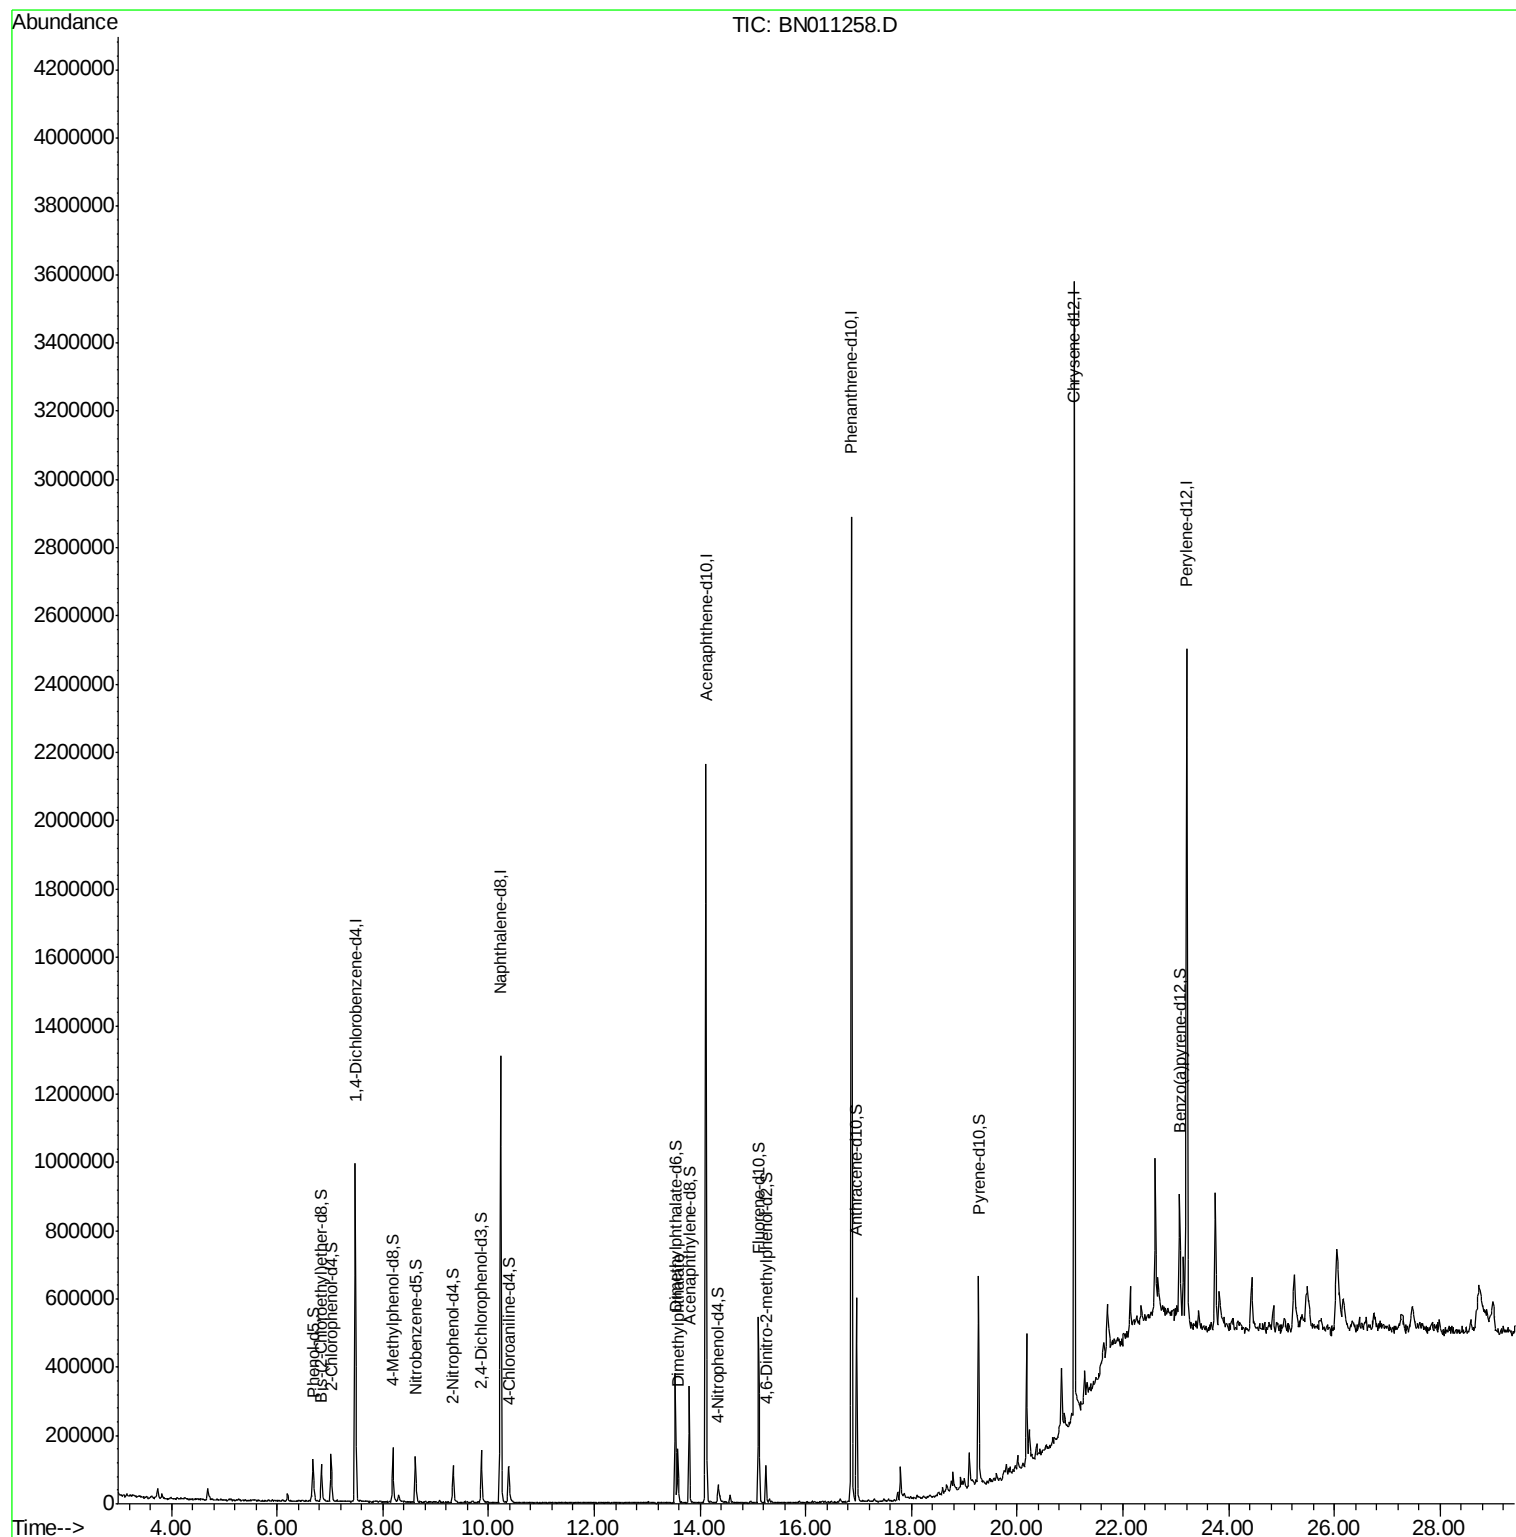

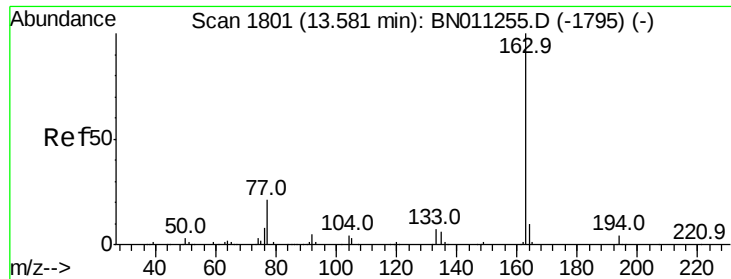


#45
 Dimethylphthalate
 Concen: 1.663 ng/ul
 RT: 13.58 min Scan# 1801
 Delta R.T. -0.01 min
 Lab File: BN011258.D
 Acq: 25 Jul 2020 02:27

Instrument :
 BNA_N
 ClientSampleId :
 C0AD9

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.5	3.4	5.0
164	10.0	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 7/27/2020 12:21:42 PM

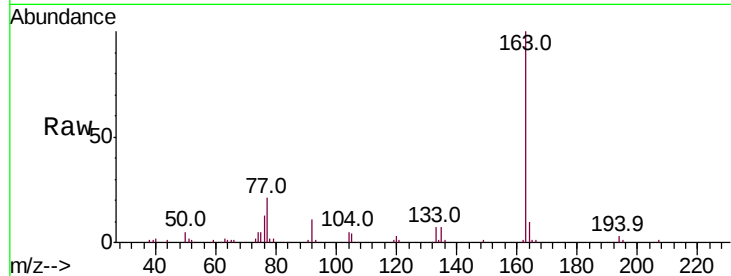

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

