

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
 Data File : BN011262.D
 Acq On : 25 Jul 2020 04:50
 Operator : CG/JU
 Sample : L3388-06
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD2

Manual Integrations
 APPROVED

mohammad
 7/27/2020 12:21:52 PM

Quant Time: Jul 25 05:33:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 25 04:23:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	244990	20.00	ng/ul	0.00
18) Naphthalene-d8	10.23	136	990694	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.11	164	617204	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.86	188	1381343	20.00	ng/ul	0.00
78) Chrysene-d12	21.08	240	1382995	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	1219253	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.15	96	5744m	0.90	ng/uL	0.00
5) Phenol-d5	6.68	99	104916	5.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	63058	6.06	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	90892	5.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	89242	5.56	ng/ul	0.00
19) Nitrobenzene-d5	8.62	128	45484	5.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.33	143	44209	5.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.86	165	86951	5.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.37	131	115069	6.59	ng/ul	0.00
44) Dimethylphthalate-d6	13.53	166	310181	6.20	ng/ul	0.00
47) Acenaphthylene-d8	13.80	160	331989	5.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	30284m	3.39	ng/ul	0.00
58) Fluorene-d10	15.11	176	267934	6.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	29803	3.54	ng/ul	0.00
71) Anthracene-d10	16.96	188	402649	5.99	ng/ul	0.00
79) Pyrene-d10	19.27	212	479804	6.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.07	264	386443	5.85	ng/ul	-0.01

Target Compounds					Ovalue	
45) Dimethylphthalate	13.58	163	105078	1.987	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
Data File : BN011262.D
Acq On : 25 Jul 2020 04:50
Operator : CG/JU
Sample : L3388-06
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AD2

Manual Integrations
APPROVED

mohammad
7/27/2020 12:21:52 PM

Quant Time: Jul 25 05:33:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 25 04:23:15 2020
Response via : Initial Calibration

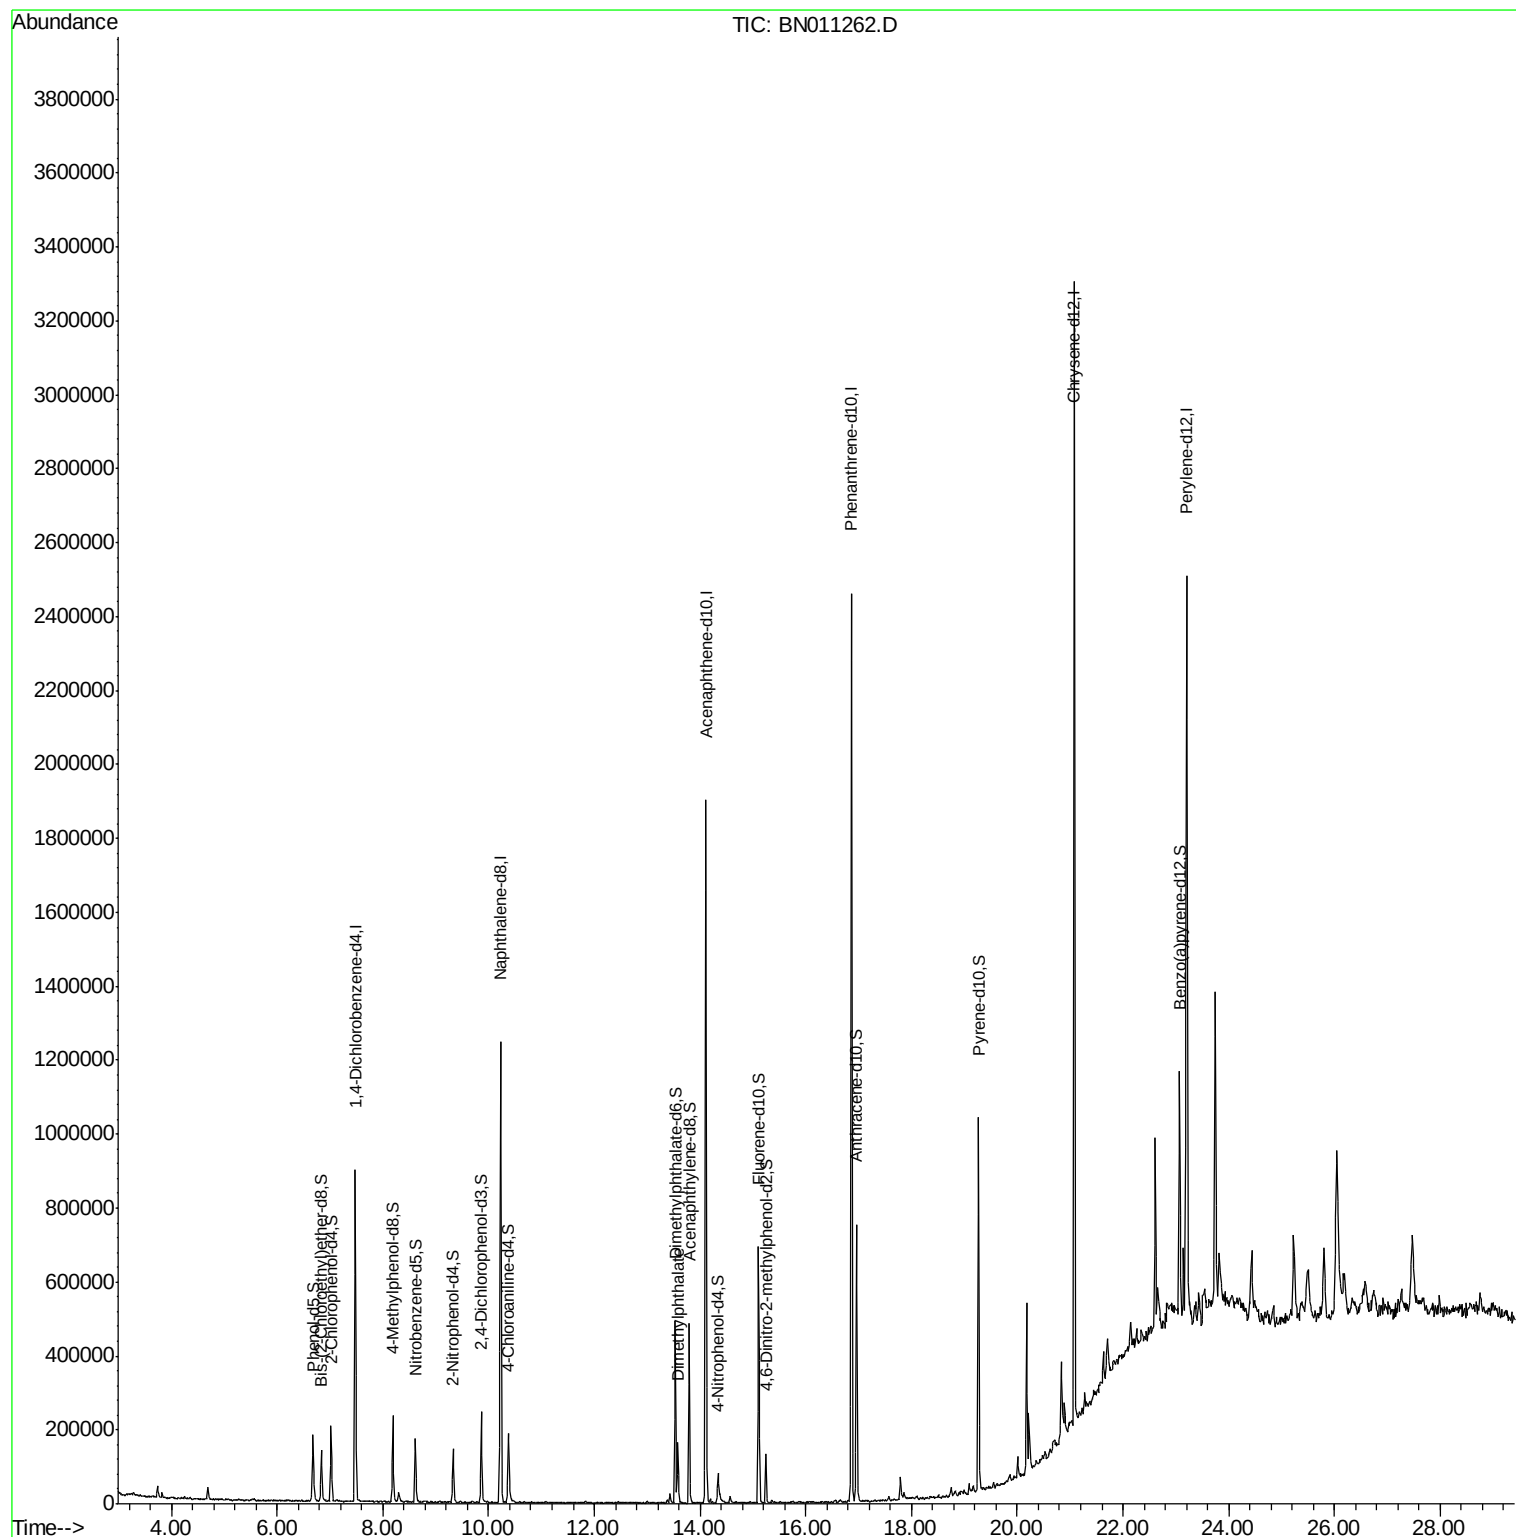

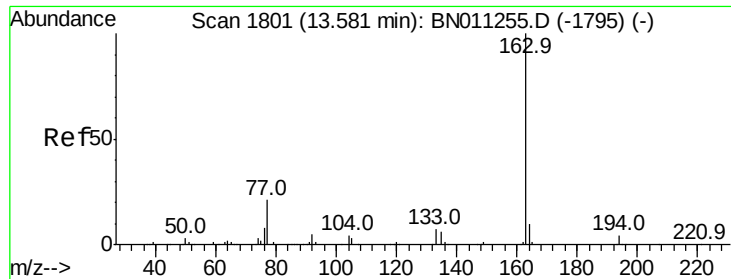

#45
 Dimethylphthalate
 Concen: 1.987 ng/ul
 RT: 13.58 min Scan# 1801
 Delta R.T. -0.01 min
 Lab File: BN011262.D
 Acq: 25 Jul 2020 04:50

Instrument :
 BNA_N
 ClientSampleId :
 C0AD2

Tot Ion:	163	Resp:	105078
Ion Ratio	Lower	Upper	
163	100		
194	3.7	3.4	5.0
164	9.4	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 7/27/2020 12:21:52 PM

