

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
 Data File : BN011252.D
 Acq On : 24 Jul 2020 21:40
 Operator : CG/JU
 Sample : L3388-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.493	84	86	91	rVB6	4356	5398	0.14%	0.025%
2	3.534	91	93	98	rBV5	3503	4935	0.13%	0.023%
3	3.740	122	128	132	rBV	24209	38956	1.00%	0.180%
4	3.823	138	142	145	rBV4	13093	19016	0.49%	0.088%
5	4.252	211	215	220	rVB6	6604	10205	0.26%	0.047%
6	4.352	229	232	235	rBV3	3542	4228	0.11%	0.019%
7	4.699	286	291	298	rVB	27910	45688	1.18%	0.211%
8	5.564	434	438	441	rVB5	4855	6361	0.16%	0.029%
9	6.211	545	548	550	rVB4	5005	5987	0.15%	0.028%
10	6.681	617	628	638	rBV2	88942	178748	4.61%	0.824%
11	6.840	649	655	665	rBV	84642	146848	3.79%	0.677%
12	7.028	681	687	693	rBV	102481	170155	4.39%	0.784%
13	7.128	701	704	709	rBV5	5602	9416	0.24%	0.043%
14	7.481	756	764	772	rBV	935693	1488002	38.36%	6.857%
15	8.193	879	885	898	rBV2	111639	193487	4.99%	0.892%
16	8.305	898	904	909	rBV4	17148	32653	0.84%	0.150%
17	8.616	952	957	965	rBV	94795	168730	4.35%	0.778%
18	9.075	1032	1035	1038	rVB2	4204	4251	0.11%	0.020%
19	9.246	1057	1064	1066	rBV5	2792	5024	0.13%	0.023%
20	9.334	1073	1079	1092	rVB	74213	125820	3.24%	0.580%
21	9.863	1164	1169	1178	rBV2	95506	170451	4.39%	0.785%
22	9.981	1185	1189	1198	rBV4	23540	37866	0.98%	0.174%
23	10.228	1224	1231	1239	rBV	1281865	2002057	51.61%	9.226%
24	10.381	1250	1257	1266	rBV2	91456	179514	4.63%	0.827%
25	10.763	1318	1322	1325	rBV3	2429	4757	0.12%	0.022%
26	10.863	1336	1339	1345	rVB5	2613	4302	0.11%	0.020%
27	12.463	1607	1611	1617	rBV3	4115	6065	0.16%	0.028%
28	12.722	1650	1655	1658	rVB5	5232	6024	0.16%	0.028%
29	13.369	1762	1765	1770	rBV3	4036	6125	0.16%	0.028%
30	13.534	1788	1793	1797	rBV	278424	379246	9.78%	1.748%
31	13.581	1797	1801	1807	rVB	149892	212695	5.48%	0.980%
32	13.798	1831	1838	1845	rBV	193548	281783	7.26%	1.298%
33	14.110	1884	1891	1901	rBV2	1967704	2831629	73.00%	13.048%
34	14.351	1928	1932	1942	rBV6	16093	40642	1.05%	0.187%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
 Data File : BN011252.D
 Acq On : 24 Jul 2020 21:40
 Operator : CG/JU
 Sample : L3388-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
 Title : SVOA CALIBRATION

35	14.569	1965	1969	1976	rBV3	16344	21444	0.55%	0.099%
36	14.940	2029	2032	2033	rBV3	3800	4186	0.11%	0.019%
37	14.963	2033	2036	2039	rVV3	6814	8730	0.23%	0.040%
38	15.116	2056	2062	2069	rBV	284674	416712	10.74%	1.920%
39	15.245	2080	2084	2090	rBV4	27856	43174	1.11%	0.199%
40	15.363	2099	2104	2106	rBV3	3712	4776	0.12%	0.022%
41	16.128	2231	2234	2237	rVB3	4011	4006	0.10%	0.018%
42	16.657	2320	2324	2329	rBV	7594	10322	0.27%	0.048%
43	16.863	2353	2359	2369	rBV	2567722	3447732	88.88%	15.887%
44	16.963	2369	2376	2388	rVB	272122	401356	10.35%	1.849%
45	17.128	2399	2404	2407	rBV3	3271	4886	0.13%	0.023%
46	17.651	2490	2493	2498	rBV5	3418	5306	0.14%	0.024%
47	17.745	2505	2509	2511	rBV4	3147	4485	0.12%	0.021%
48	17.792	2511	2517	2524	rVV4	35143	51864	1.34%	0.239%
49	17.857	2524	2528	2534	rVB	15876	24976	0.64%	0.115%
50	18.022	2555	2556	2560	rBV3	3633	4299	0.11%	0.020%
51	18.357	2610	2613	2616	rBV4	6490	6168	0.16%	0.028%
52	18.445	2626	2628	2631	rBV3	3330	4231	0.11%	0.019%
53	18.486	2633	2635	2638	rVB3	3962	4646	0.12%	0.021%
54	18.563	2646	2648	2651	rBV4	3731	4308	0.11%	0.020%
55	18.904	2704	2706	2709	rVB2	5008	4136	0.11%	0.019%
56	18.939	2709	2712	2714	rBV3	10611	12452	0.32%	0.057%
57	18.963	2714	2716	2718	rVV3	4972	5631	0.15%	0.026%
58	18.992	2718	2721	2727	rVB7	12425	16436	0.42%	0.076%
59	19.092	2735	2738	2741	rVB5	12206	12746	0.33%	0.059%
60	19.210	2755	2758	2761	rBV5	14991	12924	0.33%	0.060%
61	19.269	2763	2768	2777	rVV	277136	392170	10.11%	1.807%
62	19.410	2790	2792	2793	rBV2	9353	5266	0.14%	0.024%
63	19.528	2808	2812	2815	rBV5	15363	18974	0.49%	0.087%
64	19.563	2815	2818	2823	rVV5	38831	48071	1.24%	0.222%
65	19.763	2849	2852	2855	rBV3	19098	20023	0.52%	0.092%
66	20.180	2919	2923	2927	rBV4	128606	168409	4.34%	0.776%
67	20.239	2931	2933	2936	rVV3	49949	53262	1.37%	0.245%
68	20.269	2936	2938	2942	rVB5	29537	36072	0.93%	0.166%
69	20.369	2953	2955	2959	rVB5	20629	14699	0.38%	0.068%
70	20.833	3030	3034	3040	rBV3	101441	179285	4.62%	0.826%
71	21.080	3071	3076	3084	rBV	3178079	3878873	100.00%	17.874%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
Data File : BN011252.D
Acq On : 24 Jul 2020 21:40
Operator : CG/JU
Sample : L3388-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Title : SVOA CALIBRATION

72	21.275	3107	3109	3113	rBV4	55879	53795	1.39%	0.248%
73	21.698	3178	3181	3190	rVB7	72266	138596	3.57%	0.639%
74	23.210	3432	3438	3448	rVB2	1863897	3324426	85.71%	15.319%


Sum of corrected areas: 21700917

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN072420\
Data File : BN011252.D
Acq On : 24 Jul 2020 21:40
Operator : CG/JU
Sample : L3388-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD6

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

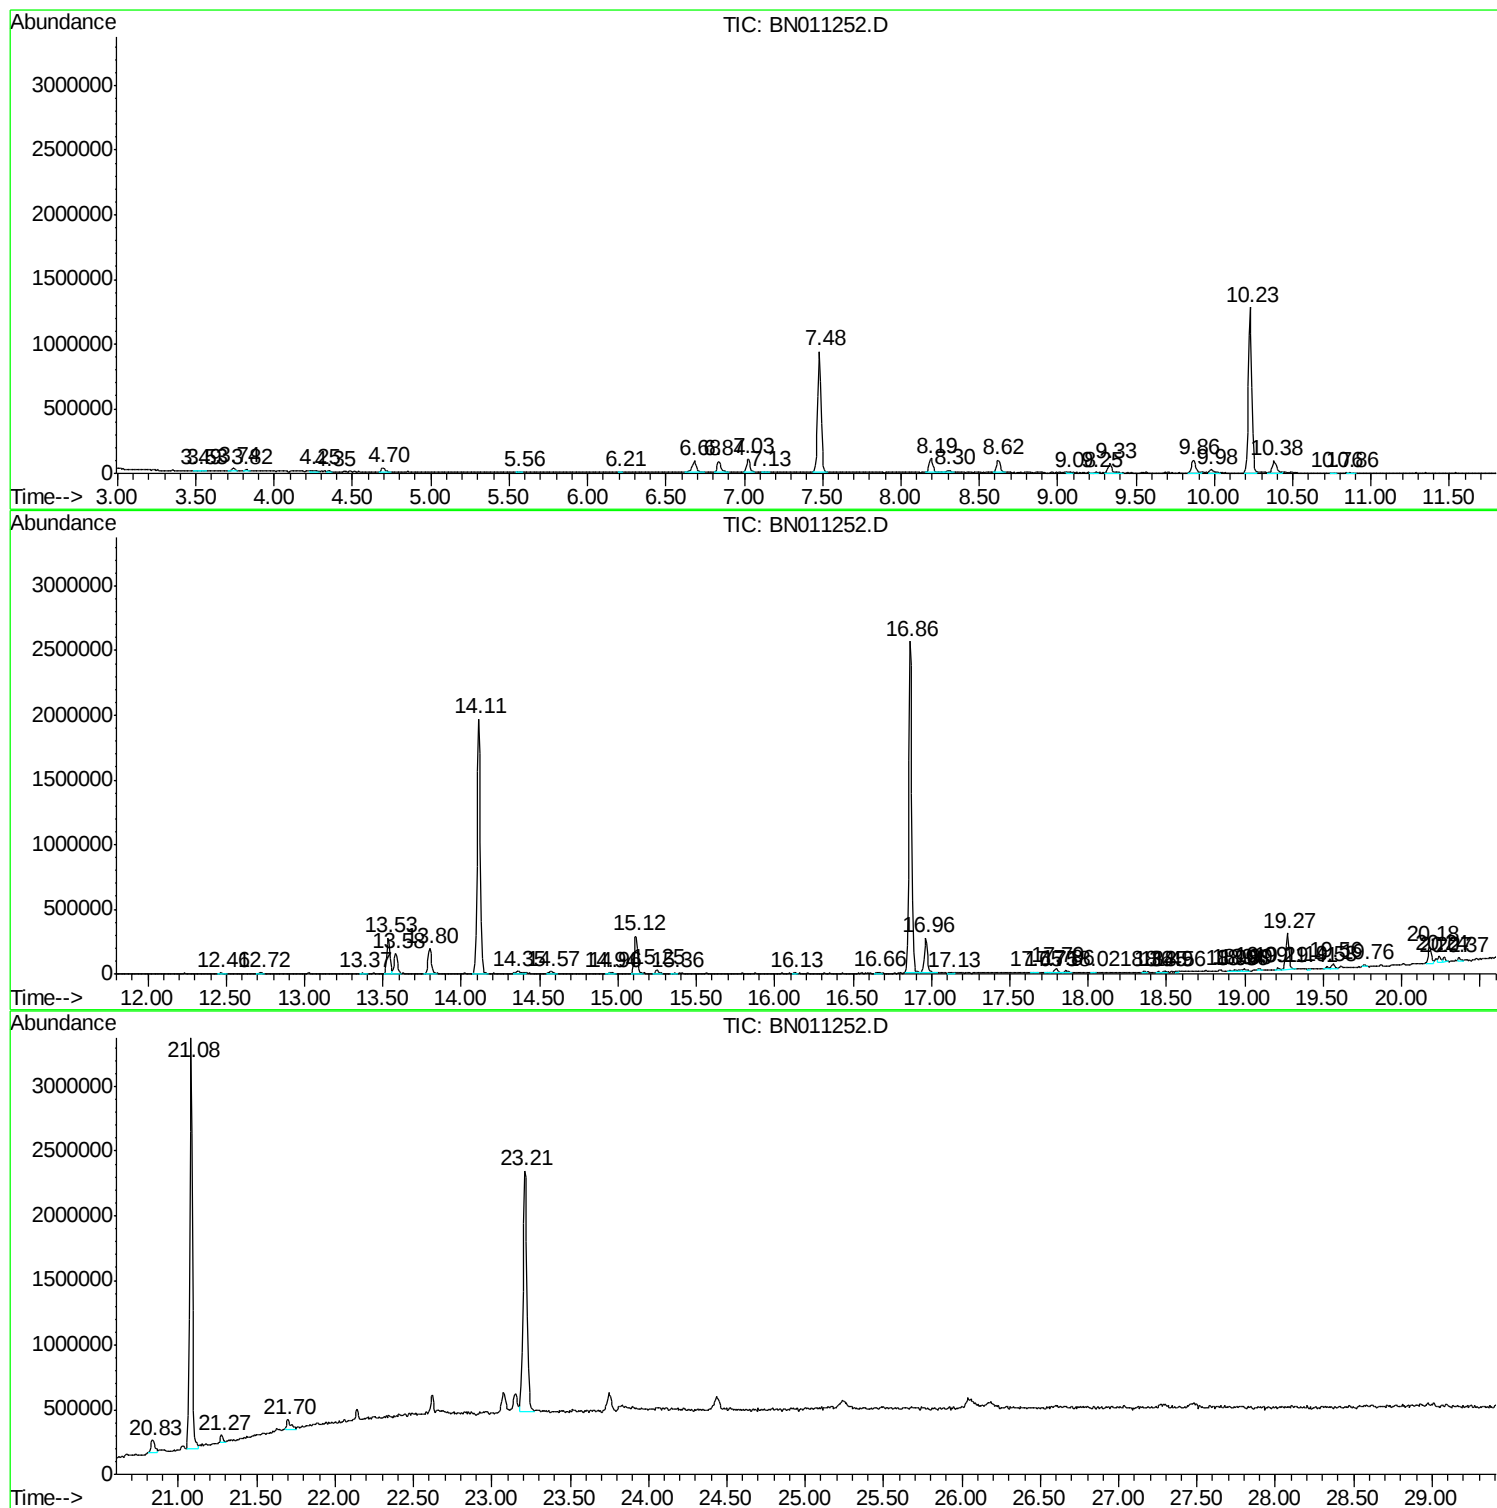

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN072420\
Data_File : BN011252.D
Acq_On : 24 Jul 2020 21:400
Operator : CG/JUU
Sample : L3388-100
Misc :
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_N
ClientSampleId :
C0AD6

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN071520MA.MM
Quant_Title : SVOA CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
