

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
 Data File : BN015662.D
 Acq On : 23 Jul 2021 09:35
 Operator : CG/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Jul 23 12:36:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 23 12:32:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.744	152	12017	0.400	ng	0.00
7) Naphthalene-d8	10.521	136	52344	0.400	ng	0.00
13) Acenaphthene-d10	14.370	164	26009	0.400	ng	0.00
19) Phenanthrene-d10	17.115	188	48805	0.400	ng	0.00
29) Chrysene-d12	21.312	240	38200	0.400	ng	0.00
35) Perylene-d12	23.628	264	34702	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.346	112	2903	0.084	ng	0.00
5) Phenol-d6	6.914	99	3206	0.078	ng	0.00
8) Nitrobenzene-d5	8.886	82	3525	0.094	ng	0.00
11) 2-Methylnaphthalene-d10	12.114	152	7821	0.090	ng	0.00
14) 2,4,6-Tribromophenol	15.867	330	678	0.058	ng	0.00
15) 2-Fluorobiphenyl	13.000	172	11879	0.115	ng	0.00
27) Fluoranthene-d10	19.157	212	12083	0.081	ng	0.00
31) Terphenyl-d14	19.763	244	10245	0.115	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.281	88	390	0.096	ng	96
3) n-Nitrosodimethylamine	3.659	42	766	0.077	ng	93
6) bis(2-Chloroethyl)ether	7.172	93	3483	0.094	ng	99
9) Naphthalene	10.571	128	14489	0.097	ng	99
10) Hexachlorobutadiene	10.863	225	2737	0.098	ng	# 99
12) 2-Methylnaphthalene	12.190	142	9067	0.093	ng	99
16) Acenaphthylene	14.091	152	9276	0.077	ng	100
17) Acenaphthene	14.434	154	7641	0.094	ng	100
18) Fluorene	15.423	166	8772	0.089	ng	99
20) 4,6-Dinitro-2-methylph...	15.512	198	145	0.036	ng	# 42
21) 4-Bromophenyl-phenylether	16.312	248	2602	0.085	ng	96
22) Hexachlorobenzene	16.433	284	3255	0.096	ng	99
23) Atrazine	16.592	200	1490	0.067	ng	97
24) Pentachlorophenol	16.774	266	472	0.056	ng	94
25) Phenanthrene	17.164	178	14643	0.093	ng	99
26) Anthracene	17.249	178	10609	0.079	ng	100
28) Fluoranthene	19.187	202	14472	0.083	ng	99
30) Pyrene	19.549	202	14586	0.101	ng	100
32) Benzo(a)anthracene	21.302	228	10670	0.078	ng	99
33) Chrysene	21.355	228	14202	0.101	ng	99
34) Bis(2-ethylhexyl)phtha...	21.238	149	3939	0.060	ng	100
36) Indeno(1,2,3-cd)pyrene	25.993	276	11308	0.079	ng	99
37) Benzo(b)fluoranthene	22.974	252	12436	0.093	ng	94
38) Benzo(k)fluoranthene	22.974	252	12436	0.091	ng	94
39) Benzo(a)pyrene	23.522	252	9264	0.079	ng	# 92
40) Dibenzo(a,h)anthracene	26.011	278	8492	0.075	ng	95
41) Benzo(g,h,i)perylene	26.719	276	10876	0.089	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015662.D
Acq On : 23 Jul 2021 09:35
Operator : CG/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Jul 23 12:36:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 23 12:32:24 2021
Response via : Initial Calibration




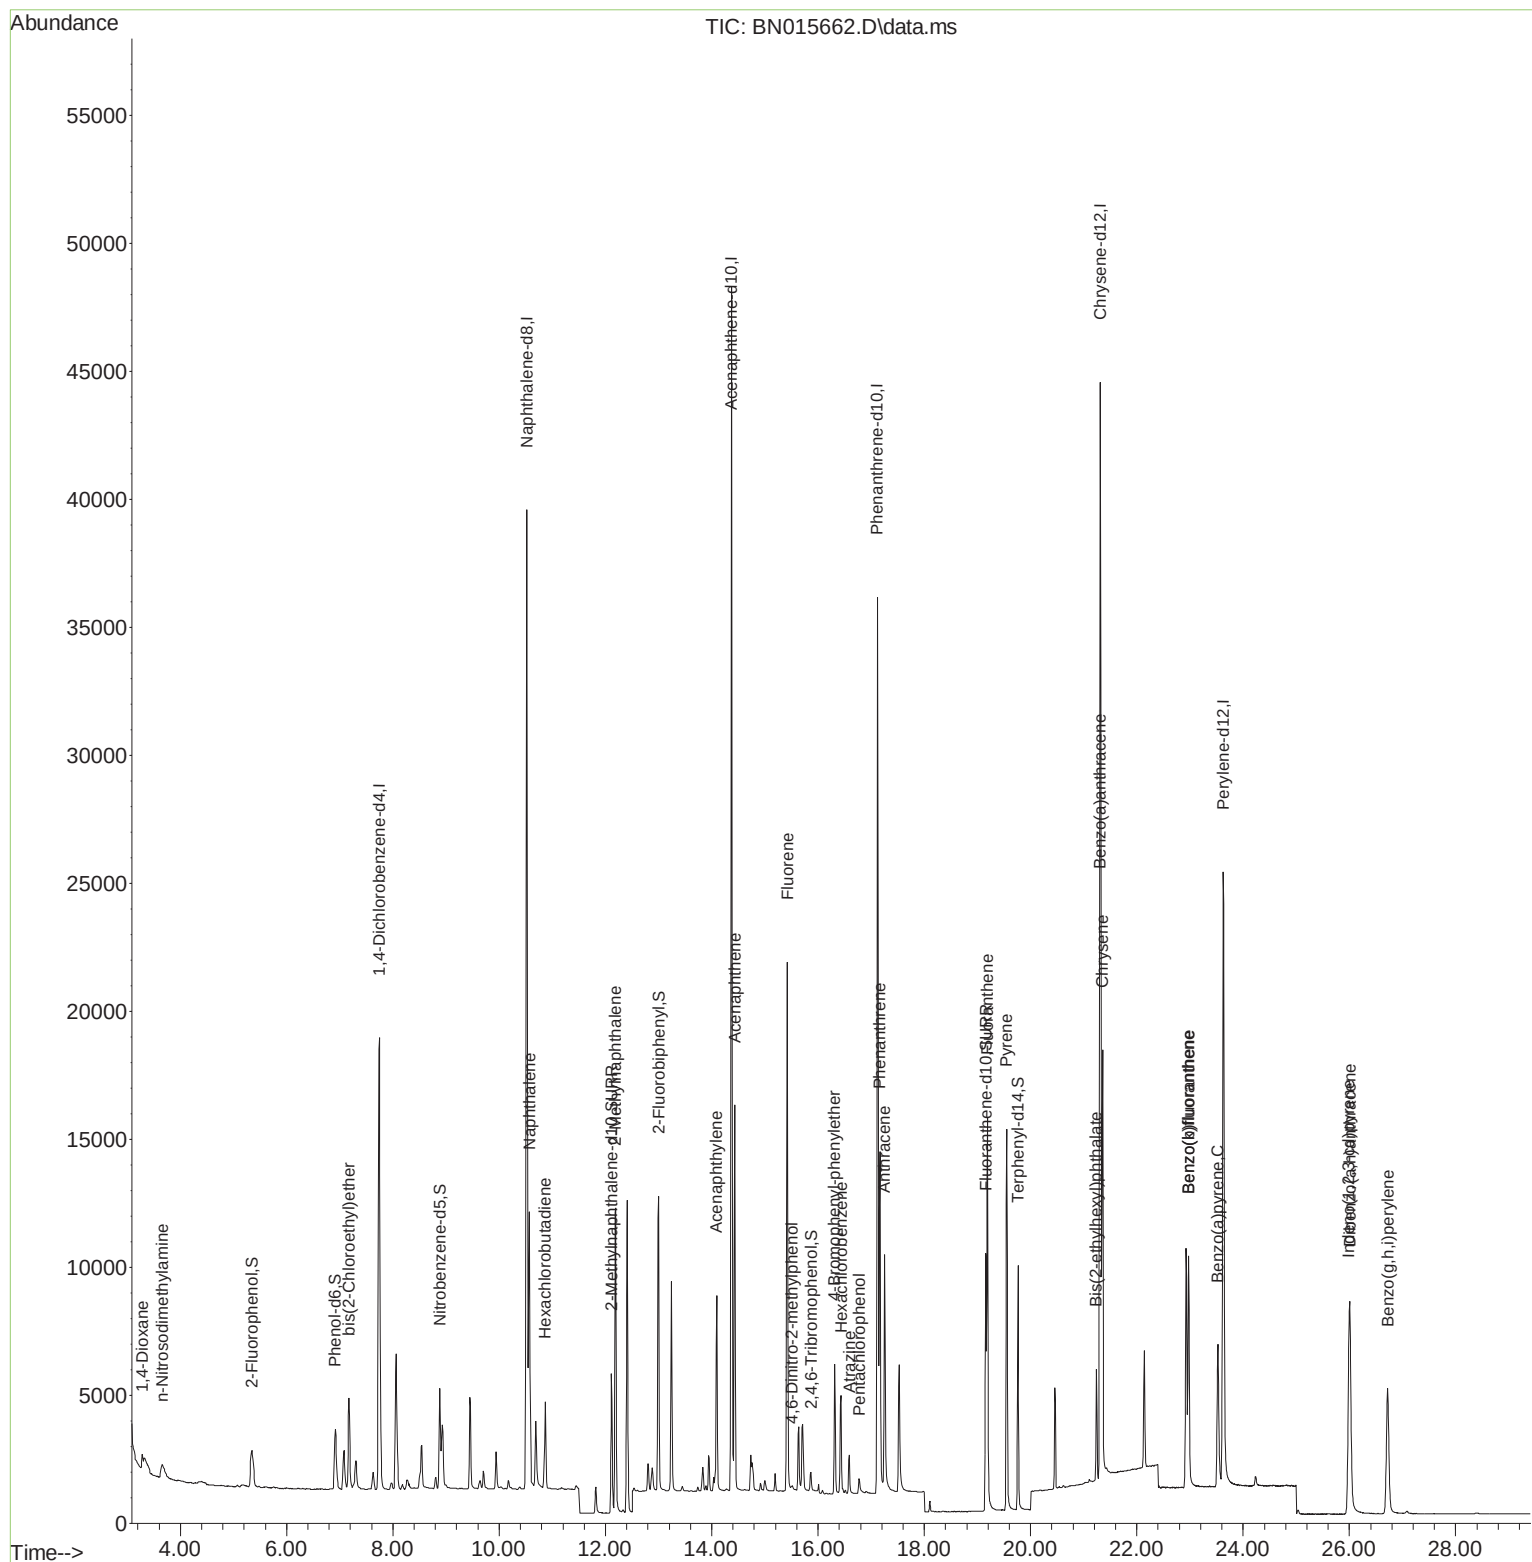


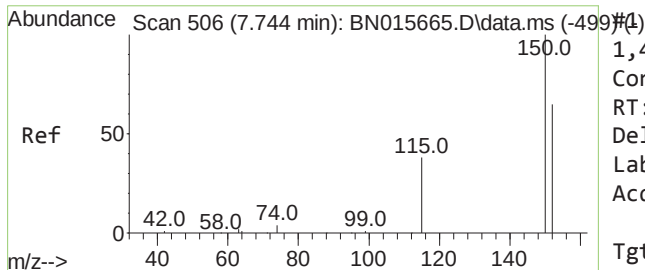

1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.744 min Scan# 506
 Delta R.T. -0.000 min
 Lab File: BN015662.D
 Acq: 23 Jul 2021 09:35




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:152 Resp: 12017
 Ion Ratio Lower Upper
 152 100
 150 153.5 123.4 185.0
 115 57.9 47.2 70.8

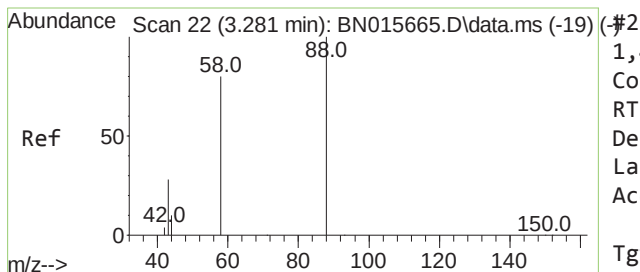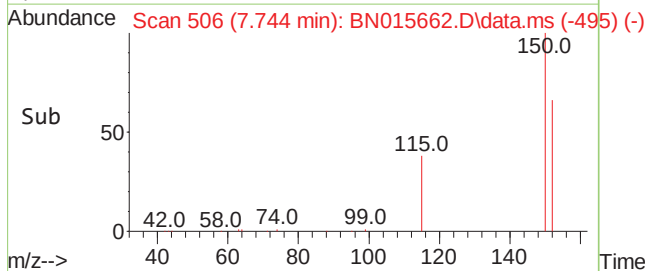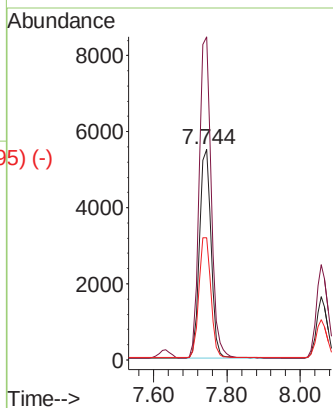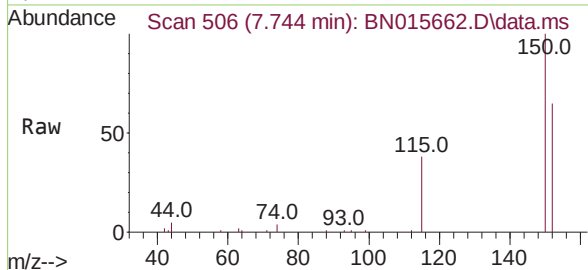

1,4-Dioxane
 Concen: 0.096 ng
 RT: 3.281 min Scan# 22
 Delta R.T. 0.000 min
 Lab File: BN015662.D
 Acq: 23 Jul 2021 09:35

Tgt Ion: 88 Resp: 390
 Ion Ratio Lower Upper
 88 100
 43 34.9 23.5 35.3
 58 78.2 64.2 96.4


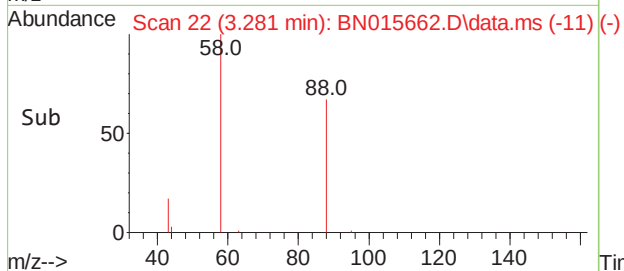




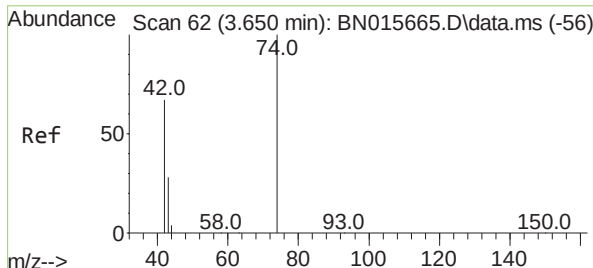

#3
n-Nitrosodimethylamine
Concen: 0.077 ng
RT: 3.659 min Scan# 63
Delta R.T. 0.009 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	42	Resp:	766
Ion	Ratio	Lower	Upper
42	100		
74	160.6	121.0	181.6
44	6.4	6.2	9.4

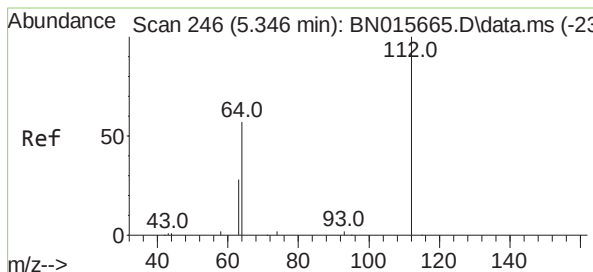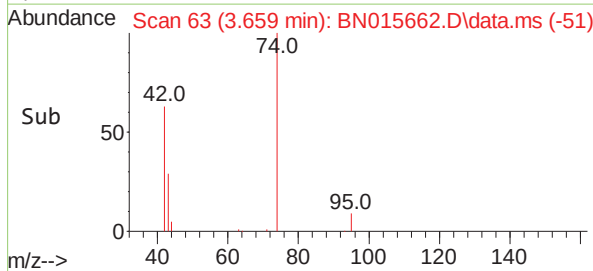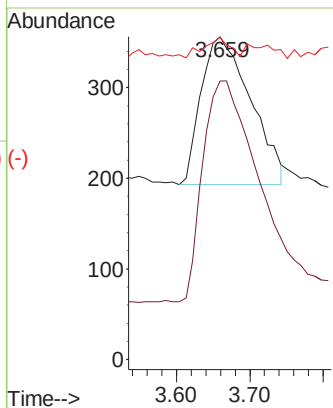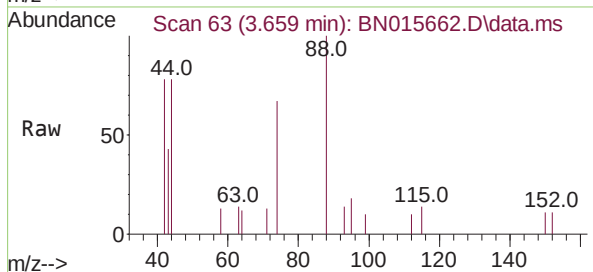

#4
2-Fluorophenol
Concen: 0.084 ng
RT: 5.346 min Scan# 246
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	112	Resp:	2903
Ion	Ratio	Lower	Upper
112	100		
64	55.5	44.9	67.3
63	28.0	22.6	33.8


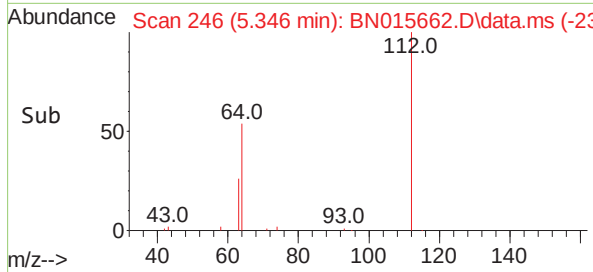
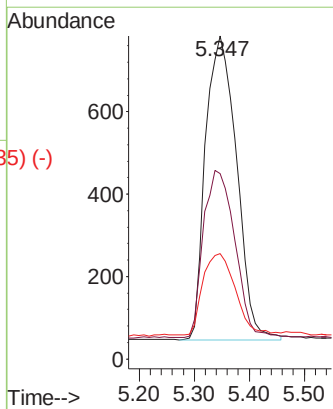
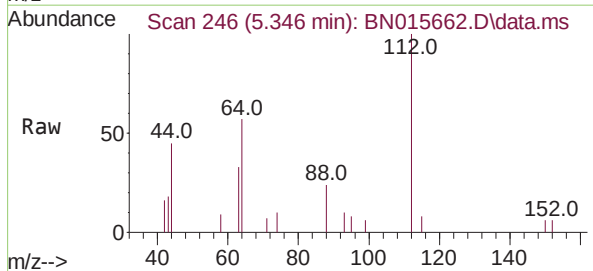


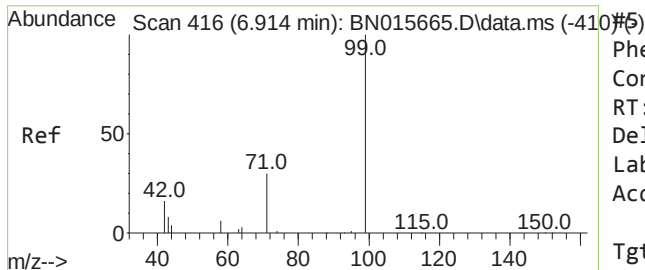

Phenol-d6
Concen: 0.078 ng
RT: 6.914 min Scan# 416
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion: 99 Resp: 3206
Ion Ratio Lower Upper
99 100
42 17.0 13.8 20.6
71 30.1 24.2 36.2

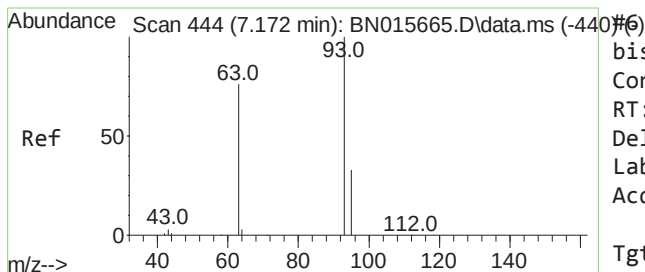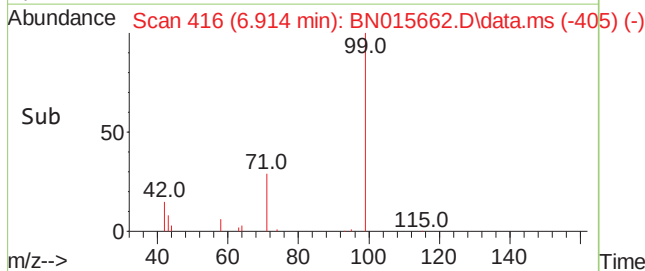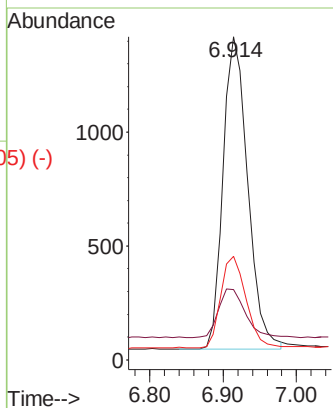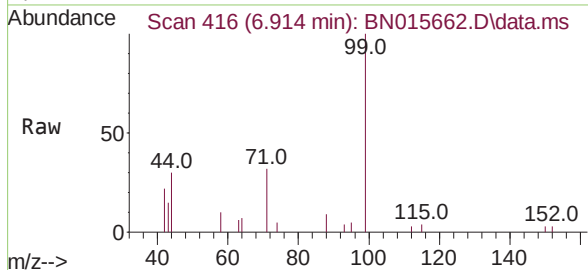


bis(2-Chloroethyl)ether
Concen: 0.094 ng
RT: 7.172 min Scan# 444
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion: 93 Resp: 3483
Ion Ratio Lower Upper
93 100
63 76.0 59.9 89.9
95 33.1 26.3 39.5

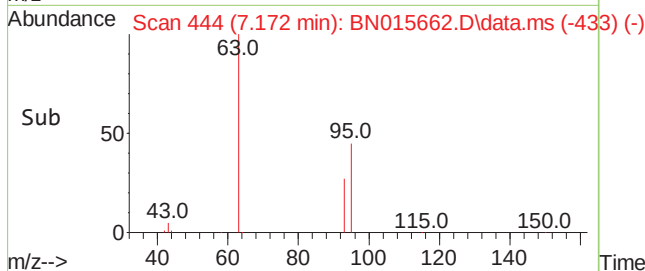




Abundance Scan 742 (10.521 min): BN015665.D\data.ms (-737) (-)

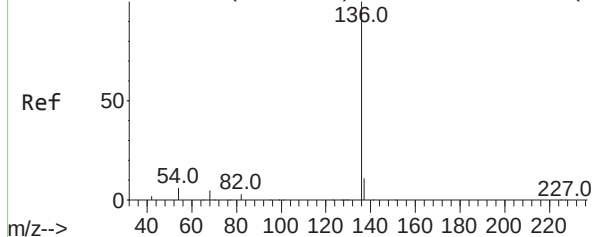


Naphthalene-d8
Concen: 0.400 ng
RT: 10.521 min Scan# 742
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:	136	Resp:	52344
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.7	13.1
54	6.4	5.2	7.8
68	5.4	4.4	6.6

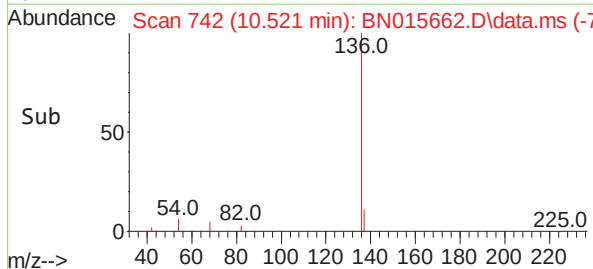
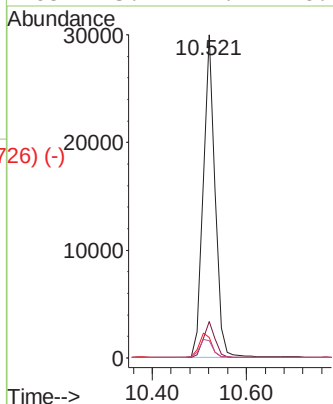
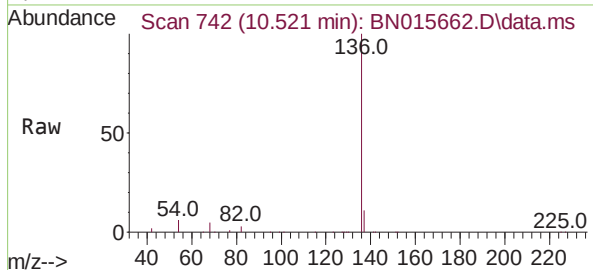



Abundance Scan 613 (8.886 min): BN015665.D\data.ms (-610) (-)

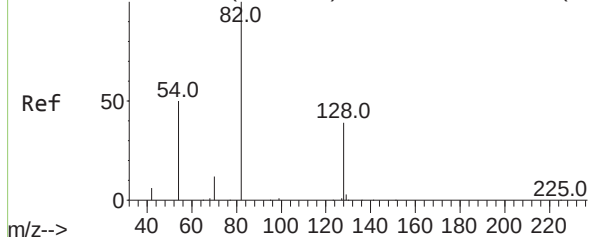

Nitrobenzene-d5
Concen: 0.094 ng
RT: 8.886 min Scan# 613
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	82	Resp:	3525
Ion	Ratio	Lower	Upper
82	100		
128	40.2	31.2	46.8
54	51.8	40.2	60.4


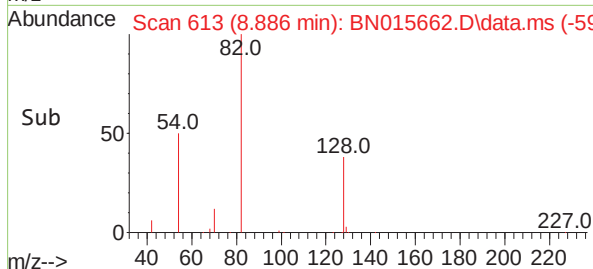
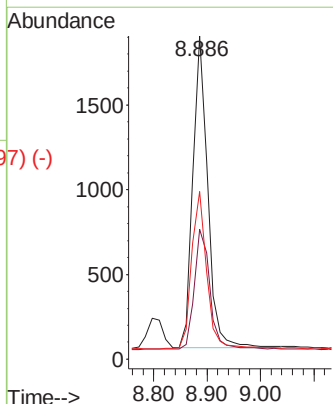
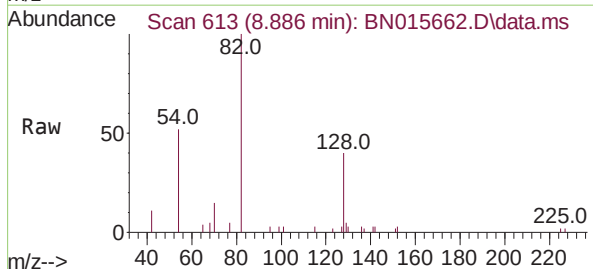


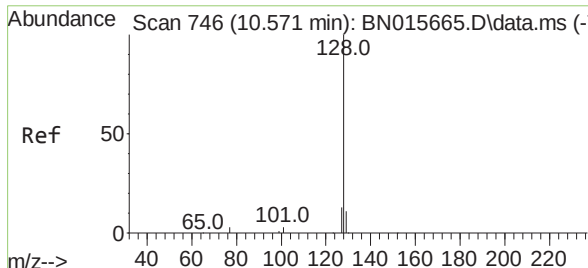

Scan 746 (10.571 min): BN015665.D\data.ms (-749)
 Naphthalene
 Concen: 0.097 ng
 RT: 10.571 min Scan# 746
 Delta R.T. 0.000 min
 Lab File: BN015662.D
 Acq: 23 Jul 2021 09:35




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion:	128	Resp:	14489
Ion	Ratio	Lower	Upper
128	100		
129	11.4	8.8	13.2
127	13.1	10.2	15.4

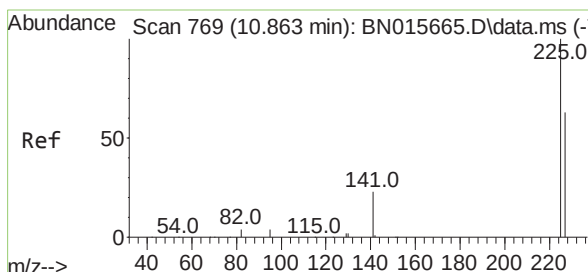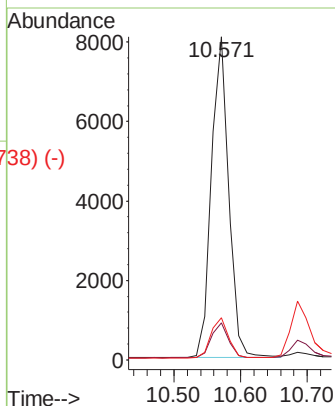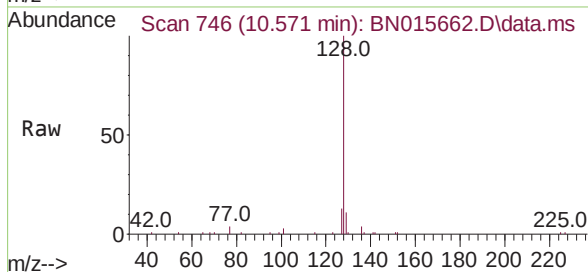


Scan 769 (10.863 min): BN015665.D\data.ms (-7610)
 Hexachlorobutadiene
 Concen: 0.098 ng
 RT: 10.863 min Scan# 769
 Delta R.T. 0.000 min
 Lab File: BN015662.D
 Acq: 23 Jul 2021 09:35

Tgt Ion:	225	Resp:	2737
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.8	50.6	76.0

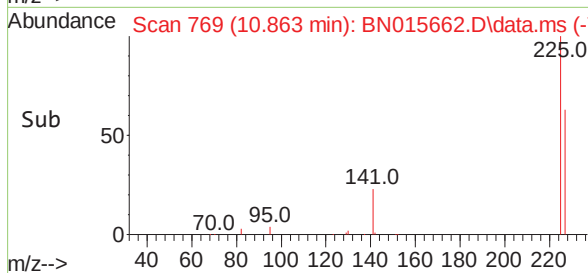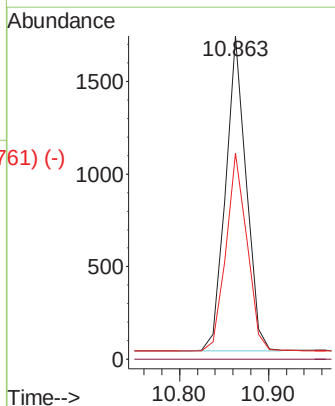




Abundance Scan 956 (12.114 min): BN015665.D\data.ms (-943) #11




2-Methylnaphthalene-d10
Concen: 0.090 ng
RT: 12.114 min Scan# 956
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:152 Resp: 7821
Ion Ratio Lower Upper
152 100
151 20.7 16.4 24.6

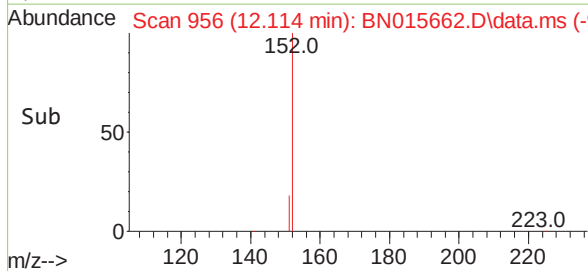

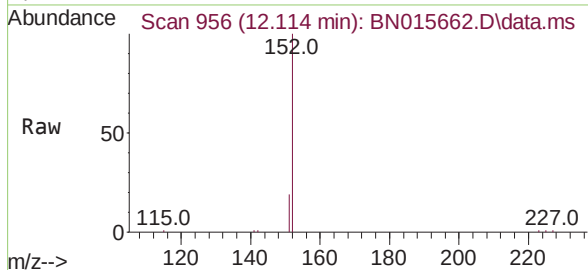


Abundance Scan 973 (12.190 min): BN015665.D\data.ms (-963) #12

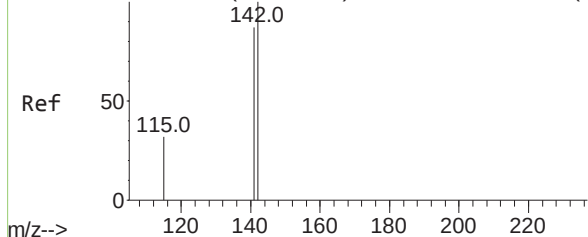


2-Methylnaphthalene
Concen: 0.093 ng
RT: 12.190 min Scan# 973
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:142 Resp: 9067
Ion Ratio Lower Upper
142 100
141 88.1 69.5 104.3
115 33.5 26.1 39.1

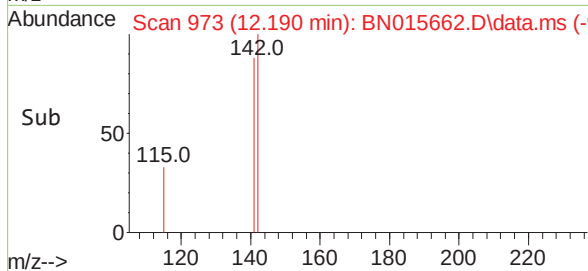




Abundance Scan 1191 (14.370 min): BN015665.D\data.ms (-1191) (-)




Acenaphthene-d10
Concen: 0.400 ng
RT: 14.370 min Scan# 1191
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:164 Resp: 26009
Ion Ratio Lower Upper
164 100
162 100.0 80.6 120.8
160 45.3 37.0 55.4

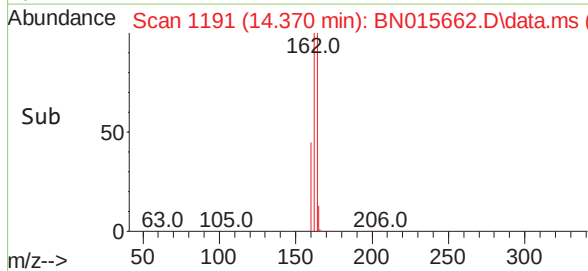
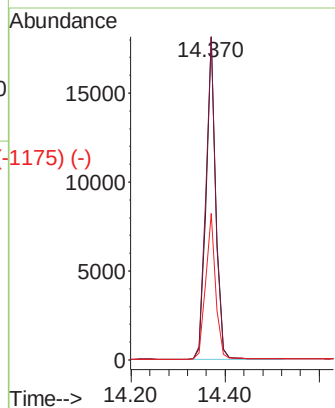
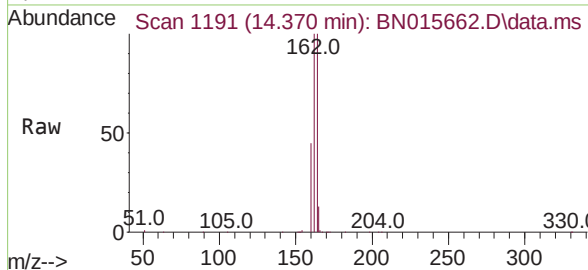


Abundance Scan 1309 (15.867 min): BN015665.D\data.ms (-1309) (-)



2,4,6-Tribromophenol
Concen: 0.058 ng
RT: 15.867 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Tgt Ion:330 Resp: 678
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.6 28.7 43.1

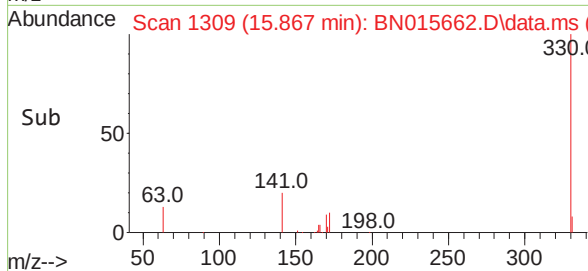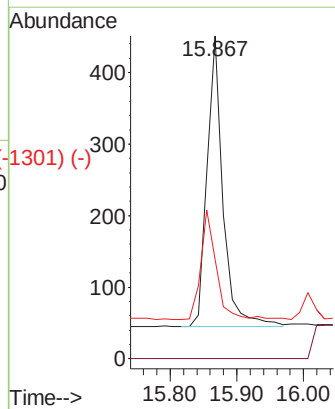




Abundance Scan 1083 (13.000 min): BN015665.D\data.ms (-1075) (-)

2-Fluorobiphenyl
Concen: 0.115 ng
RT: 13.000 min Scan# 1083
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

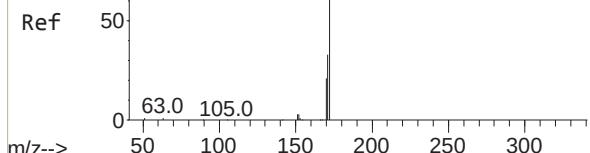


Tgt Ion:	172	Resp:	11879
Ion	Ratio	Lower	Upper
172	100		
171	33.9	26.6	40.0
170	21.9	17.2	25.8

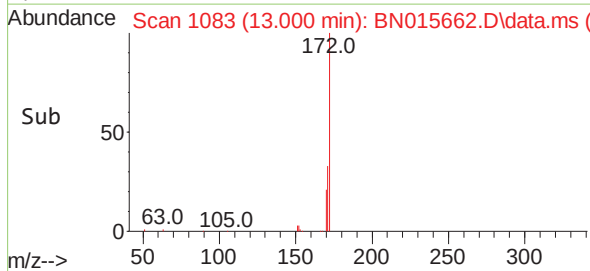
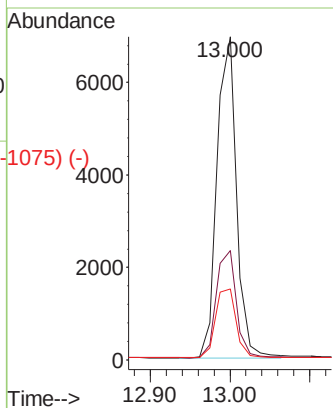
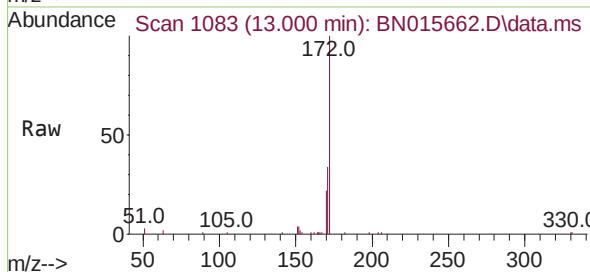


Abundance Scan 1169 (14.091 min): BN015665.D\data.ms (-1153) (-)

Acenaphthylene
Concen: 0.077 ng
RT: 14.091 min Scan# 1169
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

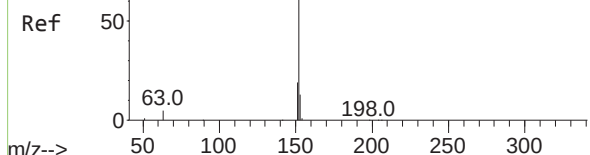


Tgt Ion:	152	Resp:	9276
Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.4	23.2
153	13.2	10.3	15.5

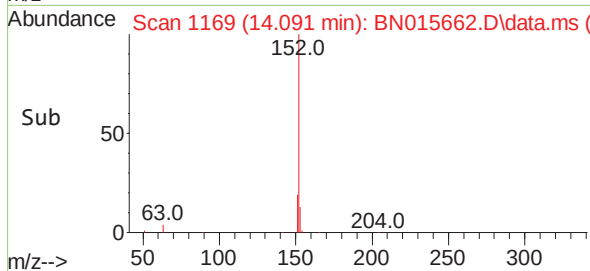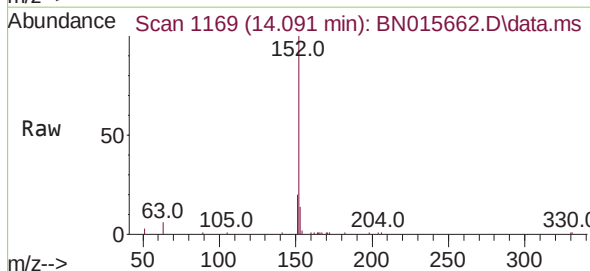




Abundance Scan 1196 (14.434 min): BN015665.D\data.ms (-1197) (-)

Acenaphthene
Concen: 0.094 ng
RT: 14.434 min Scan# 1196
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

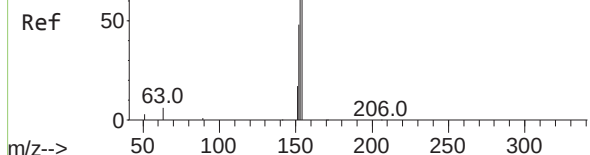


Tgt Ion:	154	Resp:	7641
Ion	Ratio	Lower	Upper
154	100		
153	113.0	90.6	136.0
152	55.5	44.6	67.0

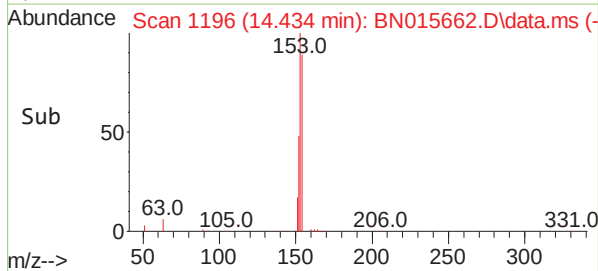
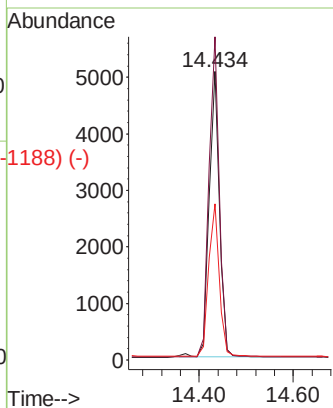
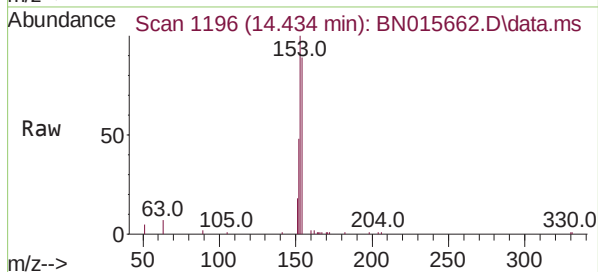


Abundance Scan 1274 (15.423 min): BN015665.D\data.ms (-1275) (-)

Fluorene
Concen: 0.089 ng
RT: 15.423 min Scan# 1274
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

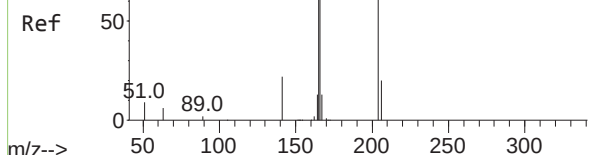


Tgt Ion:	166	Resp:	8772
Ion	Ratio	Lower	Upper
166	100		
165	97.3	78.3	117.5
167	13.3	10.8	16.2

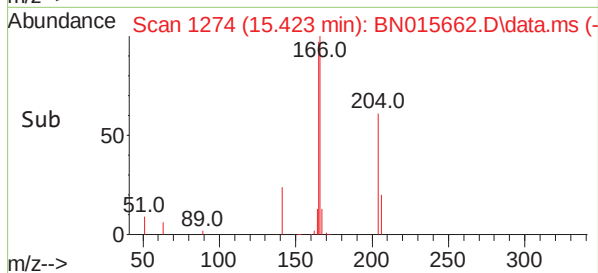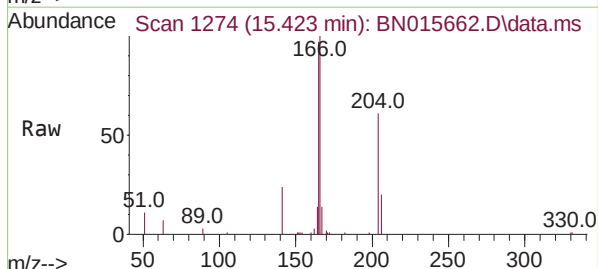



Abundance Scan 1411 (17.115 min): BN015665.D\data.ms (-1419) (-)

Phenanthrene-d10
Concen: 0.400 ng
RT: 17.115 min Scan# 1411
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

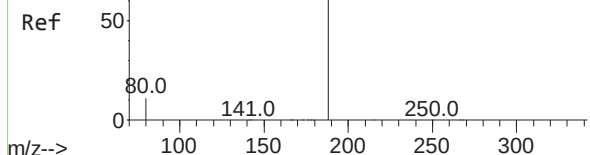

Tgt Ion:	188	Resp:	48805
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.1	9.2	13.8

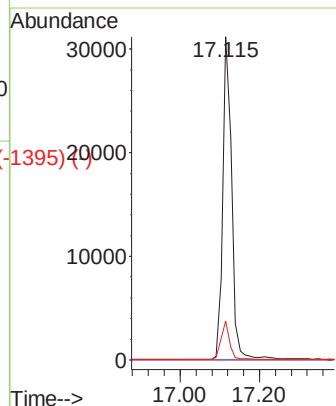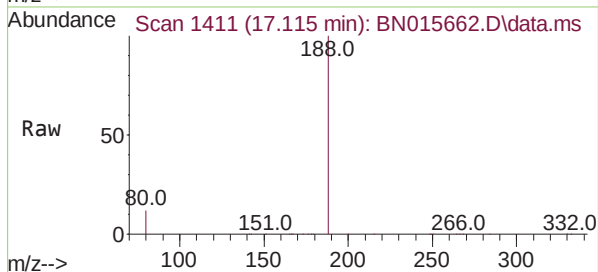



Abundance Scan 1411 (17.115 min): BN015662.D\data.ms (-1395) (-)

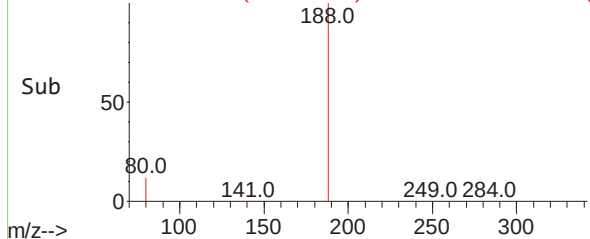


Abundance Scan 1281 (15.512 min): BN015665.D\data.ms (-1279) (-)

4,6-Dinitro-2-methylphenol
Concen: 0.036 ng
RT: 15.512 min Scan# 1281
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Tgt Ion:	198	Resp:	145
Ion	Ratio	Lower	Upper
198	100		
182	48.7	17.2	25.8#
77	0.0	0.0	0.0

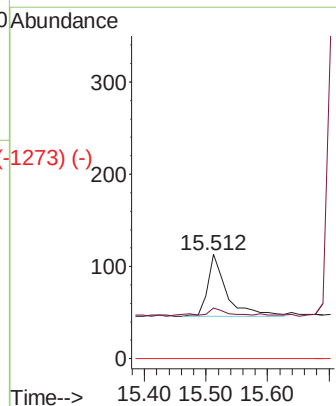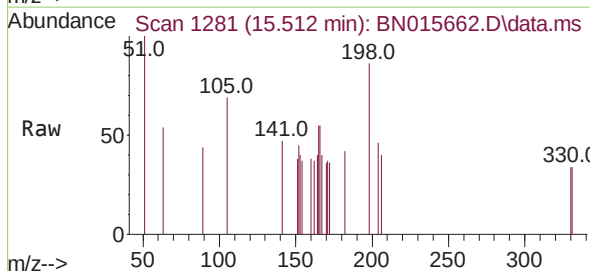

Abundance Scan 1281 (15.512 min): BN015662.D\data.ms (-1273) (-)

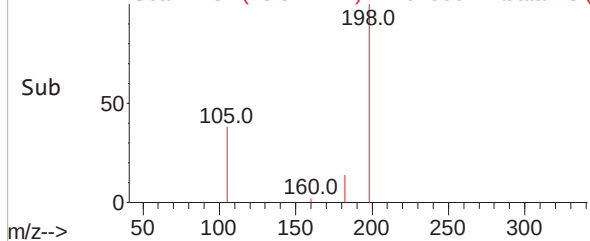




Abundance Scan 1345 (16.312 min): BN015665.D\data.ms (-1340) (-)

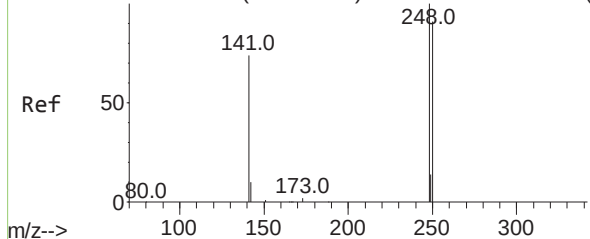


4-Bromophenyl-phenylether
Concen: 0.085 ng
RT: 16.312 min Scan# 1345
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:	248	Resp:	2602
Ion	Ratio	Lower	Upper
248	100		
250	92.3	72.9	109.3
141	80.9	59.1	88.7

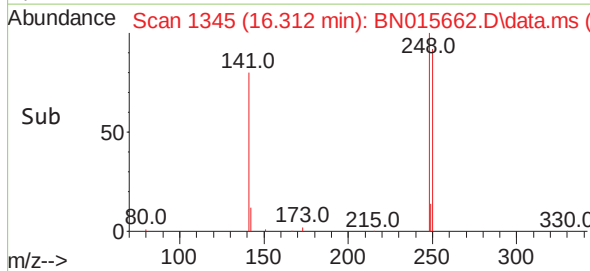
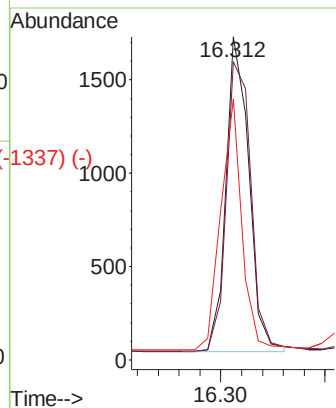
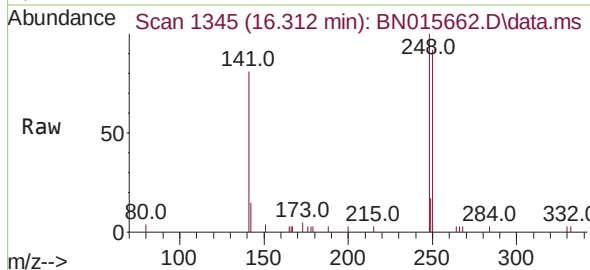


Abundance Scan 1355 (16.433 min): BN015665.D\data.ms (-1340) (-)

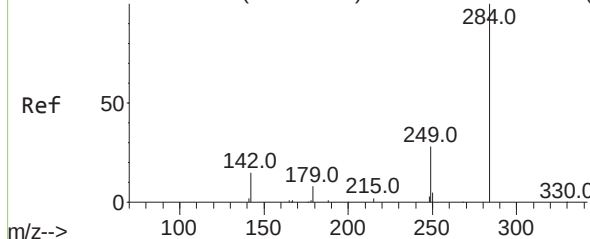


Hexachlorobenzene
Concen: 0.096 ng
RT: 16.433 min Scan# 1355
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	284	Resp:	3255
Ion	Ratio	Lower	Upper
284	100		
142	35.2	27.5	41.3
249	30.7	25.0	37.6

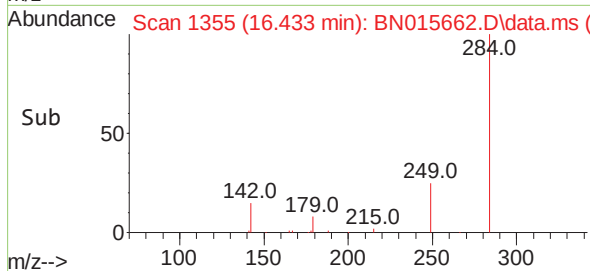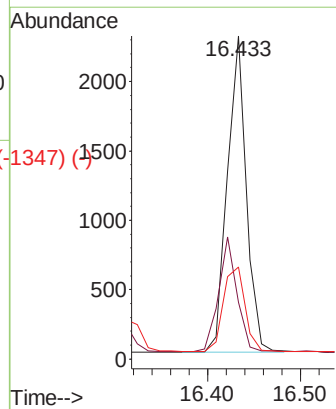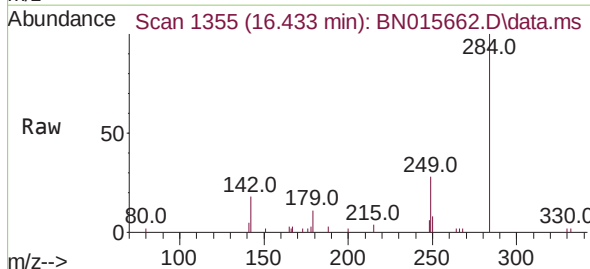



Abundance Scan 1368 (16.592 min): BN015665.D\data.ms (-1325) (-)




Atrazine
Concen: 0.067 ng
RT: 16.592 min Scan# 1368
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:	200	Resp:	1490
Ion	Ratio	Lower	Upper
200	100		
173	25.3	17.8	26.8
215	51.0	39.8	59.8

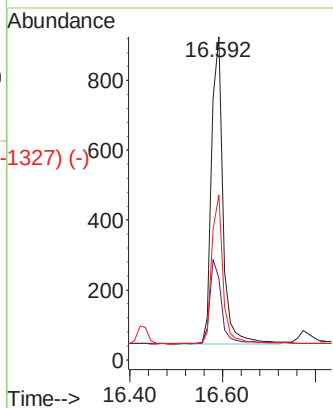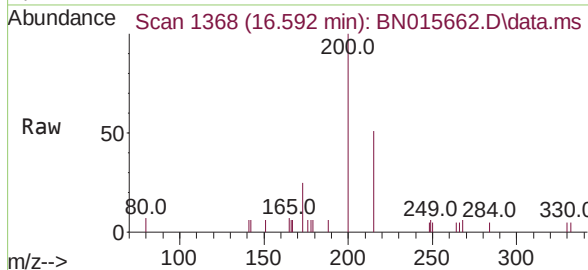

Abundance Scan 1368 (16.592 min): BN015662.D\data.ms (-1327) (-)


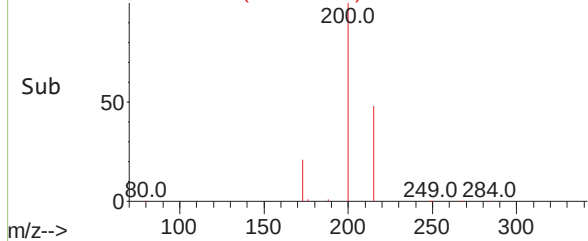


Abundance Scan 1383 (16.774 min): BN015665.D\data.ms (-1374) (-)




Pentachlorophenol
Concen: 0.056 ng
RT: 16.774 min Scan# 1383
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Tgt Ion:	266	Resp:	472
Ion	Ratio	Lower	Upper
266	100		
264	59.1	51.0	76.4
268	59.3	51.8	77.8



Abundance Scan 1383 (16.774 min): BN015662.D\data.ms (-1375) (-)






Abundance Scan 1415 (17.164 min): BN015665.D\data.ms (-1425) (-)

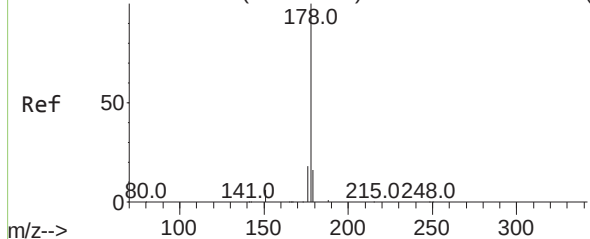


Phenanthrene
Concen: 0.093 ng
RT: 17.164 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	178	Resp:	14643
Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.0	22.6
179	16.0	12.4	18.6

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

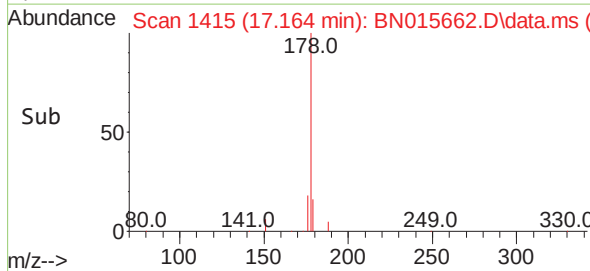
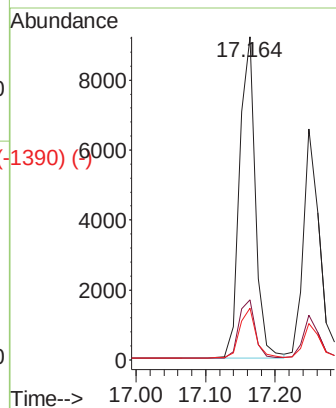
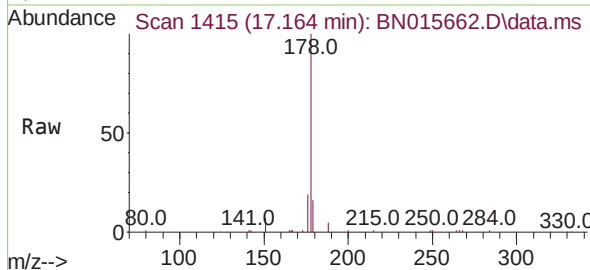


Abundance Scan 1422 (17.249 min): BN015665.D\data.ms (-1425) (-)

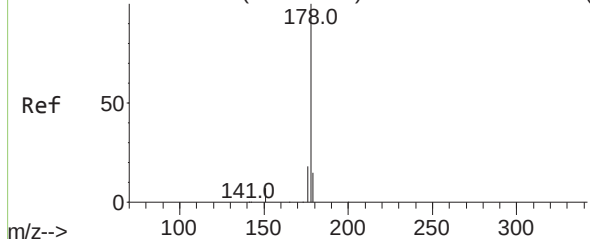


Anthracene
Concen: 0.079 ng
RT: 17.249 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	178	Resp:	10609
Ion	Ratio	Lower	Upper
178	100		
176	18.2	14.6	21.8
179	15.0	12.2	18.2

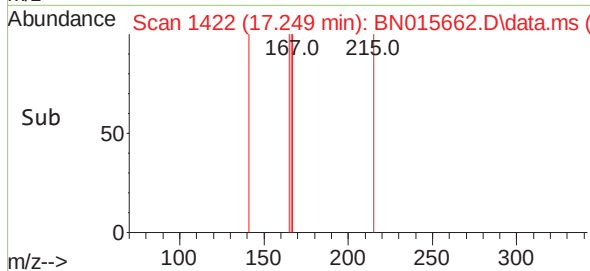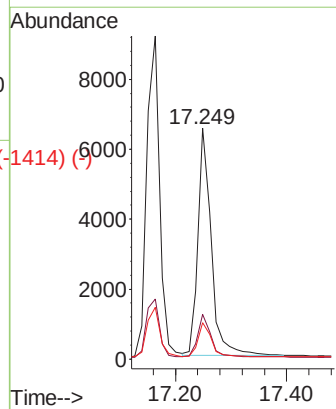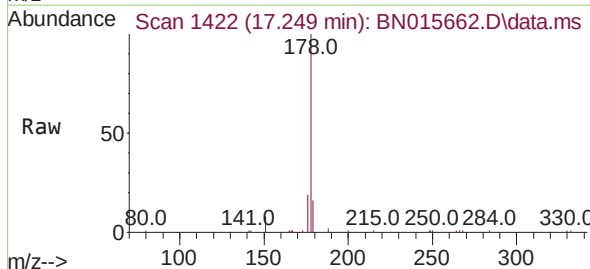



Abundance Scan 1715 (19.157 min): BN015665.D\data.ms (-1#25) (-)




Fluoranthene-d10
Concen: 0.081 ng
RT: 19.157 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:212 Resp: 12083
Ion Ratio Lower Upper
212 100
106 14.3 11.5 17.3
104 7.7 6.2 9.4

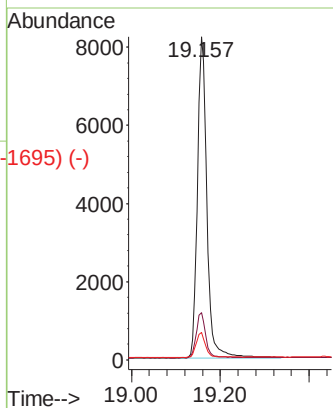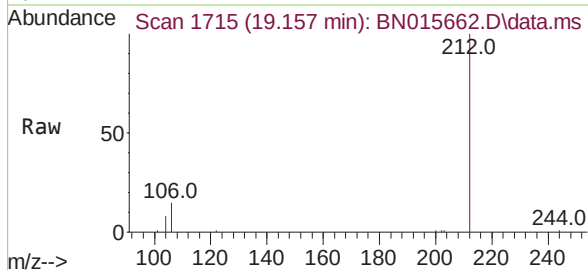

Abundance Scan 1715 (19.157 min): BN015662.D\data.ms (-1695) (-)


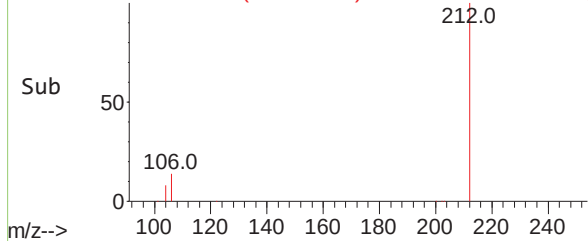


Abundance Scan 1721 (19.187 min): BN015665.D\data.ms (-1#23) (-)




Fluoranthene
Concen: 0.083 ng
RT: 19.187 min Scan# 1721
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Tgt Ion:202 Resp: 14472
Ion Ratio Lower Upper
202 100
101 11.5 9.5 14.3
203 17.0 13.8 20.6



Abundance Scan 1721 (19.187 min): BN015662.D\data.ms (-1681) (-)

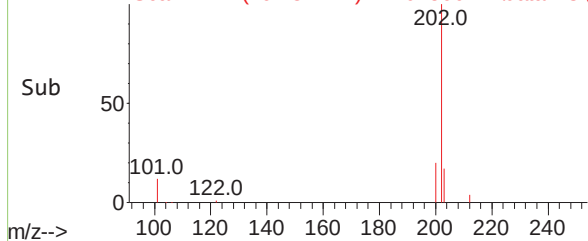




Abundance Scan 2009 (21.312 min): BN015665.D\data.ms (-1990) (-)

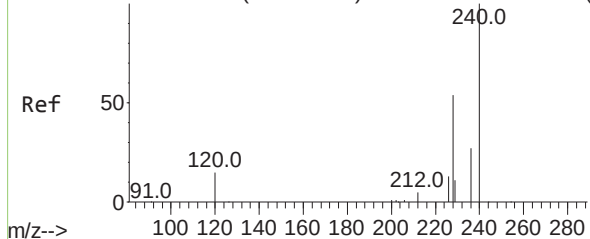


Chrysene-d12
Concen: 0.400 ng
RT: 21.312 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:	240	Resp:	38200
Ion	Ratio	Lower	Upper
240	100		
120	15.7	12.2	18.4
236	26.9	21.5	32.3

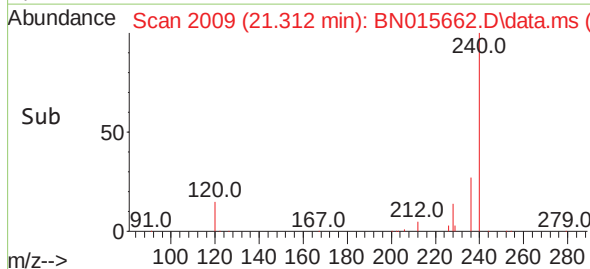
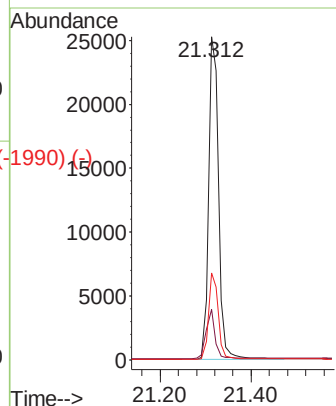
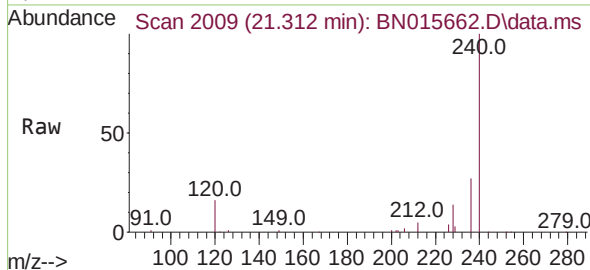


Abundance Scan 1794 (19.549 min): BN015665.D\data.ms (-1754) (-)

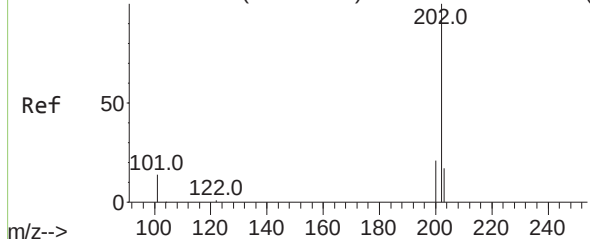

Pyrene
Concen: 0.101 ng
RT: 19.549 min Scan# 1794
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Tgt Ion:	202	Resp:	14586
Ion	Ratio	Lower	Upper
202	100		
200	20.6	16.4	24.6
203	17.2	13.9	20.9

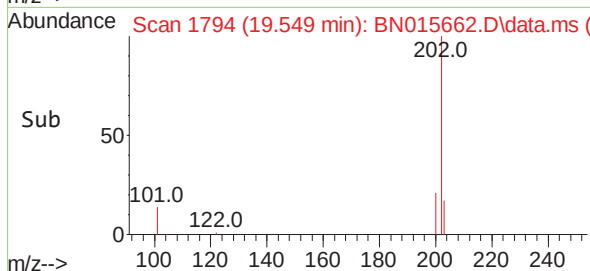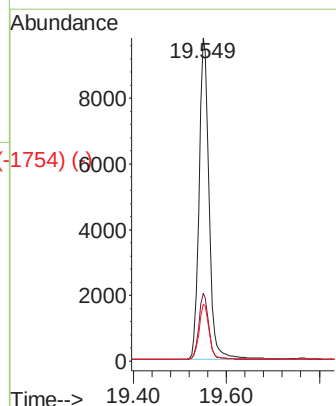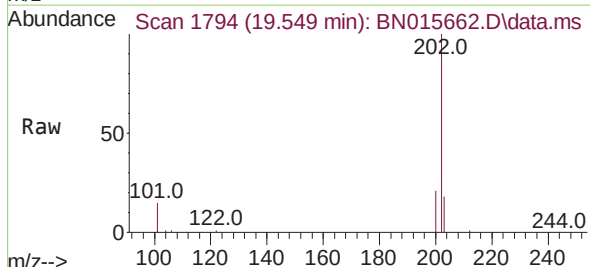



Abundance Scan 1837 (19.763 min): BN015665.D\data.ms (-1823) (-)

Terphenyl-d14
Concen: 0.115 ng
RT: 19.763 min Scan# 1837
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

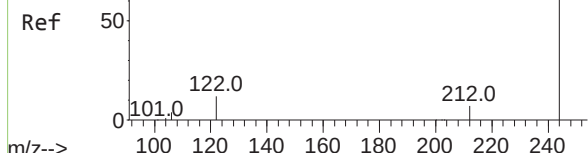

Tgt Ion:	244	Resp:	10245
Ion	Ratio	Lower	Upper
244	100		
212	8.4	6.1	9.1
122	13.6	10.1	15.1

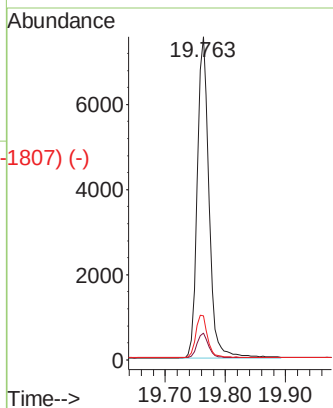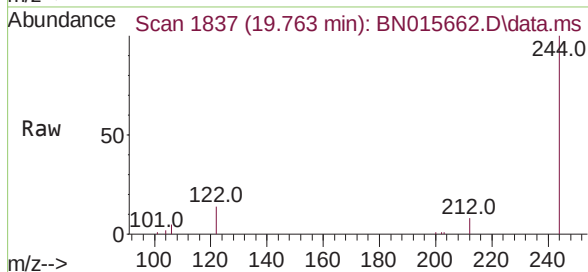




Abundance Scan 1837 (19.763 min): BN015662.D\data.ms (-1807) (-)

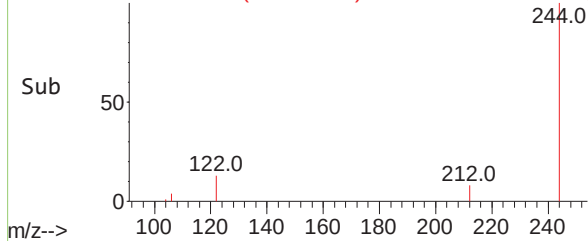


Abundance Scan 2008 (21.302 min): BN015665.D\data.ms (-2032) (-)


Benzo(a)anthracene
Concen: 0.078 ng
RT: 21.302 min Scan# 2008
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	228	Resp:	10670
Ion	Ratio	Lower	Upper
228	100		
226	27.0	21.4	32.0
229	20.3	15.5	23.3



Abundance Scan 2008 (21.302 min): BN015662.D\data.ms (-1989) (-)




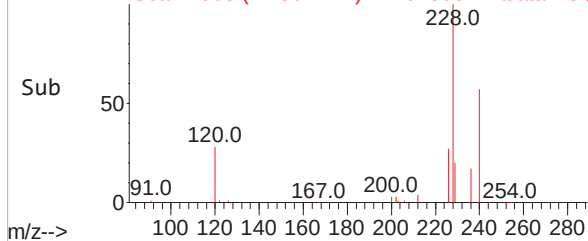


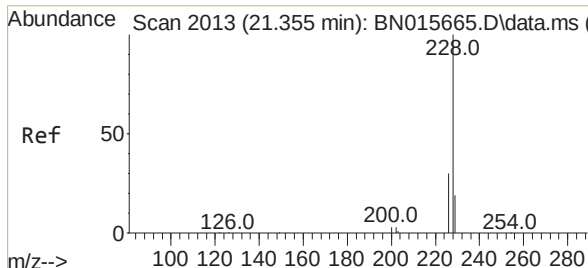

Scan 2013 (21.355 min): BN015665.D\data.ms (-2030) (-)
Chrysene
 Concen: 0.101 ng
 RT: 21.355 min Scan# 2013
 Delta R.T. 0.000 min
 Lab File: BN015662.D
 Acq: 23 Jul 2021 09:35




Instrument :
 BNA_N
ClientSampleId :
 SSTDICC0.1

Tgt Ion:	228	Resp:	14202
Ion	Ratio	Lower	Upper
228	100		
226	29.1	23.5	35.3
229	20.2	15.6	23.4

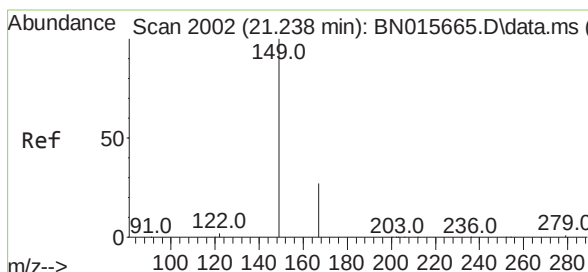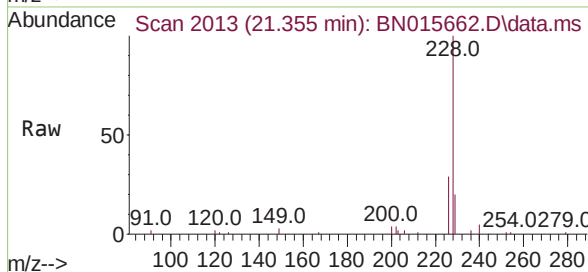

Scan 2002 (21.238 min): BN015665.D\data.ms (-1936) (-)
Bis(2-ethylhexyl)phthalate
 Concen: 0.060 ng
 RT: 21.238 min Scan# 2002
 Delta R.T. 0.000 min
 Lab File: BN015662.D
 Acq: 23 Jul 2021 09:35


Tgt Ion:	149	Resp:	3939
Ion	Ratio	Lower	Upper
149	100		
167	27.9	22.2	33.4
279	3.9	2.8	4.2

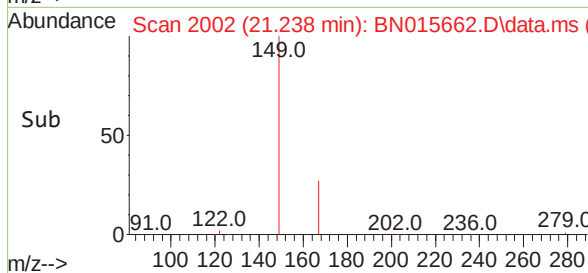




Abundance Scan 2469 (23.628 min): BN015665.D\data.ms (-2425) (-)

Perylene-d12
Concen: 0.400 ng
RT: 23.628 min Scan# 2469
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

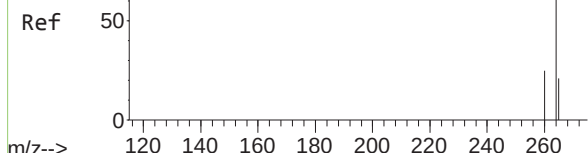





Tgt Ion:	264	Resp:	34702
Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.8	29.8
265	25.7	20.0	30.0

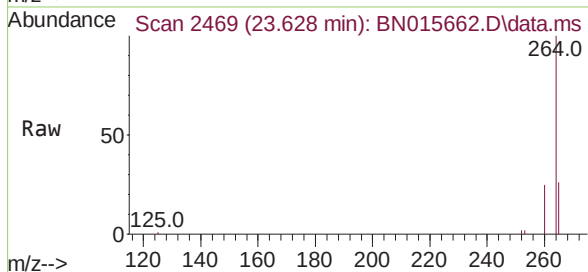


Abundance Scan 3161 (25.997 min): BN015665.D\data.ms (-3132) (-)

Indeno(1,2,3-cd)pyrene
Concen: 0.079 ng
RT: 25.993 min Scan# 3160
Delta R.T. -0.003 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	276	Resp:	11308
Ion	Ratio	Lower	Upper
276	100		
138	27.6	21.8	32.6
277	25.1	19.9	29.9

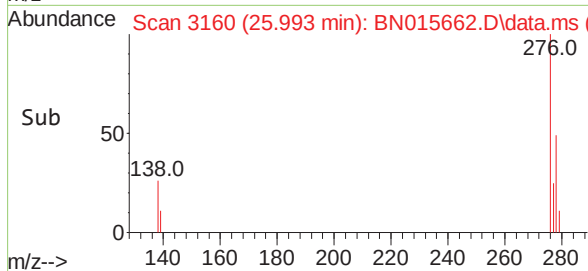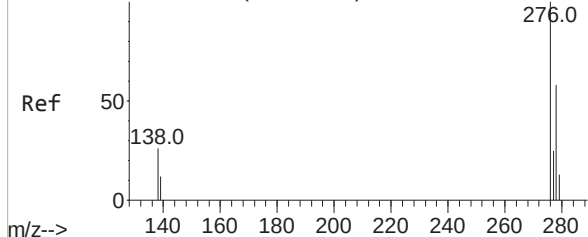

Abundance Scan 2265 (22.930 min): BN015665.D\data.ms (-230) (-)





Benzo(b)fluoranthene
Concen: 0.093 ng
RT: 22.974 min Scan# 2278
Delta R.T. 0.045 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Tgt Ion:	252	Resp:	12436
Ion	Ratio	Lower	Upper
252	100		
253	24.6	17.6	26.4
125	13.1	8.8	13.2

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Abundance Scan 2278 (22.974 min): BN015662.D\data.ms

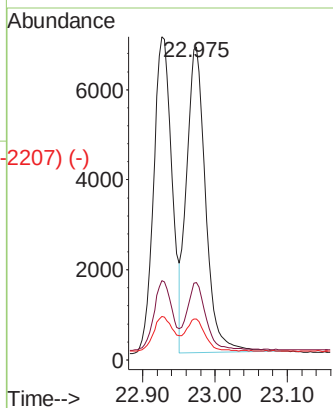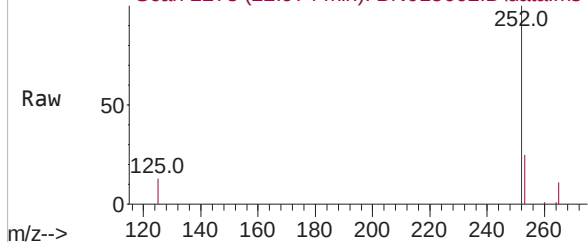

Abundance Scan 2278 (22.974 min): BN015662.D\data.ms (-2207) (-)

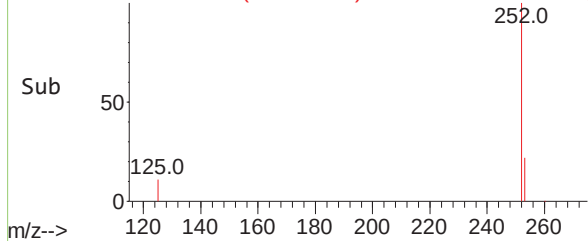



Abundance Scan 2278 (22.974 min): BN015665.D\data.ms (-230) (-)

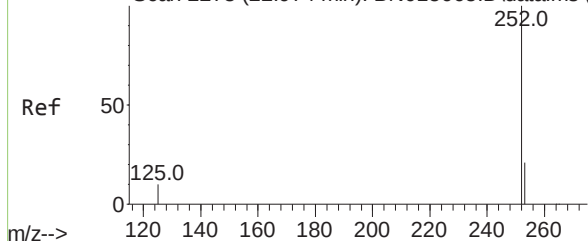


Benzo(k)fluoranthene
Concen: 0.091 ng
RT: 22.974 min Scan# 2278
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	252	Resp:	12436
Ion	Ratio	Lower	Upper
252	100		
253	24.6	17.5	26.3
125	13.1	8.8	13.2


Abundance Scan 2278 (22.974 min): BN015662.D\data.ms

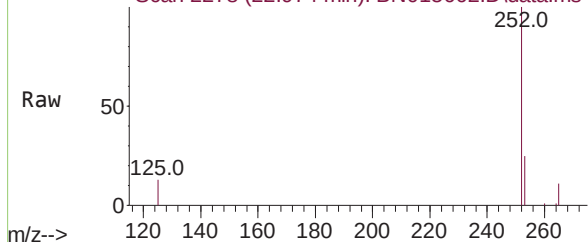

Abundance Scan 2278 (22.974 min): BN015662.D\data.ms (-2190) (-)

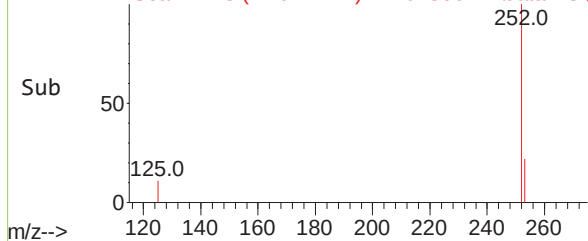



Abundance Scan 2439 (23.525 min): BN015665.D\data.ms (-2381) (-)




Benzo(a)pyrene
Concen: 0.079 ng
RT: 23.522 min Scan# 2438
Delta R.T. -0.003 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Tgt Ion:	252	Resp:	9264
Ion	Ratio	Lower	Upper
252	100		
253	26.2	18.0	27.0
125	16.7	10.4	15.6#


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

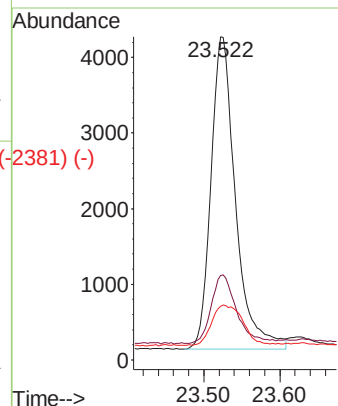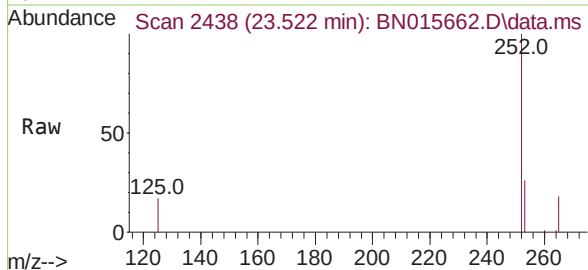

Abundance Scan 2438 (23.522 min): BN015662.D\data.ms (-2381) (-)





Abundance Scan 3166 (26.014 min): BN015665.D\data.ms (-3145) (-)




Dibenzo(a,h)anthracene
Concen: 0.075 ng
RT: 26.011 min Scan# 3165
Delta R.T. -0.003 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35


Tgt Ion:	278	Resp:	8492
Ion	Ratio	Lower	Upper
278	100		
139	20.9	14.6	22.0
279	26.0	19.3	28.9

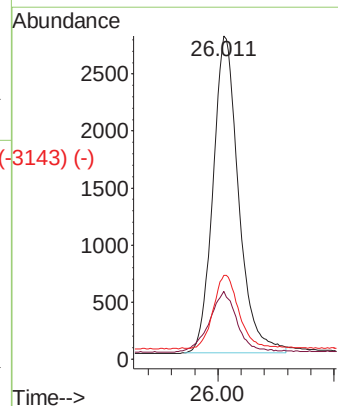

Abundance Scan 3165 (26.011 min): BN015662.D\data.ms (-3143) (-)

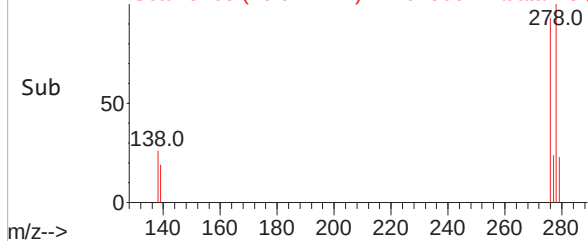


Abundance Scan 3372 (26.719 min): BN015665.D\data.ms (-3341) (-)

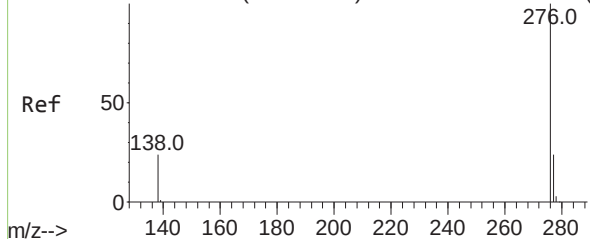


Benzo(g,h,i)perylene
Concen: 0.089 ng
RT: 26.719 min Scan# 3372
Delta R.T. 0.000 min
Lab File: BN015662.D
Acq: 23 Jul 2021 09:35

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Abundance Scan 3372 (26.719 min): BN015662.D\data.ms

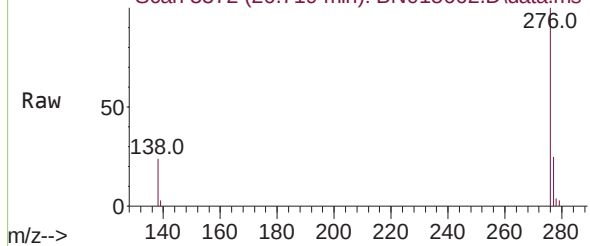

Tgt Ion:	276	Resp:	10876
Ion	Ratio	Lower	Upper
276	100		
277	25.0	19.1	28.7
138	24.4	19.1	28.7

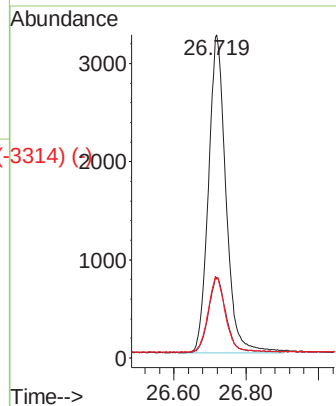

Abundance Scan 3372 (26.719 min): BN015662.D\data.ms (-3314) (-)

