
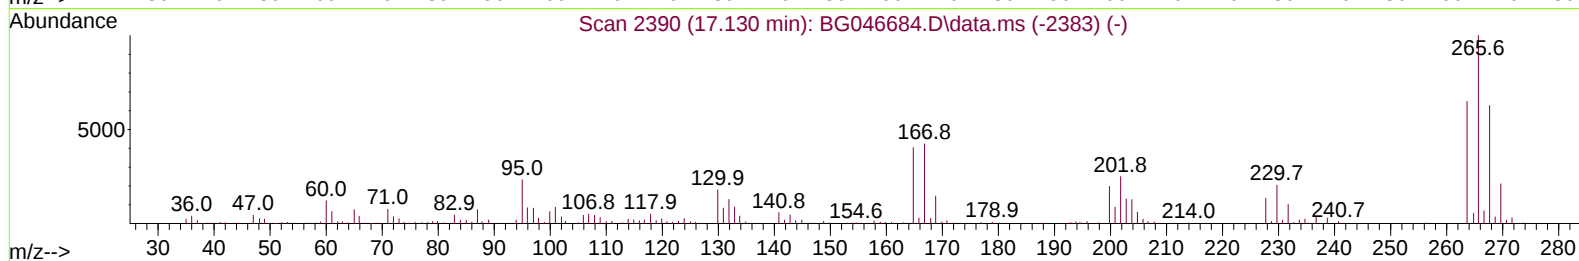
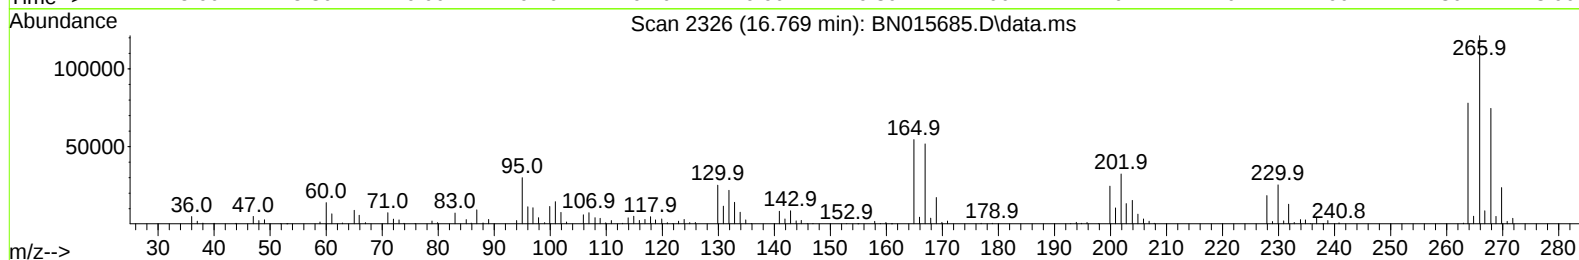


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015685.D
Acq On : 24 Jul 2021 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 06:59:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:59:38 2021
Response via : Initial Calibration

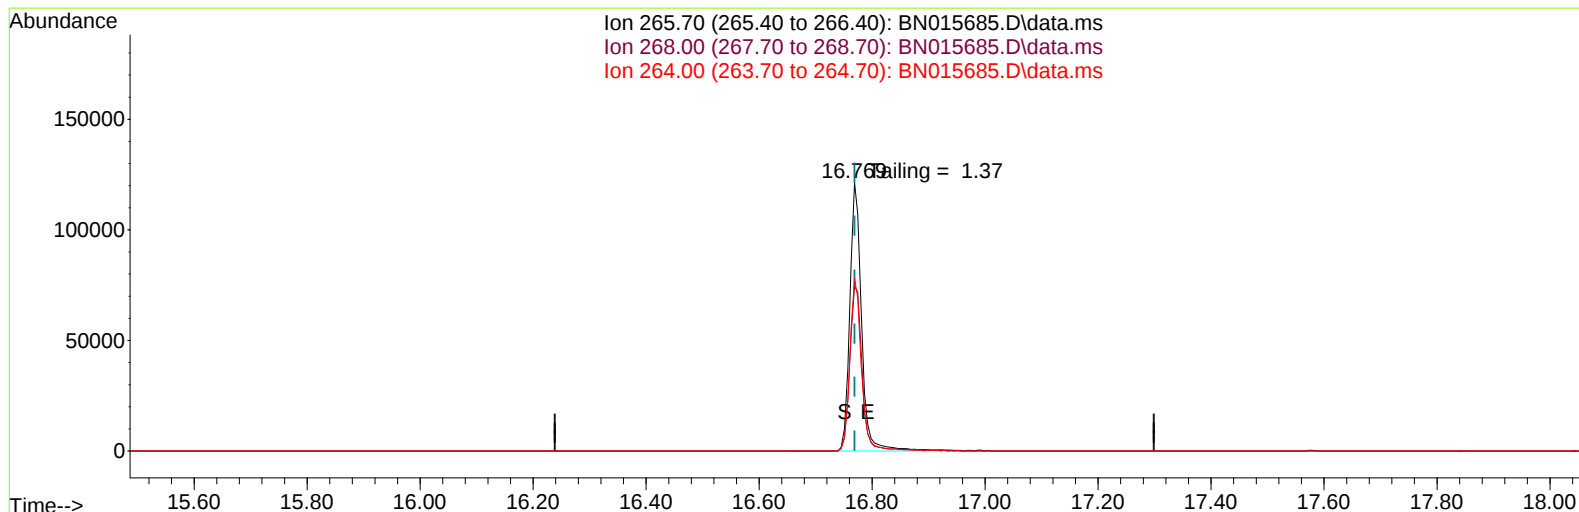

TIC: BN015685.D\data.ms

(70) Pentachlorophenol (C)




16.769min (0.000) 26842.48 ng

response 175474

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.43
264.00	61.60	64.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015685.D
Acq On : 24 Jul 2021 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 06:59:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:59:38 2021
Response via : Initial Calibration

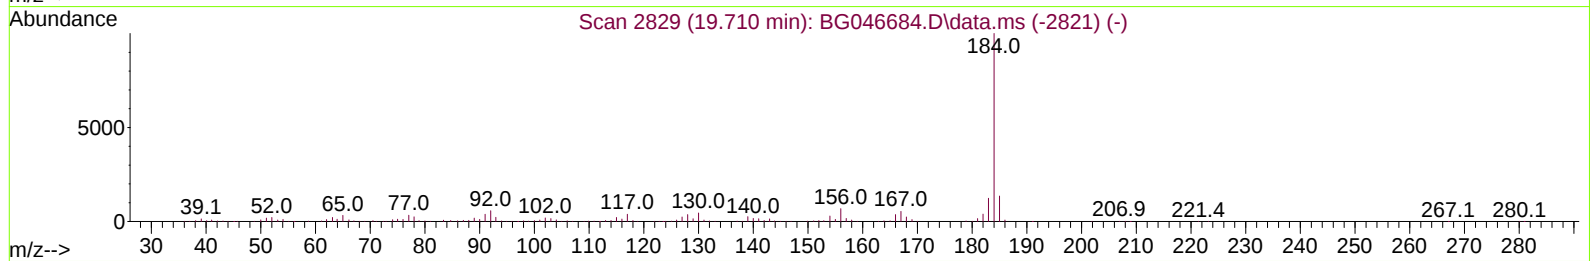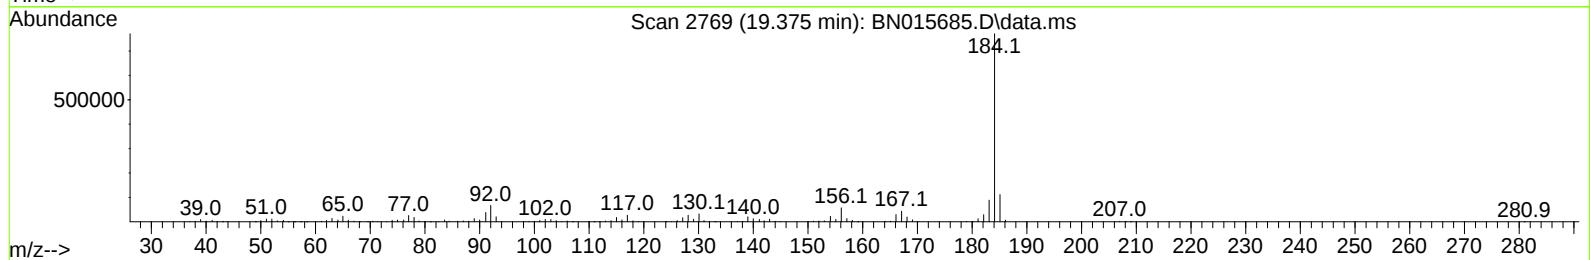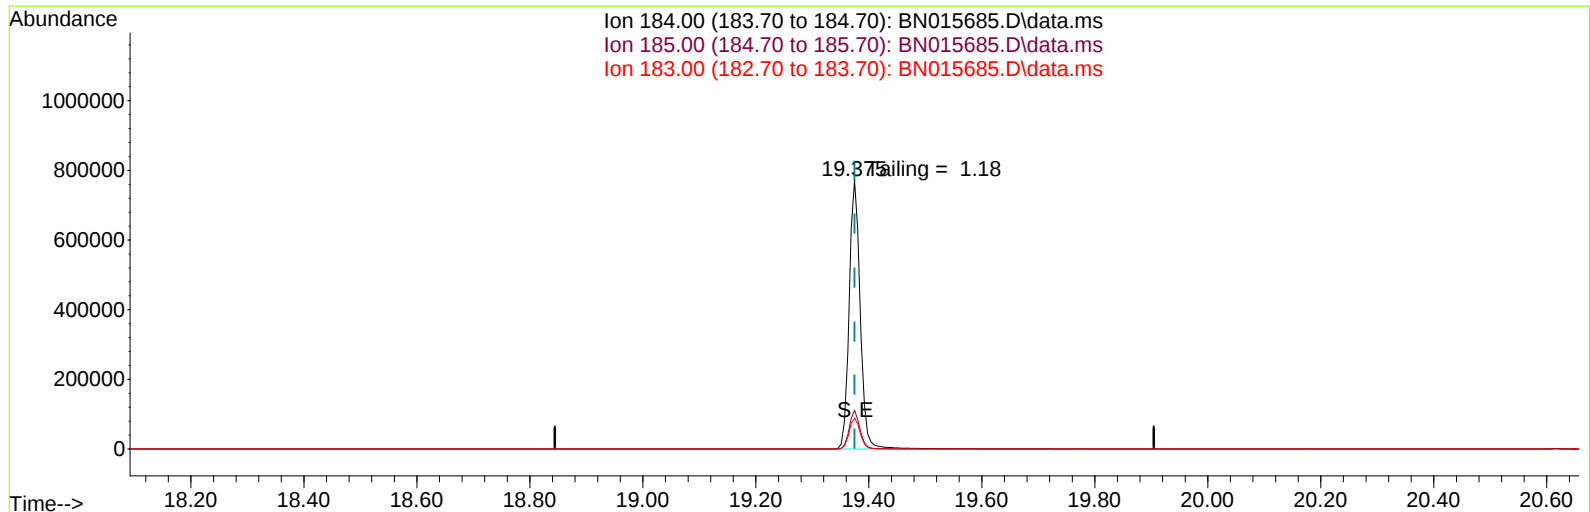

TIC: BN015685.D\data.ms

(77) Benzidine

19.375min (0.000) 0.00 ng

response 1052144

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	11.54
0.00	0.00	0.00