

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
 Data File : BN015664.D
 Acq On : 23 Jul 2021 11:24
 Operator : CG/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Jul 23 12:34:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 23 12:32:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.744	152	12636	0.400	ng	0.00
7) Naphthalene-d8	10.521	136	54268	0.400	ng	0.00
13) Acenaphthene-d10	14.370	164	27929	0.400	ng	0.00
19) Phenanthrene-d10	17.115	188	50488	0.400	ng	0.00
29) Chrysene-d12	21.323	240	46876	0.400	ng	# 0.01
35) Perylene-d12	23.632	264	38235	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.346	112	24343	0.669	ng	0.00
5) Phenol-d6	6.914	99	28802	0.665	ng	0.00
8) Nitrobenzene-d5	8.886	82	28359	0.727	ng	0.00
11) 2-Methylnaphthalene-d10	12.114	152	65305	0.724	ng	0.00
14) 2,4,6-Tribromophenol	15.867	330	7418	0.591	ng	0.00
15) 2-Fluorobiphenyl	13.000	172	88892	0.800	ng	0.00
27) Fluoranthene-d10	19.157	212	108916	0.703	ng	0.00
31) Terphenyl-d14	19.763	244	87264	0.801	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.281	88	3303	0.774	ng	98
3) n-Nitrosodimethylamine	3.641	42	7624	0.730	ng	99
6) bis(2-Chloroethyl)ether	7.172	93	29503	0.758	ng	100
9) Naphthalene	10.571	128	116044	0.748	ng	100
10) Hexachlorobutadiene	10.863	225	22132	0.761	ng	# 99
12) 2-Methylnaphthalene	12.189	142	75980	0.754	ng	100
16) Acenaphthylene	14.091	152	94396	0.733	ng	100
17) Acenaphthene	14.434	154	64515	0.737	ng	100
18) Fluorene	15.423	166	78499	0.741	ng	100
20) 4,6-Dinitro-2-methylph...	15.512	198	2099	0.505	ng	# 85
21) 4-Bromophenyl-phenylether	16.312	248	24010	0.760	ng	99
22) Hexachlorobenzene	16.433	284	27653	0.791	ng	99
23) Atrazine	16.592	200	14795	0.640	ng	100
24) Pentachlorophenol	16.774	266	5013	0.571	ng	98
25) Phenanthrene	17.164	178	124156	0.760	ng	100
26) Anthracene	17.249	178	103086	0.737	ng	100
28) Fluoranthene	19.187	202	139125	0.775	ng	100
30) Pyrene	19.549	202	134563	0.761	ng	100
32) Benzo(a)anthracene	21.302	228	118110	0.701	ng	99
33) Chrysene	21.355	228	129435	0.751	ng	100
34) Bis(2-ethylhexyl)phtha...	21.249	149	37241	0.466	ng	100
36) Indeno(1,2,3-cd)pyrene	26.000	276	111944	0.711	ng	100
37) Benzo(b)fluoranthene	22.930	252	120369	0.817	ng	100
38) Benzo(k)fluoranthene	22.978	252	121363	0.803	ng	100
39) Benzo(a)pyrene	23.529	252	95855	0.742	ng	98
40) Dibenzo(a,h)anthracene	26.017	278	88975	0.710	ng	99
41) Benzo(g,h,i)perylene	26.722	276	103705	0.766	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015664.D
Acq On : 23 Jul 2021 11:24
Operator : CG/JU
Sample : SSTDIC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Quant Time: Jul 23 12:34:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 23 12:32:24 2021
Response via : Initial Calibration

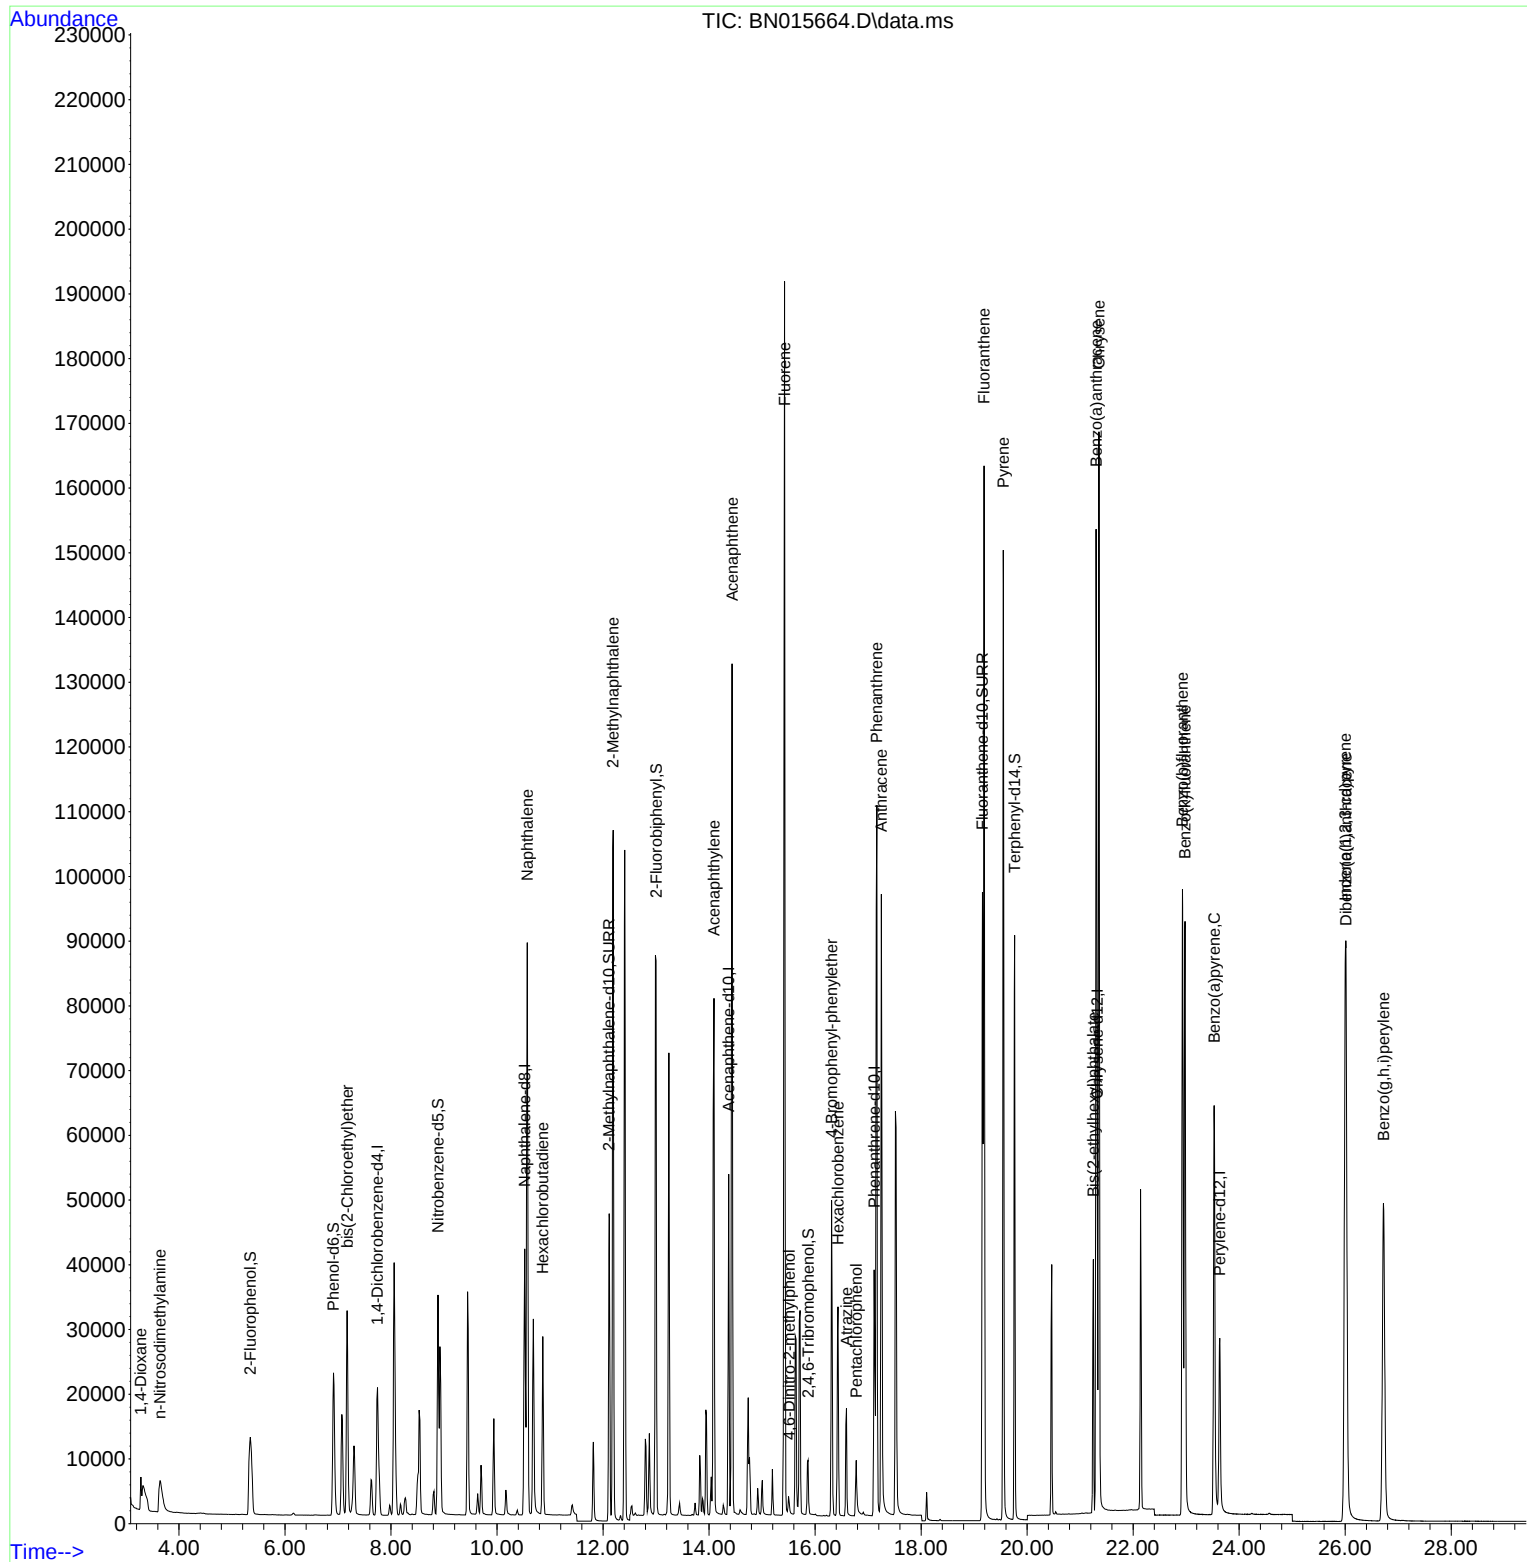







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.744 min Scan# 506
 Delta R.T. -0.000 min
 Lab File: BN015664.D
 Acq: 23 Jul 2021 11:24

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion: 152 Resp: 12636




Ion	Ratio	Lower	Upper
152	100		
150	155.7	123.4	185.0
115	59.0	47.2	70.8

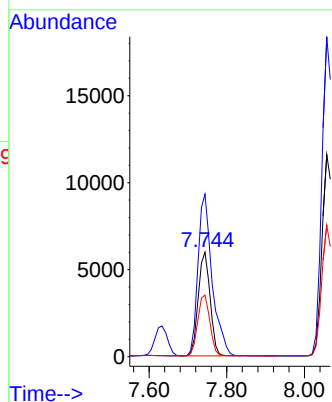


#2
 1,4-Dioxane
 Concen: 0.774 ng
 RT: 3.281 min Scan# 22
 Delta R.T. -0.000 min
 Lab File: BN015664.D
 Acq: 23 Jul 2021 11:24

Tgt Ion: 88 Resp: 3303

Ion	Ratio	Lower	Upper
88	100		
43	28.2	23.5	35.3
58	78.7	64.2	96.4






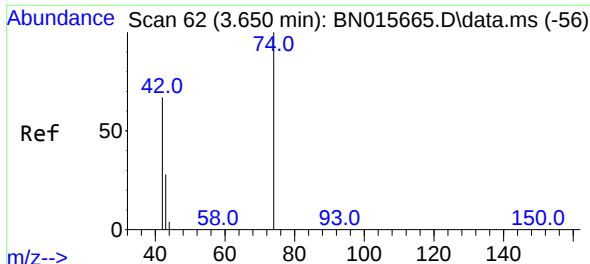


#3
n-Nitrosodimethylamine
Concen: 0.730 ng
RT: 3.641 min Scan# 61
Delta R.T. -0.009 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion: 42 Resp: 7624




Ion	Ratio	Lower	Upper
42	100		
74	149.8	121.0	181.6
44	7.9	6.2	9.4

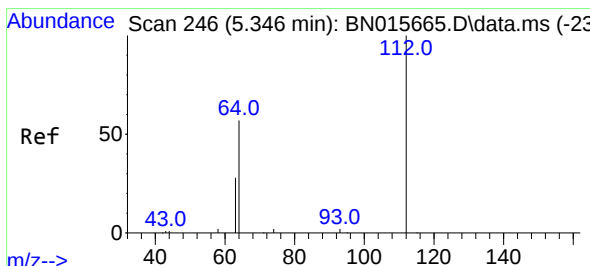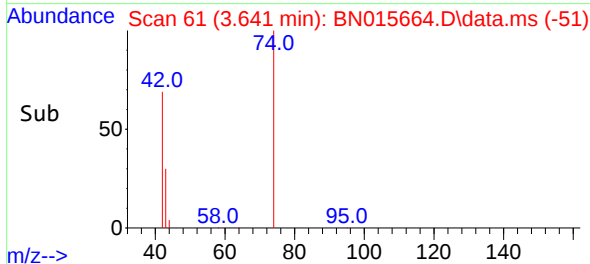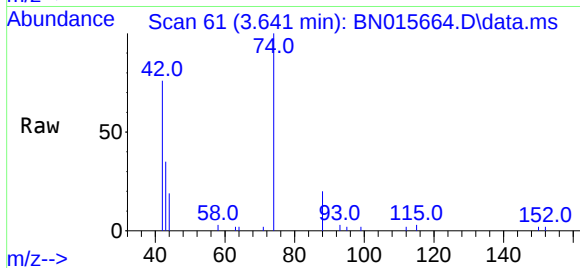


#4
2-Fluorophenol
Concen: 0.669 ng
RT: 5.346 min Scan# 246
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion: 112 Resp: 24343

Ion	Ratio	Lower	Upper
112	100		
64	56.3	44.9	67.3
63	28.2	22.6	33.8

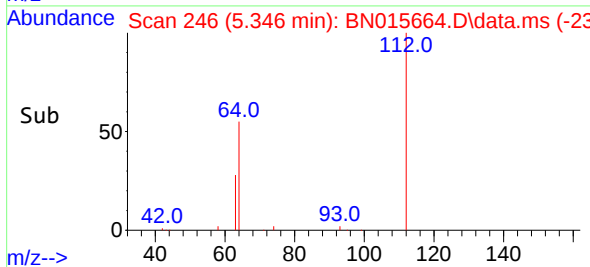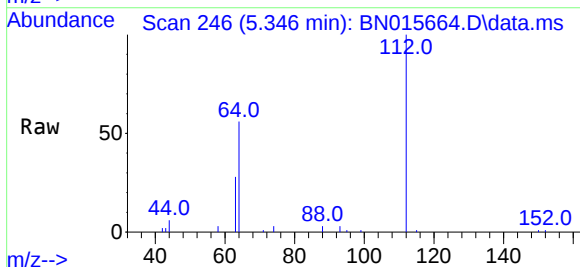







#5
Phenol-d6
Concen: 0.665 ng
RT: 6.914 min Scan# 416
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion: 99 Resp: 28802




Ion	Ratio	Lower	Upper
99	100		
42	16.8	13.8	20.6
71	30.3	24.2	36.2

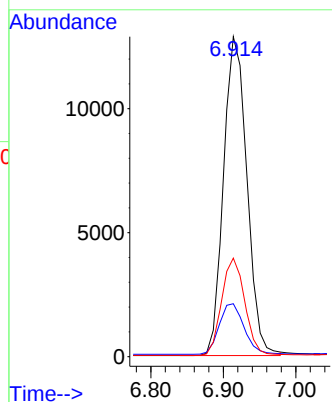


#6
bis(2-Chloroethyl)ether
Concen: 0.758 ng
RT: 7.172 min Scan# 444
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion: 93 Resp: 29503

Ion	Ratio	Lower	Upper
93	100		
63	75.3	59.9	89.9
95	32.8	26.3	39.5









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.521 min Scan# 742
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	136	Resp:	54268
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.7	13.1
54	6.5	5.2	7.8
68	5.6	4.4	6.6



#8
Nitrobenzene-d5
Concen: 0.727 ng
RT: 8.886 min Scan# 613
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:	82	Resp:	28359
Ion	Ratio	Lower	Upper
82	100		
128	39.7	31.2	46.8
54	48.1	40.2	60.4









#9
Naphthalene
Concen: 0.748 ng
RT: 10.571 min Scan# 746
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:128 Resp: 116044
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 12.8 10.2 15.4

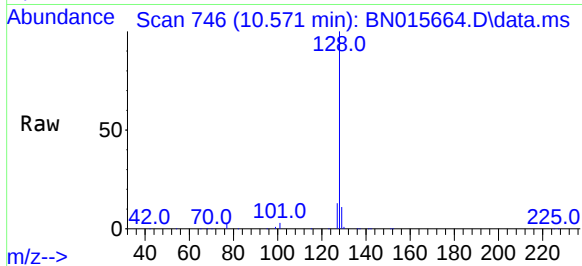

#10
Hexachlorobutadiene
Concen: 0.761 ng
RT: 10.863 min Scan# 769
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:225 Resp: 22132
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 50.6 76.0




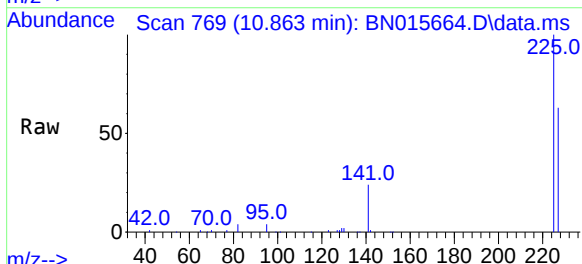


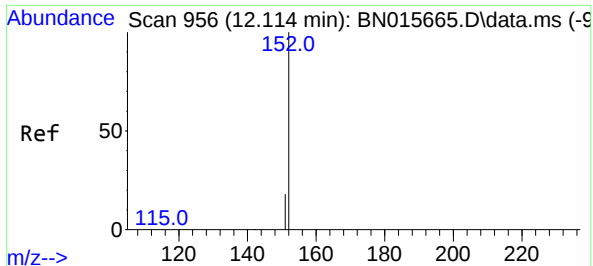

#11
2-Methylnaphthalene-d10
Concen: 0.724 ng
RT: 12.114 min Scan# 956
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 65305
Ion Ratio Lower Upper
152 100
151 20.4 16.4 24.6

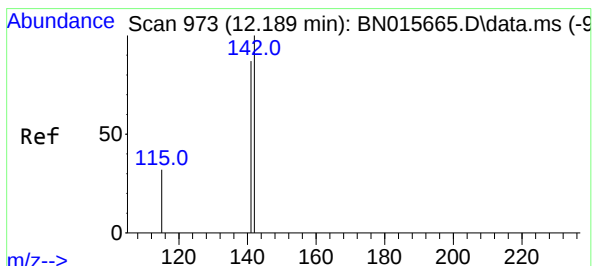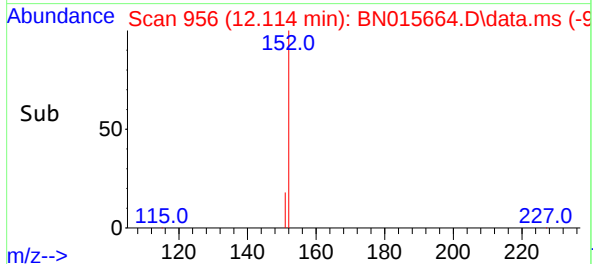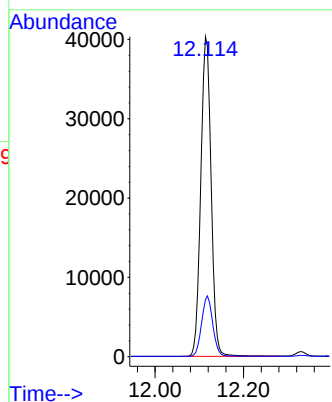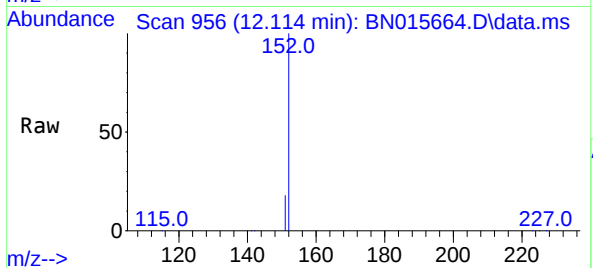

#12
2-Methylnaphthalene
Concen: 0.754 ng
RT: 12.189 min Scan# 973
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:142 Resp: 75980
Ion Ratio Lower Upper
142 100
141 87.3 69.5 104.3
115 32.3 26.1 39.1


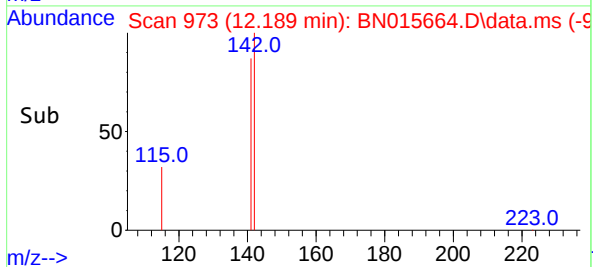

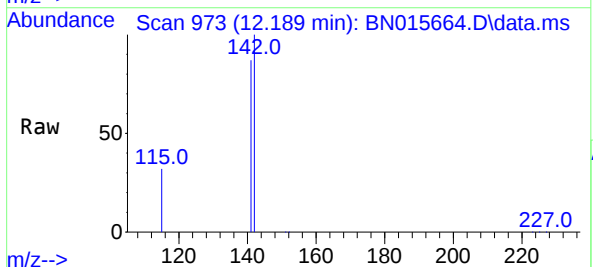




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.370 min Scan# 1191
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:164 Resp: 27929
Ion Ratio Lower Upper
164 100
162 101.3 80.6 120.8
160 45.8 37.0 55.4

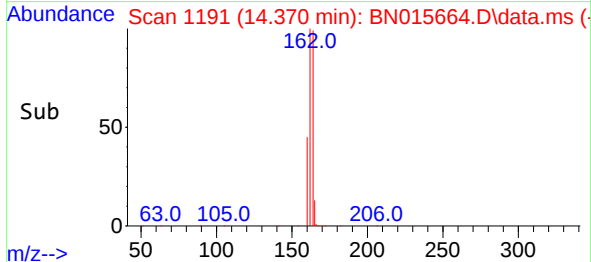

#14
2,4,6-Tribromophenol
Concen: 0.591 ng
RT: 15.867 min Scan# 1309
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:330 Resp: 7418
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.0 28.7 43.1


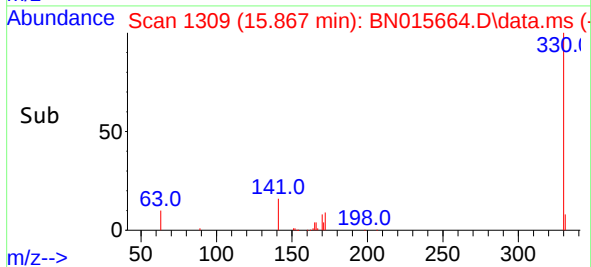

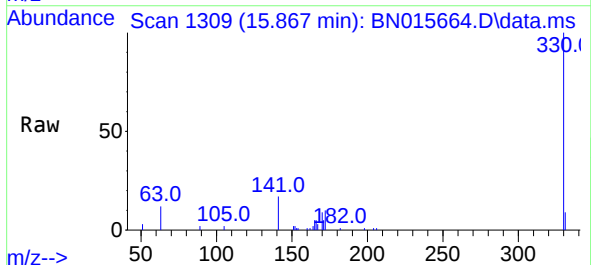




#15
2-Fluorobiphenyl
Concen: 0.800 ng
RT: 13.000 min Scan# 1083
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:172 Resp: 88892
Ion Ratio Lower Upper
172 100
171 33.1 26.6 40.0
170 21.4 17.2 25.8

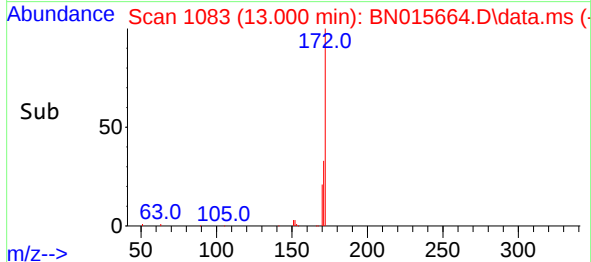

#16
Acenaphthylene
Concen: 0.733 ng
RT: 14.091 min Scan# 1169
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:152 Resp: 94396
Ion Ratio Lower Upper
152 100
151 19.2 15.4 23.2
153 13.1 10.3 15.5


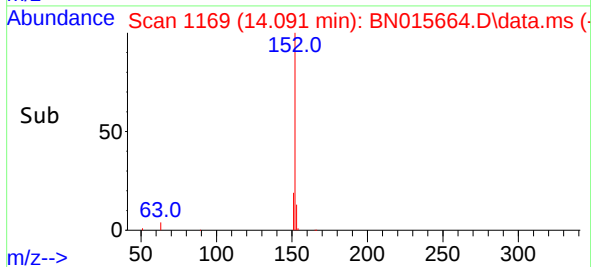

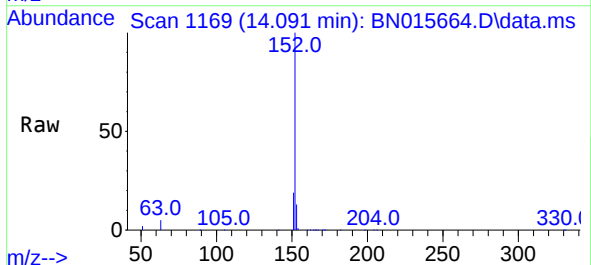




#17
Acenaphthene
Concen: 0.737 ng
RT: 14.434 min Scan# 1196
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:154 Resp: 64515
Ion Ratio Lower Upper
154 100
153 113.1 90.6 136.0
152 55.1 44.6 67.0



#18
Fluorene
Concen: 0.741 ng
RT: 15.423 min Scan# 1274
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:166 Resp: 78499
Ion Ratio Lower Upper
166 100
165 98.0 78.3 117.5
167 13.5 10.8 16.2









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.115 min Scan# 1411
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:188 Resp: 50488
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.8 9.2 13.8



#20
4,6-Dinitro-2-methylphenol
Concen: 0.505 ng
RT: 15.512 min Scan# 1281
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:198 Resp: 2099
Ion Ratio Lower Upper
198 100
182 14.3 17.2 25.8#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.760 ng
RT: 16.312 min Scan# 1345
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	248	Resp:	24010
Ion	Ratio	Lower	Upper
248	100		
250	91.0	72.9	109.3
141	72.7	59.1	88.7



#22
Hexachlorobenzene
Concen: 0.791 ng
RT: 16.433 min Scan# 1355
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:	284	Resp:	27653
Ion	Ratio	Lower	Upper
284	100		
142	34.2	27.5	41.3
249	30.9	25.0	37.6









#23
Atrazine
Concen: 0.640 ng
RT: 16.592 min Scan# 1368
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	200	Resp:	14795
Ion Ratio	Lower	Upper	
200	100		
173	22.1	17.8	26.8
215	49.8	39.8	59.8

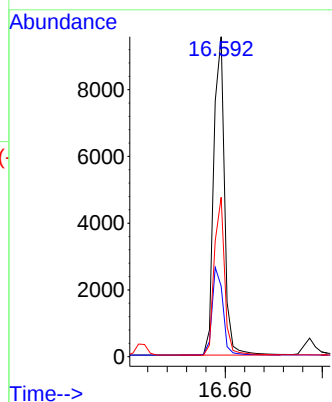

#24
Pentachlorophenol
Concen: 0.571 ng
RT: 16.774 min Scan# 1383
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:	266	Resp:	5013
Ion Ratio	Lower	Upper	
266	100		
264	62.4	51.0	76.4
268	63.7	51.8	77.8









#25
Phenanthrene
Concen: 0.760 ng
RT: 17.164 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:178 Resp: 124156
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.6
179 15.3 12.4 18.6

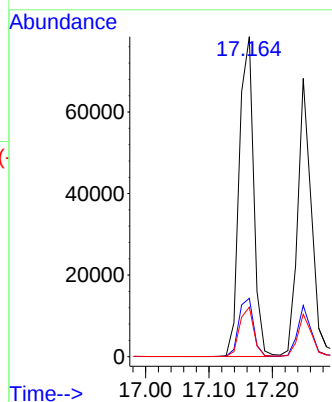

#26
Anthracene
Concen: 0.737 ng
RT: 17.249 min Scan# 1422
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:178 Resp: 103086
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.3 12.2 18.2



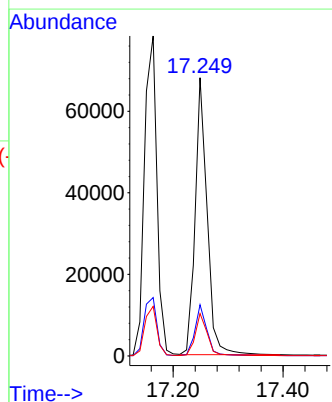





#27
Fluoranthene-d10
Concen: 0.703 ng
RT: 19.157 min Scan# 1715
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:212 Resp: 108916
Ion Ratio Lower Upper
212 100
106 14.4 11.5 17.3
104 7.8 6.2 9.4

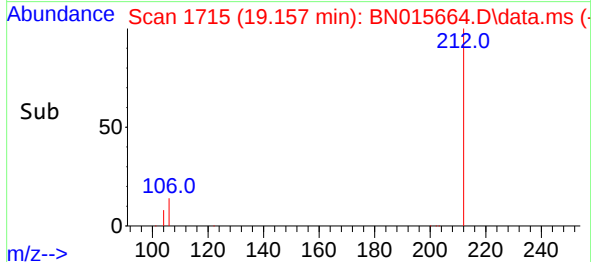

#28
Fluoranthene
Concen: 0.775 ng
RT: 19.187 min Scan# 1721
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:202 Resp: 139125
Ion Ratio Lower Upper
202 100
101 11.8 9.5 14.3
203 17.3 13.8 20.6









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.323 min Scan# 2010
Delta R.T. 0.011 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:240 Resp: 46876
Ion Ratio Lower Upper
240 100
120 6.4 12.2 18.4#
236 25.3 21.5 32.3



#30
Pyrene
Concen: 0.761 ng
RT: 19.549 min Scan# 1794
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:202 Resp: 134563
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.4 13.9 20.9









#31
Terphenyl-d14
Concen: 0.801 ng
RT: 19.763 min Scan# 1837
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:244 Resp: 87264
Ion Ratio Lower Upper
244 100
212 7.6 6.1 9.1
122 12.9 10.1 15.1



#32
Benzo(a)anthracene
Concen: 0.701 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:228 Resp: 118110
Ion Ratio Lower Upper
228 100
226 27.0 21.4 32.0
229 19.2 15.5 23.3

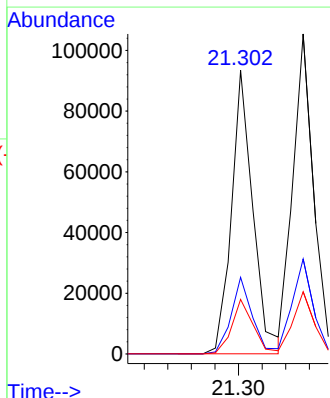







#33
Chrysene
Concen: 0.751 ng
RT: 21.355 min Scan# 2013
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion:228 Resp: 129435




Ion	Ratio	Lower	Upper
228	100		
226	29.7	23.5	35.3
229	19.4	15.6	23.4




#34
Bis(2-ethylhexyl)phthalate
Concen: 0.466 ng
RT: 21.249 min Scan# 2003
Delta R.T. 0.011 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:149 Resp: 37241


Ion	Ratio	Lower	Upper
149	100		
167	27.7	22.2	33.4
279	3.5	2.8	4.2

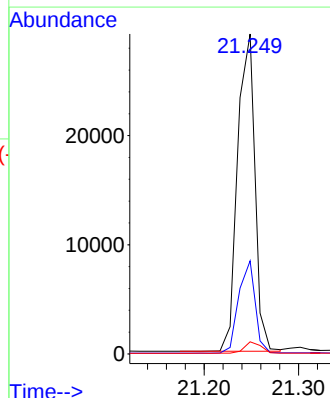






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.632 min Scan# 2470
Delta R.T. 0.003 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8







Tgt Ion:264 Resp: 38235
Ion Ratio Lower Upper
264 100
260 24.8 19.8 29.8
265 25.3 20.0 30.0

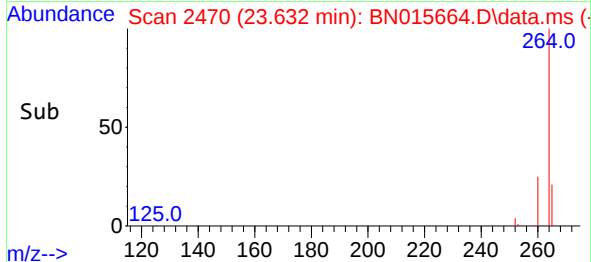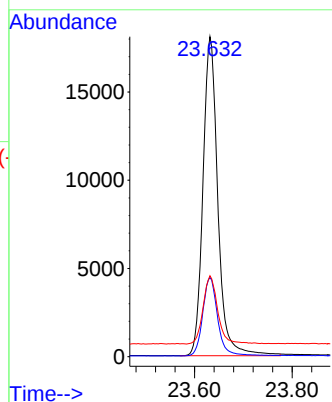

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.711 ng
RT: 26.000 min Scan# 3162
Delta R.T. 0.003 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:276 Resp: 111944
Ion Ratio Lower Upper
276 100
138 27.3 21.8 32.6
277 25.0 19.9 29.9




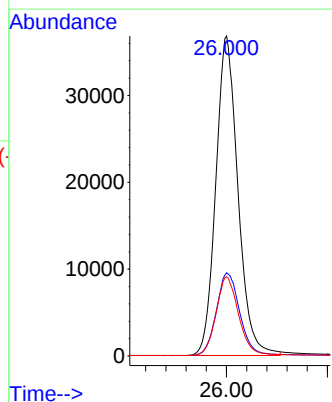




#37
Benzo(b)fluoranthene
Concen: 0.817 ng
RT: 22.930 min Scan# 2265
Delta R.T. -0.000 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:252 Resp: 120369
Ion Ratio Lower Upper
252 100
253 21.9 17.6 26.4
125 10.8 8.8 13.2

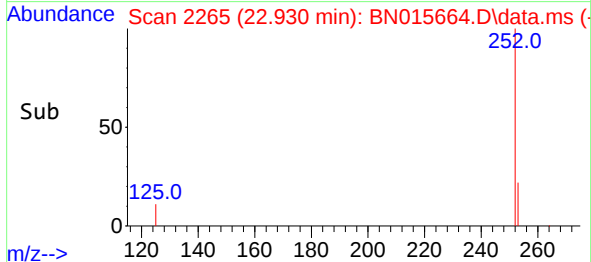

#38
Benzo(k)fluoranthene
Concen: 0.803 ng
RT: 22.978 min Scan# 2279
Delta R.T. 0.003 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:252 Resp: 121363
Ion Ratio Lower Upper
252 100
253 21.8 17.5 26.3
125 10.8 8.8 13.2


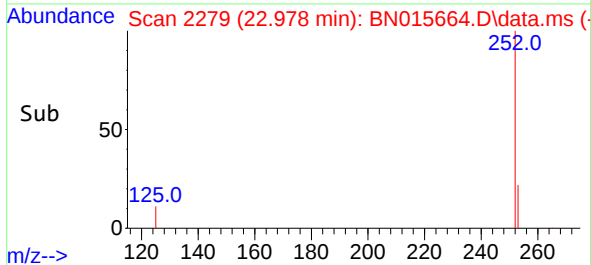

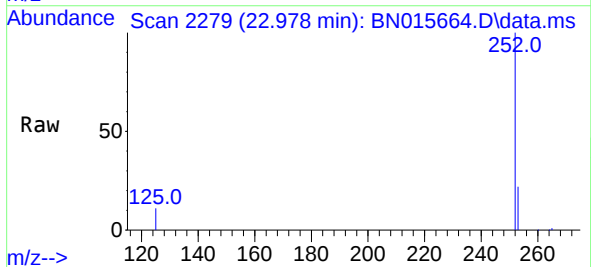




#39
Benzo(a)pyrene
Concen: 0.742 ng
RT: 23.529 min Scan# 2440
Delta R.T. 0.003 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:252	Resp:	95855
Ion Ratio	Lower	Upper
252	100	
253	21.8	18.0 27.0
125	12.0	10.4 15.6

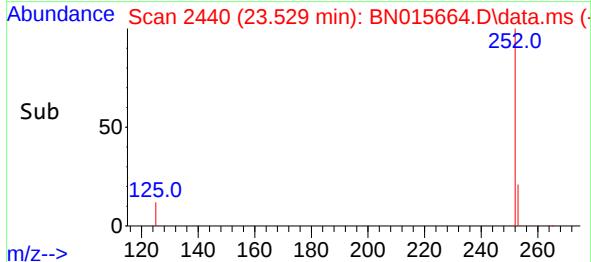

#40
Dibenzo(a,h)anthracene
Concen: 0.710 ng
RT: 26.017 min Scan# 3167
Delta R.T. 0.003 min
Lab File: BN015664.D
Acq: 23 Jul 2021 11:24

Tgt Ion:278	Resp:	88975
Ion Ratio	Lower	Upper
278	100	
139	18.0	14.6 22.0
279	23.6	19.3 28.9



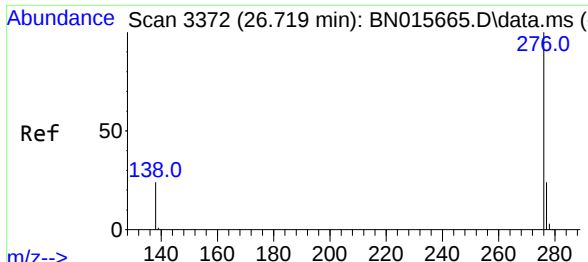

#41
 Benzo(g,h,i)perylene
 Concen: 0.766 ng
 RT: 26.722 min Scan# 3373
 Delta R.T. 0.003 min
 Lab File: BN015664.D
 Acq: 23 Jul 2021 11:24

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Tgt Ion:	276	Resp:	103705
Ion	Ratio	Lower	Upper
276	100		
277	23.4	19.1	28.7
138	23.3	19.1	28.7

