

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
 Data File : BN015666.D
 Acq On : 23 Jul 2021 12:37
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Jul 23 13:07:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 23 12:32:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.744	152	13004	0.400	ng	0.00
7) Naphthalene-d8	10.521	136	54881	0.400	ng	0.00
13) Acenaphthene-d10	14.370	164	28745	0.400	ng	0.00
19) Phenanthrene-d10	17.115	188	53213	0.400	ng	0.00
29) Chrysene-d12	21.323	240	51933	0.400	ng	# 0.01
35) Perylene-d12	23.628	264	43157	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.347	112	52311	1.396	ng	0.00
5) Phenol-d6	6.914	99	63330	1.420	ng	0.00
8) Nitrobenzene-d5	8.886	82	64351	1.632	ng	0.00
11) 2-Methylnaphthalene-d10	12.114	152	136112	1.491	ng	0.00
14) 2,4,6-Tribromophenol	15.868	330	18743	1.452	ng	0.00
15) 2-Fluorobiphenyl	13.000	172	183884	1.609	ng	0.00
27) Fluoranthene-d10	19.157	212	245908	1.505	ng	0.00
31) Terphenyl-d14	19.763	244	193453	1.603	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.281	88	6480	1.476	ng	98
3) n-Nitrosodimethylamine	3.641	42	16727	1.556	ng	100
6) bis(2-Chloroethyl)ether	7.172	93	61237	1.528	ng	100
9) Naphthalene	10.572	128	238603	1.520	ng	100
10) Hexachlorobutadiene	10.863	225	45025	1.530	ng	# 99
12) 2-Methylnaphthalene	12.190	142	156389	1.534	ng	100
16) Acenaphthylene	14.091	152	214028	1.614	ng	100
17) Acenaphthene	14.434	154	138221	1.535	ng	98
18) Fluorene	15.423	166	170129	1.560	ng	99
20) 4,6-Dinitro-2-methylph...	15.512	198	7055	1.611	ng	# 76
21) 4-Bromophenyl-phenylether	16.312	248	53064	1.593	ng	97
22) Hexachlorobenzene	16.434	284	57956	1.573	ng	100
23) Atrazine	16.592	200	37534	1.540	ng	99
24) Pentachlorophenol	16.774	266	14436	1.560	ng	99
25) Phenanthrene	17.164	178	267899	1.556	ng	100
26) Anthracene	17.249	178	238164	1.617	ng	100
28) Fluoranthene	19.187	202	304174	1.607	ng	100
30) Pyrene	19.550	202	300736	1.535	ng	100
32) Benzo(a)anthracene	21.302	228	281904	1.511	ng	100
33) Chrysene	21.355	228	296791	1.554	ng	100
34) Bis(2-ethylhexyl)phtha...	21.249	149	108550	1.225	ng	100
36) Indeno(1,2,3-cd)pyrene	25.997	276	271897	1.530	ng	100
37) Benzo(b)fluoranthene	22.930	252	282564	1.699	ng	100
38) Benzo(k)fluoranthene	22.975	252	274946	1.612	ng	99
39) Benzo(a)pyrene	23.526	252	234091	1.605	ng	98
40) Dibenzo(a,h)anthracene	26.014	278	217770	1.539	ng	99
41) Benzo(g,h,i)perylene	26.723	276	242922	1.590	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015666.D
Acq On : 23 Jul 2021 12:37
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Jul 23 13:07:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 23 12:32:24 2021
Response via : Initial Calibration

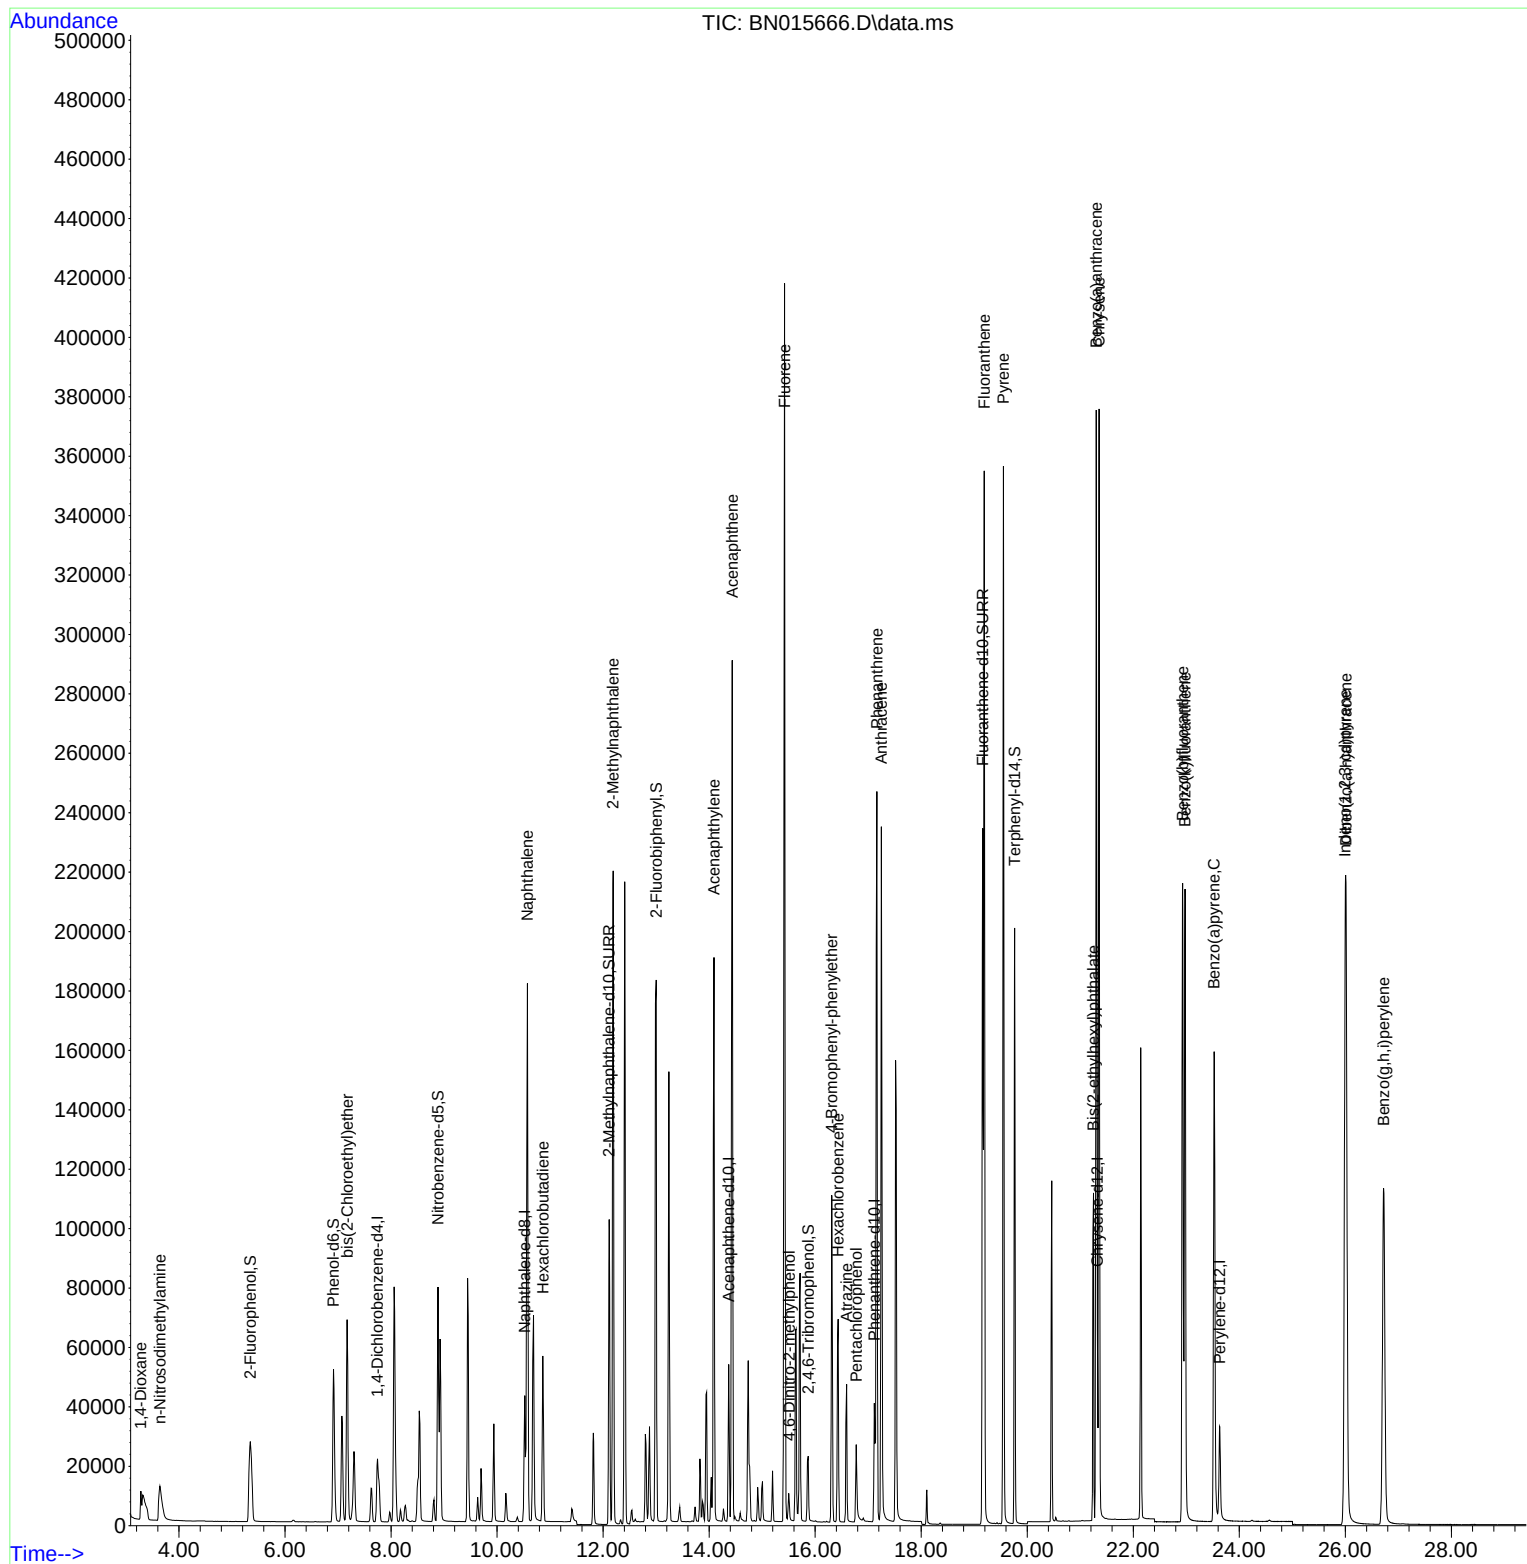







#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.744 min Scan# 506
 Delta R.T. -0.000 min
 Lab File: BN015666.D
 Acq: 23 Jul 2021 12:37

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:152 Resp: 13004




Ion	Ratio	Lower	Upper
152	100		
150	155.3	123.4	185.0
115	58.5	47.2	70.8

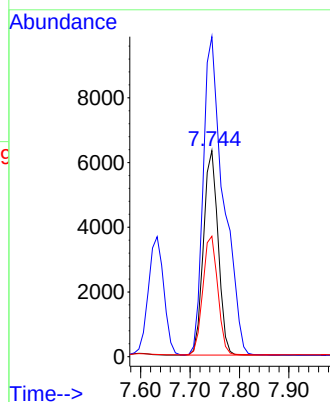


#2
 1,4-Dioxane
 Concen: 1.476 ng
 RT: 3.281 min Scan# 22
 Delta R.T. 0.000 min
 Lab File: BN015666.D
 Acq: 23 Jul 2021 12:37

Tgt Ion: 88 Resp: 6480

Ion	Ratio	Lower	Upper
88	100		
43	28.3	23.5	35.3
58	78.0	64.2	96.4



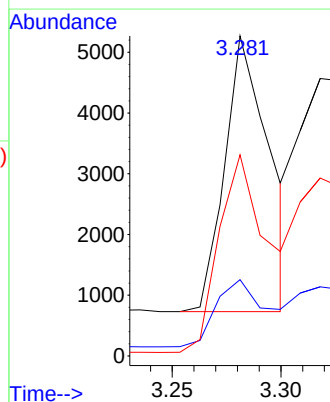





#3
n-Nitrosodimethylamine
Concen: 1.556 ng
RT: 3.641 min Scan# 61
Delta R.T. -0.009 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 16727
Ion Ratio Lower Upper
42 100
74 151.2 121.0 181.6
44 7.5 6.2 9.4



#4
2-Fluorophenol
Concen: 1.396 ng
RT: 5.347 min Scan# 246
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion: 112 Resp: 52311
Ion Ratio Lower Upper
112 100
64 56.2 44.9 67.3
63 28.0 22.6 33.8









#5
Phenol-d6
Concen: 1.420 ng
RT: 6.914 min Scan# 416
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 63330
Ion Ratio Lower Upper
99 100
42 16.8 13.8 20.6
71 30.0 24.2 36.2



#6
bis(2-Chloroethyl)ether
Concen: 1.528 ng
RT: 7.172 min Scan# 444
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion: 93 Resp: 61237
Ion Ratio Lower Upper
93 100
63 74.7 59.9 89.9
95 32.8 26.3 39.5









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.521 min Scan# 742
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	54881
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.7	13.1
54	6.6	5.2	7.8
68	5.6	4.4	6.6



#8
Nitrobenzene-d5
Concen: 1.632 ng
RT: 8.886 min Scan# 613
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:	82	Resp:	64351
Ion	Ratio	Lower	Upper
82	100		
128	41.3	31.2	46.8
54	47.2	40.2	60.4



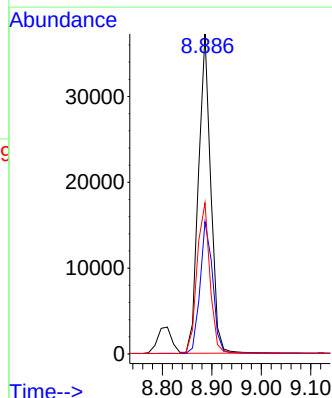





#9
Naphthalene
Concen: 1.520 ng
RT: 10.572 min Scan# 746
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:128 Resp: 238603
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 12.7 10.2 15.4

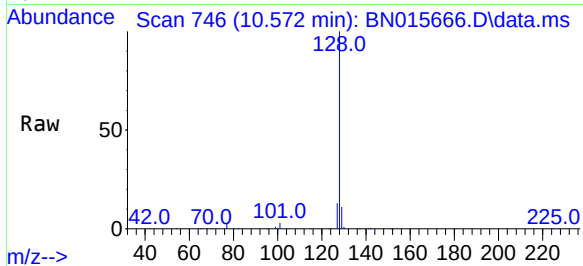

#10
Hexachlorobutadiene
Concen: 1.530 ng
RT: 10.863 min Scan# 769
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:225 Resp: 45025
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 50.6 76.0




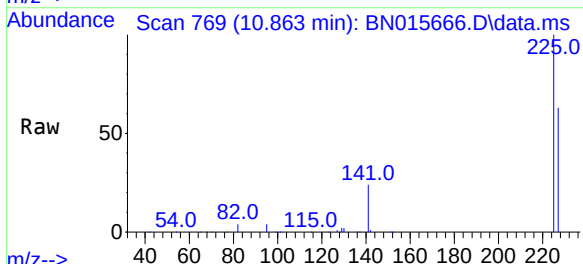


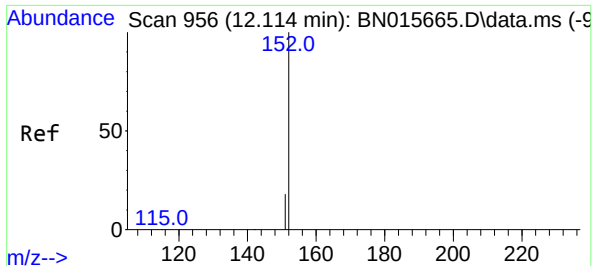

#11
2-Methylnaphthalene-d10
Concen: 1.491 ng
RT: 12.114 min Scan# 956
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 136112
Ion Ratio Lower Upper
152 100
151 20.4 16.4 24.6

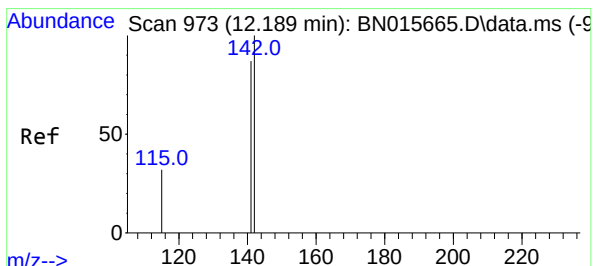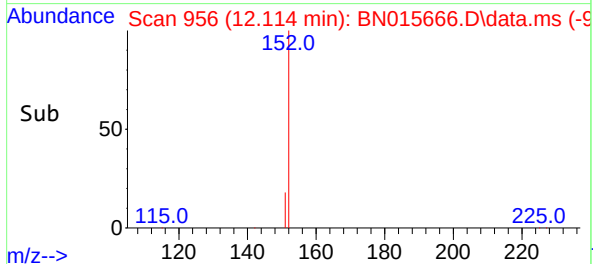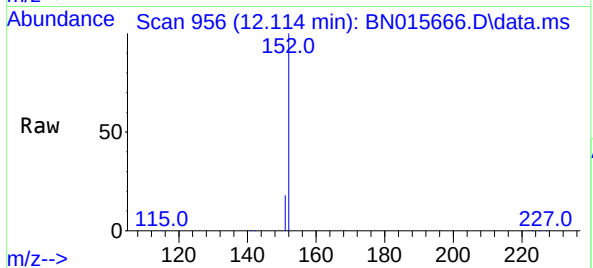

#12
2-Methylnaphthalene
Concen: 1.534 ng
RT: 12.190 min Scan# 973
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:142 Resp: 156389
Ion Ratio Lower Upper
142 100
141 86.7 69.5 104.3
115 32.6 26.1 39.1


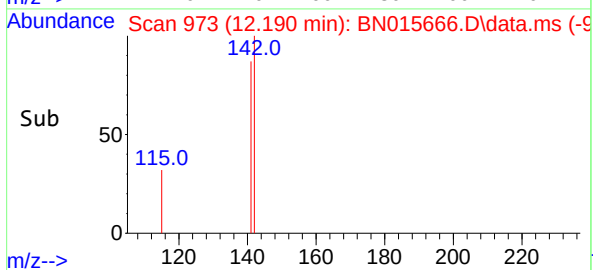

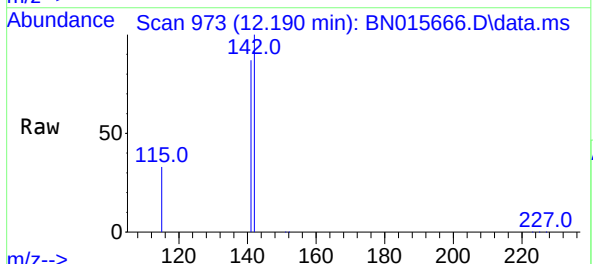




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.370 min Scan# 1191
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 28745
Ion Ratio Lower Upper
164 100
162 102.6 80.6 120.8
160 46.1 37.0 55.4

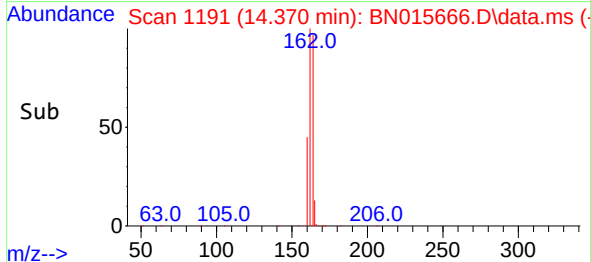

#14
2,4,6-Tribromophenol
Concen: 1.452 ng
RT: 15.868 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:330 Resp: 18743
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.8 28.7 43.1


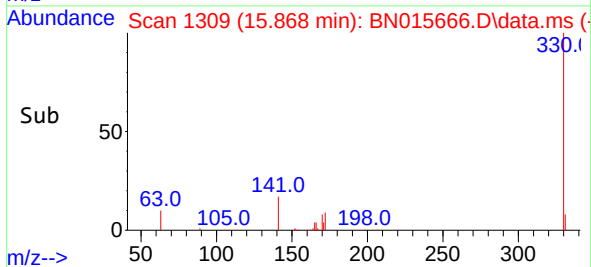

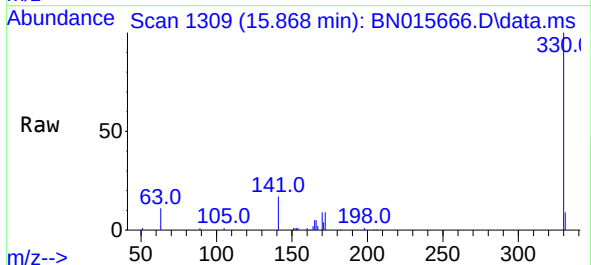




#15
2-Fluorobiphenyl
Concen: 1.609 ng
RT: 13.000 min Scan# 1083
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 183884
Ion Ratio Lower Upper
172 100
171 33.5 26.6 40.0
170 21.6 17.2 25.8

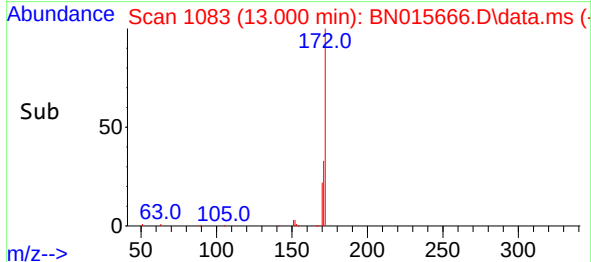

#16
Acenaphthylene
Concen: 1.614 ng
RT: 14.091 min Scan# 1169
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:152 Resp: 214028
Ion Ratio Lower Upper
152 100
151 19.2 15.4 23.2
153 13.1 10.3 15.5


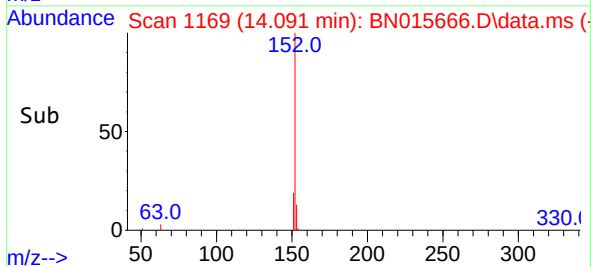

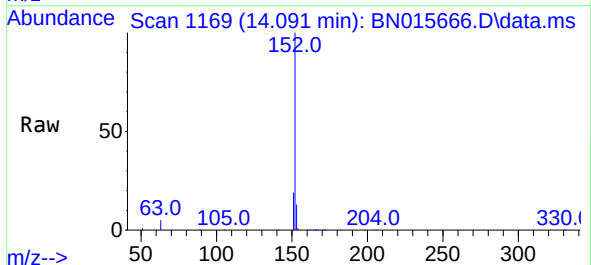




#17
Acenaphthene
Concen: 1.535 ng
RT: 14.434 min Scan# 1196
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 138221
Ion Ratio Lower Upper
154 100
153 112.0 90.6 136.0
152 54.3 44.6 67.0

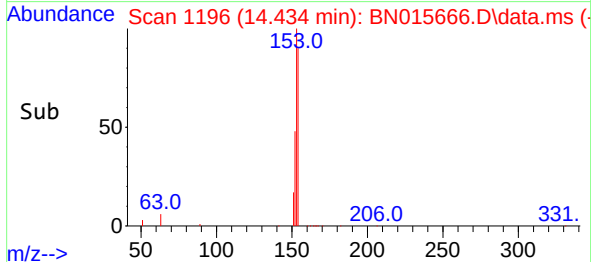

#18
Fluorene
Concen: 1.560 ng
RT: 15.423 min Scan# 1274
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:166 Resp: 170129
Ion Ratio Lower Upper
166 100
165 97.1 78.3 117.5
167 13.4 10.8 16.2


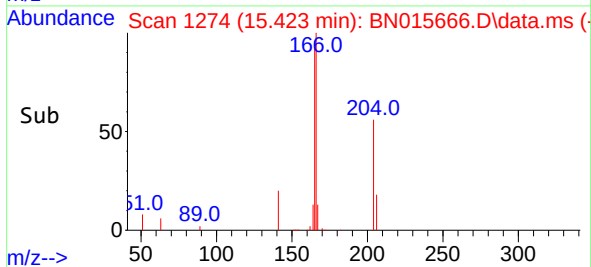

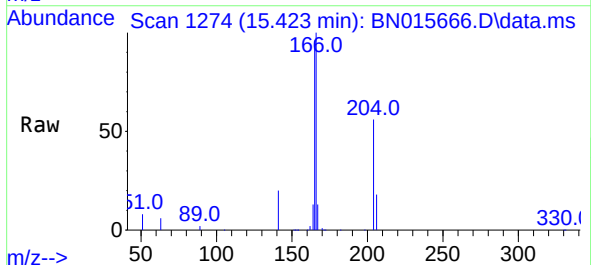




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.115 min Scan# 1411
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 53213
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.1 9.2 13.8



#20
4,6-Dinitro-2-methylphenol
Concen: 1.611 ng
RT: 15.512 min Scan# 1281
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:198 Resp: 7055
Ion Ratio Lower Upper
198 100
182 10.0 17.2 25.8#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 1.593 ng
RT: 16.312 min Scan# 1345
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:248 Resp: 53064




Ion	Ratio	Lower	Upper
248	100		
250	91.1	72.9	109.3
141	68.8	59.1	88.7

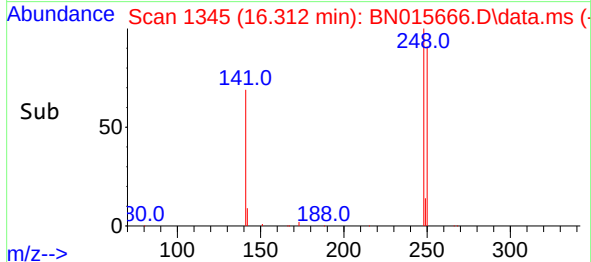


#22
Hexachlorobenzene
Concen: 1.573 ng
RT: 16.434 min Scan# 1355
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:284 Resp: 57956

Ion	Ratio	Lower	Upper
284	100		
142	34.4	27.5	41.3
249	31.3	25.0	37.6


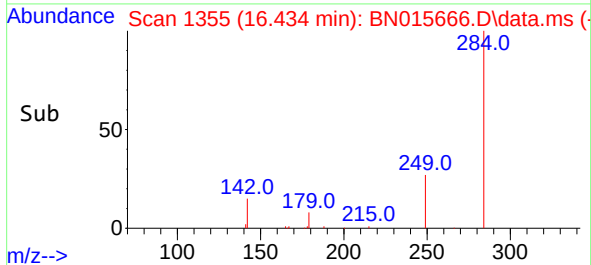

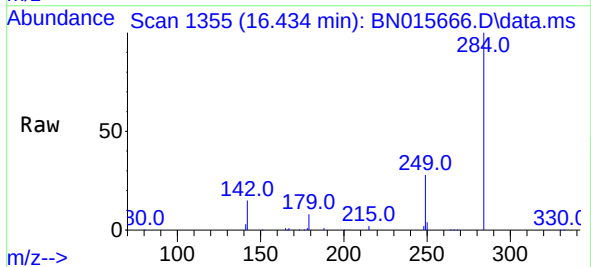




#23
Atrazine
Concen: 1.540 ng
RT: 16.592 min Scan# 1368
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 37534
Ion Ratio Lower Upper
200 100
173 22.4 17.8 26.8
215 48.9 39.8 59.8



#24
Pentachlorophenol
Concen: 1.560 ng
RT: 16.774 min Scan# 1383
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:266 Resp: 14436
Ion Ratio Lower Upper
266 100
264 63.1 51.0 76.4
268 63.9 51.8 77.8









#25
Phenanthrene
Concen: 1.556 ng
RT: 17.164 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 267899
Ion Ratio Lower Upper
178 100
176 18.7 15.0 22.6
179 15.3 12.4 18.6



#26
Anthracene
Concen: 1.617 ng
RT: 17.249 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:178 Resp: 238164
Ion Ratio Lower Upper
178 100
176 18.1 14.6 21.8
179 15.3 12.2 18.2









#27
Fluoranthene-d10
Concen: 1.505 ng
RT: 19.157 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 245908
Ion Ratio Lower Upper
212 100
106 14.5 11.5 17.3
104 7.9 6.2 9.4

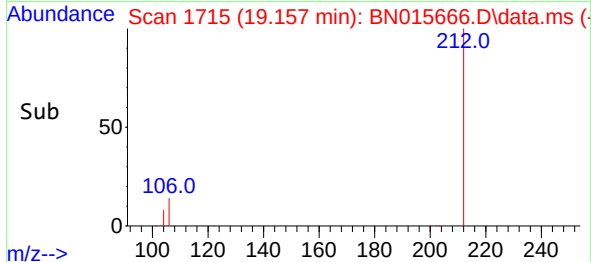

#28
Fluoranthene
Concen: 1.607 ng
RT: 19.187 min Scan# 1721
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:202 Resp: 304174
Ion Ratio Lower Upper
202 100
101 11.9 9.5 14.3
203 17.3 13.8 20.6


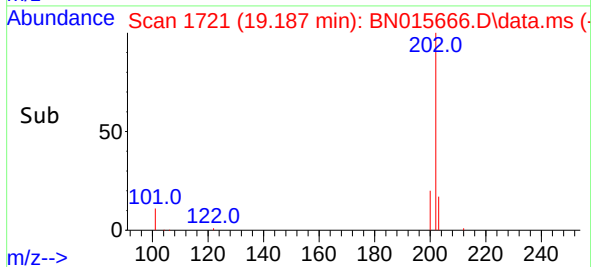

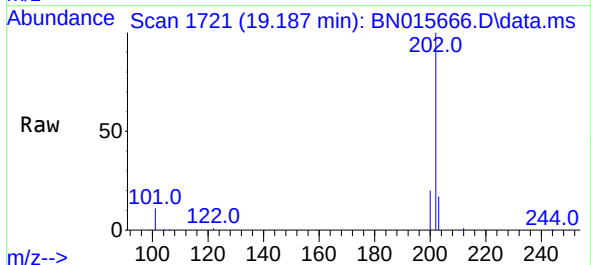




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.323 min Scan# 2010
Delta R.T. 0.011 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:240 Resp: 51933
Ion Ratio Lower Upper
240 100
120 5.8 12.2 18.4#
236 25.2 21.5 32.3

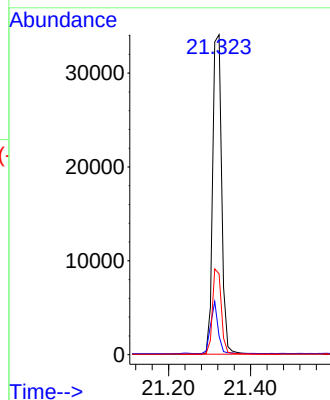

#30
Pyrene
Concen: 1.535 ng
RT: 19.550 min Scan# 1794
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:202 Resp: 300736
Ion Ratio Lower Upper
202 100
200 20.6 16.4 24.6
203 17.4 13.9 20.9



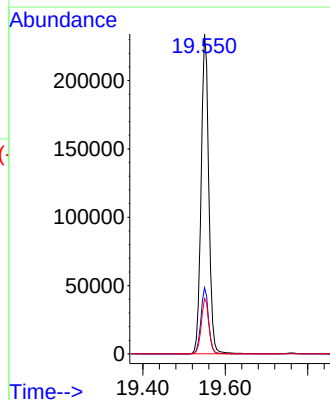



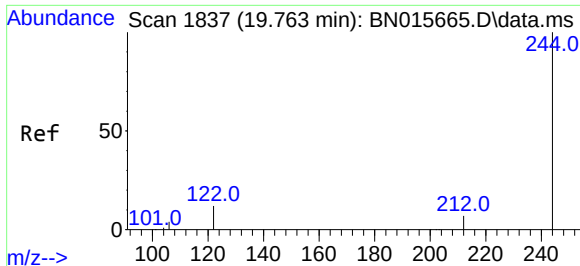

#31
Terphenyl-d14
Concen: 1.603 ng
RT: 19.763 min Scan# 1837
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:244 Resp: 193453
Ion Ratio Lower Upper
244 100
212 7.6 6.1 9.1
122 12.7 10.1 15.1

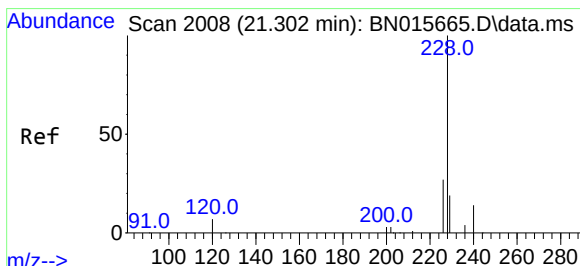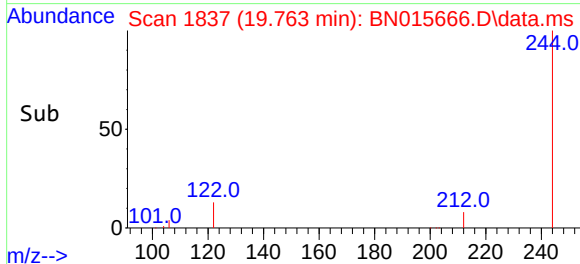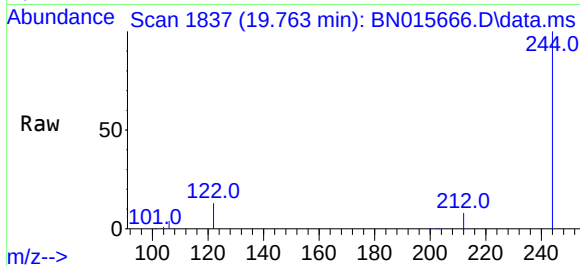

#32
Benzo(a)anthracene
Concen: 1.511 ng
RT: 21.302 min Scan# 2008
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:228 Resp: 281904
Ion Ratio Lower Upper
228 100
226 26.4 21.4 32.0
229 19.6 15.5 23.3


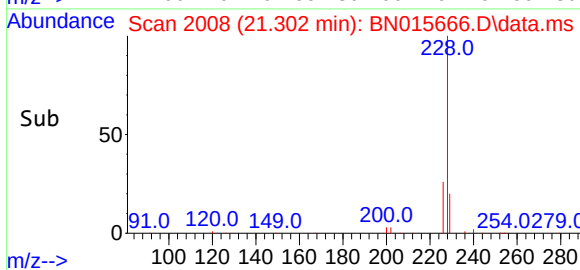

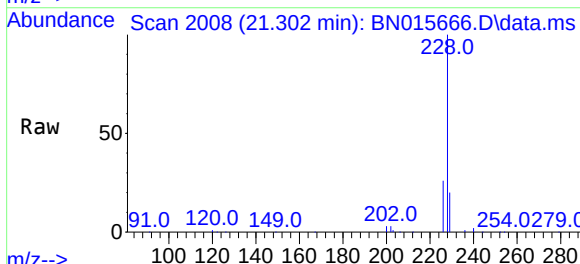


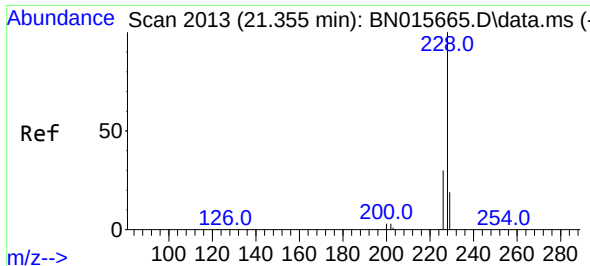

#33
Chrysene
Concen: 1.554 ng
RT: 21.355 min Scan# 2013
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	228	Resp:	296791
Ion	Ratio	Lower	Upper
228	100		
226	29.1	23.5	35.3
229	19.6	15.6	23.4

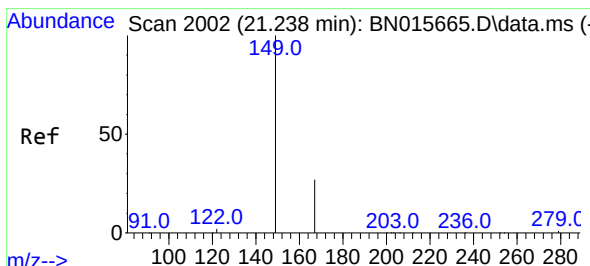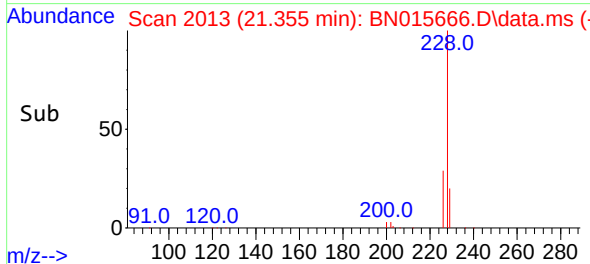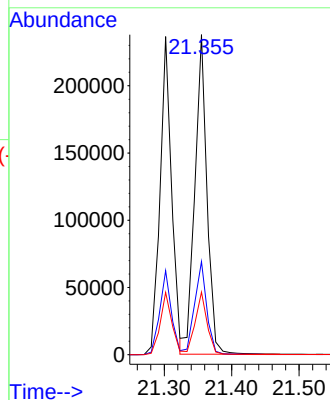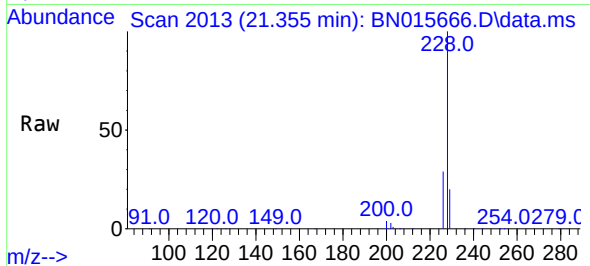

#34
Bis(2-ethylhexyl)phthalate
Concen: 1.225 ng
RT: 21.249 min Scan# 2003
Delta R.T. 0.011 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37


Tgt Ion:	149	Resp:	108550
Ion	Ratio	Lower	Upper
149	100		
167	28.0	22.2	33.4
279	3.6	2.8	4.2

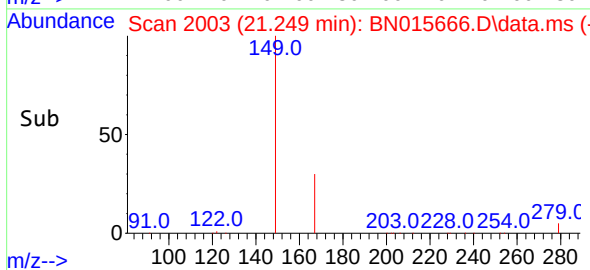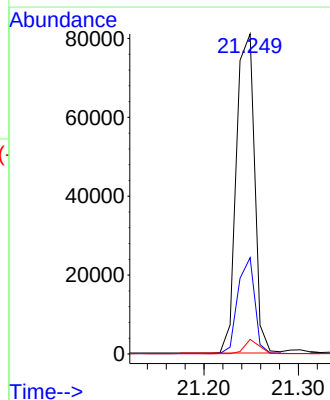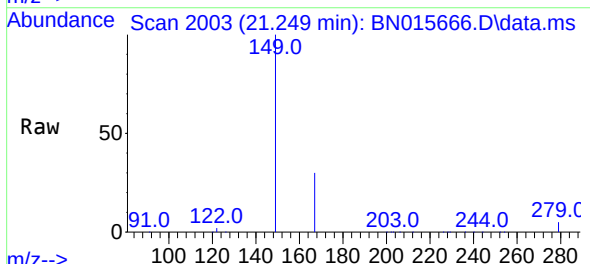






#35
Perylene-d12
Concen: 0.400 ng
RT: 23.628 min Scan# 2469
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6



Tgt Ion:264 Resp: 43157




Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.8	29.8
265	24.3	20.0	30.0

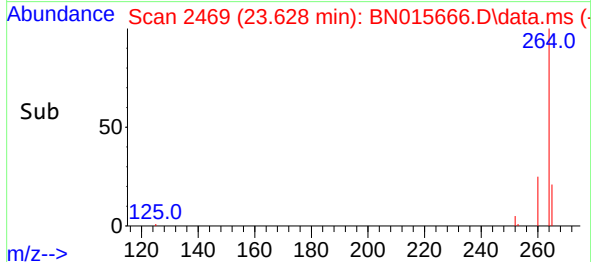


#36
Indeno(1,2,3-cd)pyrene
Concen: 1.530 ng
RT: 25.997 min Scan# 3161
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:276 Resp: 271897

Ion	Ratio	Lower	Upper
276	100		
138	27.4	21.8	32.6
277	25.0	19.9	29.9









#37
Benzo(b)fluoranthene
Concen: 1.699 ng
RT: 22.930 min Scan# 2265
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 282564
Ion Ratio Lower Upper
252 100
253 22.1 17.6 26.4
125 10.8 8.8 13.2



#38
Benzo(k)fluoranthene
Concen: 1.612 ng
RT: 22.975 min Scan# 2278
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:252 Resp: 274946
Ion Ratio Lower Upper
252 100
253 21.5 17.5 26.3
125 10.8 8.8 13.2




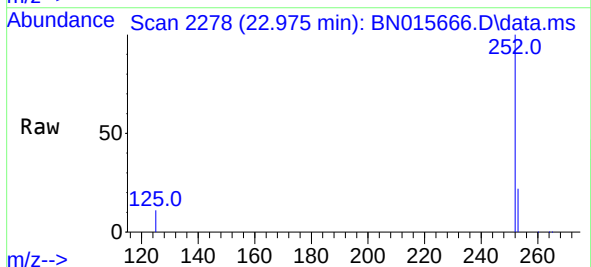




#39
Benzo(a)pyrene
Concen: 1.605 ng
RT: 23.526 min Scan# 2439
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 234091
Ion Ratio Lower Upper
252 100
253 21.6 18.0 27.0
125 12.0 10.4 15.6

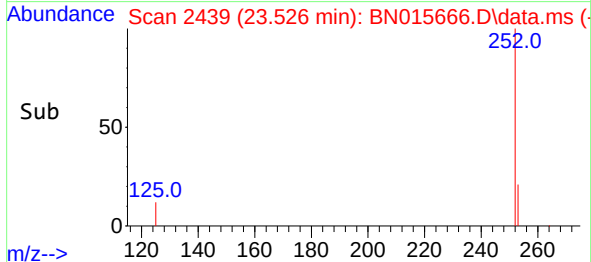

#40
Dibenzo(a,h)anthracene
Concen: 1.539 ng
RT: 26.014 min Scan# 3166
Delta R.T. 0.000 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Tgt Ion:278 Resp: 217770
Ion Ratio Lower Upper
278 100
139 18.2 14.6 22.0
279 23.6 19.3 28.9



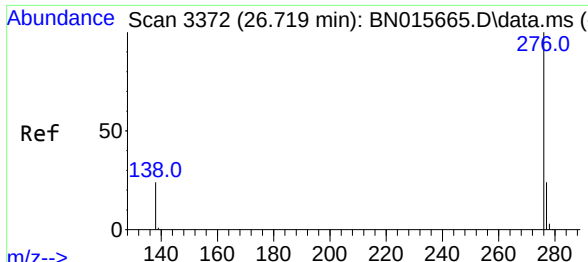

#41
Benzo(g,h,i)perylene
Concen: 1.590 ng
RT: 26.723 min Scan# 3373
Delta R.T. 0.004 min
Lab File: BN015666.D
Acq: 23 Jul 2021 12:37

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Tgt Ion:276 Resp: 242922
Ion Ratio Lower Upper
276 100
277 23.8 19.1 28.7
138 23.5 19.1 28.7

