

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
 Data File : BN015686.D
 Acq On : 24 Jul 2021 12:27
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jul 25 06:59:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 23 14:45:01 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.735	152	13490	0.400	ng	0.00
7) Naphthalene-d8	10.508	136	59834	0.400	ng	#-0.01
13) Acenaphthene-d10	14.358	164	32294	0.400	ng	-0.01
19) Phenanthrene-d10	17.115	188	61354	0.400	ng	# 0.00
29) Chrysene-d12	21.312	240	58567	0.400	ng	# 0.00
35) Perylene-d12	23.618	264	56529	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.337	112	14622	0.450	ng	0.00
5) Phenol-d6	6.905	99	17392	0.457	ng	0.00
8) Nitrobenzene-d5	8.873	82	16949	0.404	ng	-0.01
11) 2-Methylnaphthalene-d10	12.109	152	35508	0.398	ng	0.00
14) 2,4,6-Tribromophenol	15.855	330	5130	0.511	ng	-0.01
15) 2-Fluorobiphenyl	12.987	172	49138	0.373	ng	-0.01
27) Fluoranthene-d10	19.152	212	65926	0.403	ng	0.00
31) Terphenyl-d14	19.758	244	52714	0.378	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.281	88	2185	0.543	ng	# 68
3) n-Nitrosodimethylamine	3.631	42	4119	0.414	ng	# 94
6) bis(2-Chloroethyl)ether	7.163	93	15464	0.404	ng	99
9) Naphthalene	10.559	128	62380	0.393	ng	99
10) Hexachlorobutadiene	10.863	225	11798	0.391	ng	# 99
12) 2-Methylnaphthalene	12.181	142	41236	0.403	ng	98
16) Acenaphthylene	14.078	152	53303	0.395	ng	100
17) Acenaphthene	14.421	154	35881	0.383	ng	99
18) Fluorene	15.411	166	44367	0.397	ng	100
20) 4,6-Dinitro-2-methylph...	15.499	198	1957	0.557	ng	# 86
21) 4-Bromophenyl-phenylether	16.312	248	13747	0.385	ng	# 76
22) Hexachlorobenzene	16.421	284	15433	0.380	ng	100
23) Atrazine	16.579	200	10068	0.474	ng	# 94
24) Pentachlorophenol	16.774	266	4198	0.536	ng	99
25) Phenanthrene	17.151	178	71225	0.385	ng	100
26) Anthracene	17.249	178	61091	0.397	ng	100
28) Fluoranthene	19.182	202	80914	0.405	ng	100
30) Pyrene	19.544	202	80674	0.384	ng	100
32) Benzo(a)anthracene	21.291	228	75166	0.410	ng	99
33) Chrysene	21.344	228	78643	0.387	ng	99
34) Bis(2-ethylhexyl)phtha...	21.238	149	35982	0.601	ng	99
36) Indeno(1,2,3-cd)pyrene	25.983	276	87080	0.425	ng	99
37) Benzo(b)fluoranthene	22.920	252	79987	0.376	ng	100
38) Benzo(k)fluoranthene	22.968	252	79757	0.375	ng	99
39) Benzo(a)pyrene	23.515	252	68538	0.398	ng	100
40) Dibenzo(a,h)anthracene	26.000	278	70069	0.435	ng	100
41) Benzo(g,h,i)perylene	26.702	276	73670	0.393	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015686.D
Acq On : 24 Jul 2021 12:27
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Jul 25 06:59:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 23 14:45:01 2021
Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.735 min Scan# 505
Delta R.T. -0.009 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 13490
Ion Ratio Lower Upper
152 100
150 155.4 123.4 185.0
115 59.1 47.2 70.8



#2
1,4-Dioxane
Concen: 0.543 ng
RT: 3.281 min Scan# 22
Delta R.T. 0.000 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion: 88 Resp: 2185
Ion Ratio Lower Upper
88 100
43 90.2 23.5 35.3#
58 78.7 64.2 96.4









#3
n-Nitrosodimethylamine
Concen: 0.414 ng
RT: 3.631 min Scan# 60
Delta R.T. -0.018 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 4119
Ion Ratio Lower Upper
42 100
74 158.4 121.0 181.6
44 0.0 6.2 9.4#



#4
2-Fluorophenol
Concen: 0.450 ng
RT: 5.337 min Scan# 245
Delta R.T. -0.009 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion: 112 Resp: 14622
Ion Ratio Lower Upper
112 100
64 55.9 44.9 67.3
63 27.7 22.6 33.8









#5
Phenol-d6
Concen: 0.457 ng
RT: 6.905 min Scan# 415
Delta R.T. -0.009 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 17392
Ion Ratio Lower Upper
99 100
42 16.4 13.8 20.6
71 30.4 24.2 36.2



#6
bis(2-Chloroethyl)ether
Concen: 0.404 ng
RT: 7.163 min Scan# 443
Delta R.T. -0.009 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion: 93 Resp: 15464
Ion Ratio Lower Upper
93 100
63 74.2 59.9 89.9
95 32.7 26.3 39.5









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.508 min Scan# 741
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	59834
Ion Ratio	Lower	Upper	
136	100		
137	11.0	8.7	13.1
54	9.1	5.2	7.8#
68	7.5	4.4	6.6#



#8
Nitrobenzene-d5
Concen: 0.404 ng
RT: 8.873 min Scan# 612
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:	82	Resp:	16949
Ion Ratio	Lower	Upper	
82	100		
128	35.0	31.2	46.8
54	52.7	40.2	60.4









#9
Naphthalene
Concen: 0.393 ng
RT: 10.559 min Scan# 745
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128 Resp: 62380
Ion Ratio Lower Upper
128 100
129 11.1 8.8 13.2
127 13.2 10.2 15.4



#10
Hexachlorobutadiene
Concen: 0.391 ng
RT: 10.863 min Scan# 769
Delta R.T. 0.000 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:225 Resp: 11798
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.9 50.6 76.0









#11
2-Methylnaphthalene-d10
Concen: 0.398 ng
RT: 12.109 min Scan# 955
Delta R.T. -0.004 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 35508
Ion Ratio Lower Upper
152 100
151 20.4 16.4 24.6

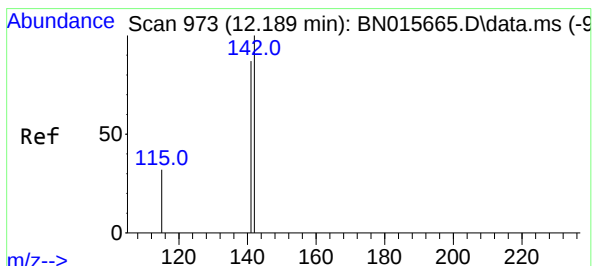

#12
2-Methylnaphthalene
Concen: 0.403 ng
RT: 12.181 min Scan# 971
Delta R.T. -0.009 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:142 Resp: 41236
Ion Ratio Lower Upper
142 100
141 88.5 69.5 104.3
115 33.4 26.1 39.1









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.358 min Scan# 1190
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 32294
Ion Ratio Lower Upper
164 100
162 105.3 80.6 120.8
160 48.5 37.0 55.4



#14
2,4,6-Tribromophenol
Concen: 0.511 ng
RT: 15.855 min Scan# 1308
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:330 Resp: 5130
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.1 28.7 43.1









#15
2-Fluorobiphenyl
Concen: 0.373 ng
RT: 12.987 min Scan# 1082
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	49138
Ion Ratio	Lower	Upper	
172	100		
171	34.3	26.6	40.0
170	22.7	17.2	25.8



#16
Acenaphthylene
Concen: 0.395 ng
RT: 14.078 min Scan# 1168
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:	152	Resp:	53303
Ion Ratio	Lower	Upper	
152	100		
151	19.3	15.4	23.2
153	13.1	10.3	15.5









#17
Acenaphthene
Concen: 0.383 ng
RT: 14.421 min Scan# 1195
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 35881
Ion Ratio Lower Upper
154 100
153 112.4 90.6 136.0
152 54.4 44.6 67.0



#18
Fluorene
Concen: 0.397 ng
RT: 15.411 min Scan# 1273
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:166 Resp: 44367
Ion Ratio Lower Upper
166 100
165 97.8 78.3 117.5
167 13.5 10.8 16.2









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.115 min Scan# 1411
Delta R.T. 0.000 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 61354
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.4 9.2 13.8#



#20
4,6-Dinitro-2-methylphenol
Concen: 0.557 ng
RT: 15.499 min Scan# 1280
Delta R.T. -0.013 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:198 Resp: 1957
Ion Ratio Lower Upper
198 100
182 15.1 17.2 25.8#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.385 ng
RT: 16.312 min Scan# 1345
Delta R.T. 0.000 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 13747
Ion Ratio Lower Upper
248 100
250 101.5 72.9 109.3
141 40.2 59.1 88.7#



#22
Hexachlorobenzene
Concen: 0.380 ng
RT: 16.421 min Scan# 1354
Delta R.T. -0.012 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:284 Resp: 15433
Ion Ratio Lower Upper
284 100
142 34.3 27.5 41.3
249 31.0 25.0 37.6









#23
Atrazine
Concen: 0.474 ng
RT: 16.579 min Scan# 1367
Delta R.T. -0.012 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 10068
Ion Ratio Lower Upper
200 100
173 27.8 17.8 26.8#
215 47.4 39.8 59.8



#24
Pentachlorophenol
Concen: 0.536 ng
RT: 16.774 min Scan# 1383
Delta R.T. 0.000 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:266 Resp: 4198
Ion Ratio Lower Upper
266 100
264 62.9 51.0 76.4
268 63.6 51.8 77.8









#25
Phenanthrene
Concen: 0.385 ng
RT: 17.151 min Scan# 1414
Delta R.T. -0.012 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 71225
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.3 12.4 18.6



#26
Anthracene
Concen: 0.397 ng
RT: 17.249 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:178 Resp: 61091
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.3 12.2 18.2









#27
Fluoranthene-d10
Concen: 0.403 ng
RT: 19.152 min Scan# 1714
Delta R.T. -0.005 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 65926
Ion Ratio Lower Upper
212 100
106 14.1 11.5 17.3
104 7.7 6.2 9.4



#28
Fluoranthene
Concen: 0.405 ng
RT: 19.182 min Scan# 1720
Delta R.T. -0.005 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:202 Resp: 80914
Ion Ratio Lower Upper
202 100
101 11.8 9.5 14.3
203 17.3 13.8 20.6









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.312 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 58567
Ion Ratio Lower Upper
240 100
120 7.7 12.2 18.4#
236 26.1 21.5 32.3



#30
Pyrene
Concen: 0.384 ng
RT: 19.544 min Scan# 1793
Delta R.T. -0.005 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:202 Resp: 80674
Ion Ratio Lower Upper
202 100
200 20.6 16.4 24.6
203 17.5 13.9 20.9









#31
Terphenyl-d14
Concen: 0.378 ng
RT: 19.758 min Scan# 1836
Delta R.T. -0.005 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 52714
Ion Ratio Lower Upper
244 100
212 7.6 6.1 9.1
122 11.9 10.1 15.1



#32
Benzo(a)anthracene
Concen: 0.410 ng
RT: 21.291 min Scan# 2007
Delta R.T. -0.011 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:228 Resp: 75166
Ion Ratio Lower Upper
228 100
226 27.4 21.4 32.0
229 19.1 15.5 23.3









#33
Chrysene
Concen: 0.387 ng
RT: 21.344 min Scan# 2012
Delta R.T. -0.011 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	228	Resp:	78643
Ion Ratio	Lower	Upper	
228	100		
226	30.0	23.5	35.3
229	19.3	15.6	23.4



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.601 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27


Tgt Ion:	149	Resp:	35982
Ion Ratio	Lower	Upper	
149	100		
167	28.2	22.2	33.4
279	3.6	2.8	4.2








#35
Perylene-d12
Concen: 0.400 ng
RT: 23.618 min Scan# 2466
Delta R.T. -0.010 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:264 Resp: 56529
Ion Ratio Lower Upper
264 100
260 24.8 19.8 29.8
265 24.8 20.0 30.0



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.425 ng
RT: 25.983 min Scan# 3157
Delta R.T. -0.014 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27


Tgt Ion:276 Resp: 87080
Ion Ratio Lower Upper
276 100
138 27.9 21.8 32.6
277 25.0 19.9 29.9








#37
Benzo(b)fluoranthene
Concen: 0.376 ng
RT: 22.920 min Scan# 2262
Delta R.T. -0.010 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 79987
Ion Ratio Lower Upper
252 100
253 22.1 17.6 26.4
125 11.3 8.8 13.2



#38
Benzo(k)fluoranthene
Concen: 0.375 ng
RT: 22.968 min Scan# 2276
Delta R.T. -0.007 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:252 Resp: 79757
Ion Ratio Lower Upper
252 100
253 22.3 17.5 26.3
125 11.1 8.8 13.2









#39
Benzo(a)pyrene
Concen: 0.398 ng
RT: 23.515 min Scan# 2436
Delta R.T. -0.010 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252	Resp:	68538
Ion Ratio	Lower	Upper
252	100	
253	22.2	18.0 27.0
125	12.9	10.4 15.6



#40
Dibenzo(a,h)anthracene
Concen: 0.435 ng
RT: 26.000 min Scan# 3162
Delta R.T. -0.014 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Tgt Ion:278	Resp:	70069
Ion Ratio	Lower	Upper
278	100	
139	18.2	14.6 22.0
279	23.9	19.3 28.9



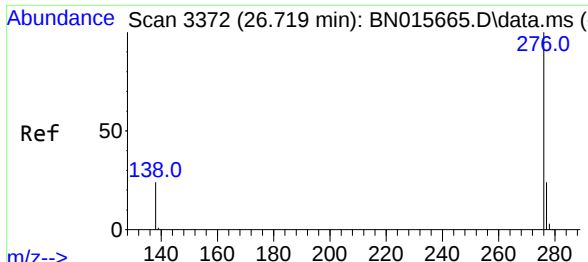

#41
Benzo(g,h,i)perylene
Concen: 0.393 ng
RT: 26.702 min Scan# 3367
Delta R.T. -0.017 min
Lab File: BN015686.D
Acq: 24 Jul 2021 12:27

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 73670
Ion Ratio Lower Upper
276 100
277 23.8 19.1 28.7
138 24.1 19.1 28.7

