
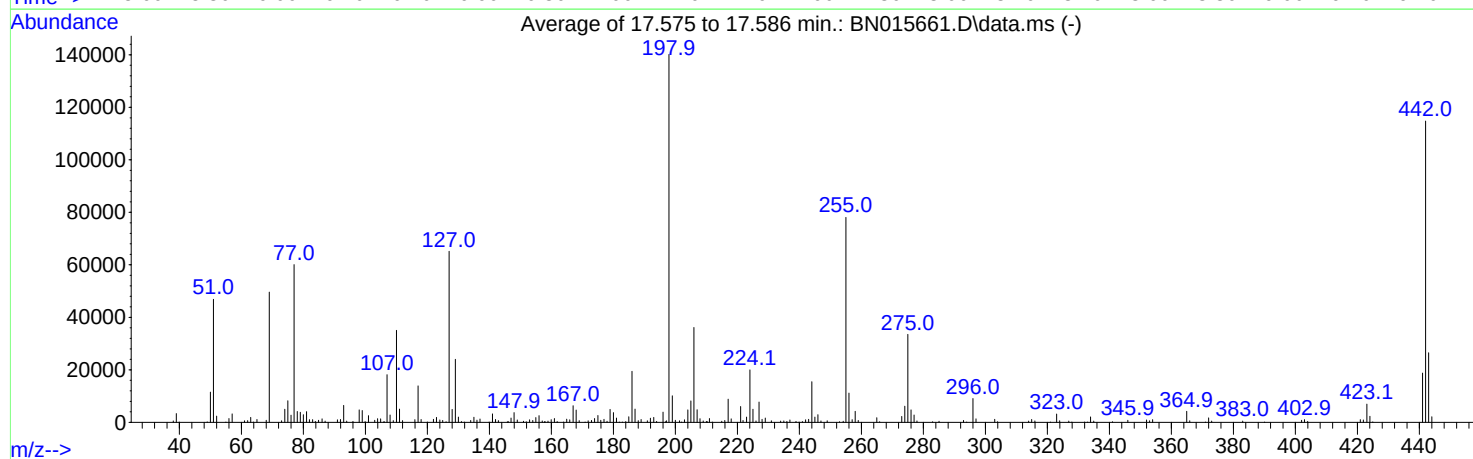


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
 Data File : BN015661.D
 Acq On : 23 Jul 2021 08:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 23 14:45:01 2021

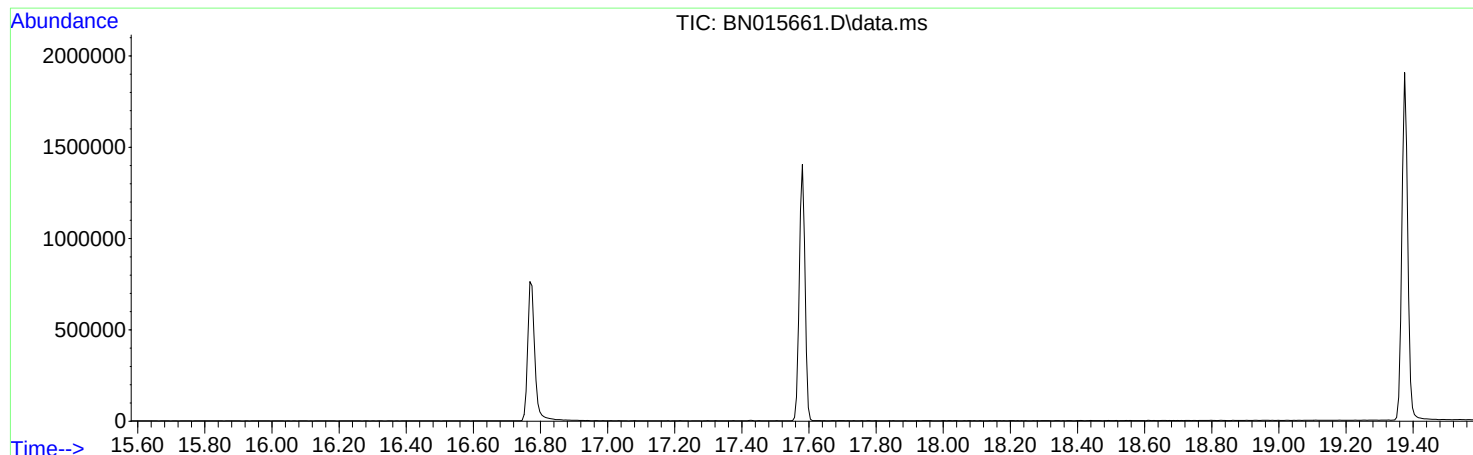




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	46869	PASS
68	69	0.00	2	1.7	824	PASS
69	198	0.00	100	35.4	49613	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	65144	PASS
197	198	0.00	2	0.4	629	PASS
198	198	100	100	100.0	140109	PASS
199	198	5	9	7.2	10100	PASS
275	198	10	60	23.9	33507	PASS
365	198	1	100	3.0	4206	PASS
441	198	0.01	100	13.4	18752	PASS
442	442	50	100	100.0	114755	PASS
443	442	15	24	23.1	26493	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015661.D
Acq On : 23 Jul 2021 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 23 09:44:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 23 09:44:30 2021
Response via : Initial Calibration

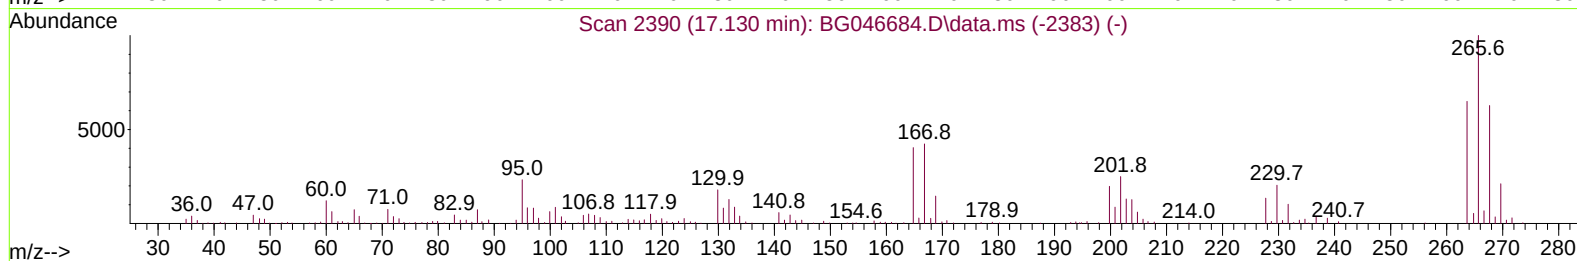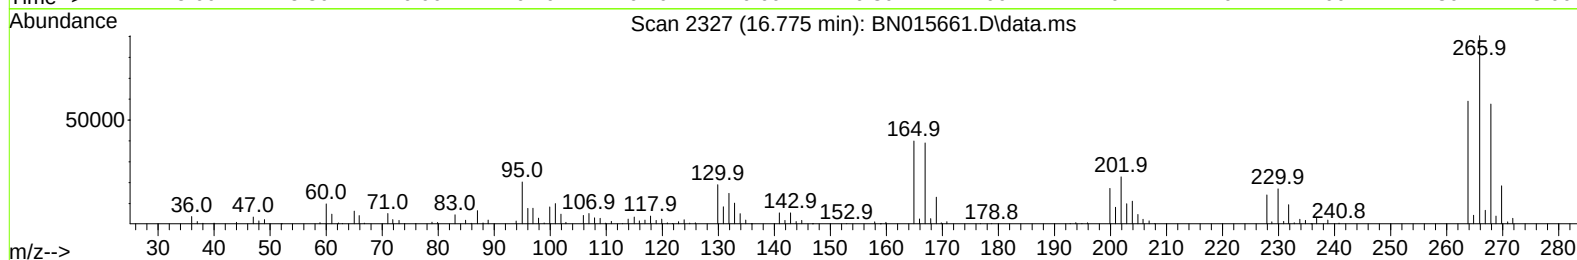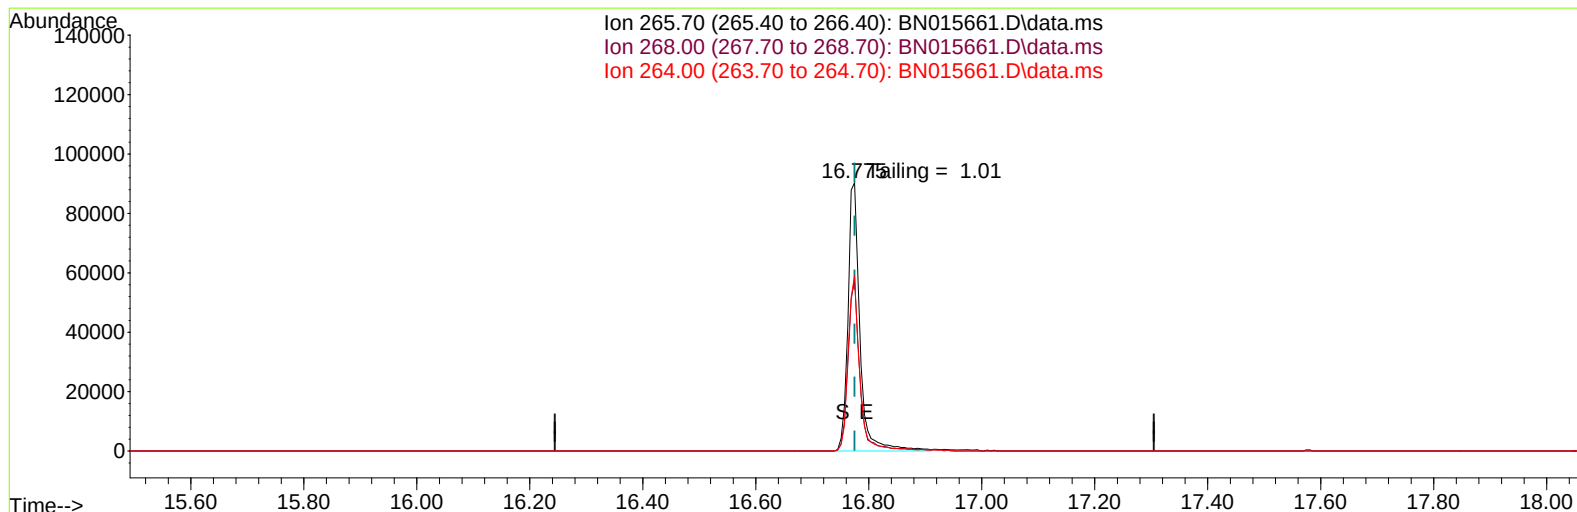

TIC: BN015661.D\data.ms

(70) Pentachlorophenol (C)

16.775min (0.000) 19763.90 ng




response 133698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.83
264.00	61.60	65.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015661.D
Acq On : 23 Jul 2021 08:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 23 09:44:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 23 09:44:30 2021
Response via : Initial Calibration

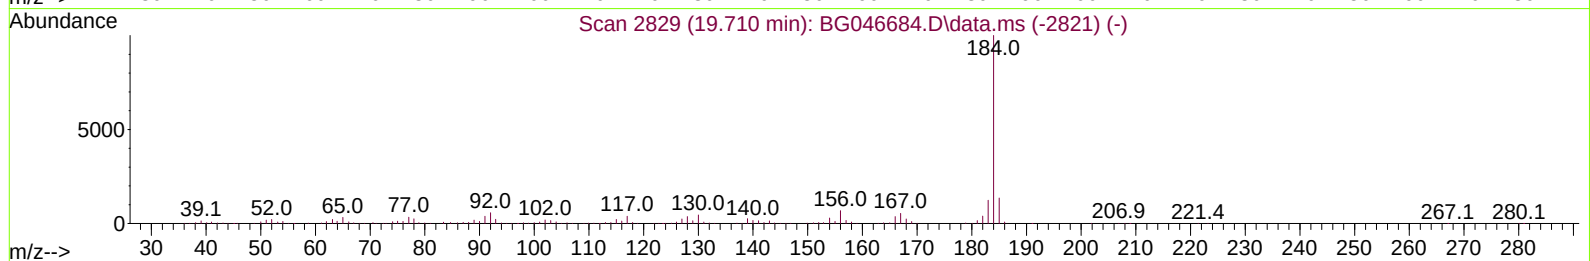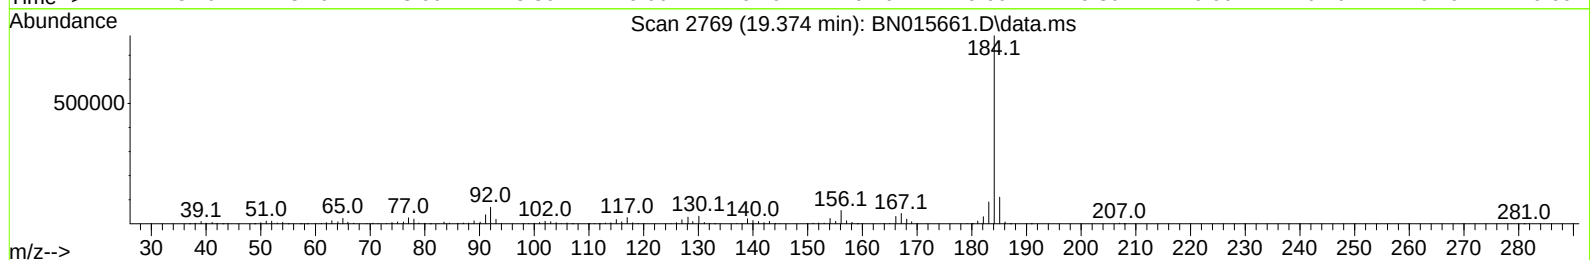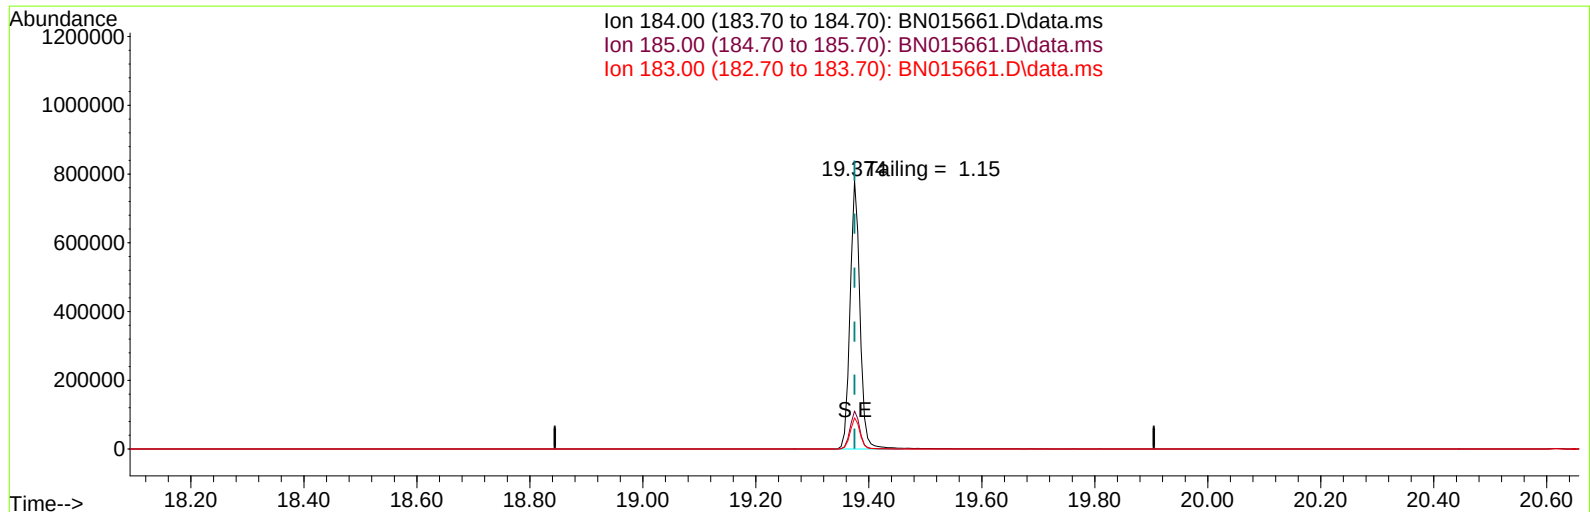

TIC: BN015661.D\data.ms

(77) Benzidine

19.374min (0.000) 0.00 ng

response 956828

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.21
183.00	13.20	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/24/2021	BNA_N	<u>BN015661.D</u>
Compound Name	Response	Retention Time
DDT	474335	20.621
DDD	3139	20.174
DDE	588	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3727	478062	0.78