
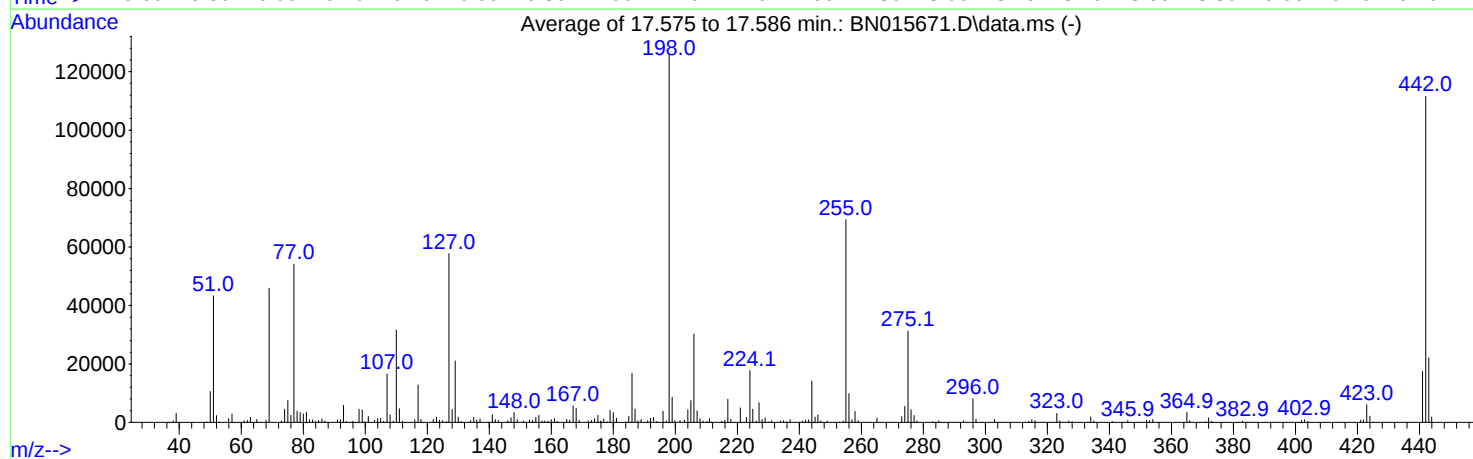


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
 Data File : BN015671.D
 Acq On : 23 Jul 2021 17:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 23 14:45:01 2021

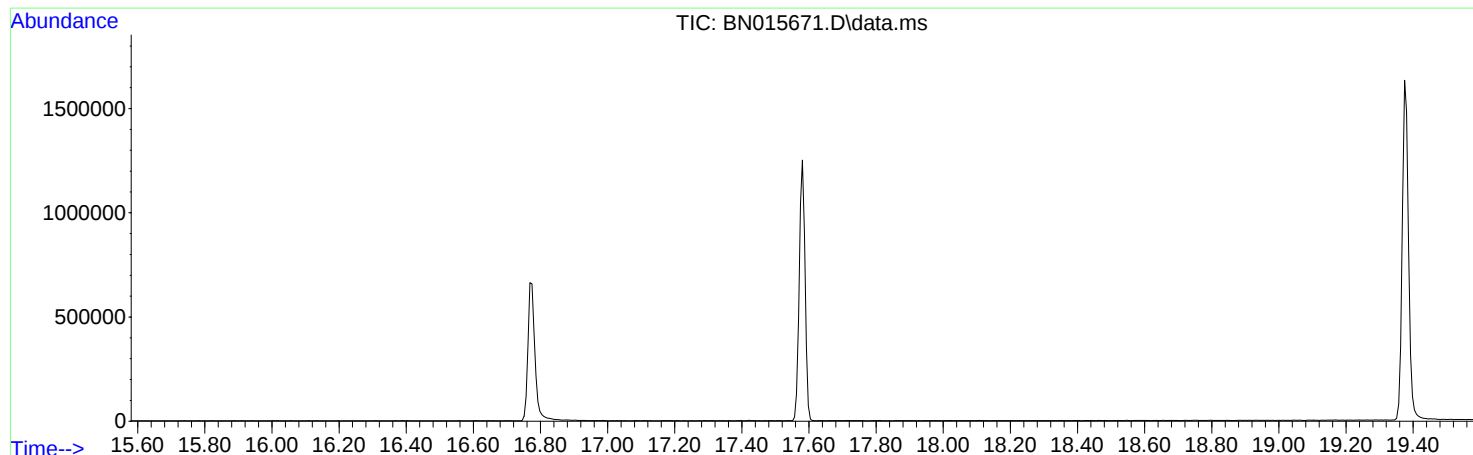




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	43317	PASS
68	69	0.00	2	1.7	758	PASS
69	198	0.00	100	36.4	45864	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.9	57773	PASS
197	198	0.00	2	0.4	527	PASS
198	198	100	100	100.0	125883	PASS
199	198	5	9	6.8	8616	PASS
275	198	10	60	24.8	31269	PASS
365	198	1	100	2.7	3381	PASS
441	198	0.01	100	13.8	17402	PASS
442	442	50	100	100.0	111560	PASS
443	442	15	24	19.8	22053	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015671.D
Acq On : 23 Jul 2021 17:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 23 17:54:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 23 09:44:30 2021
Response via : Initial Calibration

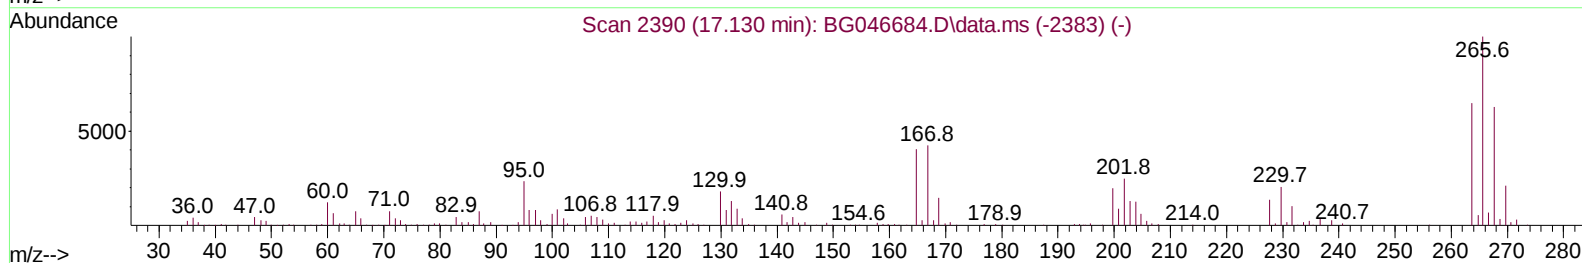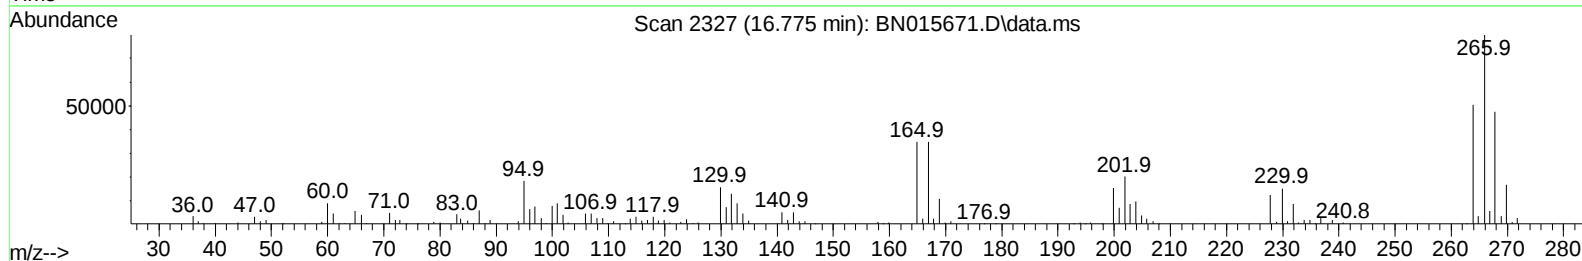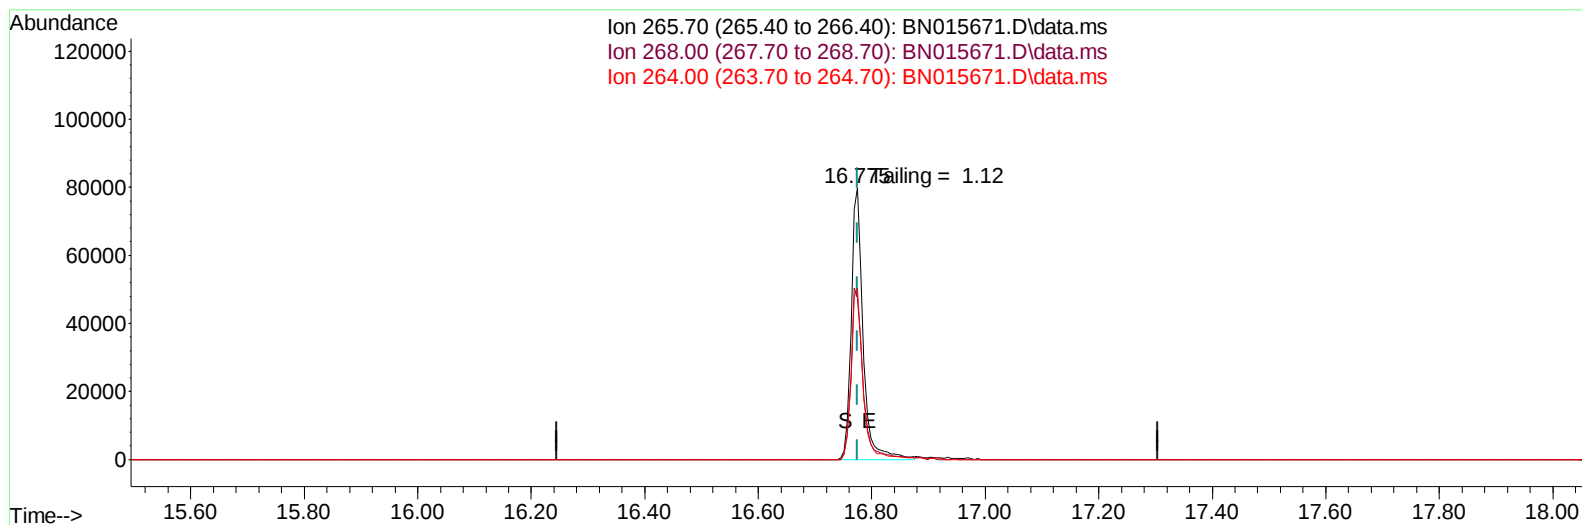

TIC: BN015671.D\data.ms

(70) Pentachlorophenol (C)

16.775min (0.000) 21360.36 ng




response 116671

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.50
264.00	61.60	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015671.D
Acq On : 23 Jul 2021 17:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 23 17:54:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 23 09:44:30 2021
Response via : Initial Calibration

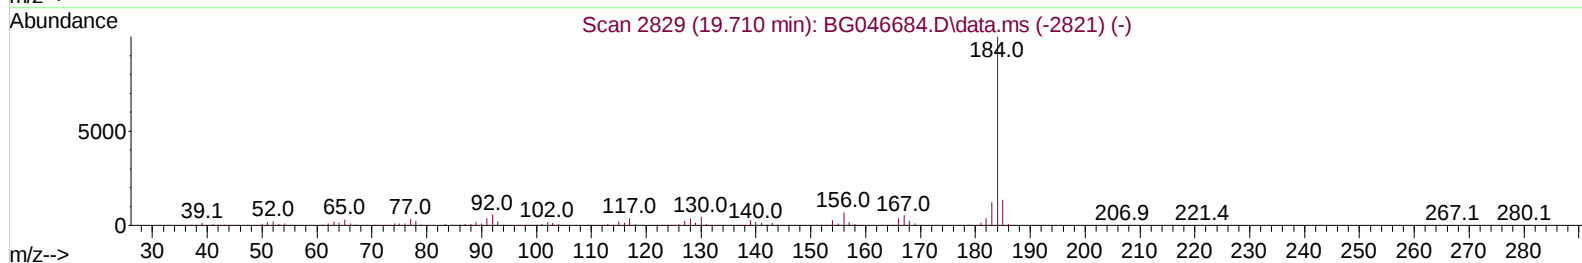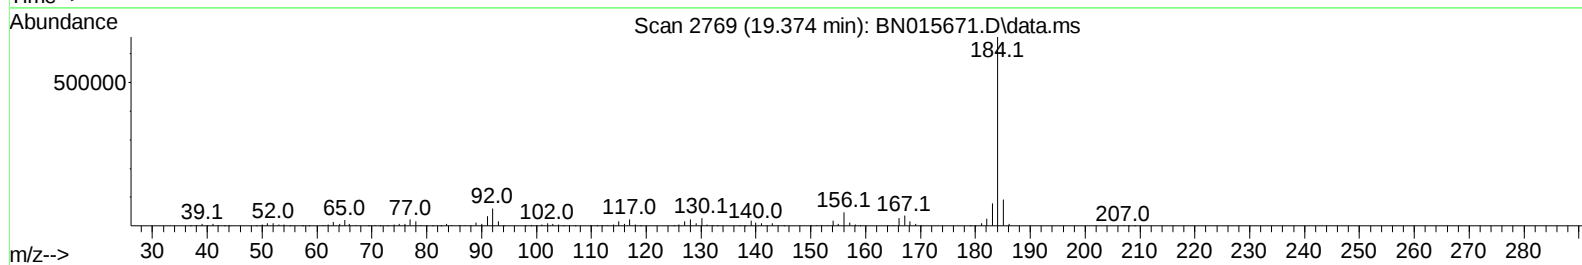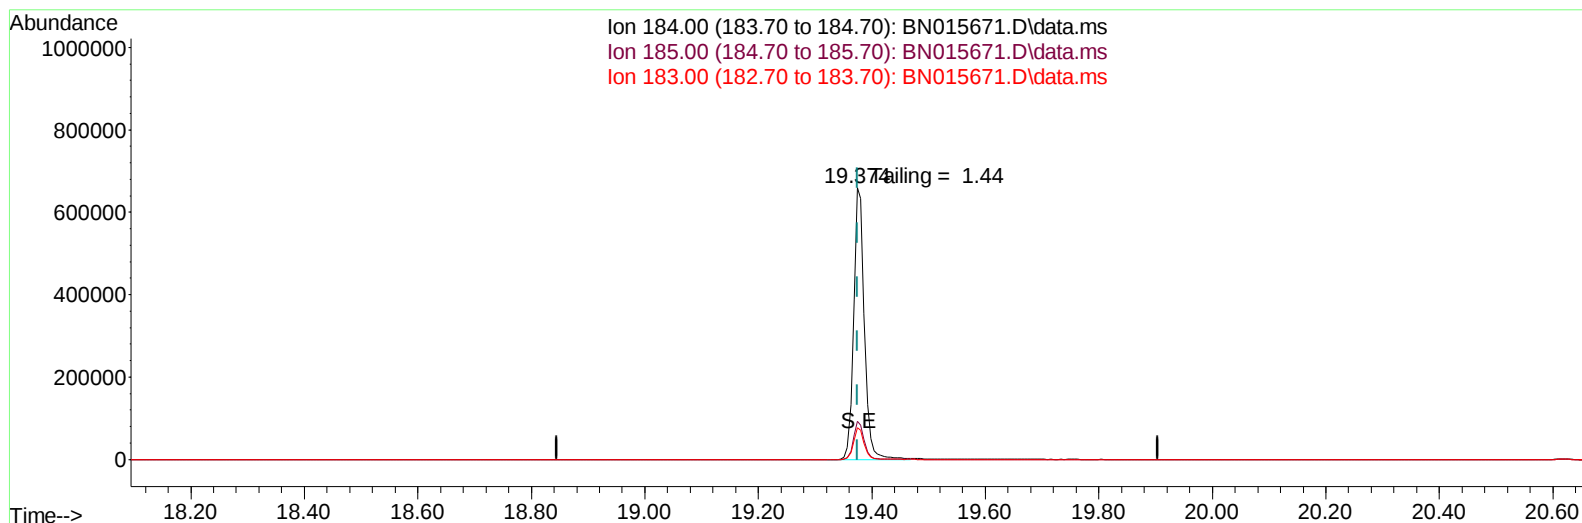

TIC: BN015671.D\data.ms

(77) Benzidine

19.374min (0.000) 0.00 ng

response 878034

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.08
183.00	13.20	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/24/2021	BNA_N	<u>BN015671.D</u>
Compound Name	Response	Retention Time
DDT	419694	20.621
DDD	3093	20.18
DDE	390	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3483	423177	0.82