
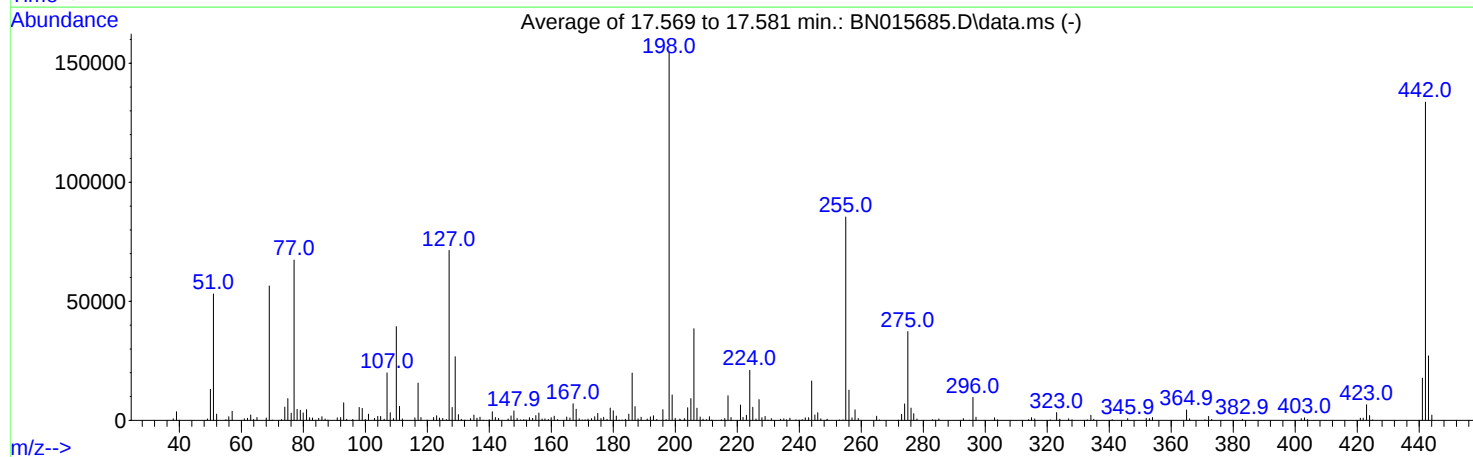


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
 Data File : BN015685.D
 Acq On : 24 Jul 2021 09:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 23 14:45:01 2021

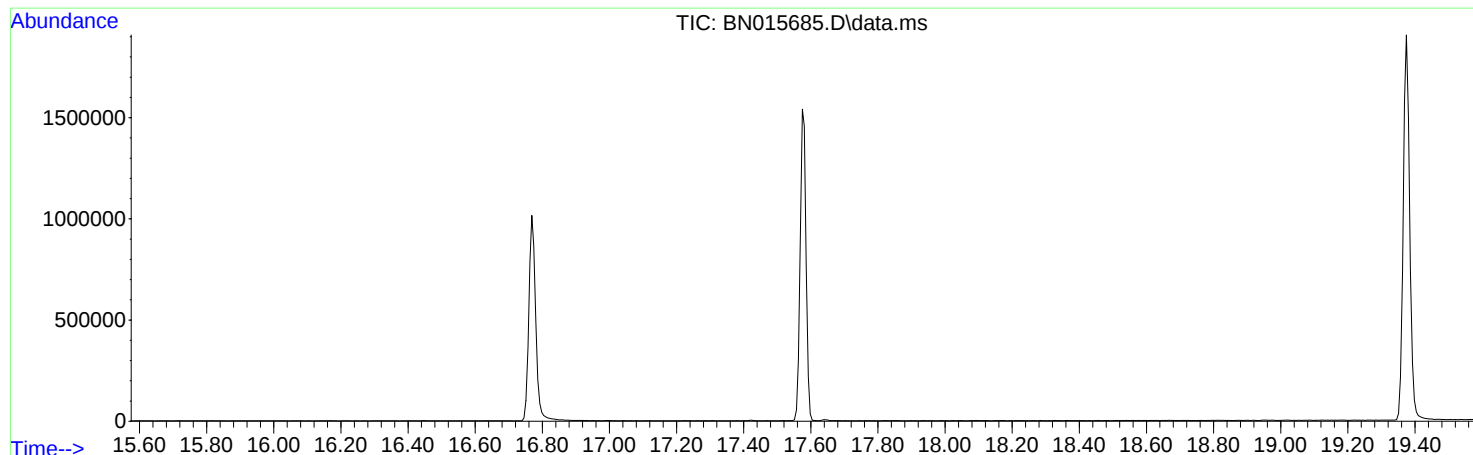




AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	53072	PASS
68	69	0.00	2	1.7	988	PASS
69	198	0.00	100	36.6	56485	PASS
70	69	0.00	2	0.2	110	PASS
127	198	10	80	46.2	71371	PASS
197	198	0.00	2	0.2	352	PASS
198	198	100	100	100.0	154509	PASS
199	198	5	9	6.9	10669	PASS
275	198	10	60	24.2	37320	PASS
365	198	1	100	2.8	4372	PASS
441	198	0.01	100	11.5	17739	PASS
442	442	50	100	100.0	133643	PASS
443	442	15	24	20.3	27079	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072421\
Data File : BN015685.D
Acq On : 24 Jul 2021 09:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 26 06:59:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:59:38 2021
Response via : Initial Calibration

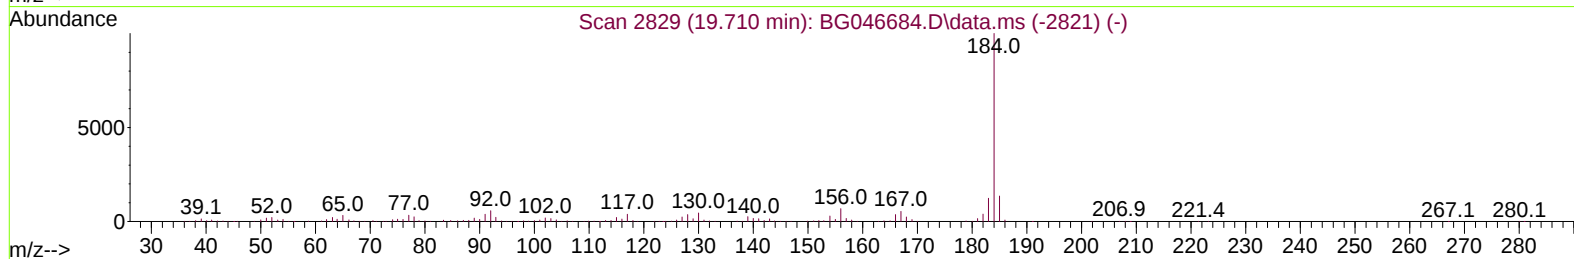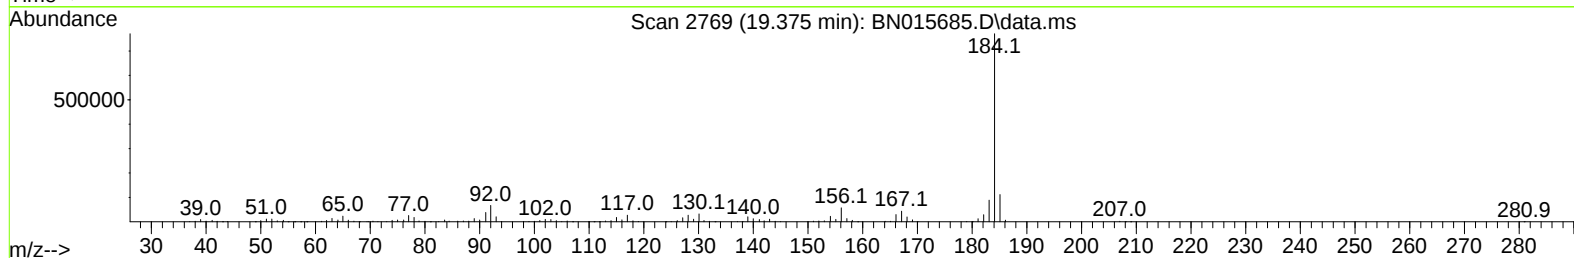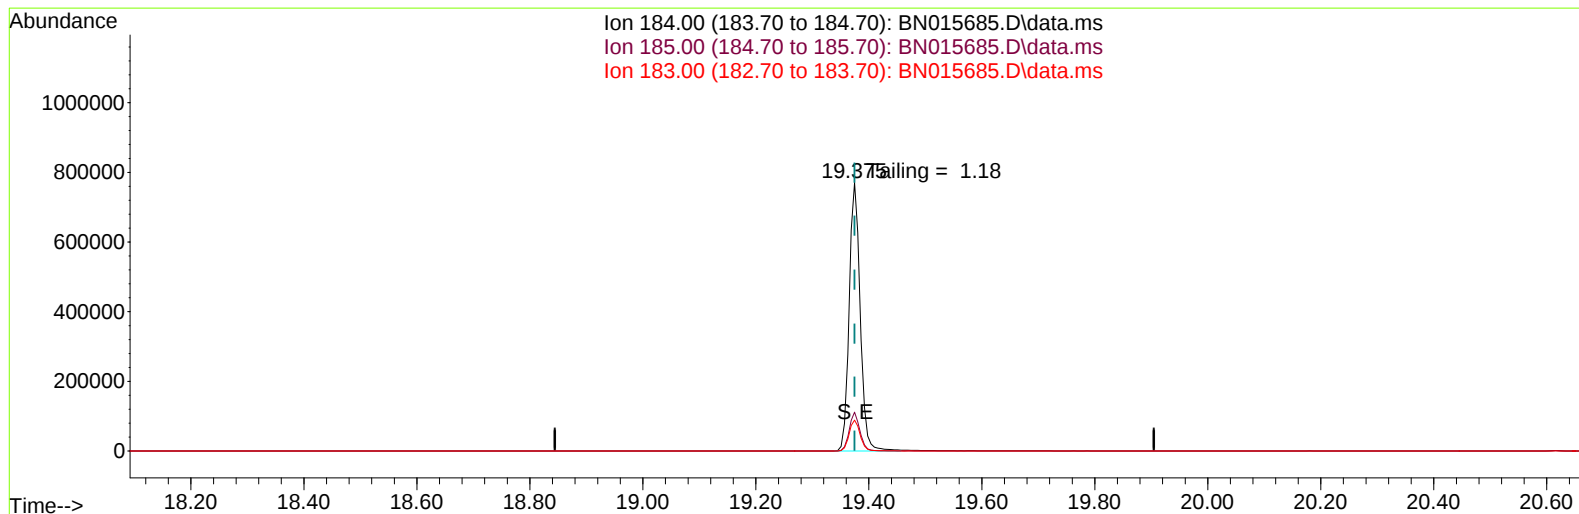

TIC: BN015685.D\data.ms

(77) Benzidine

19.375min (0.000) 0.00 ng

response 1052144

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.49
183.00	13.20	11.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/24/2021	BNA_N	<u>BN015685.D</u>
Compound Name	Response	Retention Time
DDT	383516	20.616
DDD	109884	20.175
DDE	815	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
110699	494215	22.40