

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
 Data File : BN015691.D
 Acq On : 24 Jul 2021 17:36
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Jul 26 01:34:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 26 01:23:47 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	13001	0.40	ng	0.00
7) Naphthalene-d8	10.470	136	58615	0.40	ng	0.00
13) Acenaphthene-d10	14.319	164	31665	0.40	ng	0.00
19) Phenanthrene-d10	17.078	188	61522	0.40	ng	0.00
29) Chrysene-d12	21.281	240	60001	0.40	ng	0.00
35) Perylene-d12	23.567	264	60517	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	6955	0.22	ng	0.00
5) Phenol-d6	6.868	99	8107	0.22	ng	0.00
8) Nitrobenzene-d5	8.835	82	8665	0.21	ng	0.00
11) 2-Methylnaphthalene-d10	12.065	152	17995	0.21	ng	0.00
14) 2,4,6-Tribromophenol	15.817	330	2297	0.23	ng	0.00
15) 2-Fluorobiphenyl	12.949	172	27647	0.21	ng	0.00
27) Fluoranthene-d10	19.113	212	32903	0.20	ng	0.00
31) Terphenyl-d14	19.723	244	30349	0.21	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.226	88	823	0.21	ng	# 99
3) n-Nitrosodimethylamine	3.594	42	1809	0.19	ng	# 97
6) bis(2-Chloroethyl)ether	7.126	93	7681	0.21	ng	100
9) Naphthalene	10.521	128	31855	0.20	ng	100
10) Hexachlorobutadiene	10.812	225	5980	0.20	ng	# 100
12) 2-Methylnaphthalene	12.141	142	20912	0.21	ng	99
16) Acenaphthylene	14.040	152	25049	0.19	ng	100
17) Acenaphthene	14.383	154	18180	0.20	ng	98
18) Fluorene	15.373	166	22233	0.20	ng	99
20) 4,6-Dinitro-2-methylph...	15.461	198	238	0.06	ng	# 61
21) 4-Bromophenyl-phenylether	16.275	248	6900	0.19	ng	97
22) Hexachlorobenzene	16.385	284	7949	0.20	ng	99
23) Atrazine	16.543	200	4569	0.21	ng	99
24) Pentachlorophenol	16.738	266	1902	0.21	ng	98
25) Phenanthrene	17.115	178	36745	0.20	ng	100
26) Anthracene	17.200	178	29856	0.19	ng	100
28) Fluoranthene	19.142	202	40452	0.20	ng	100
30) Pyrene	19.510	202	41534	0.19	ng	100
32) Benzo(a)anthracene	21.259	228	39133	0.21	ng	99
33) Chrysene	21.312	228	40854	0.20	ng	99
34) Bis(2-ethylhexyl)phtha...	21.206	149	15898	0.20	ng	100
36) Indeno(1,2,3-cd)pyrene	25.901	276	46685	0.21	ng	99
37) Benzo(b)fluoranthene	22.875	252	41419	0.18	ng	98
38) Benzo(k)fluoranthene	22.920	252	44777	0.20	ng	99
39) Benzo(a)pyrene	23.464	252	36817	0.20	ng	98
40) Dibenzo(a,h)anthracene	25.922	278	38256	0.22	ng	99
41) Benzo(g,h,i)perylene	26.616	276	38116	0.19	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
Data File : BN015691.D
Acq On : 24 Jul 2021 17:36
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Jul 26 01:34:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 01:23:47 2021
Response via : Initial Calibration




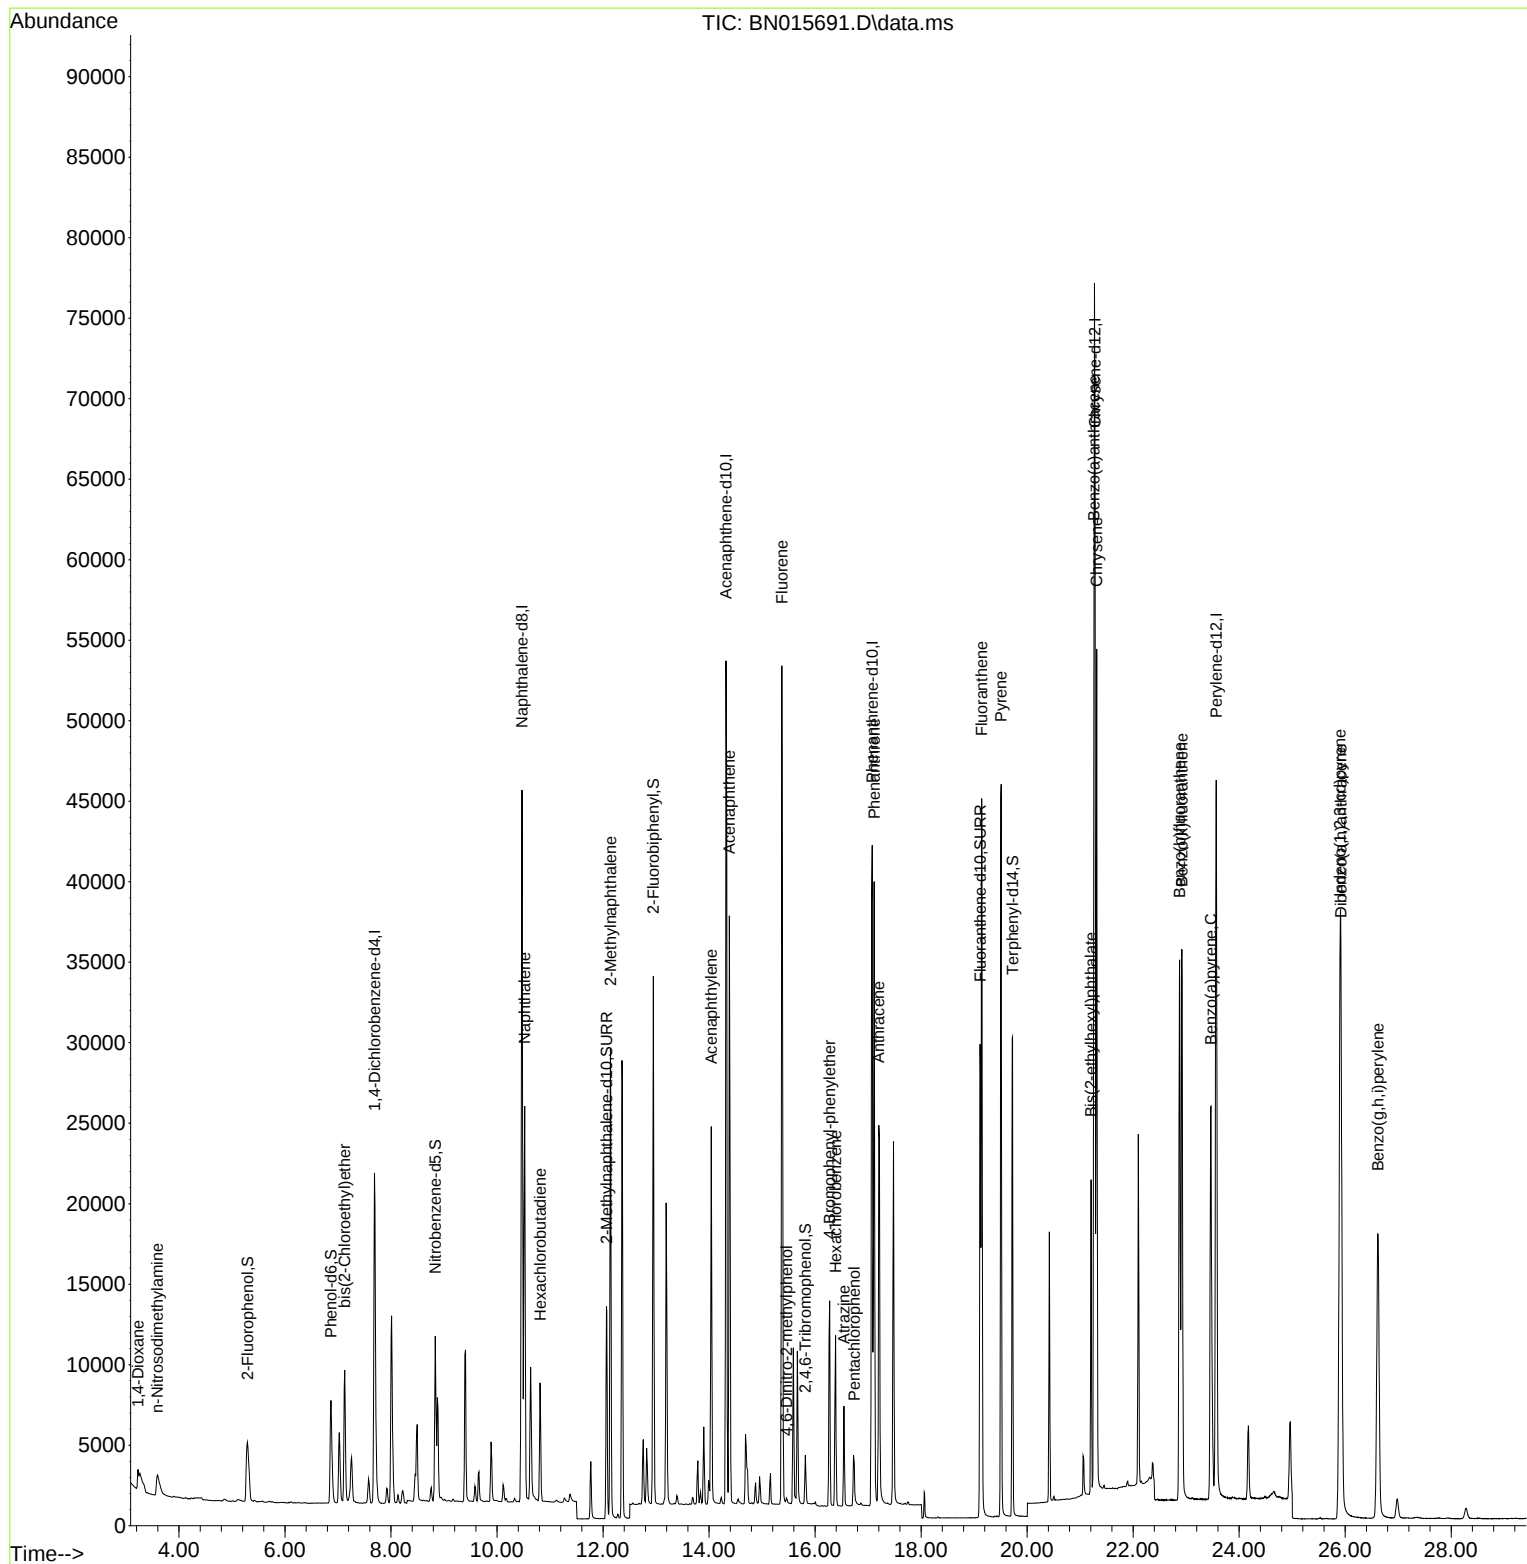


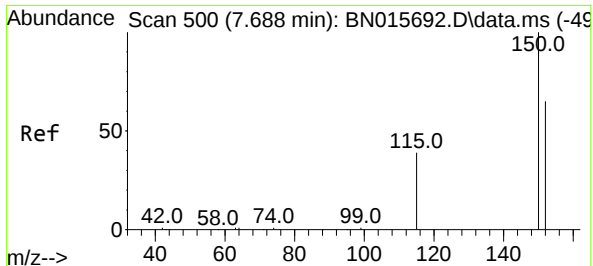

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.688 min Scan# 500
 Delta R.T. 0.000 min
 Lab File: BN015691.D
 Acq: 24 Jul 2021 17:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:152 Resp: 13001
 Ion Ratio Lower Upper
 152 100
 150 156.2 125.2 187.8
 115 60.8 48.6 73.0

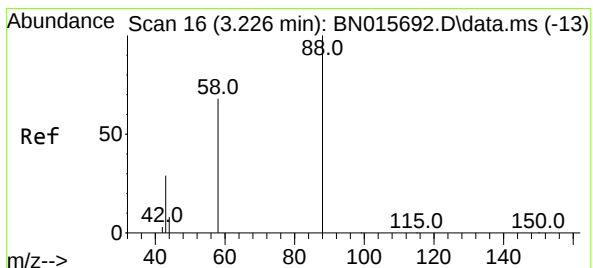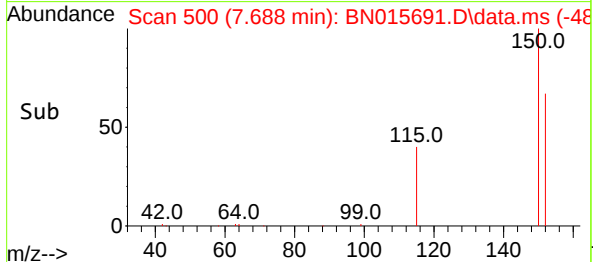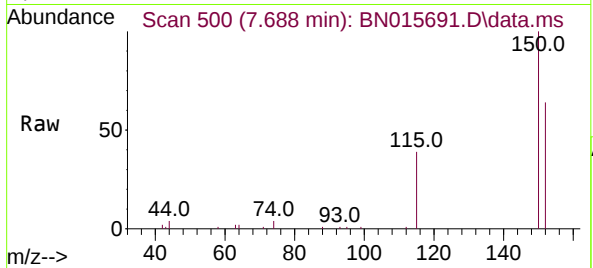

#2
 1,4-Dioxane
 Concen: 0.21 ng
 RT: 3.226 min Scan# 16
 Delta R.T. 0.000 min
 Lab File: BN015691.D
 Acq: 24 Jul 2021 17:36

Tgt Ion: 88 Resp: 823
 Ion Ratio Lower Upper
 88 100
 43 93.2 0.0 0.0#
 58 66.1 53.8 80.6


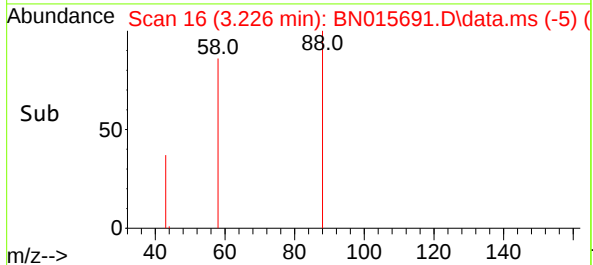

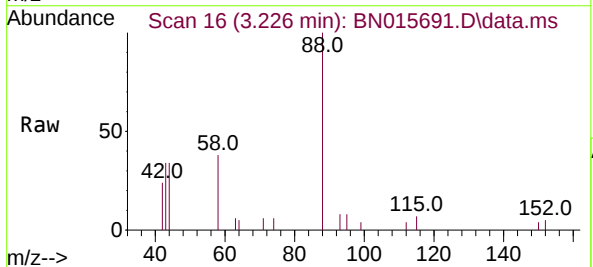


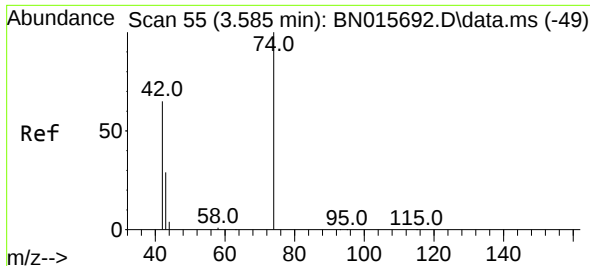

#3
n-Nitrosodimethylamine
Concen: 0.19 ng
RT: 3.594 min Scan# 56
Delta R.T. 0.009 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion: 42 Resp: 1809
Ion Ratio Lower Upper
42 100
74 155.1 126.7 190.1
44 5.4 5.8 8.8#

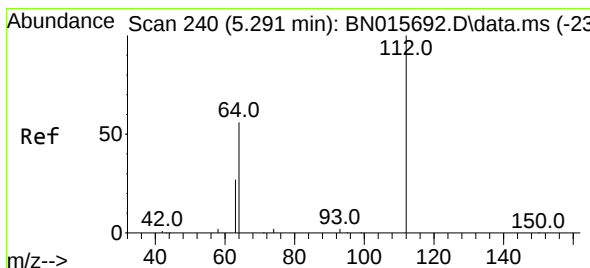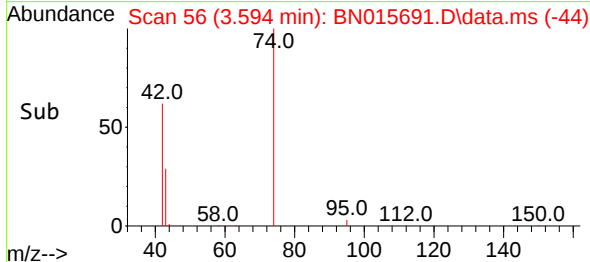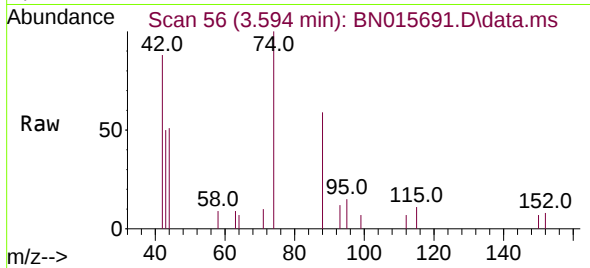

#4
2-Fluorophenol
Concen: 0.22 ng
RT: 5.291 min Scan# 240
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion: 112 Resp: 6955
Ion Ratio Lower Upper
112 100
64 55.6 44.8 67.2
63 28.2 22.2 33.4


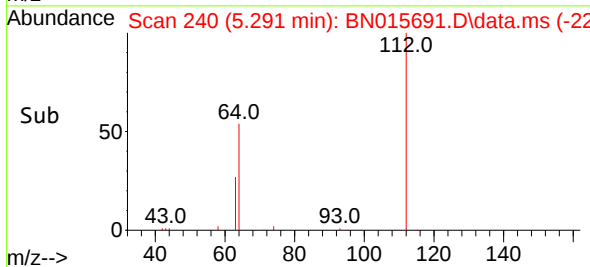

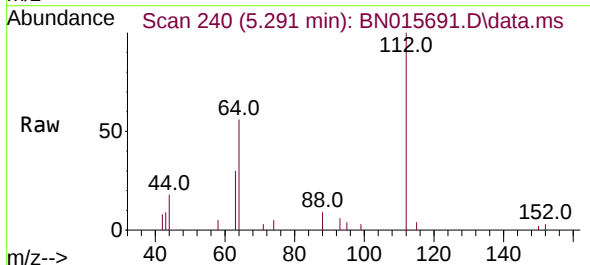




#5
Phenol-d6
Concen: 0.22 ng
RT: 6.868 min Scan# 411
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion: 99 Resp: 8107
Ion Ratio Lower Upper
99 100
42 16.5 13.4 20.0
71 30.4 24.5 36.7

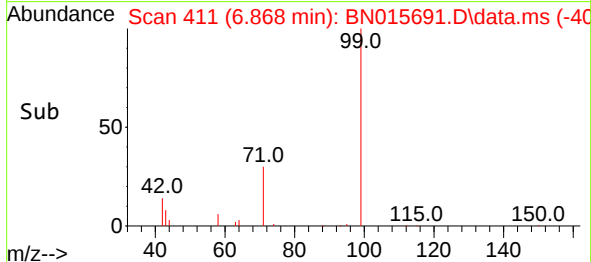

#6
bis(2-Chloroethyl)ether
Concen: 0.21 ng
RT: 7.126 min Scan# 439
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion: 93 Resp: 7681
Ion Ratio Lower Upper
93 100
63 74.5 59.8 89.8
95 32.9 26.4 39.6









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.470 min Scan# 738
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	136	Resp:	58615
Ion Ratio	Lower	Upper	
136	100		
137	11.1	8.9	13.3
54	6.5	5.0	7.4
68	5.6	4.3	6.5

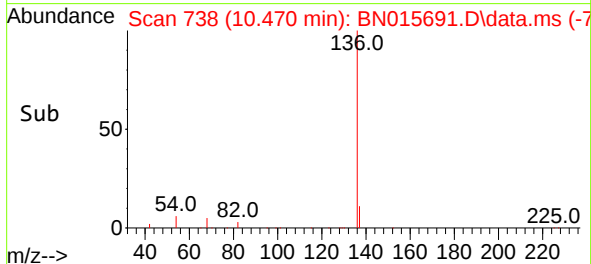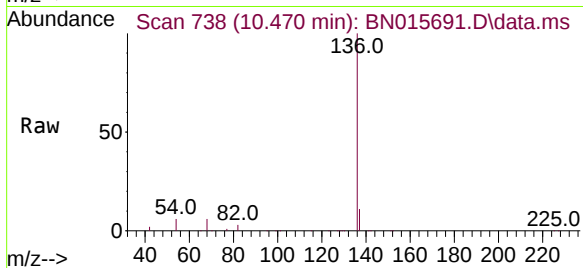

#8
Nitrobenzene-d5
Concen: 0.21 ng
RT: 8.835 min Scan# 609
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:	82	Resp:	8665
Ion Ratio	Lower	Upper	
82	100		
128	39.0	32.0	48.0
54	50.1	38.9	58.3


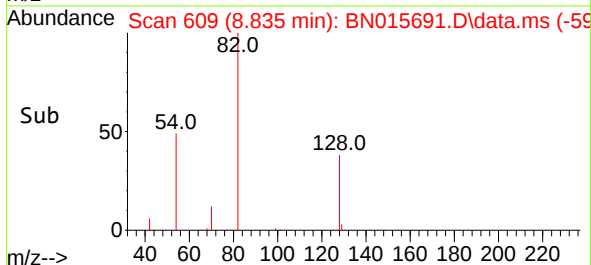
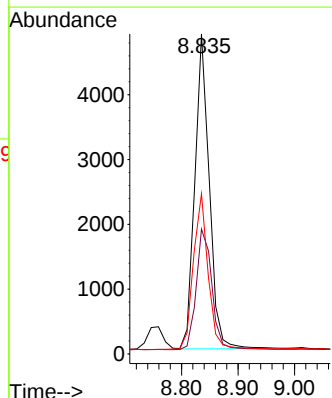
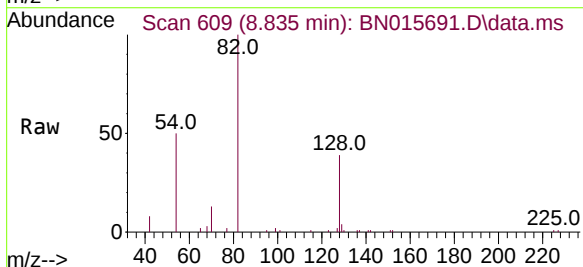




#9
Naphthalene
Concen: 0.20 ng
RT: 10.521 min Scan# 742
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	128	Resp:	31855
Ion Ratio	Lower	Upper	
128	100		
129	11.1	8.9	13.3
127	13.0	10.4	15.6

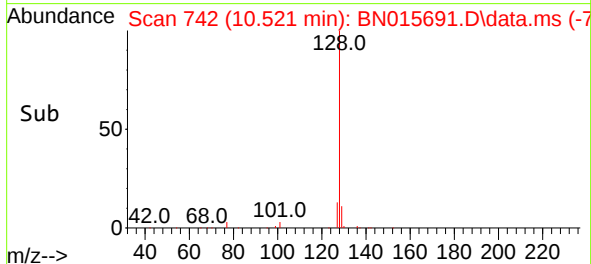

#10
Hexachlorobutadiene
Concen: 0.20 ng
RT: 10.812 min Scan# 765
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:	225	Resp:	5980
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.5	51.1	76.7







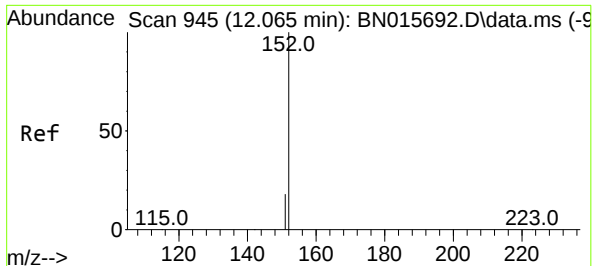

#11
2-Methylnaphthalene-d10
Concen: 0.21 ng
RT: 12.065 min Scan# 945
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:152 Resp: 17995
Ion Ratio Lower Upper
152 100
151 20.5 16.3 24.5

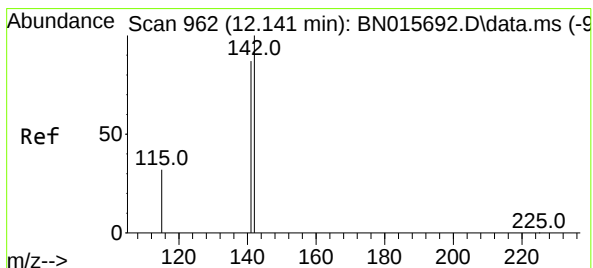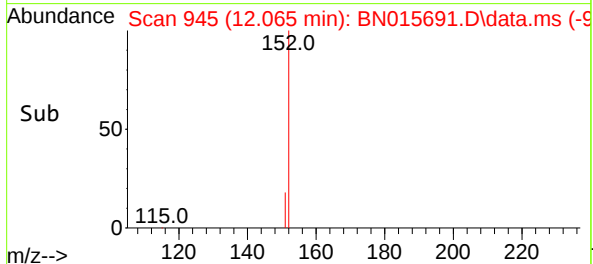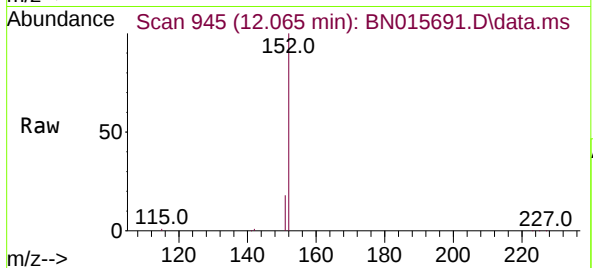

#12
2-Methylnaphthalene
Concen: 0.21 ng
RT: 12.141 min Scan# 962
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:142 Resp: 20912
Ion Ratio Lower Upper
142 100
141 87.6 69.4 104.2
115 32.9 25.9 38.9


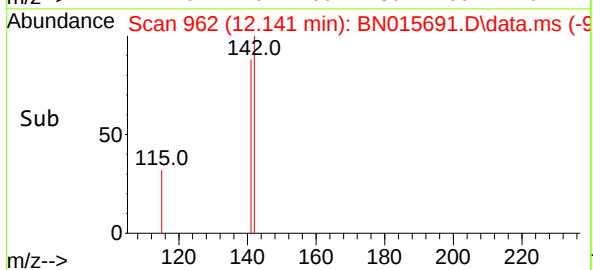

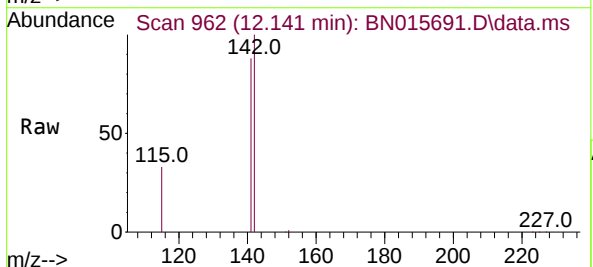




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.319 min Scan# 1187
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:164 Resp: 31665
Ion Ratio Lower Upper
164 100
162 104.7 83.6 125.4
160 48.4 38.6 58.0

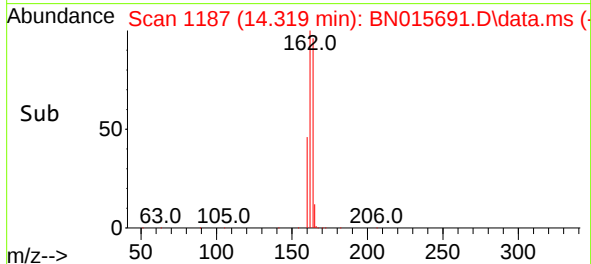

#14
2,4,6-Tribromophenol
Concen: 0.23 ng
RT: 15.817 min Scan# 1305
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:330 Resp: 2297
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.9 28.5 42.7


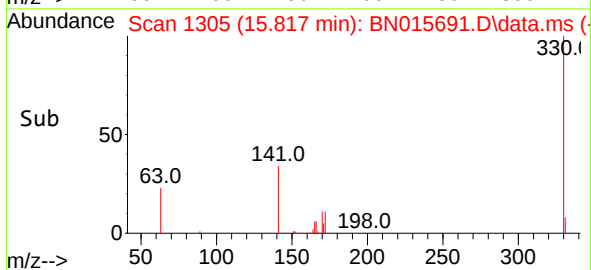






#15
2-Fluorobiphenyl
Concen: 0.21 ng
RT: 12.949 min Scan# 1079
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:	172	Resp:	27647
Ion Ratio	Lower	Upper	
172	100		
171	34.4	27.4	41.0
170	22.8	17.9	26.9

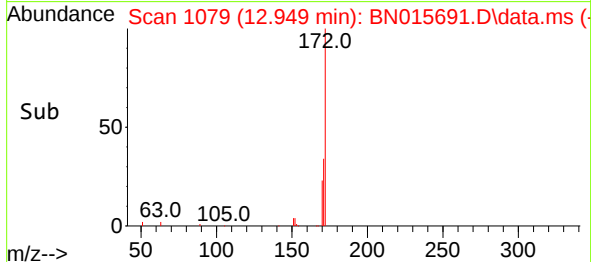

#16
Acenaphthylene
Concen: 0.19 ng
RT: 14.040 min Scan# 1165
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:	152	Resp:	25049
Ion Ratio	Lower	Upper	
152	100		
151	19.1	15.4	23.2
153	13.0	10.4	15.6


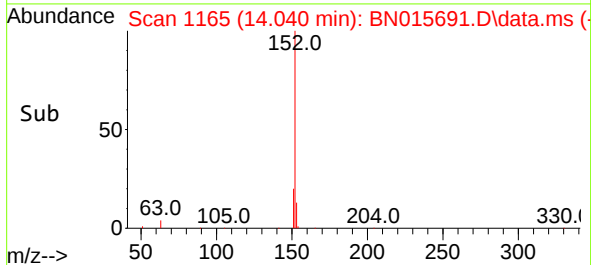




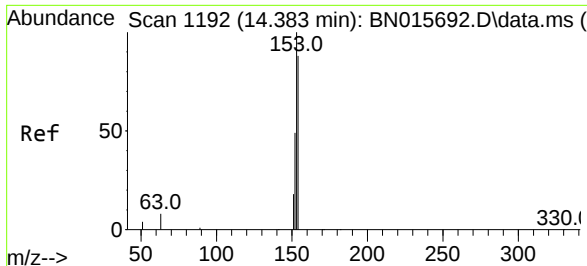

#17
Acenaphthene
Concen: 0.20 ng
RT: 14.383 min Scan# 1192
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:154 Resp: 18180
Ion Ratio Lower Upper
154 100
153 113.4 89.0 133.6
152 55.1 43.3 64.9

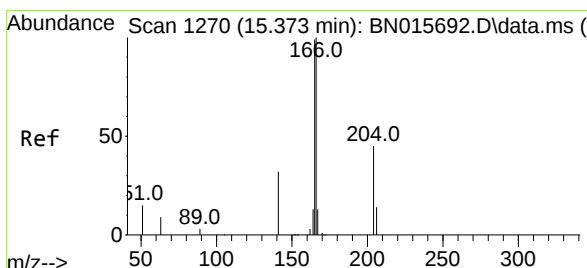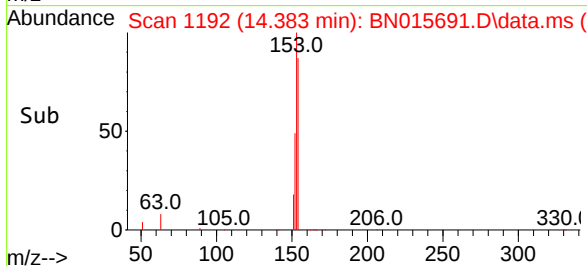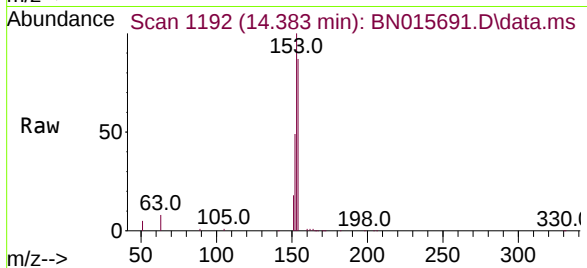

#18
Fluorene
Concen: 0.20 ng
RT: 15.373 min Scan# 1270
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:166 Resp: 22233
Ion Ratio Lower Upper
166 100
165 98.0 77.9 116.9
167 13.4 10.8 16.2


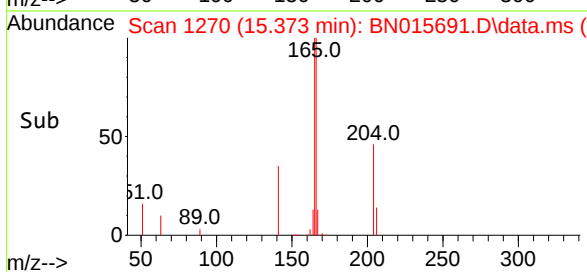

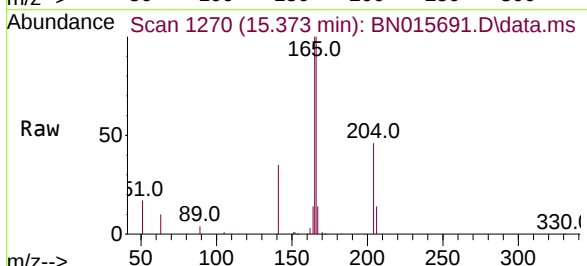




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.078 min Scan# 1408
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:188 Resp: 61522
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.0 5.3 7.9

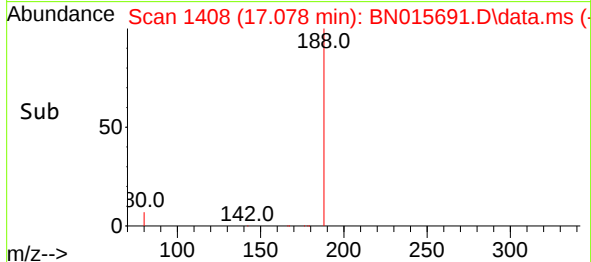

#20
4,6-Dinitro-2-methylphenol
Concen: 0.06 ng
RT: 15.461 min Scan# 1277
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:198 Resp: 238
Ion Ratio Lower Upper
198 100
182 38.4 16.4 24.6#
77 0.0 0.0 0.0




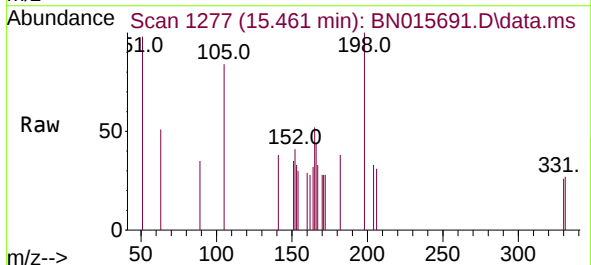


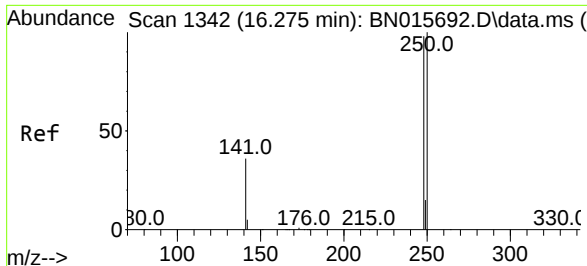

#21
4-Bromophenyl-phenylether
Concen: 0.19 ng
RT: 16.275 min Scan# 1342
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:248 Resp: 6900
Ion Ratio Lower Upper
248 100
250 100.2 81.6 122.4
141 40.0 29.4 44.0

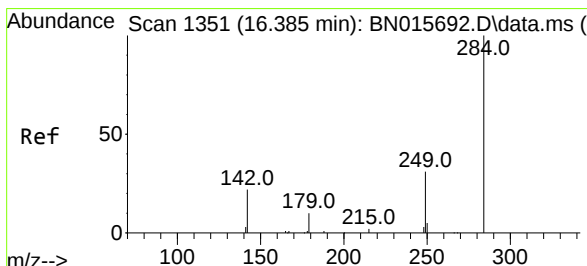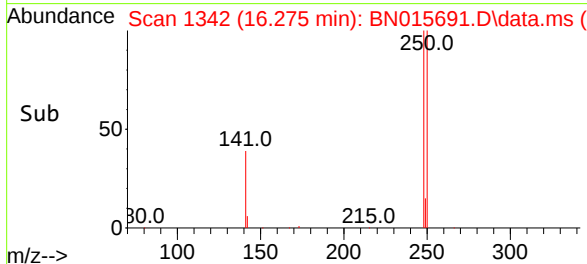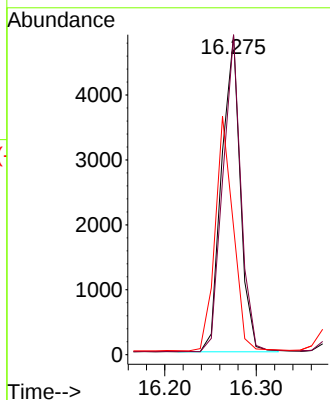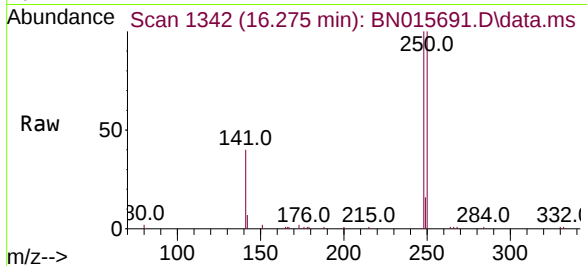

#22
Hexachlorobenzene
Concen: 0.20 ng
RT: 16.385 min Scan# 1351
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:284 Resp: 7949
Ion Ratio Lower Upper
284 100
142 34.3 27.6 41.4
249 31.3 24.6 37.0

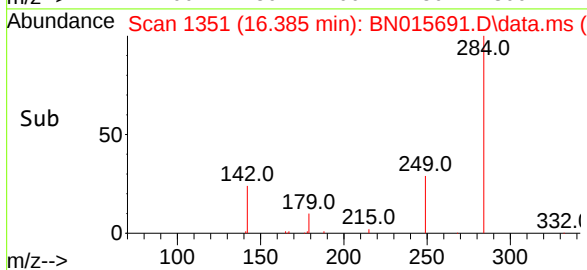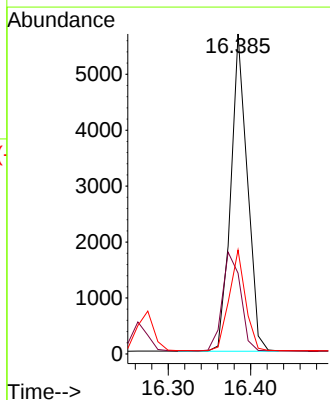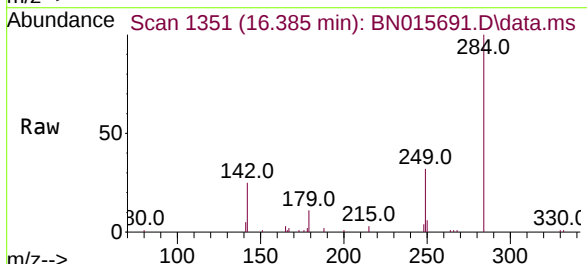

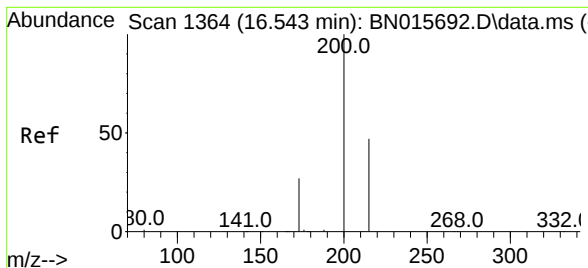

#23

Atrazine

Concen: 0.21 ng

RT: 16.543 min Scan# 1364

Delta R.T. 0.000 min

Lab File: BN015691.D

Acq: 24 Jul 2021 17:36





Instrument :

BNA_N

ClientSampleId :

SSTDIC0.2

Tgt Ion:	200	Resp:	4569
Ion	Ratio	Lower	Upper
200	100		
173	28.6	21.8	32.6
215	48.0	38.2	57.2

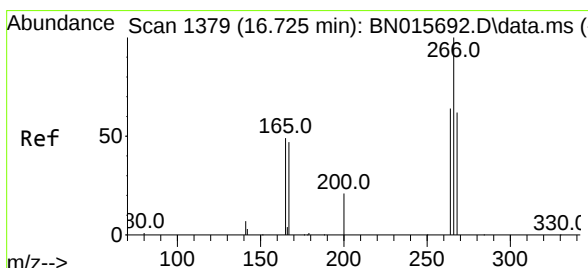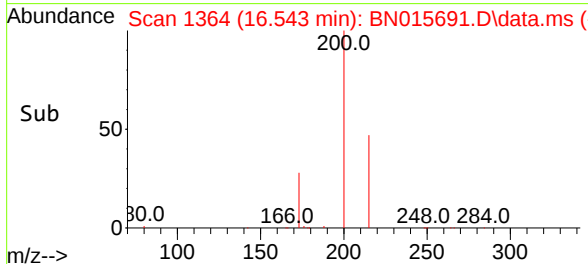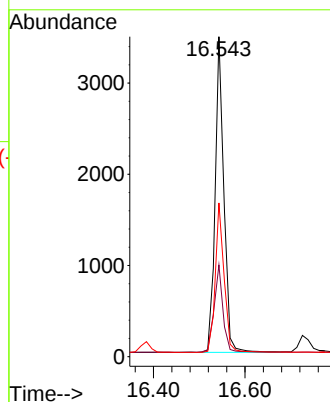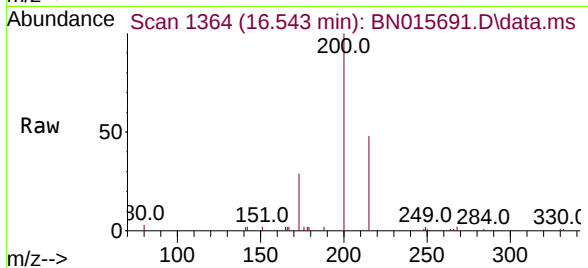

#24

Pentachlorophenol

Concen: 0.21 ng




RT: 16.738 min Scan# 1380


Delta R.T. 0.012 min

Lab File: BN015691.D

Acq: 24 Jul 2021 17:36

Tgt Ion:	266	Resp:	1902
Ion	Ratio	Lower	Upper
266	100		
264	63.2	49.9	74.9
268	66.0	50.8	76.2


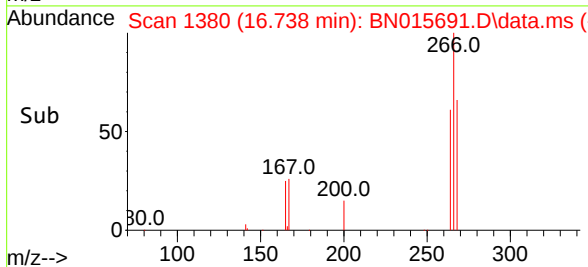
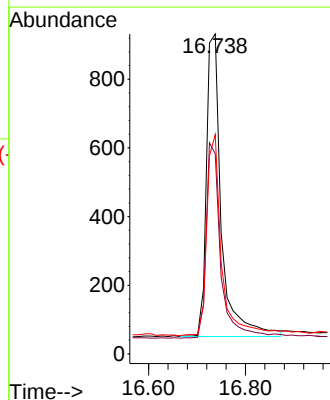
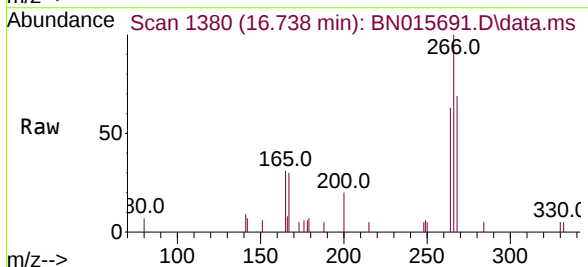


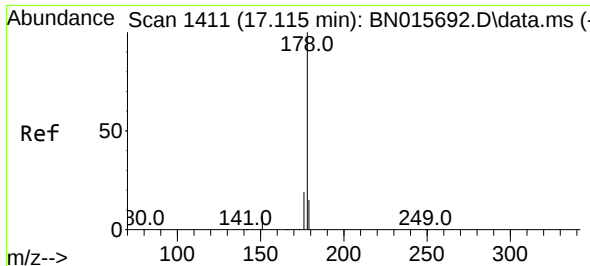

#25
Phenanthrene
Concen: 0.20 ng
RT: 17.115 min Scan# 1411
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:178 Resp: 36745
Ion Ratio Lower Upper
178 100
176 19.0 15.1 22.7
179 15.6 12.4 18.6

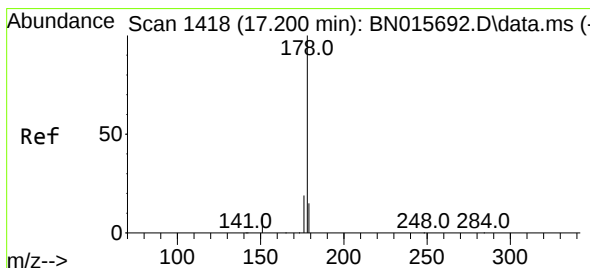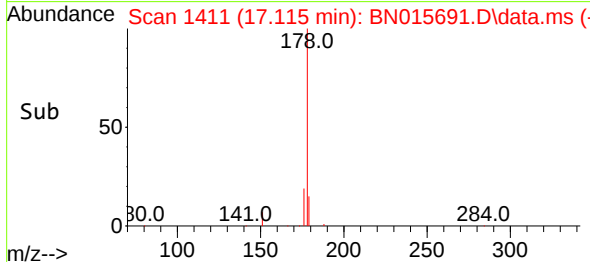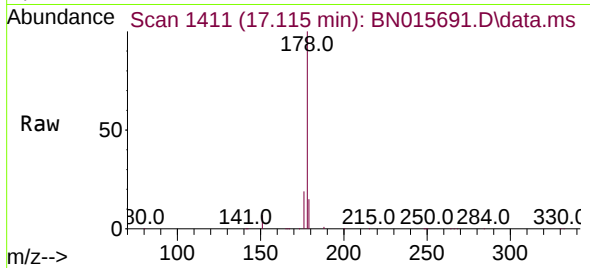

#26
Anthracene
Concen: 0.19 ng
RT: 17.200 min Scan# 1418
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:178 Resp: 29856
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.4 12.2 18.2


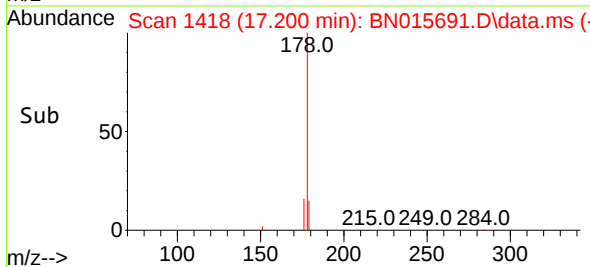

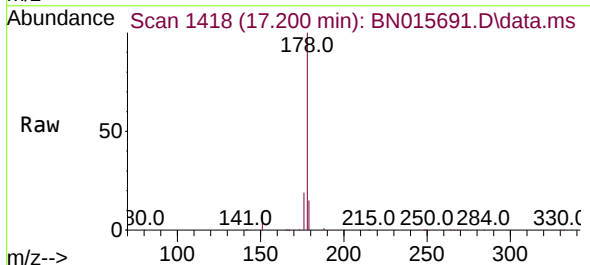




#27
Fluoranthene-d10
Concen: 0.20 ng
RT: 19.113 min Scan# 1706
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:212 Resp: 32903
Ion Ratio Lower Upper
212 100
106 14.1 11.5 17.3
104 7.9 6.3 9.5

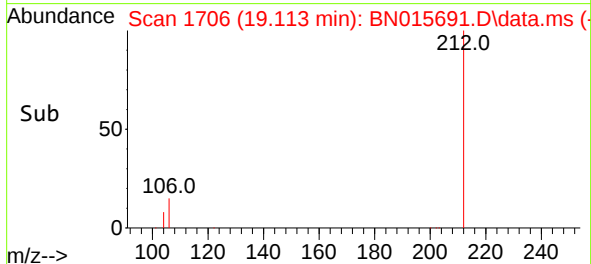

#28
Fluoranthene
Concen: 0.20 ng
RT: 19.142 min Scan# 1712
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:202 Resp: 40452
Ion Ratio Lower Upper
202 100
101 11.7 9.4 14.2
203 17.3 13.8 20.8


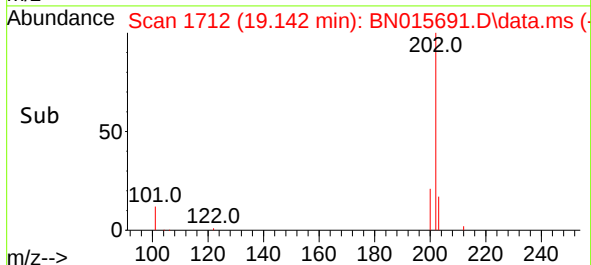




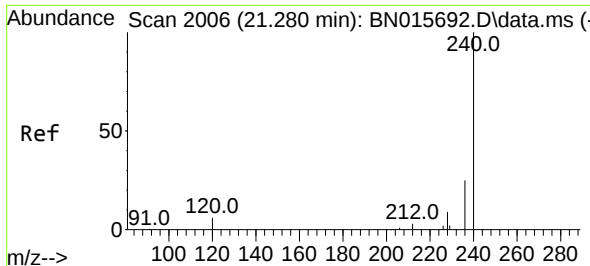

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.281 min Scan# 2006
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:240 Resp: 60001
Ion Ratio Lower Upper
240 100
120 6.4 4.9 7.3
236 25.6 20.4 30.6

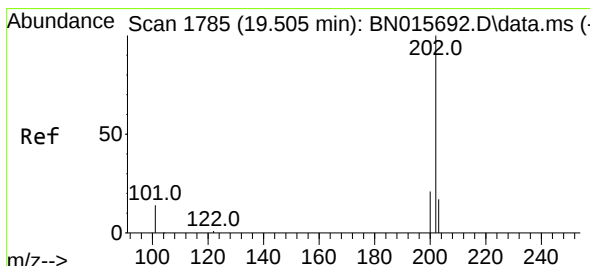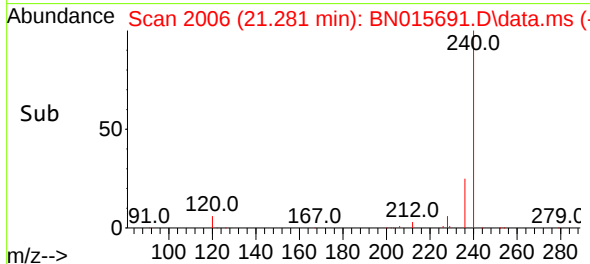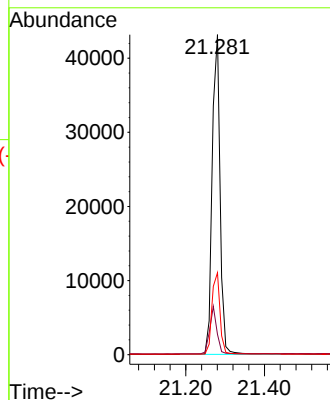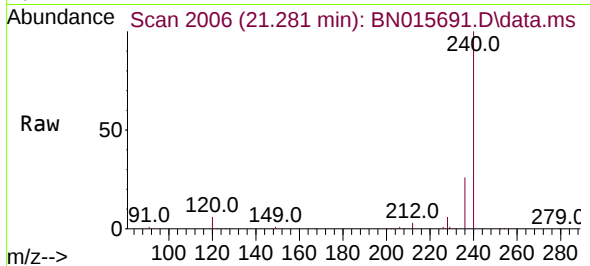

#30
Pyrene
Concen: 0.19 ng
RT: 19.510 min Scan# 1786
Delta R.T. 0.005 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:202 Resp: 41534
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.5 13.9 20.9


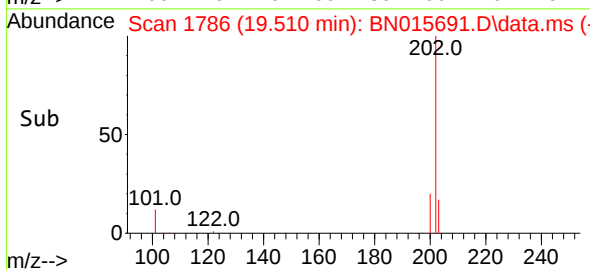
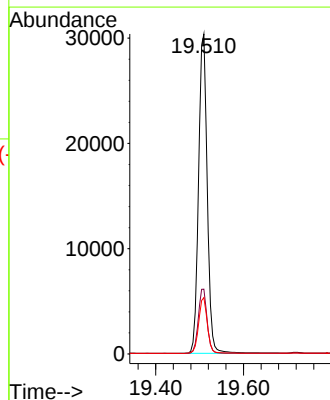
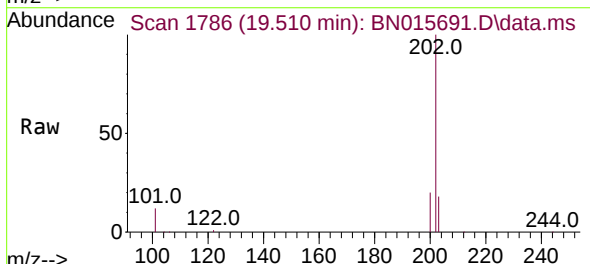




#31
Terphenyl-d14
Concen: 0.21 ng
RT: 19.723 min Scan# 1829
Delta R.T. 0.005 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:244 Resp: 30349
Ion Ratio Lower Upper
244 100
212 7.5 6.2 9.2
122 12.2 10.9 16.3

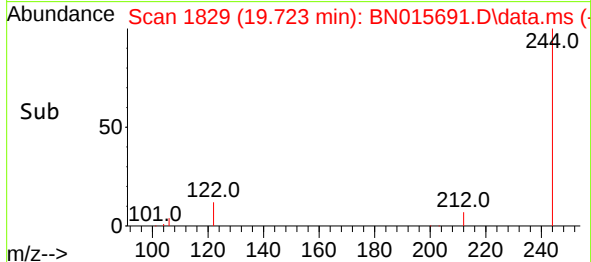

#32
Benzo(a)anthracene
Concen: 0.21 ng
RT: 21.259 min Scan# 2004
Delta R.T. 0.000 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:228 Resp: 39133
Ion Ratio Lower Upper
228 100
226 27.3 21.2 31.8
229 19.7 15.5 23.3

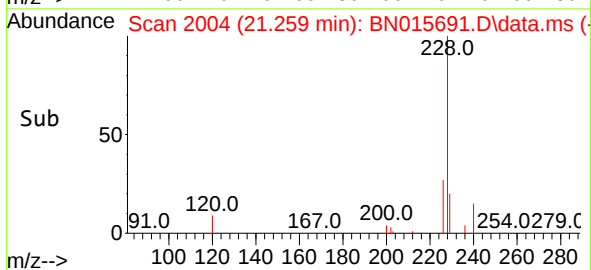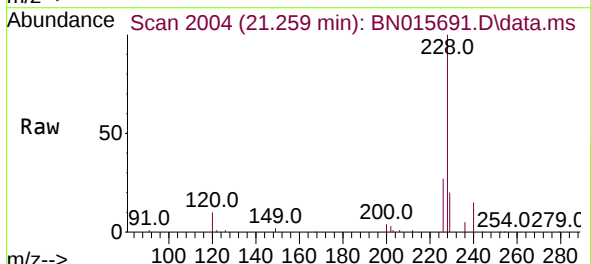

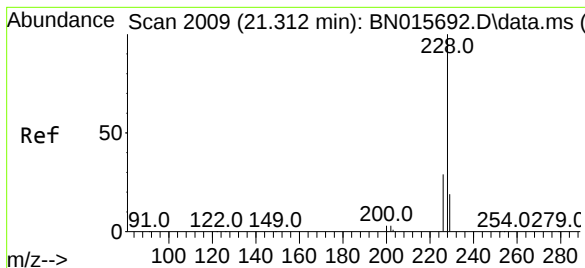

#33

Chrysene

Concen: 0.20 ng

RT: 21.312 min Scan# 2009

Delta R.T. 0.000 min

Lab File: BN015691.D

Acq: 24 Jul 2021 17:36

Tgt Ion:228 Resp: 40854

Ion Ratio Lower Upper

228 100

226 29.8 23.4 35.0





229 19.8 15.5 23.3

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.2

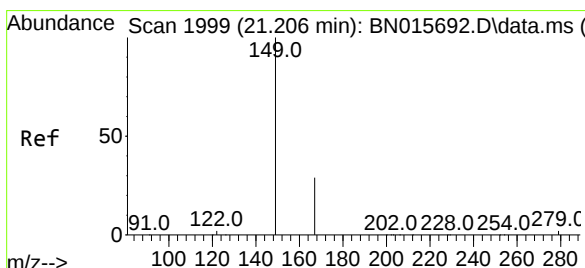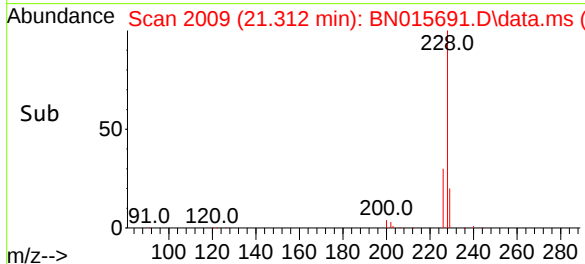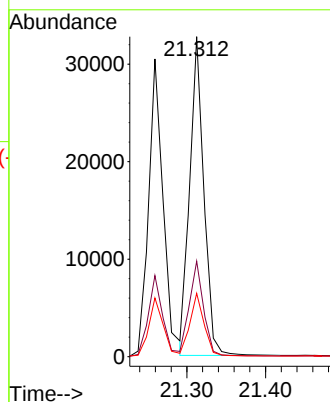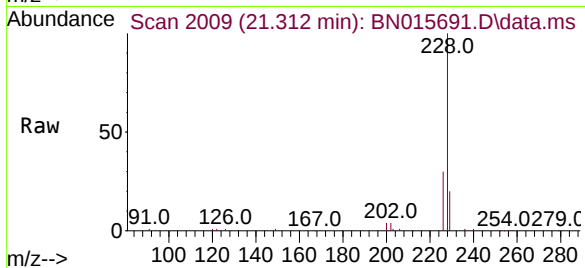

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.20 ng

RT: 21.206 min Scan# 1999

Delta R.T. 0.000 min

Lab File: BN015691.D

Acq: 24 Jul 2021 17:36




Tgt Ion:149 Resp: 15898


Ion Ratio Lower Upper

149 100

167 28.3 22.6 34.0


279 3.8 2.8 4.2

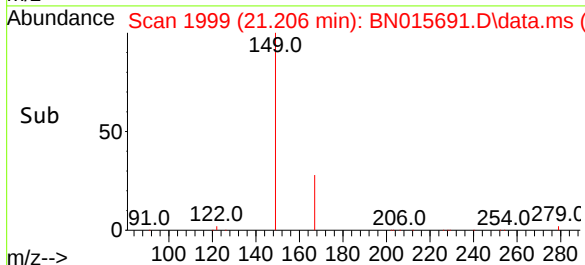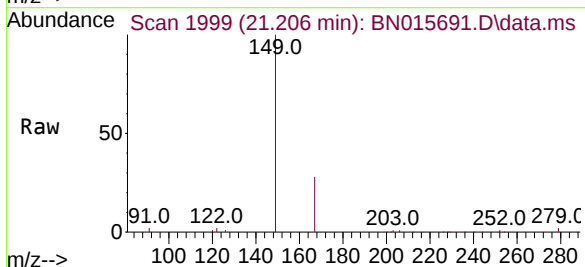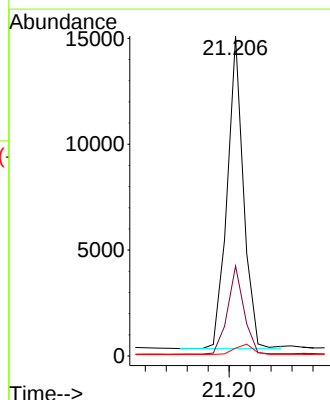






#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.567 min Scan# 2451
 Delta R.T. 0.003 min
 Lab File: BN015691.D
 Acq: 24 Jul 2021 17:36

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2







Tgt Ion:	264	Resp:	60517
Ion Ratio	Lower	Upper	
264	100		
260	25.0	19.8	29.8
265	24.0	19.0	28.6



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.21 ng
 RT: 25.901 min Scan# 3133
 Delta R.T. 0.003 min
 Lab File: BN015691.D
 Acq: 24 Jul 2021 17:36

Tgt Ion:	276	Resp:	46685
Ion Ratio	Lower	Upper	
276	100		
138	29.7	23.0	34.4
277	25.1	20.0	30.0


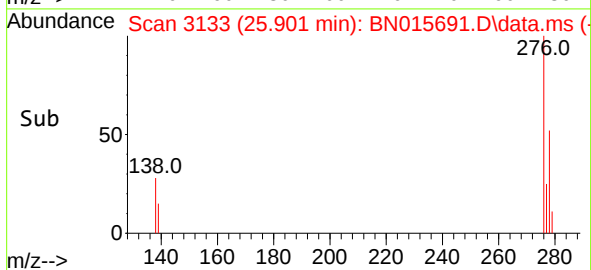






#37
Benzo(b)fluoranthene
Concen: 0.18 ng
RT: 22.875 min Scan# 2249
Delta R.T. 0.003 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:252 Resp: 41419
Ion Ratio Lower Upper
252 100
253 22.7 17.5 26.3
125 11.5 8.9 13.3

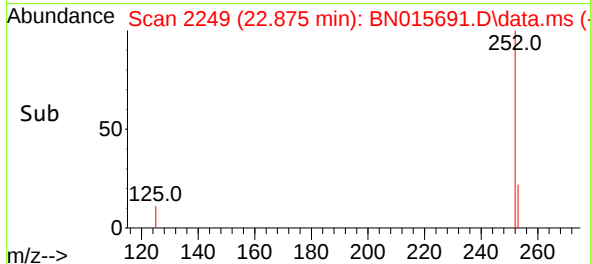

#38
Benzo(k)fluoranthene
Concen: 0.20 ng
RT: 22.920 min Scan# 2262
Delta R.T. 0.003 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Tgt Ion:252 Resp: 44777
Ion Ratio Lower Upper
252 100
253 22.6 17.6 26.4
125 12.3 9.4 14.2

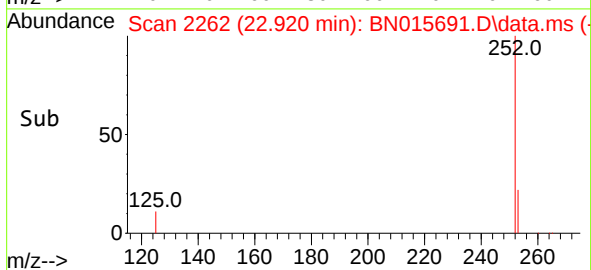



#39

Benzo(a)pyrene

Concen: 0.20 ng





RT: 23.464 min Scan# 2421

Delta R.T. 0.003 min

Lab File: BN015691.D

Acq: 24 Jul 2021 17:36

Tgt Ion:252	Resp:	36817
Ion Ratio	Lower	Upper
252	100	
253	23.3	17.7 26.5
125	13.6	10.2 15.2

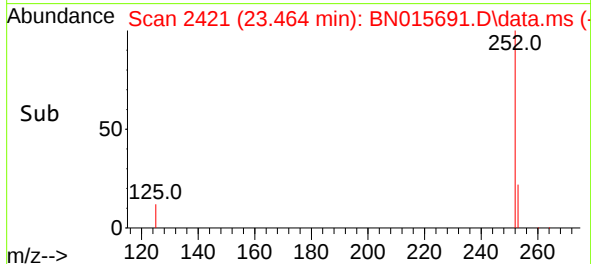

#40

Dibenzo(a,h)anthracene

Concen: 0.22 ng




RT: 25.922 min Scan# 3139


Delta R.T. 0.003 min

Lab File: BN015691.D

Acq: 24 Jul 2021 17:36

Tgt Ion:278	Resp:	38256
Ion Ratio	Lower	Upper
278	100	
139	19.6	15.1 22.7
279	24.3	19.0 28.4

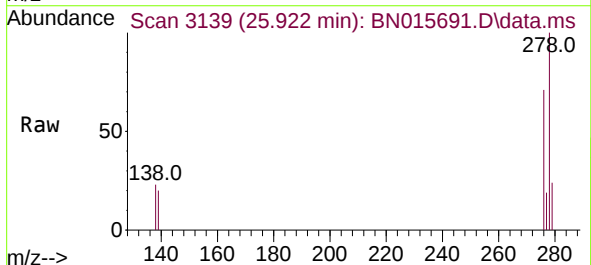

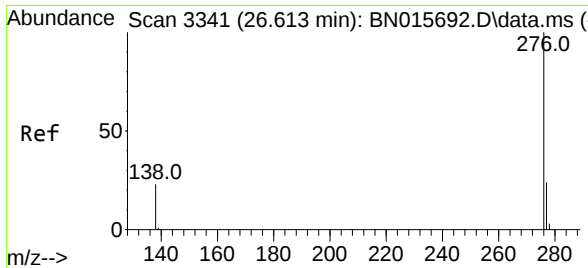

#41
Benzo(g,h,i)perylene
Concen: 0.19 ng
RT: 26.616 min Scan# 3342
Delta R.T. 0.003 min
Lab File: BN015691.D
Acq: 24 Jul 2021 17:36

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Tgt Ion:276 Resp: 38116
Ion Ratio Lower Upper
276 100
277 23.9 19.4 29.0
138 24.1 19.0 28.6

