
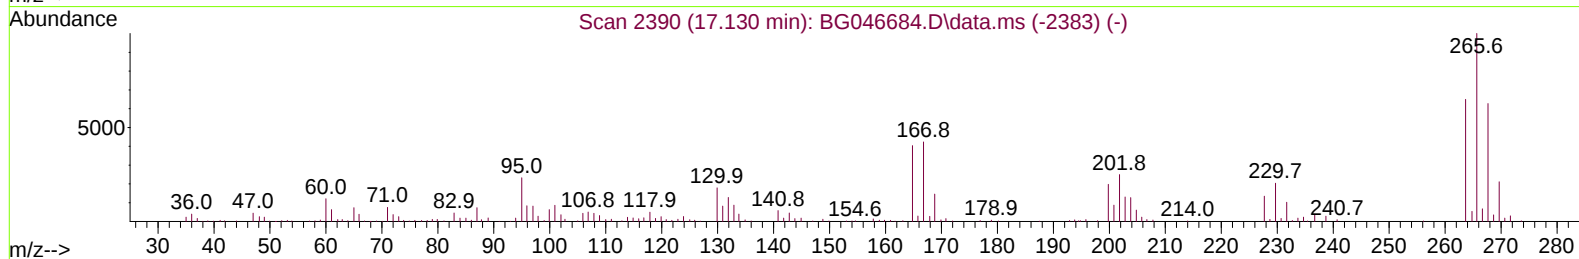
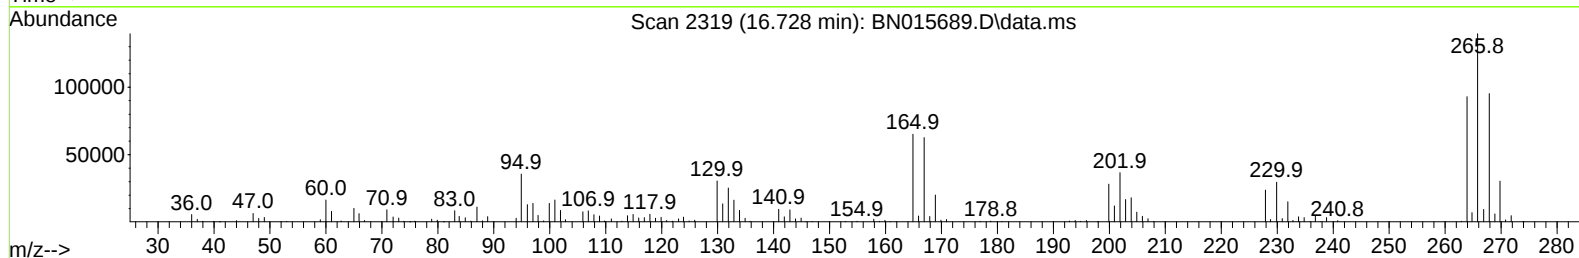


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
Data File : BN015689.D
Acq On : 24 Jul 2021 15:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 06:53:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:53:05 2021
Response via : Initial Calibration

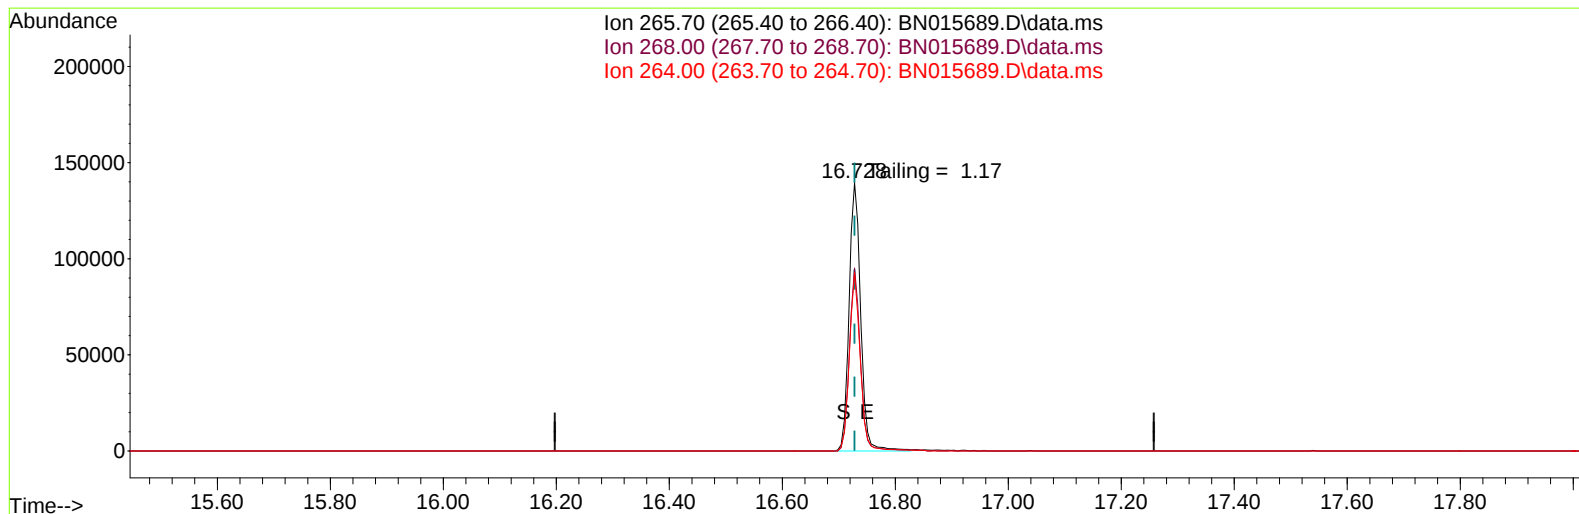

TIC: BN015689.D\data.ms

(70) Pentachlorophenol (C)




16.728min (0.000) 26744.29 ng

response 200018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.21
264.00	61.60	66.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
Data File : BN015689.D
Acq On : 24 Jul 2021 15:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 06:53:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 06:53:05 2021
Response via : Initial Calibration

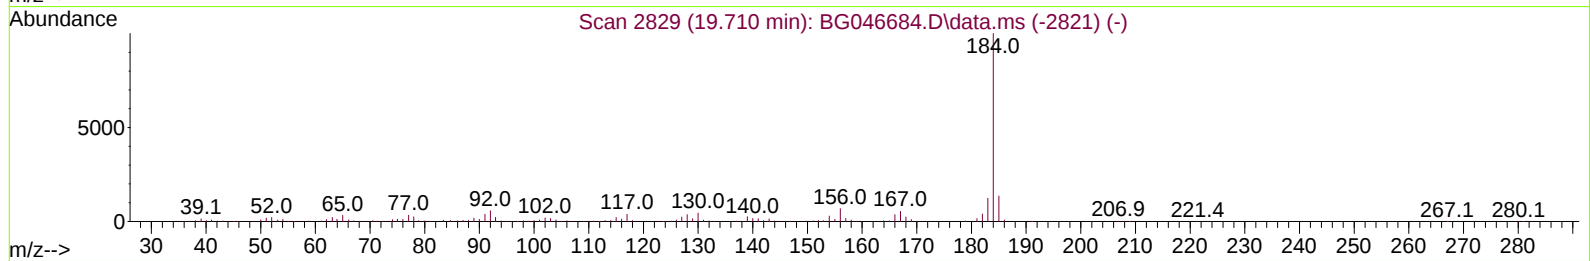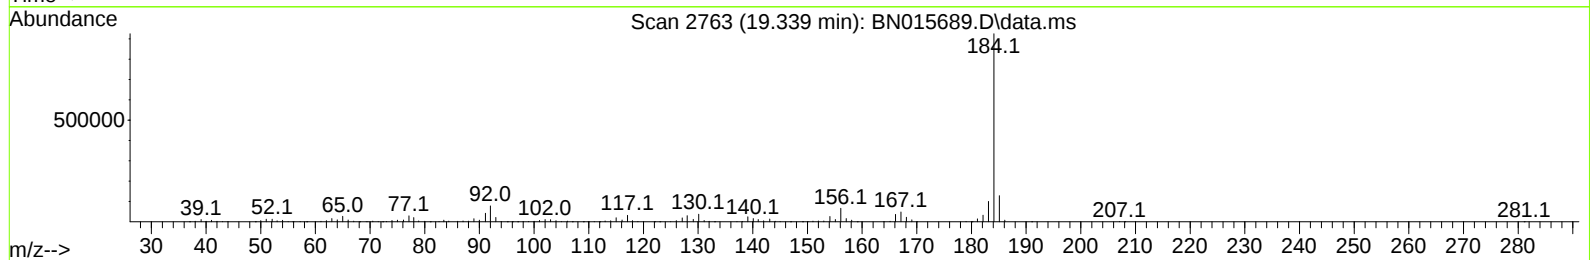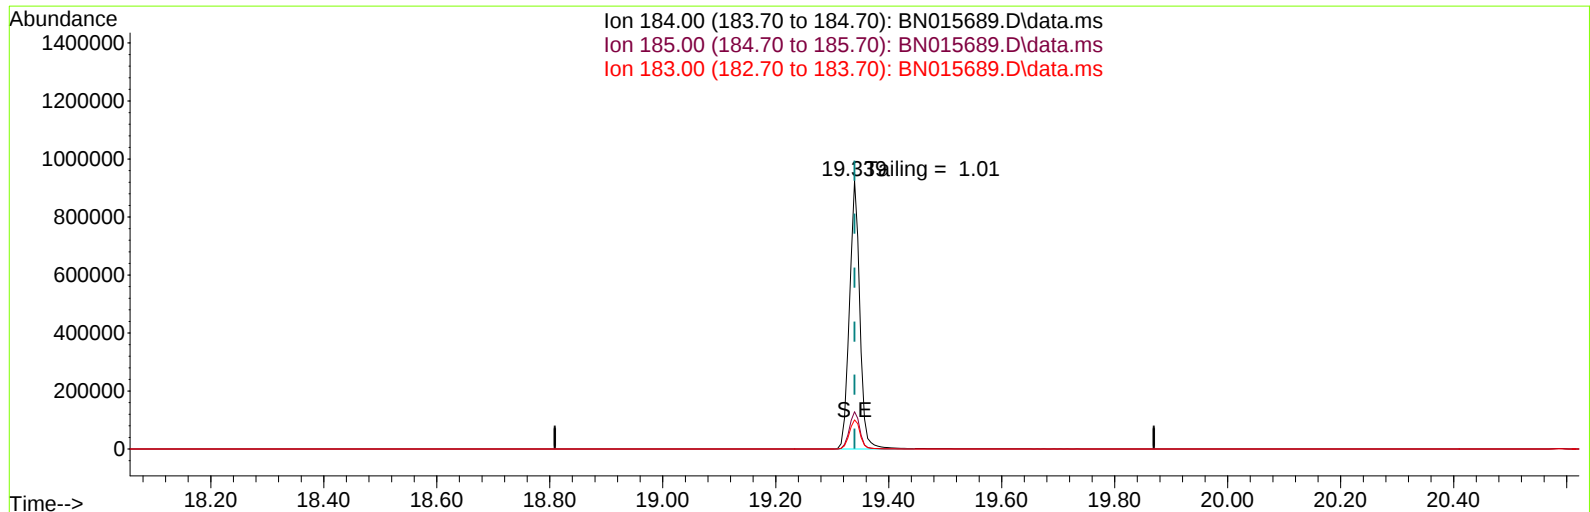

TIC: BN015689.D\data.ms

(77) Benzidine

19.339min (0.000) 0.00 ng

response 1187049

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.90
183.00	13.20	10.87
0.00	0.00	0.00