

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
 Data File : BN015692.D
 Acq On : 24 Jul 2021 18:13
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Jul 26 01:35:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 26 01:23:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	13917	0.400	ng	0.00
7) Naphthalene-d8	10.470	136	63092	0.400	ng	0.00
13) Acenaphthene-d10	14.319	164	34700	0.400	ng	0.00
19) Phenanthrene-d10	17.078	188	67562	0.400	ng	0.00
29) Chrysene-d12	21.280	240	65853	0.400	ng	0.00
35) Perylene-d12	23.563	264	65232	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	14378	0.429	ng	0.00
5) Phenol-d6	6.868	99	17222	0.438	ng	0.00
8) Nitrobenzene-d5	8.835	82	16741	0.379	ng	0.00
11) 2-Methylnaphthalene-d10	12.065	152	37749	0.401	ng	0.00
14) 2,4,6-Tribromophenol	15.817	330	5249	0.486	ng	0.00
15) 2-Fluorobiphenyl	12.949	172	52699	0.373	ng	0.00
27) Fluoranthene-d10	19.113	212	70414	0.391	ng	0.00
31) Terphenyl-d14	19.718	244	59885	0.382	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.226	88	1812	0.436	ng	# 94
3) n-Nitrosodimethylamine	3.585	42	3950	0.385	ng	98
6) bis(2-Chloroethyl)ether	7.126	93	15920	0.403	ng	100
9) Naphthalene	10.521	128	65634	0.392	ng	100
10) Hexachlorobutadiene	10.812	225	12331	0.387	ng	# 100
12) 2-Methylnaphthalene	12.141	142	43875	0.406	ng	100
16) Acenaphthylene	14.040	152	56250	0.388	ng	100
17) Acenaphthene	14.383	154	38885	0.386	ng	100
18) Fluorene	15.373	166	47932	0.399	ng	100
20) 4,6-Dinitro-2-methylph...	15.461	198	759	0.165	ng	100
21) 4-Bromophenyl-phenylether	16.275	248	14877	0.378	ng	100
22) Hexachlorobenzene	16.385	284	16817	0.376	ng	100
23) Atrazine	16.543	200	10257	0.438	ng	100
24) Pentachlorophenol	16.725	266	4284	0.423	ng	100
25) Phenanthrene	17.115	178	78318	0.384	ng	100
26) Anthracene	17.200	178	65840	0.389	ng	100
28) Fluoranthene	19.142	202	88254	0.401	ng	100
30) Pyrene	19.505	202	89968	0.380	ng	100
32) Benzo(a)anthracene	21.259	228	86236	0.418	ng	100
33) Chrysene	21.312	228	87222	0.381	ng	100
34) Bis(2-ethylhexyl)phtha...	21.206	149	36808	0.426	ng	100
36) Indeno(1,2,3-cd)pyrene	25.898	276	98203	0.415	ng	100
37) Benzo(b)fluoranthene	22.872	252	89076	0.363	ng	100
38) Benzo(k)fluoranthene	22.916	252	92248	0.376	ng	100
39) Benzo(a)pyrene	23.460	252	78114	0.393	ng	100
40) Dibenzo(a,h)anthracene	25.918	278	80327	0.432	ng	100
41) Benzo(g,h,i)perylene	26.613	276	79911	0.369	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
Data File : BN015692.D
Acq On : 24 Jul 2021 18:13
Operator : CG/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Jul 26 01:35:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 01:23:47 2021
Response via : Initial Calibration




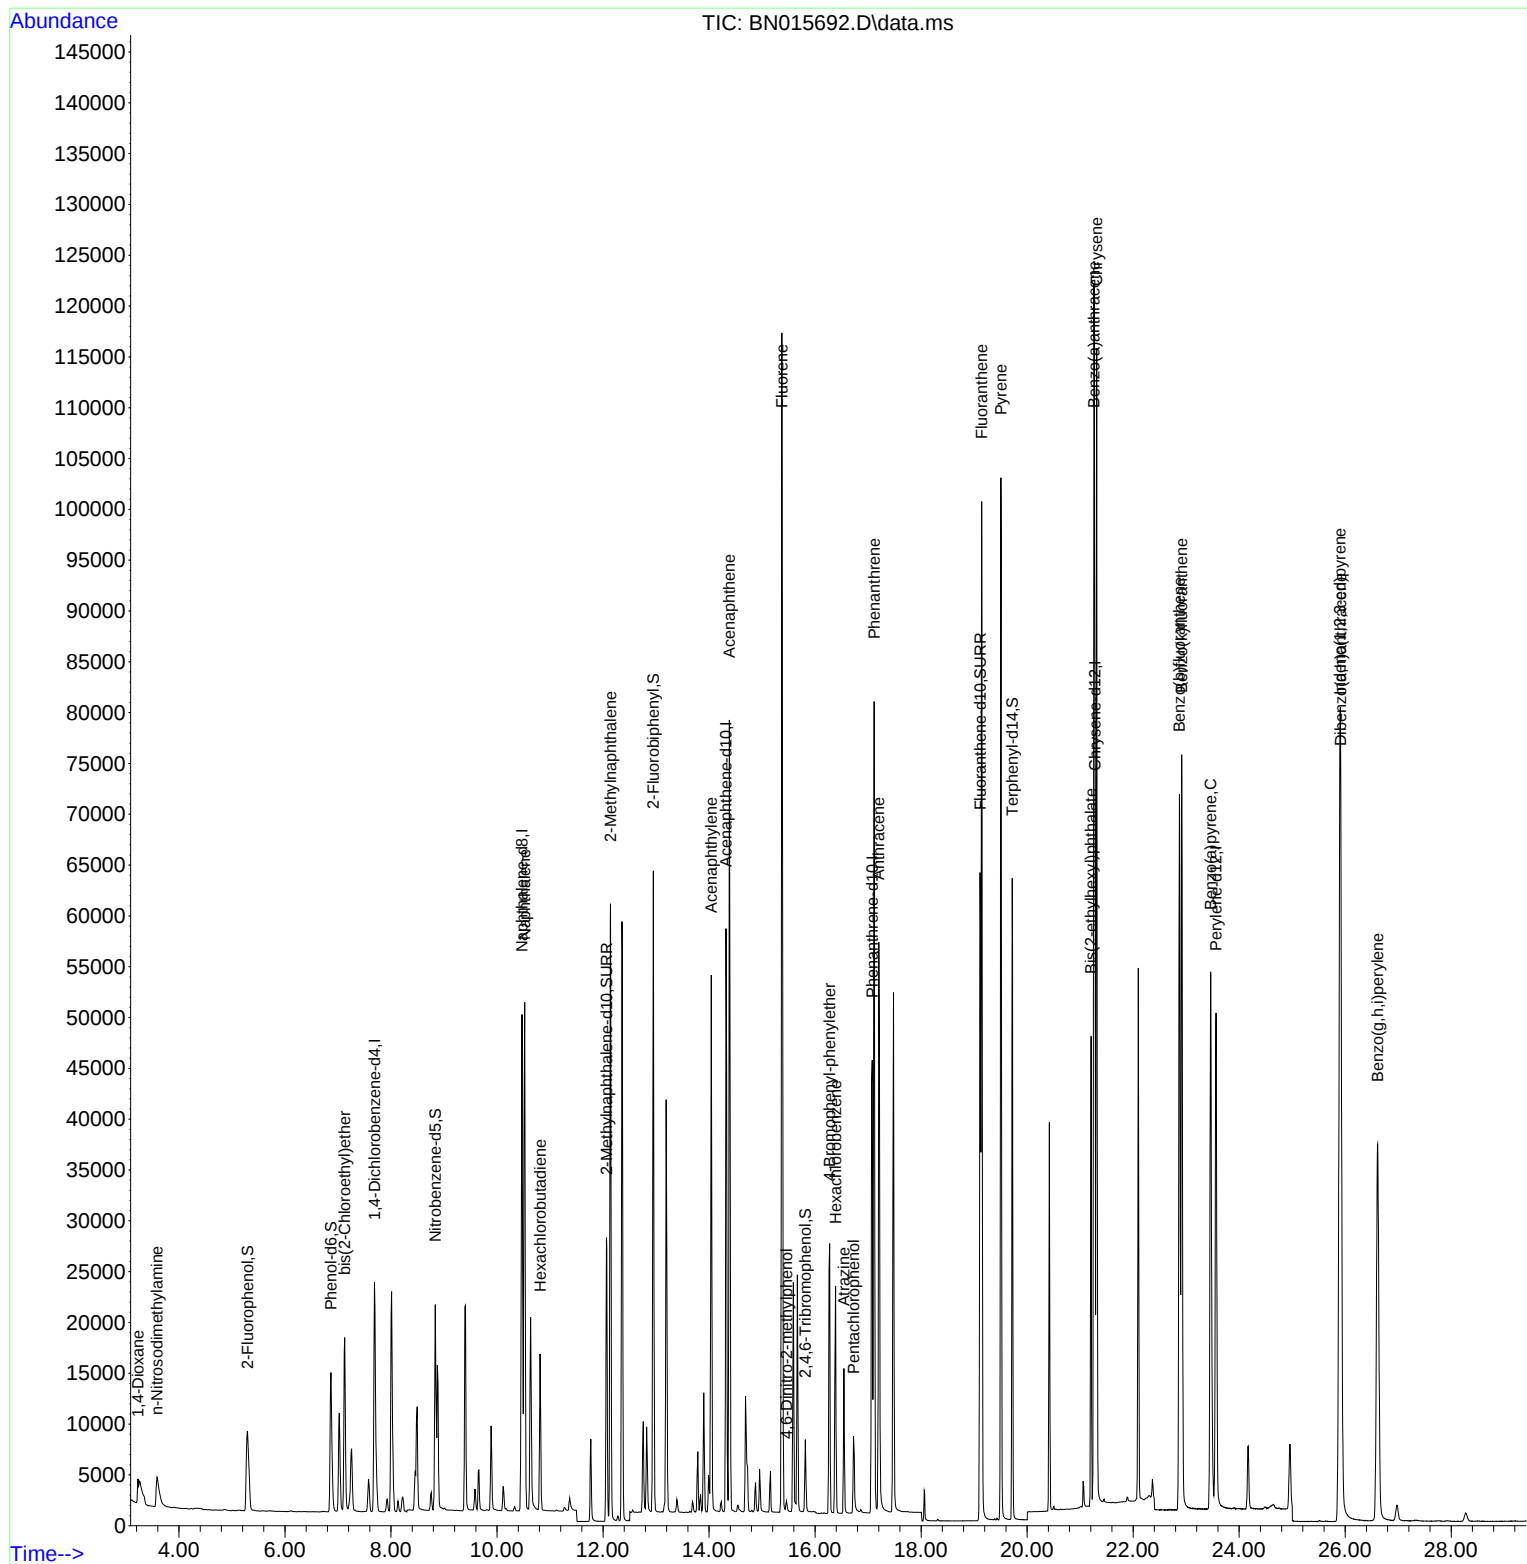




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.688 min Scan# 500
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 13917
Ion Ratio Lower Upper
152 100
150 156.5 125.2 187.8
115 60.8 48.6 73.0

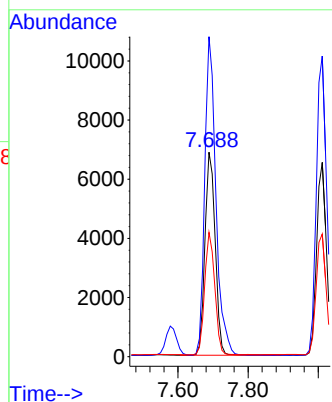

#2
1,4-Dioxane
Concen: 0.436 ng
RT: 3.226 min Scan# 16
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion: 88 Resp: 1812
Ion Ratio Lower Upper
88 100
43 26.2 0.0 0.0#
58 62.4 53.8 80.6


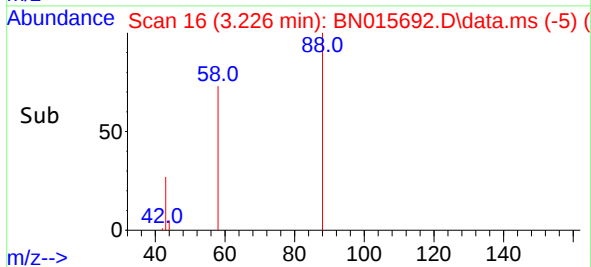
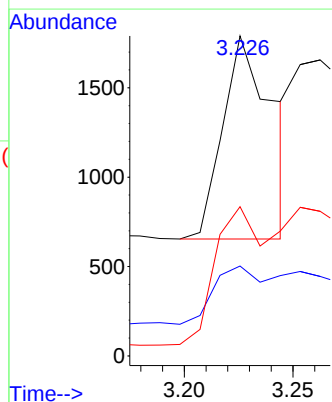
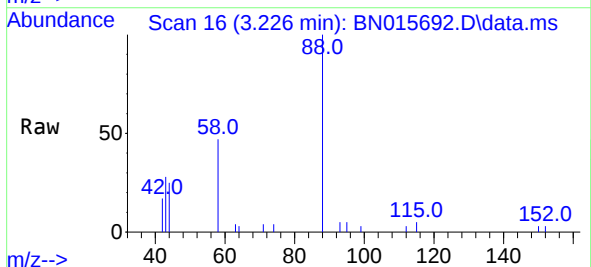




#3
n-Nitrosodimethylamine
Concen: 0.385 ng
RT: 3.585 min Scan# 55
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 42 Resp: 3950
Ion Ratio Lower Upper
42 100
74 156.1 126.7 190.1
44 7.2 5.8 8.8

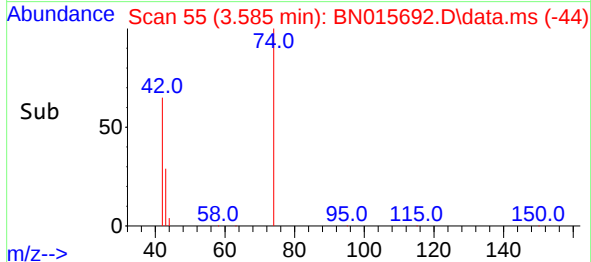

#4
2-Fluorophenol
Concen: 0.429 ng
RT: 5.291 min Scan# 240
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion: 112 Resp: 14378
Ion Ratio Lower Upper
112 100
64 56.1 44.8 67.2
63 27.8 22.2 33.4


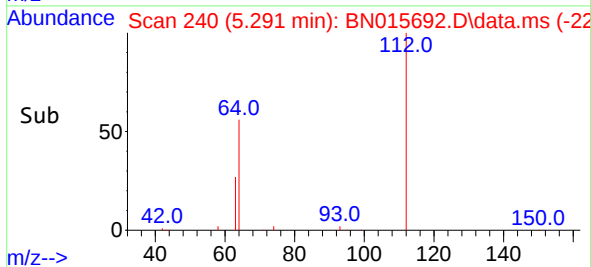

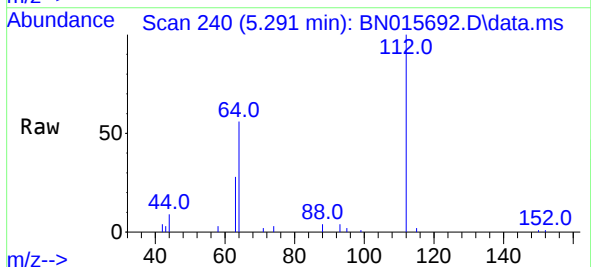




#5
Phenol-d6
Concen: 0.438 ng
RT: 6.868 min Scan# 411
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 99 Resp: 17222
Ion Ratio Lower Upper
99 100
42 16.7 13.4 20.0
71 30.6 24.5 36.7



#6
bis(2-Chloroethyl)ether
Concen: 0.403 ng
RT: 7.126 min Scan# 439
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion: 93 Resp: 15920
Ion Ratio Lower Upper
93 100
63 74.8 59.8 89.8
95 33.0 26.4 39.6


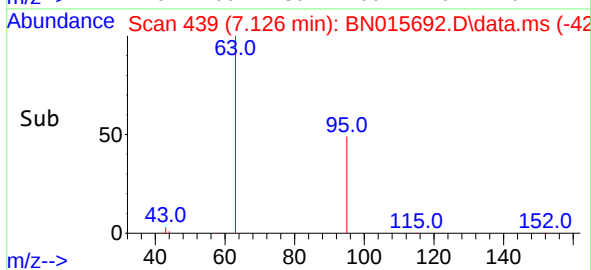






#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.470 min Scan# 738
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	136	Resp:	63092
Ion Ratio	Lower	Upper	
136	100		
137	11.1	8.9	13.3
54	6.2	5.0	7.4
68	5.4	4.3	6.5



#8
Nitrobenzene-d5
Concen: 0.379 ng
RT: 8.835 min Scan# 609
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:	82	Resp:	16741
Ion Ratio	Lower	Upper	
82	100		
128	40.0	32.0	48.0
54	48.6	38.9	58.3



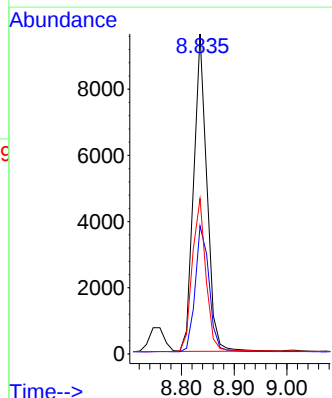





#9
Naphthalene
Concen: 0.392 ng
RT: 10.521 min Scan# 742
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	128	Resp:	65634
Ion	Ratio	Lower	Upper
128	100		
129	11.1	8.9	13.3
127	13.0	10.4	15.6

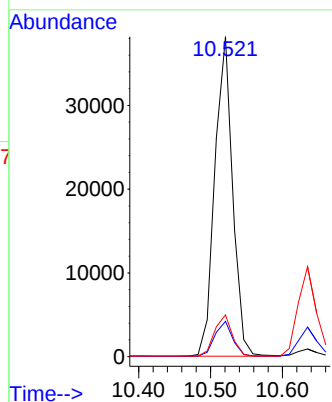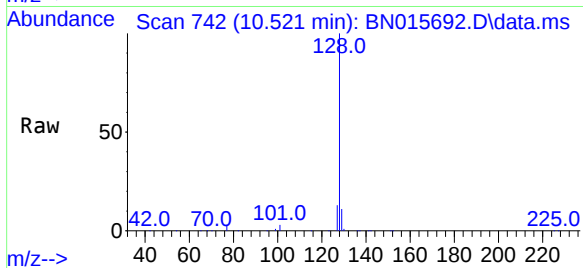

#10
Hexachlorobutadiene
Concen: 0.387 ng
RT: 10.812 min Scan# 765
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:	225	Resp:	12331
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.9	51.1	76.7


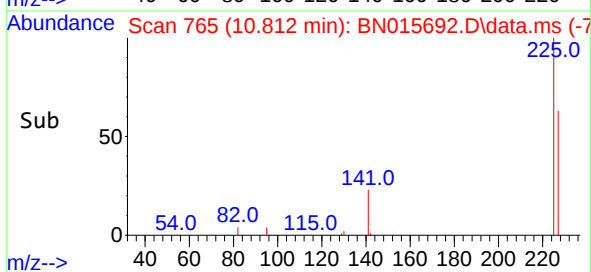

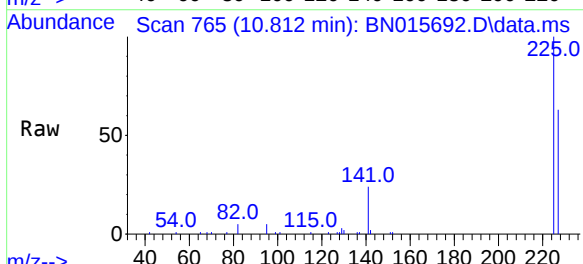


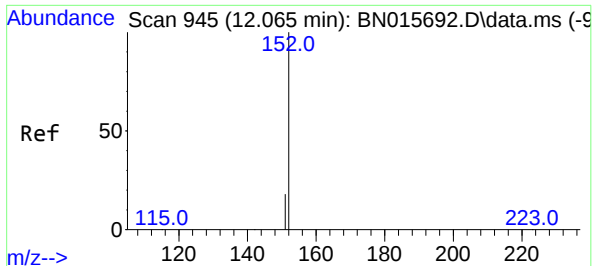

#11
2-Methylnaphthalene-d10
Concen: 0.401 ng
RT: 12.065 min Scan# 945
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 37749
Ion Ratio Lower Upper
152 100
151 20.4 16.3 24.5

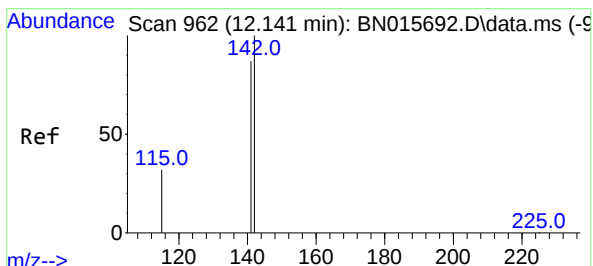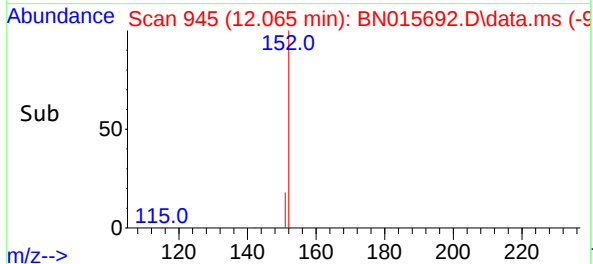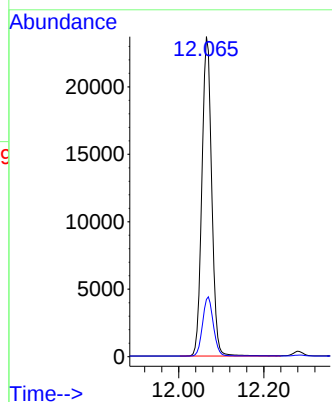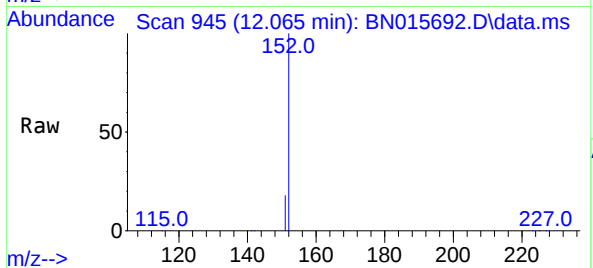

#12
2-Methylnaphthalene
Concen: 0.406 ng
RT: 12.141 min Scan# 962
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:142 Resp: 43875
Ion Ratio Lower Upper
142 100
141 86.8 69.4 104.2
115 32.4 25.9 38.9


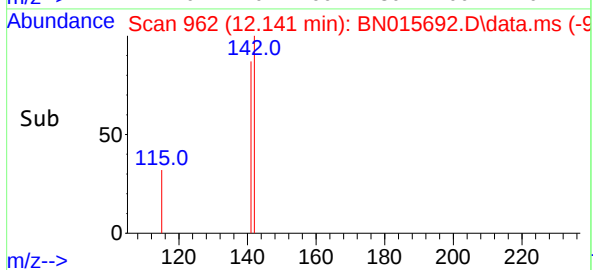
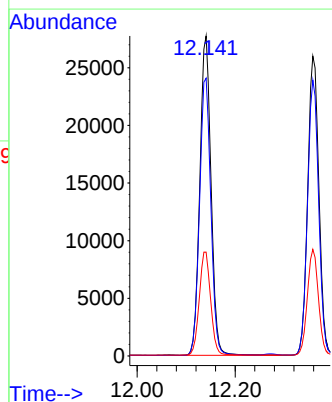
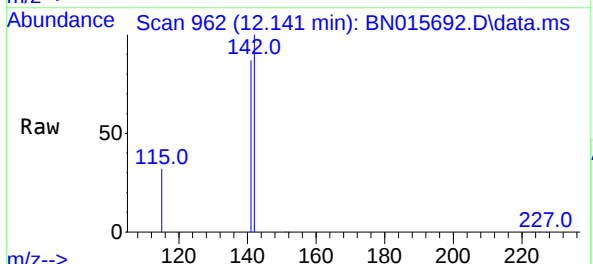




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.319 min Scan# 1187
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:164 Resp: 34700
Ion Ratio Lower Upper
164 100
162 104.5 83.6 125.4
160 48.3 38.6 58.0

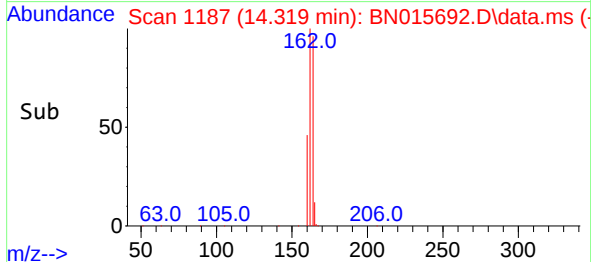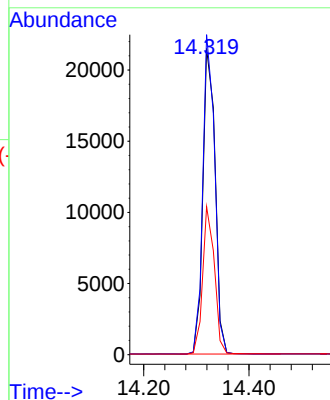

#14
2,4,6-Tribromophenol
Concen: 0.486 ng
RT: 15.817 min Scan# 1305
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:330 Resp: 5249
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 35.5 28.5 42.7

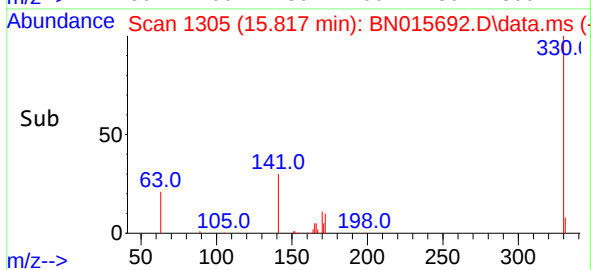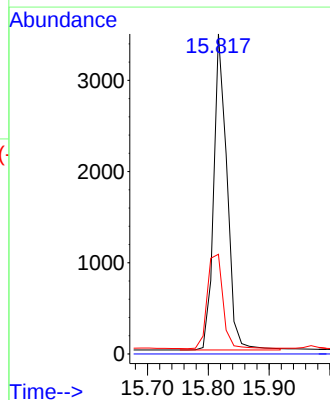







#15
2-Fluorobiphenyl
Concen: 0.373 ng
RT: 12.949 min Scan# 1079
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:172 Resp: 52699




Ion	Ratio	Lower	Upper
172	100		
171	34.2	27.4	41.0
170	22.4	17.9	26.9

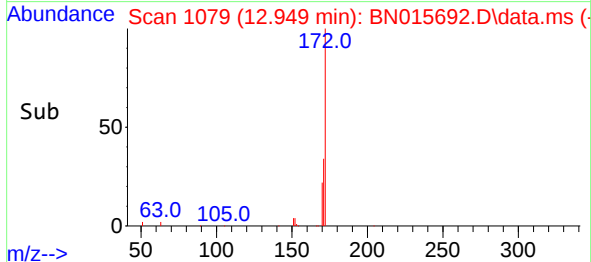


#16
Acenaphthylene
Concen: 0.388 ng
RT: 14.040 min Scan# 1165
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:152 Resp: 56250

Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.4	23.2
153	13.0	10.4	15.6


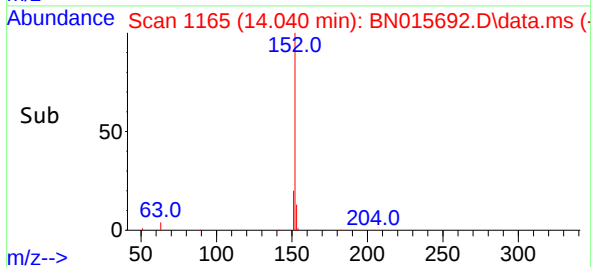

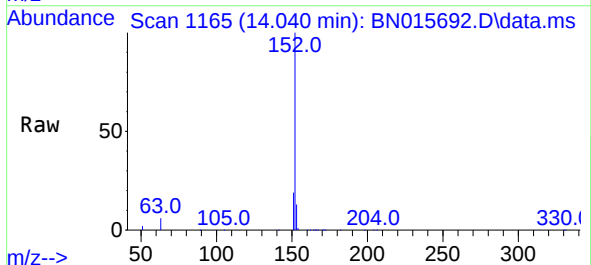




#17
Acenaphthene
Concen: 0.386 ng
RT: 14.383 min Scan# 1192
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 38885
Ion Ratio Lower Upper
154 100
153 111.3 89.0 133.6
152 54.1 43.3 64.9

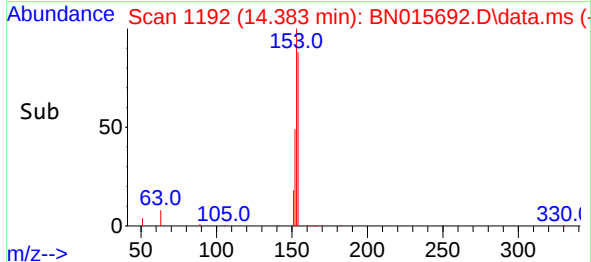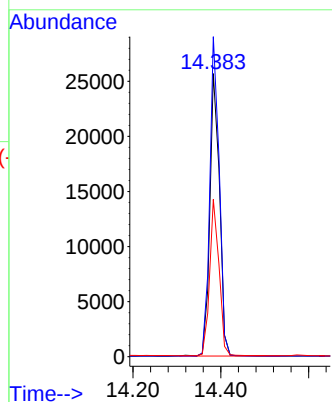

#18
Fluorene
Concen: 0.399 ng
RT: 15.373 min Scan# 1270
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:166 Resp: 47932
Ion Ratio Lower Upper
166 100
165 97.4 77.9 116.9
167 13.5 10.8 16.2


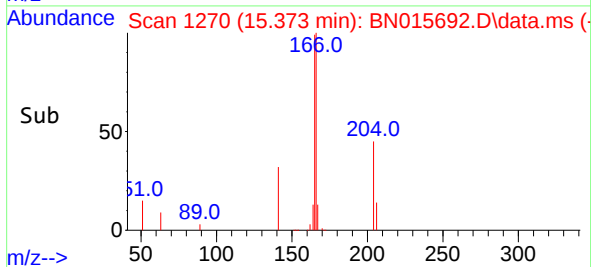
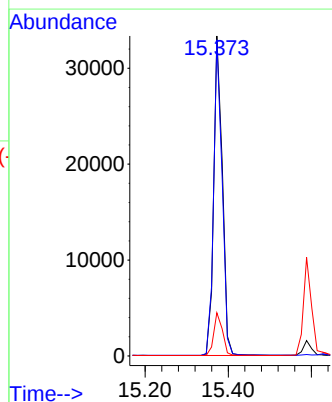
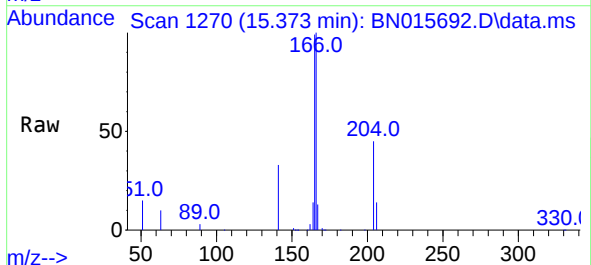




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.078 min Scan# 1408
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:188	Resp:	67562
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	6.6	5.3



#20
4,6-Dinitro-2-methylphenol
Concen: 0.165 ng
RT: 15.461 min Scan# 1277
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:198	Resp:	759
Ion Ratio	Lower	Upper
198	100	
182	20.5	16.4
77	0.0	0.0


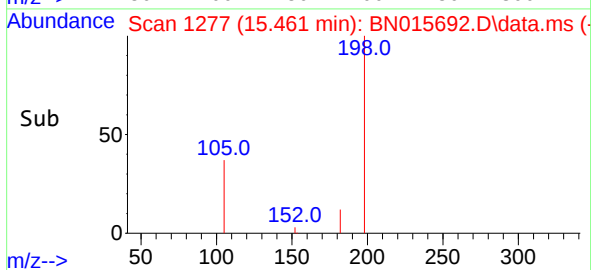




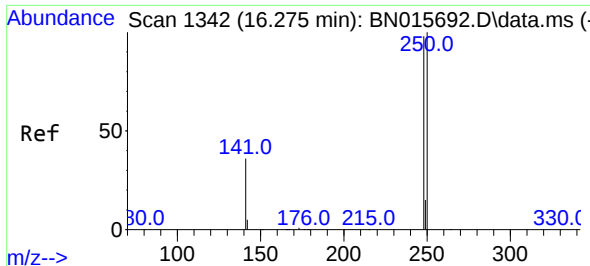

#21
4-Bromophenyl-phenylether
Concen: 0.378 ng
RT: 16.275 min Scan# 1342
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	248	Resp:	14877
Ion	Ratio	Lower	Upper
248	100		
250	102.0	81.6	122.4
141	36.7	29.4	44.0

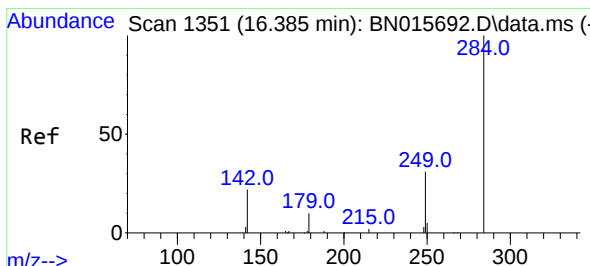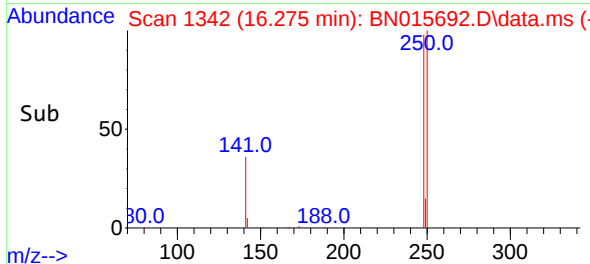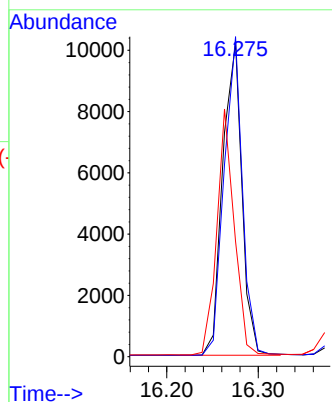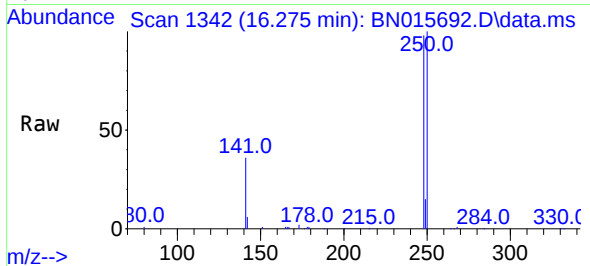

#22
Hexachlorobenzene
Concen: 0.376 ng
RT: 16.385 min Scan# 1351
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:	284	Resp:	16817
Ion	Ratio	Lower	Upper
284	100		
142	34.4	27.6	41.4
249	30.8	24.6	37.0


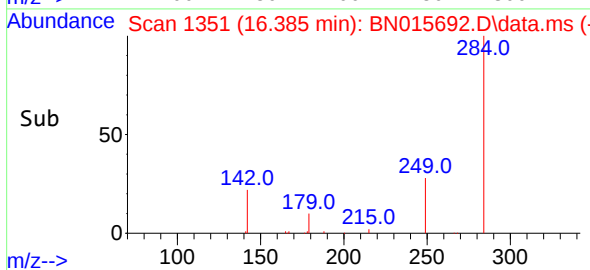

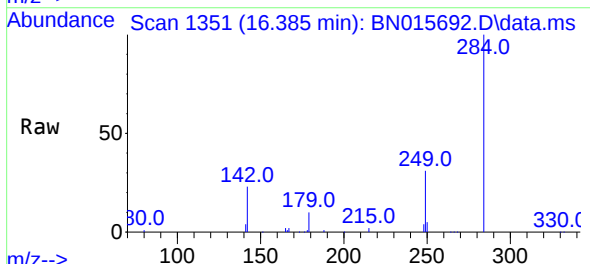


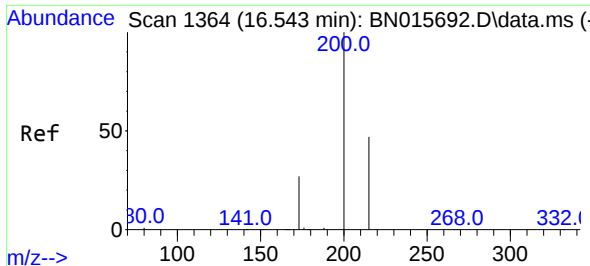

#23
Atrazine
Concen: 0.438 ng
RT: 16.543 min Scan# 1364
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	200	Resp:	10257
Ion Ratio	Lower	Upper	
200	100		
173	27.2	21.8	32.6
215	47.7	38.2	57.2

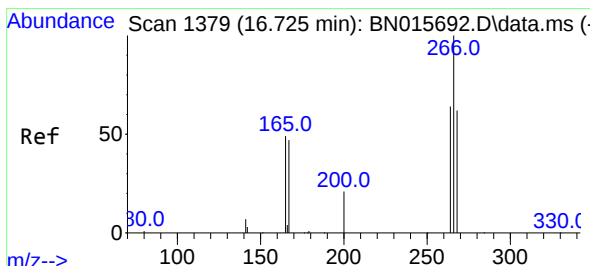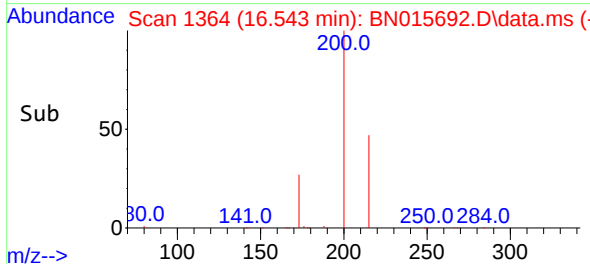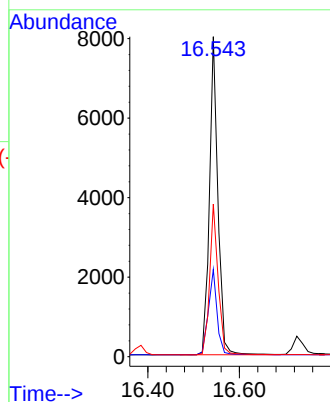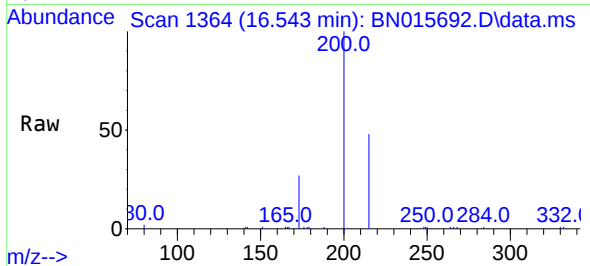

#24
Pentachlorophenol
Concen: 0.423 ng
RT: 16.725 min Scan# 1379
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:	266	Resp:	4284
Ion Ratio	Lower	Upper	
266	100		
264	61.9	49.9	74.9
268	63.7	50.8	76.2


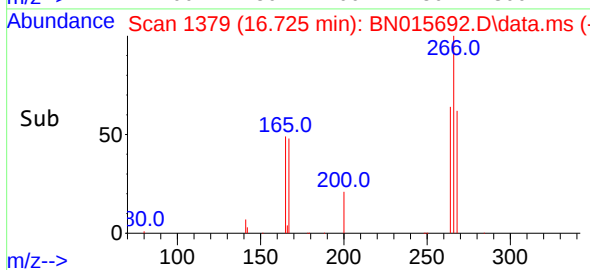
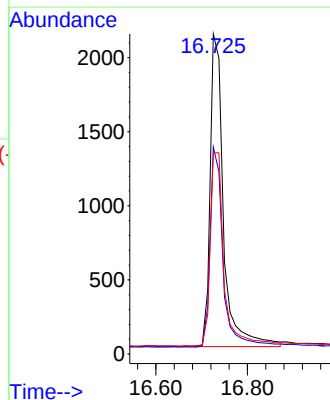
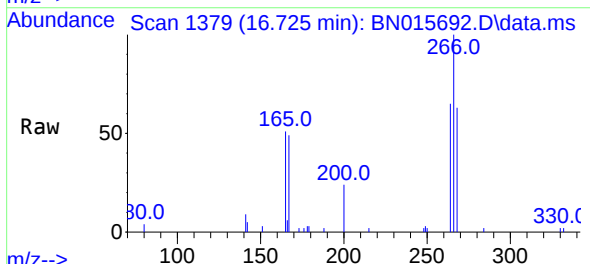




#25
Phenanthrene
Concen: 0.384 ng
RT: 17.115 min Scan# 1411
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 78318
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.5 12.4 18.6



#26
Anthracene
Concen: 0.389 ng
RT: 17.200 min Scan# 1418
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:178 Resp: 65840
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.2 12.2 18.2



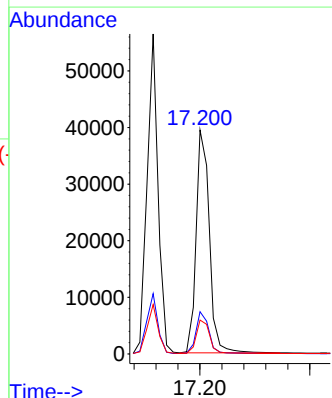





#27
Fluoranthene-d10
Concen: 0.391 ng
RT: 19.113 min Scan# 1706
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 70414
Ion Ratio Lower Upper
212 100
106 14.4 11.5 17.3
104 7.9 6.3 9.5

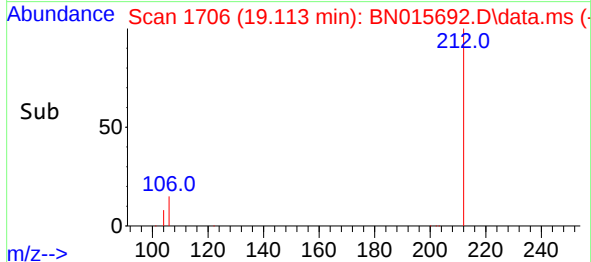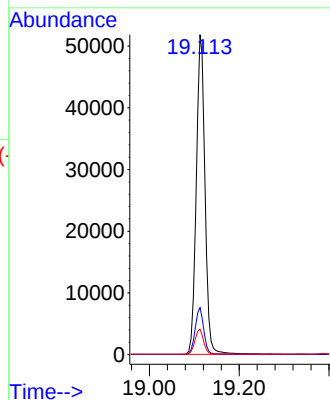

#28
Fluoranthene
Concen: 0.401 ng
RT: 19.142 min Scan# 1712
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:202 Resp: 88254
Ion Ratio Lower Upper
202 100
101 11.8 9.4 14.2
203 17.3 13.8 20.8


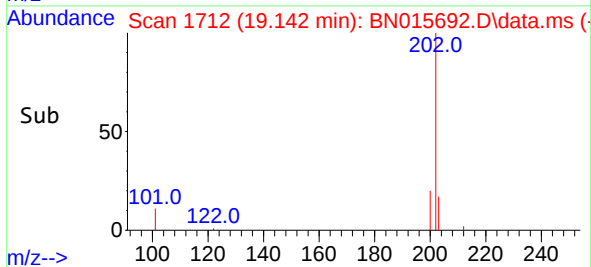
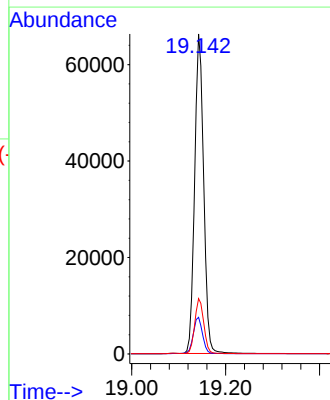
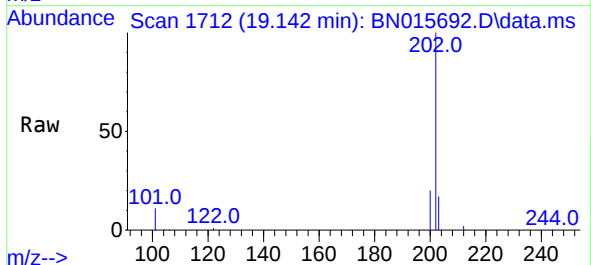


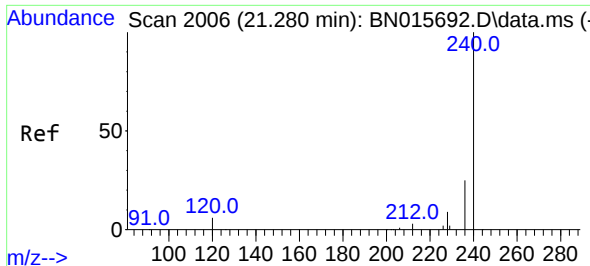

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.280 min Scan# 2006
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:240 Resp: 65853
Ion Ratio Lower Upper
240 100
120 6.1 4.9 7.3
236 25.5 20.4 30.6

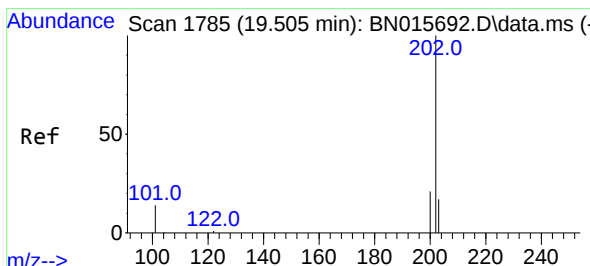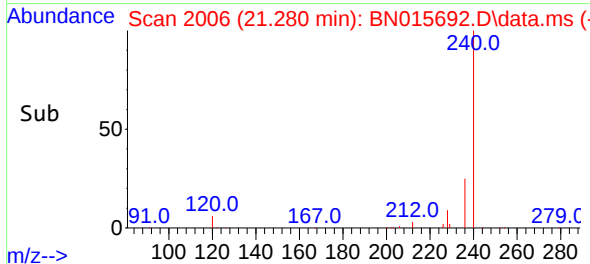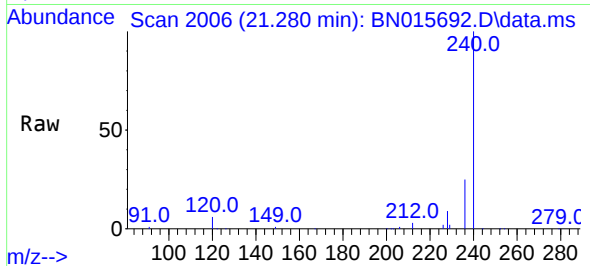

#30
Pyrene
Concen: 0.380 ng
RT: 19.505 min Scan# 1785
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:202 Resp: 89968
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.4 13.9 20.9


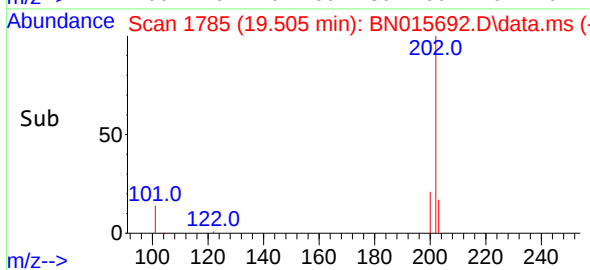

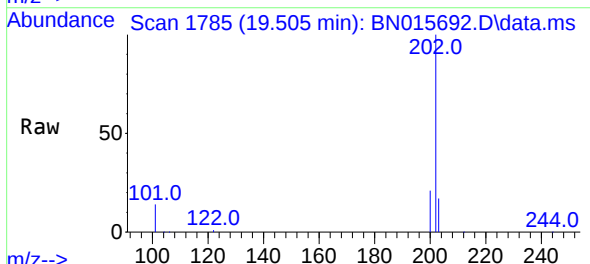


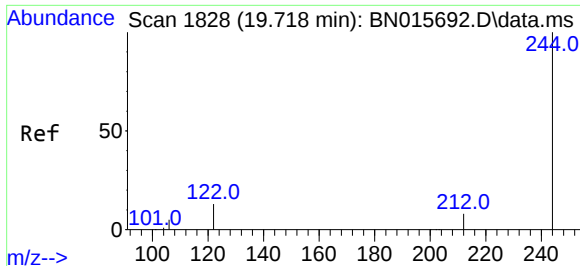

#31
Terphenyl-d14
Concen: 0.382 ng
RT: 19.718 min Scan# 1828
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:244 Resp: 59885
Ion Ratio Lower Upper
244 100
212 7.7 6.2 9.2
122 13.6 10.9 16.3

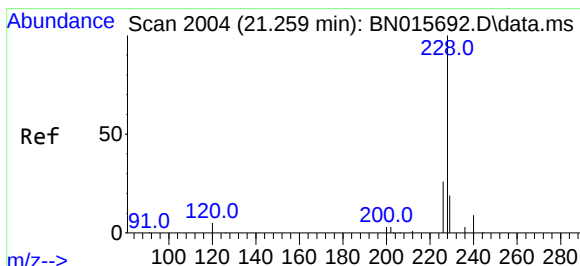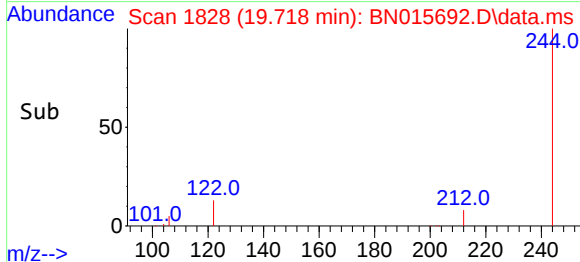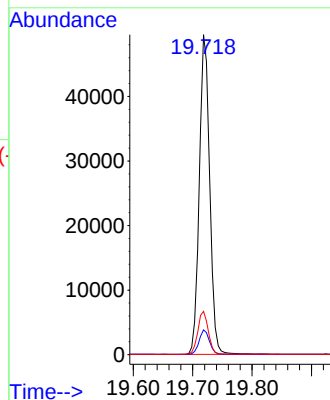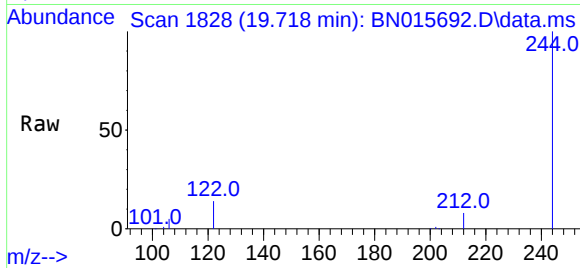

#32
Benzo(a)anthracene
Concen: 0.418 ng
RT: 21.259 min Scan# 2004
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:228 Resp: 86236
Ion Ratio Lower Upper
228 100
226 26.5 21.2 31.8
229 19.4 15.5 23.3


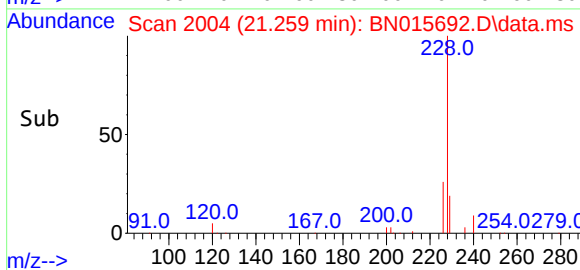
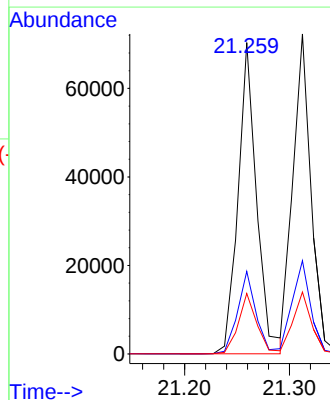
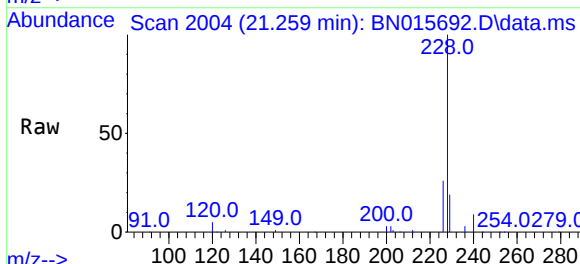


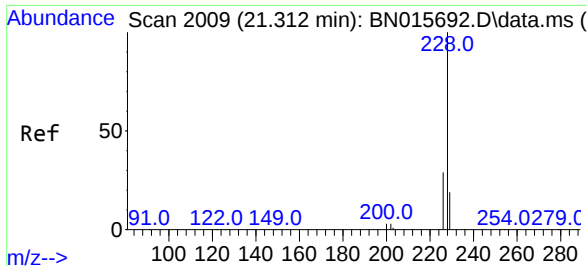

#33
Chrysene
Concen: 0.381 ng
RT: 21.312 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:	228	Resp:	87222
Ion Ratio	Lower	Upper	
228	100		
226	29.2	23.4	35.0
229	19.4	15.5	23.3

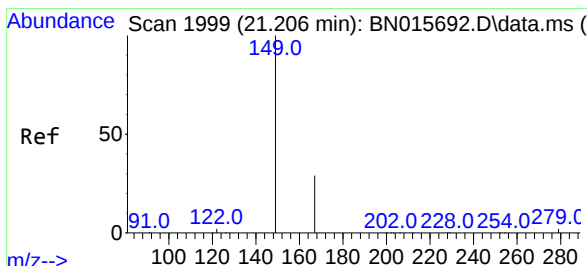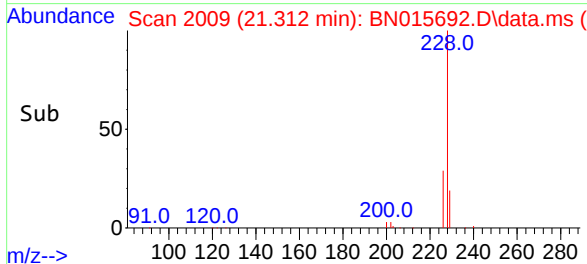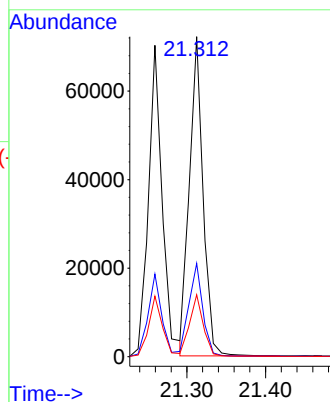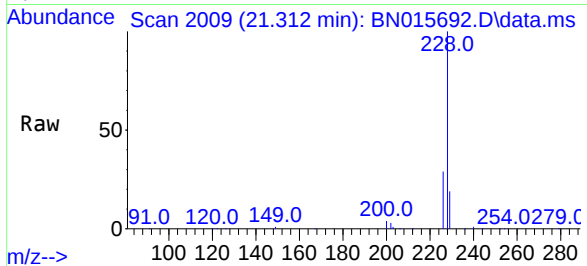

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.426 ng
RT: 21.206 min Scan# 1999
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:	149	Resp:	36808
Ion Ratio	Lower	Upper	
149	100		
167	28.3	22.6	34.0
279	3.5	2.8	4.2

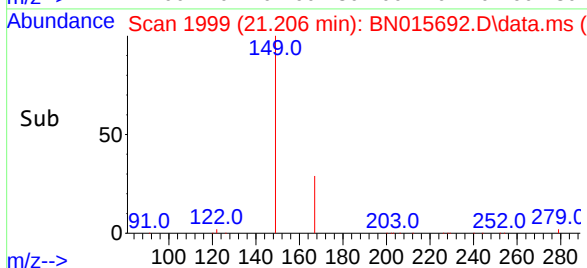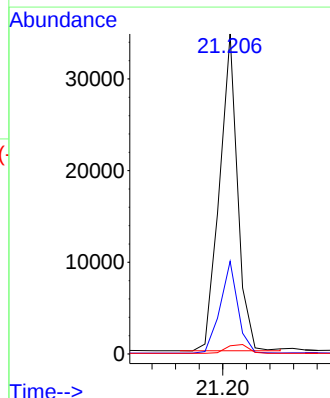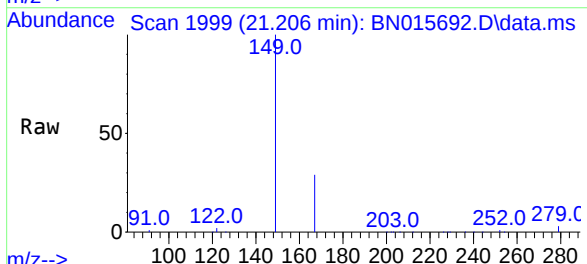







#35
Perylene-d12
Concen: 0.400 ng
RT: 23.563 min Scan# 2450
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Tgt Ion:264 Resp: 65232




Ion	Ratio	Lower	Upper
264	100		
260	24.8	19.8	29.8
265	23.8	19.0	28.6

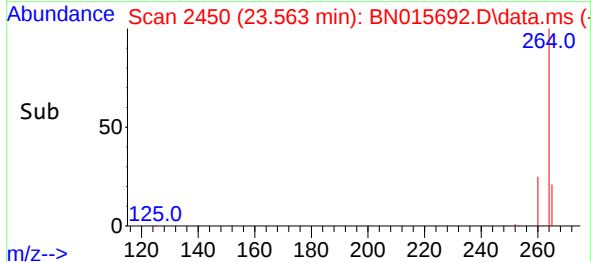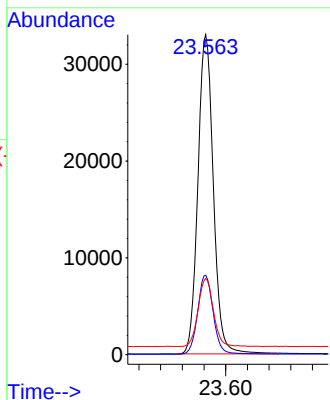


#36
Indeno(1,2,3-cd)pyrene
Concen: 0.415 ng
RT: 25.898 min Scan# 3132
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:276 Resp: 98203

Ion	Ratio	Lower	Upper
276	100		
138	28.9	23.0	34.4
277	25.0	20.0	30.0


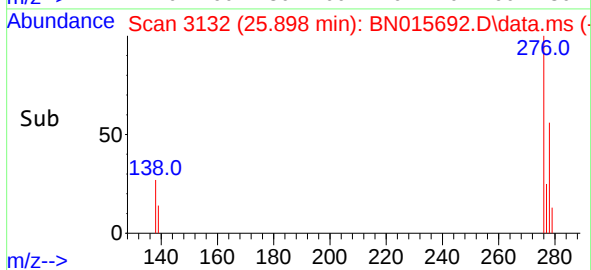
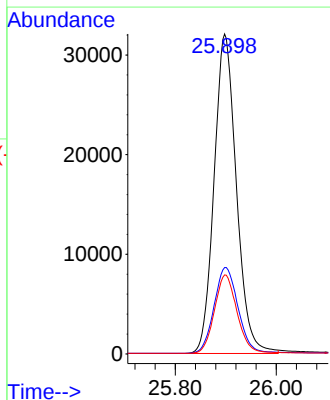





#37
Benzo(b)fluoranthene
Concen: 0.363 ng
RT: 22.872 min Scan# 2248
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:252 Resp: 89076
Ion Ratio Lower Upper
252 100
253 21.9 17.5 26.3
125 11.1 8.9 13.3

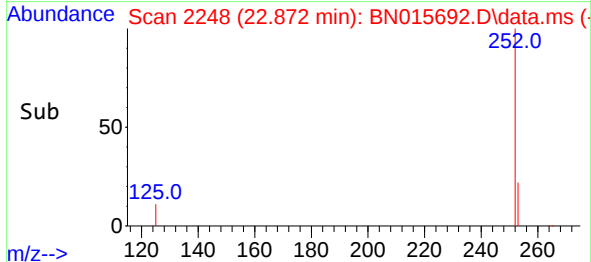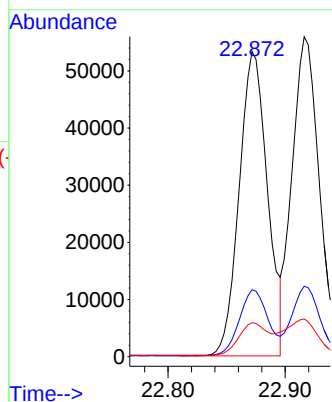

#38
Benzo(k)fluoranthene
Concen: 0.376 ng
RT: 22.916 min Scan# 2261
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:252 Resp: 92248
Ion Ratio Lower Upper
252 100
253 22.0 17.6 26.4
125 11.8 9.4 14.2


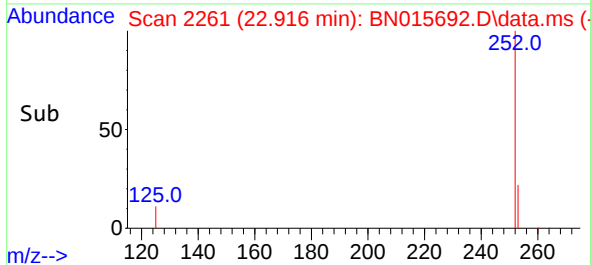

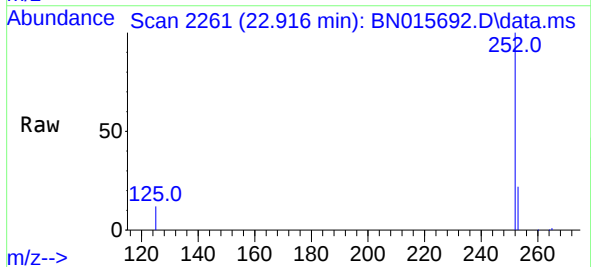




#39
Benzo(a)pyrene
Concen: 0.393 ng
RT: 23.460 min Scan# 2420
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:252 Resp: 78114
Ion Ratio Lower Upper
252 100
253 22.1 17.7 26.5
125 12.7 10.2 15.2

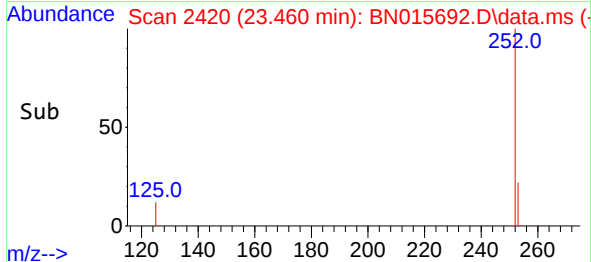

#40
Dibenzo(a,h)anthracene
Concen: 0.432 ng
RT: 25.918 min Scan# 3138
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13


Tgt Ion:278 Resp: 80327
Ion Ratio Lower Upper
278 100
139 18.9 15.1 22.7
279 23.7 19.0 28.4

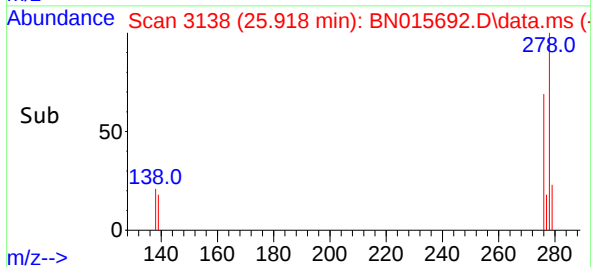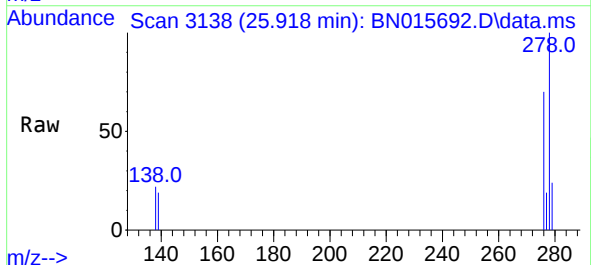

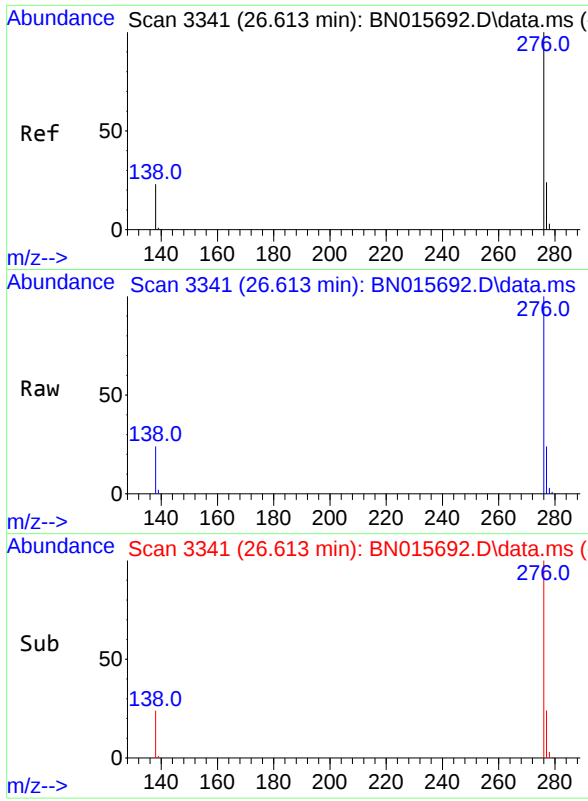

#41
Benzo(g,h,i)perylene
Concen: 0.369 ng
RT: 26.613 min Scan# 3341
Delta R.T. 0.000 min
Lab File: BN015692.D
Acq: 24 Jul 2021 18:13

Tgt Ion:	276	Resp:	79911
Ion	Ratio	Lower	Upper
276	100		
277	24.2	19.4	29.0
138	23.8	19.0	28.6

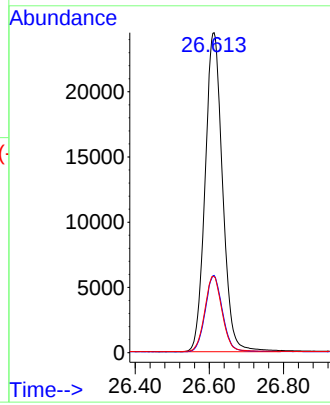

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4