

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
 Data File : BN015695.D
 Acq On : 24 Jul 2021 20:02
 Operator : CG/JU
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Jul 26 01:35:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 26 01:23:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	14221	0.400	ng	0.00
7) Naphthalene-d8	10.470	136	59214	0.400	ng	0.00
13) Acenaphthene-d10	14.319	164	32879	0.400	ng	0.00
19) Phenanthrene-d10	17.078	188	64138	0.400	ng	0.00
29) Chrysene-d12	21.280	240	62632	0.400	ng	0.00
35) Perylene-d12	23.563	264	61618	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	119169	3.482	ng	0.00
5) Phenol-d6	6.868	99	145948	3.634	ng	0.00
8) Nitrobenzene-d5	8.835	82	152827	3.683	ng	0.00
11) 2-Methylnaphthalene-d10	12.065	152	290405	3.290	ng	0.00
14) 2,4,6-Tribromophenol	15.816	330	54146	5.293	ng	0.00
15) 2-Fluorobiphenyl	12.949	172	397604	2.966	ng	0.00
27) Fluoranthene-d10	19.112	212	588940	3.441	ng	0.00
31) Terphenyl-d14	19.718	244	455505	3.056	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.225	88	13062	3.079	ng	# 87
3) n-Nitrosodimethylamine	3.567	42	36793	3.511	ng	98
6) bis(2-Chloroethyl)ether	7.126	93	125041	3.100	ng	99
9) Naphthalene	10.520	128	491886	3.130	ng	100
10) Hexachlorobutadiene	10.812	225	93670	3.136	ng	# 100
12) 2-Methylnaphthalene	12.140	142	326779	3.224	ng	100
16) Acenaphthylene	14.040	152	497377	3.622	ng	100
17) Acenaphthene	14.383	154	311825	3.267	ng	98
18) Fluorene	15.372	166	379020	3.328	ng	99
20) 4,6-Dinitro-2-methylph...	15.461	198	25341	5.819	ng	# 71
21) 4-Bromophenyl-phenylether	16.275	248	124991	3.349	ng	99
22) Hexachlorobenzene	16.384	284	129654	3.054	ng	99
23) Atrazine	16.543	200	107368	4.831	ng	97
24) Pentachlorophenol	16.725	266	60067	6.247	ng	99
25) Phenanthrene	17.115	178	607671	3.139	ng	100
26) Anthracene	17.200	178	577610	3.592	ng	100
28) Fluoranthene	19.142	202	680488	3.257	ng	100
30) Pyrene	19.509	202	706784	3.142	ng	100
32) Benzo(a)anthracene	21.259	228	699934	3.566	ng	99
33) Chrysene	21.312	228	663861	3.053	ng	99
34) Bis(2-ethylhexyl)phtha...	21.206	149	445458	5.422	ng	99
36) Indeno(1,2,3-cd)pyrene	25.897	276	753204	3.374	ng	99
37) Benzo(b)fluoranthene	22.875	252	697524	3.010	ng	100
38) Benzo(k)fluoranthene	22.919	252	686854	2.960	ng	99
39) Benzo(a)pyrene	23.464	252	640164	3.409	ng	99
40) Dibenzo(a,h)anthracene	25.918	278	614276	3.499	ng	99
41) Benzo(g,h,i)perylene	26.616	276	644489	3.153	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN072521\
Data File : BN015695.D
Acq On : 24 Jul 2021 20:02
Operator : CG/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Jul 26 01:35:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN072521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 26 01:23:47 2021
Response via : Initial Calibration




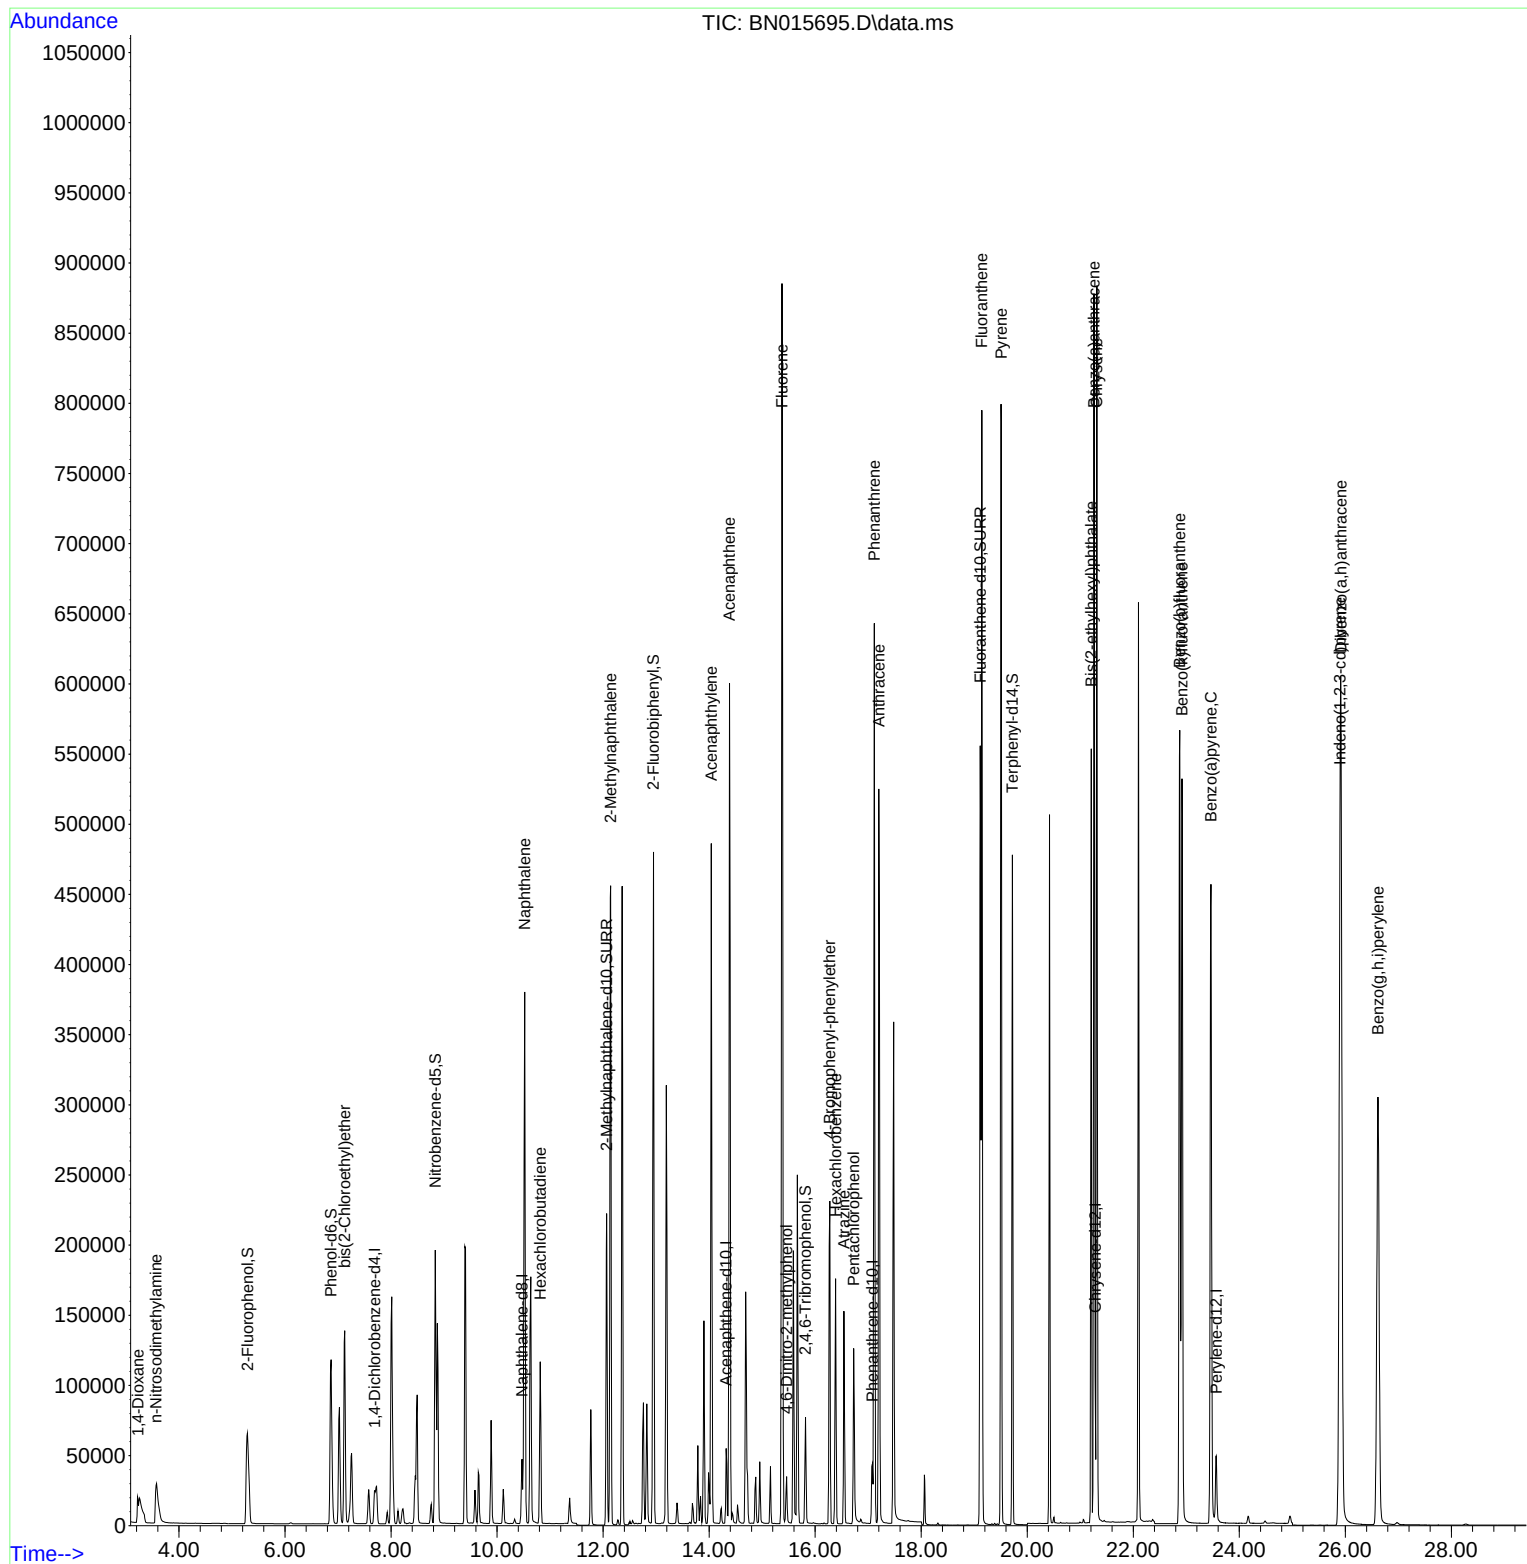




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.688 min Scan# 500
 Delta R.T. 0.000 min
 Lab File: BN015695.D
 Acq: 24 Jul 2021 20:02




Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC3.2


Tgt Ion:152 Resp: 14221
 Ion Ratio Lower Upper
 152 100
 150 158.1 125.2 187.8
 115 60.4 48.6 73.0

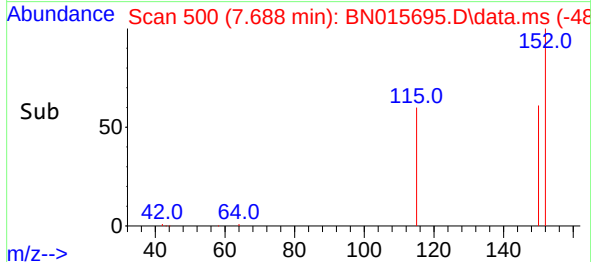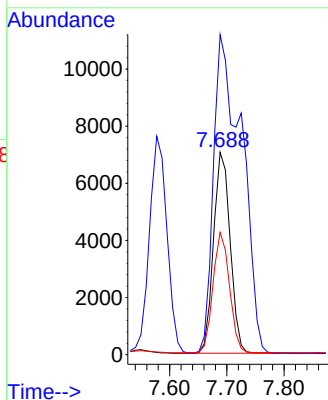

#2
 1,4-Dioxane
 Concen: 3.079 ng
 RT: 3.225 min Scan# 16
 Delta R.T. -0.000 min
 Lab File: BN015695.D
 Acq: 24 Jul 2021 20:02

Tgt Ion: 88 Resp: 13062
 Ion Ratio Lower Upper
 88 100
 43 28.3 0.0 0.0#
 58 77.7 53.8 80.6

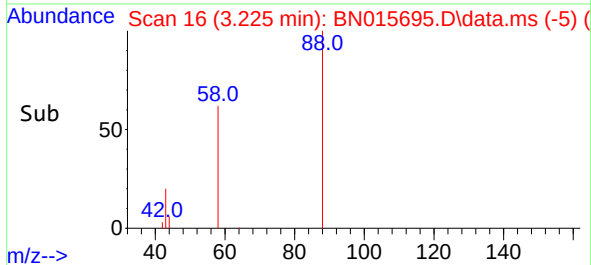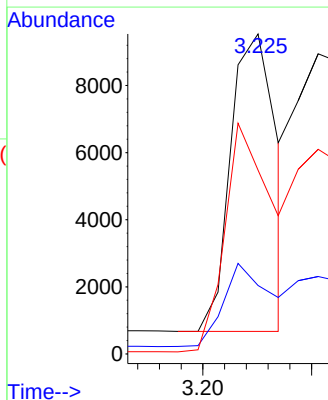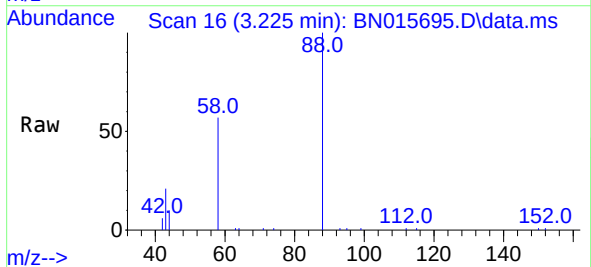







#3
n-Nitrosodimethylamine
Concen: 3.511 ng
RT: 3.567 min Scan# 53
Delta R.T. -0.019 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion: 42 Resp: 36793




Ion	Ratio	Lower	Upper
42	100		
74	155.8	126.7	190.1
44	7.0	5.8	8.8

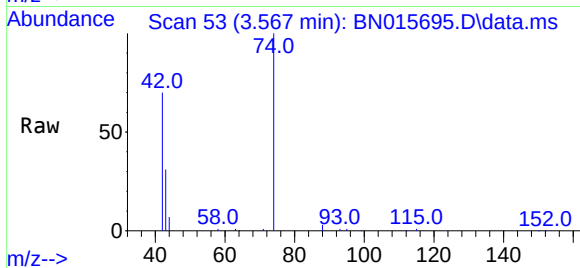


#4
2-Fluorophenol
Concen: 3.482 ng
RT: 5.291 min Scan# 240
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion: 112 Resp: 119169

Ion	Ratio	Lower	Upper
112	100		
64	55.7	44.8	67.2
63	27.7	22.2	33.4


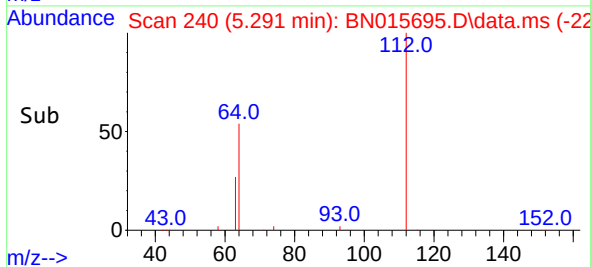

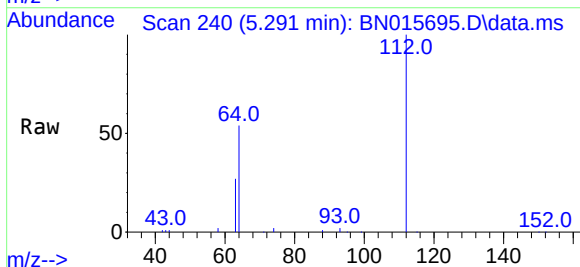




#5
Phenol-d6
Concen: 3.634 ng
RT: 6.868 min Scan# 411
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 145948
Ion Ratio Lower Upper
99 100
42 16.5 13.4 20.0
71 30.3 24.5 36.7



#6
bis(2-Chloroethyl)ether
Concen: 3.100 ng
RT: 7.126 min Scan# 439
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion: 93 Resp: 125041
Ion Ratio Lower Upper
93 100
63 74.2 59.8 89.8
95 32.8 26.4 39.6


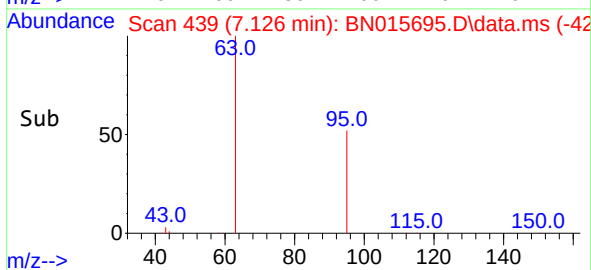






#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.470 min Scan# 738
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	59214
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	6.5	5.0	7.4
68	5.6	4.3	6.5



#8
Nitrobenzene-d5
Concen: 3.683 ng
RT: 8.835 min Scan# 609
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:	82	Resp:	152827
Ion	Ratio	Lower	Upper
82	100		
128	42.7	32.0	48.0
54	46.1	38.9	58.3

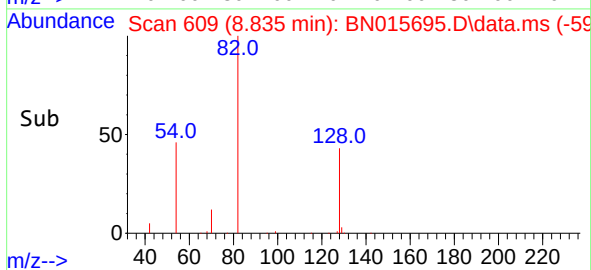







#9
Naphthalene
Concen: 3.130 ng
RT: 10.520 min Scan# 742
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:128 Resp: 491886




Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.9	13.3
127	12.8	10.4	15.6

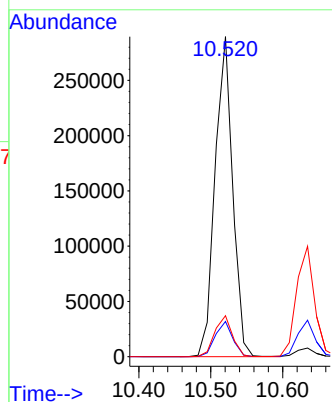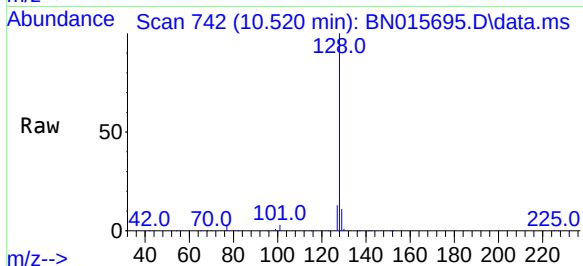


#10
Hexachlorobutadiene
Concen: 3.136 ng
RT: 10.812 min Scan# 765
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:225 Resp: 93670

Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.6	51.1	76.7


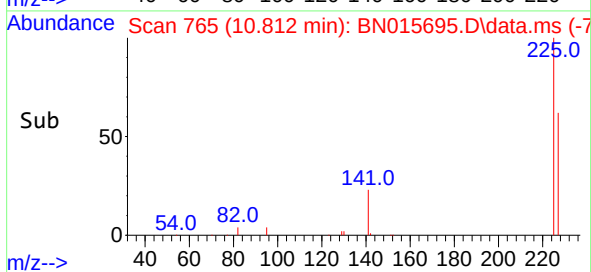

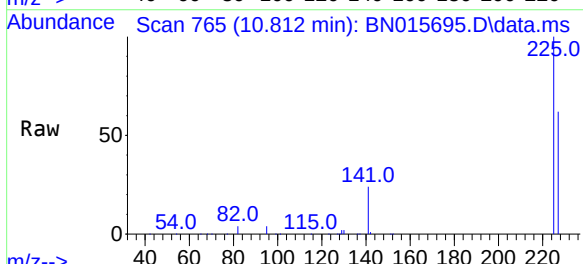


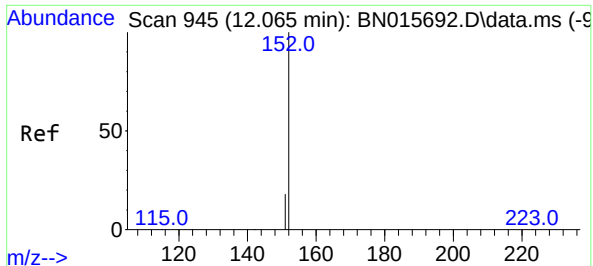

#11
2-Methylnaphthalene-d10
Concen: 3.290 ng
RT: 12.065 min Scan# 945
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 290405
Ion Ratio Lower Upper
152 100
151 20.3 16.3 24.5

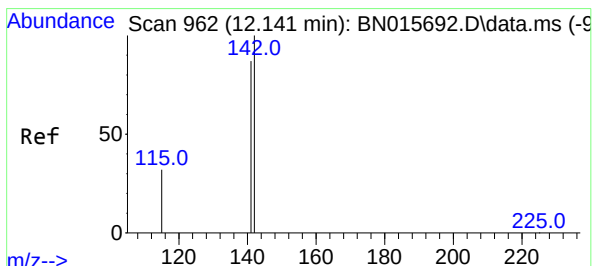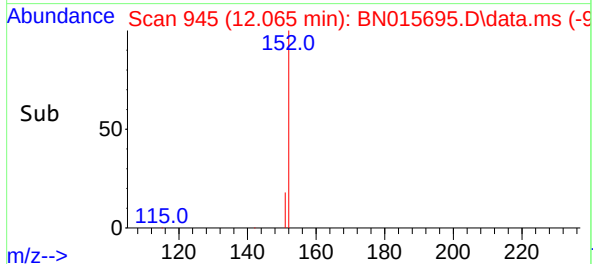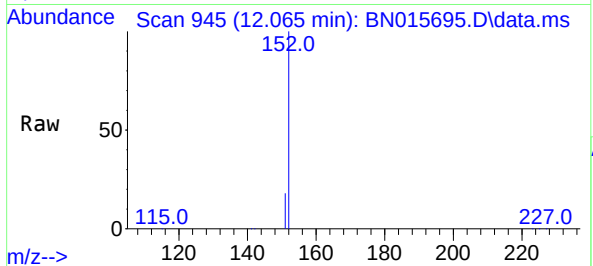

#12
2-Methylnaphthalene
Concen: 3.224 ng
RT: 12.140 min Scan# 962
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:142 Resp: 326779
Ion Ratio Lower Upper
142 100
141 87.2 69.4 104.2
115 32.3 25.9 38.9

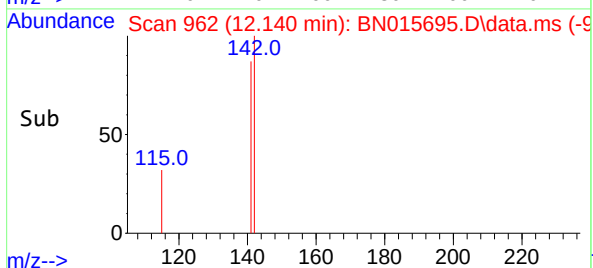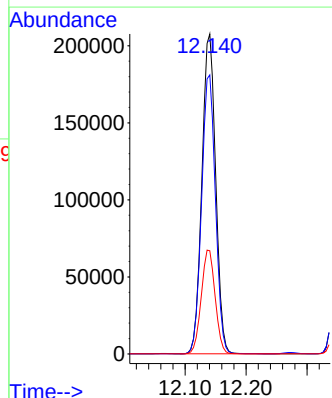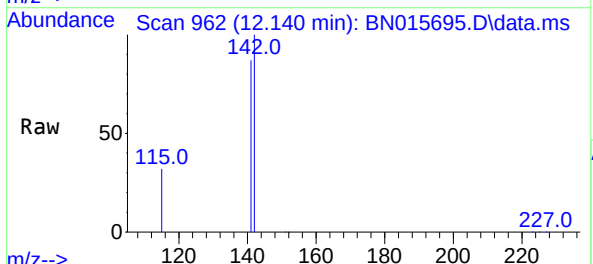







#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.319 min Scan# 1187
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:164 Resp: 32879




Ion	Ratio	Lower	Upper
164	100		
162	104.4	83.6	125.4
160	48.2	38.6	58.0




#14
2,4,6-Tribromophenol
Concen: 5.293 ng
RT: 15.816 min Scan# 1305
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:330 Resp: 54146

Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	35.5	28.5	42.7



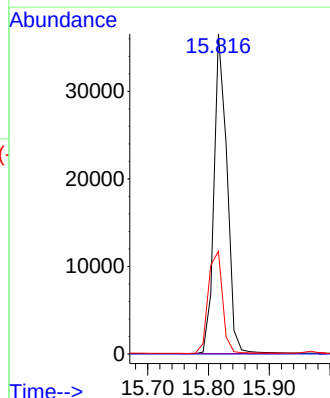





#15
2-Fluorobiphenyl
Concen: 2.966 ng
RT: 12.949 min Scan# 1079
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:172 Resp: 397604
Ion Ratio Lower Upper
172 100
171 34.0 27.4 41.0
170 22.3 17.9 26.9



#16
Acenaphthylene
Concen: 3.622 ng
RT: 14.040 min Scan# 1165
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:152 Resp: 497377
Ion Ratio Lower Upper
152 100
151 19.4 15.4 23.2
153 13.0 10.4 15.6


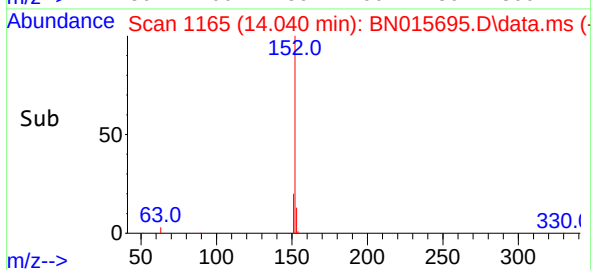




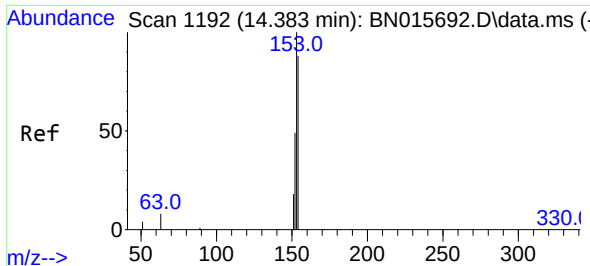

#17
Acenaphthene
Concen: 3.267 ng
RT: 14.383 min Scan# 1192
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:154 Resp: 311825
Ion Ratio Lower Upper
154 100
153 110.2 89.0 133.6
152 52.3 43.3 64.9

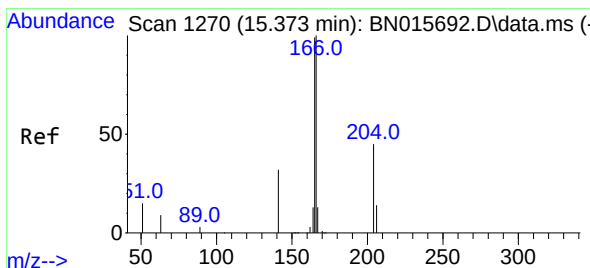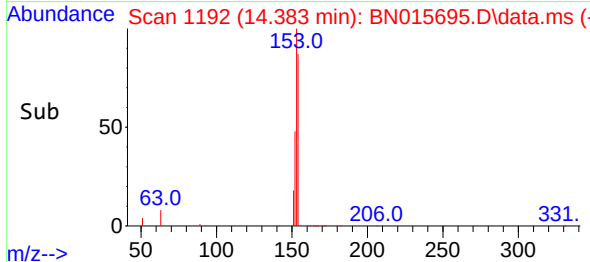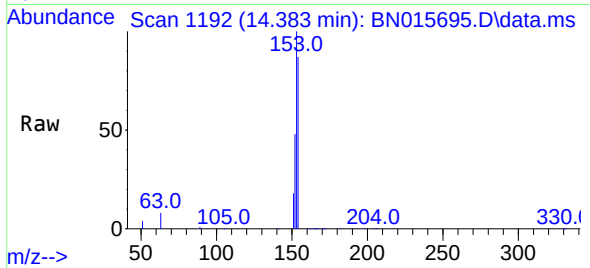

#18
Fluorene
Concen: 3.328 ng
RT: 15.372 min Scan# 1270
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:166 Resp: 379020
Ion Ratio Lower Upper
166 100
165 96.8 77.9 116.9
167 13.5 10.8 16.2


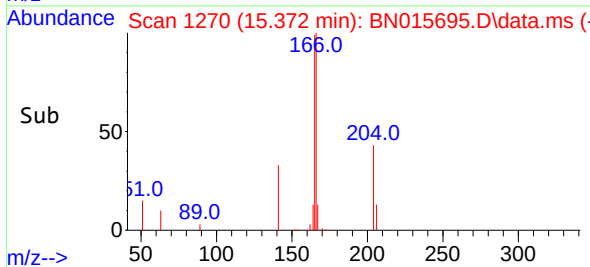

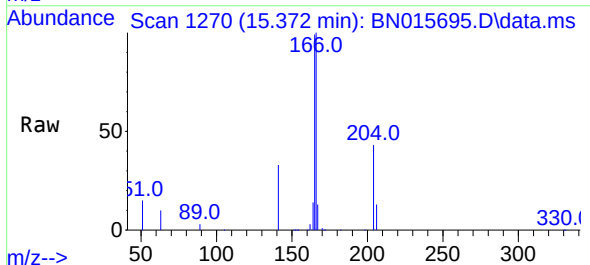




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.078 min Scan# 1408
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:188 Resp: 64138
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.8 5.3 7.9



#20
4,6-Dinitro-2-methylphenol
Concen: 5.819 ng
RT: 15.461 min Scan# 1277
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:198 Resp: 25341
Ion Ratio Lower Upper
198 100
182 7.0 16.4 24.6#
77 0.0 0.0 0.0


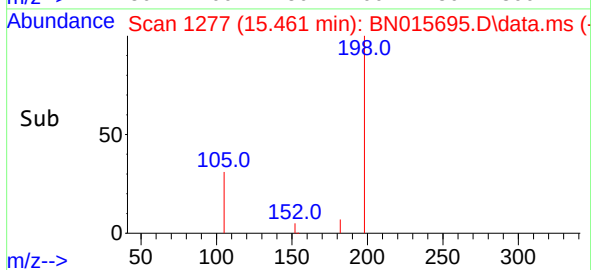




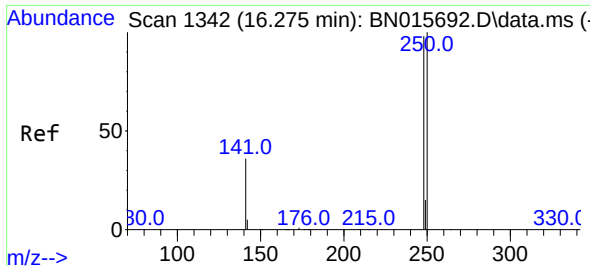

#21
4-Bromophenyl-phenylether
Concen: 3.349 ng
RT: 16.275 min Scan# 1342
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	248	Resp:	124991
Ion	Ratio	Lower	Upper
248	100		
250	101.7	81.6	122.4
141	35.5	29.4	44.0

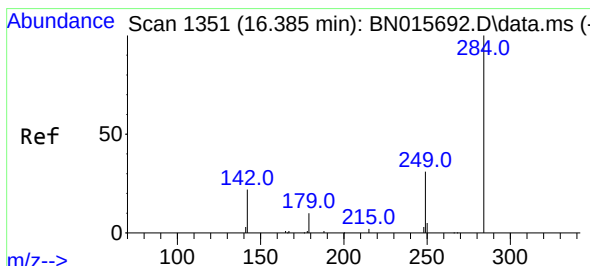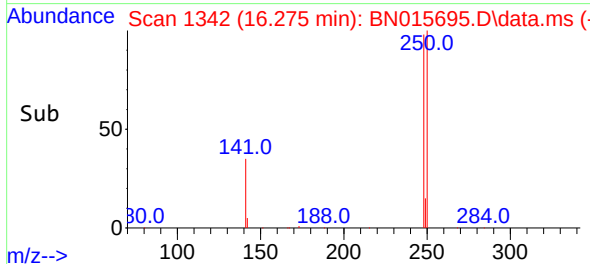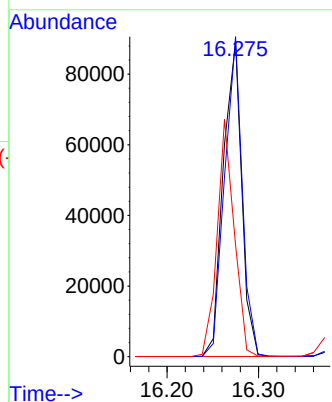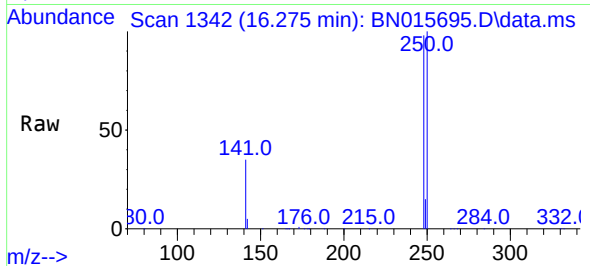

#22
Hexachlorobenzene
Concen: 3.054 ng
RT: 16.384 min Scan# 1351
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:	284	Resp:	129654
Ion	Ratio	Lower	Upper
284	100		
142	34.6	27.6	41.4
249	31.5	24.6	37.0


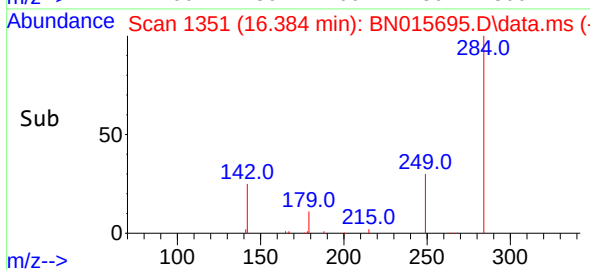
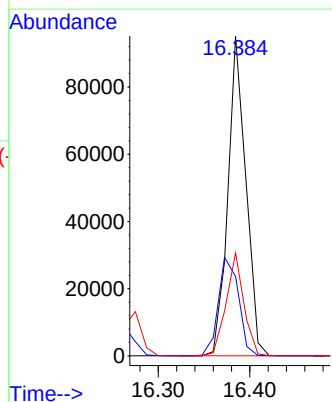
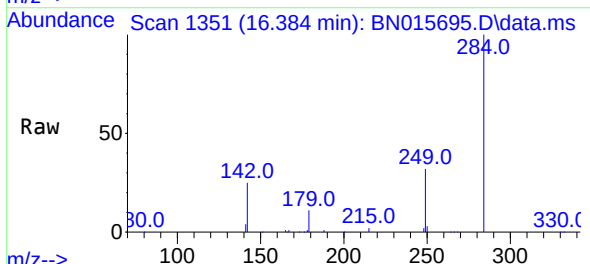


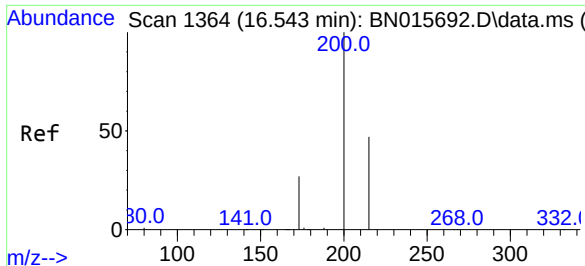

#23
Atrazine
Concen: 4.831 ng
RT: 16.543 min Scan# 1364
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:200 Resp: 107368
Ion Ratio Lower Upper
200 100
173 29.5 21.8 32.6
215 46.4 38.2 57.2

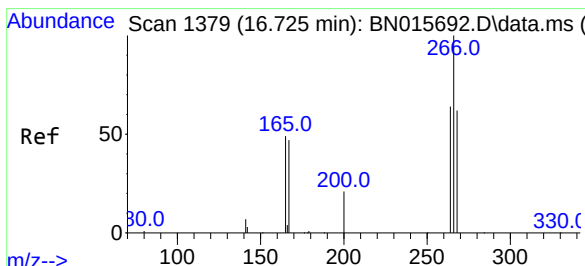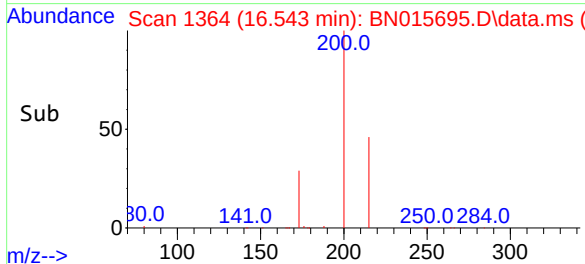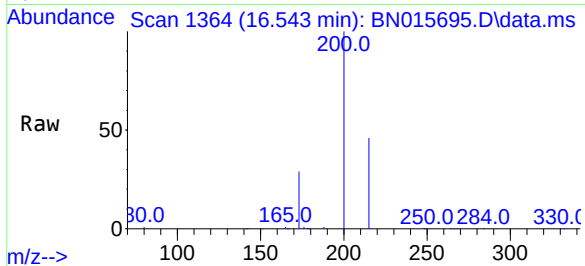

#24
Pentachlorophenol
Concen: 6.247 ng
RT: 16.725 min Scan# 1379
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:266 Resp: 60067
Ion Ratio Lower Upper
266 100
264 63.2 49.9 74.9
268 63.9 50.8 76.2


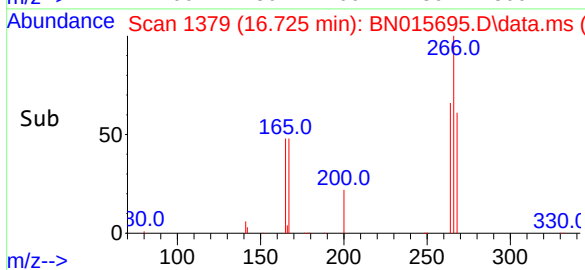

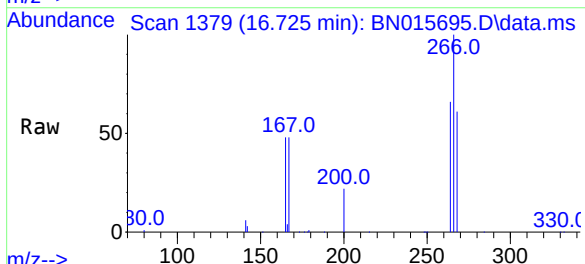




#25
Phenanthrene
Concen: 3.139 ng
RT: 17.115 min Scan# 1411
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:178 Resp: 607671
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.3 12.4 18.6

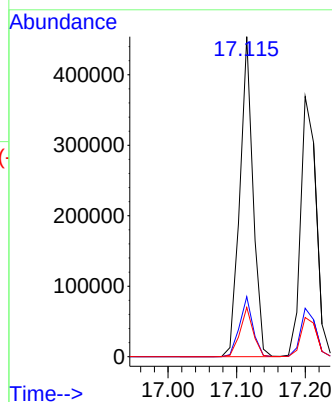

#26
Anthracene
Concen: 3.592 ng
RT: 17.200 min Scan# 1418
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:178 Resp: 577610
Ion Ratio Lower Upper
178 100
176 18.1 14.6 21.8
179 15.4 12.2 18.2


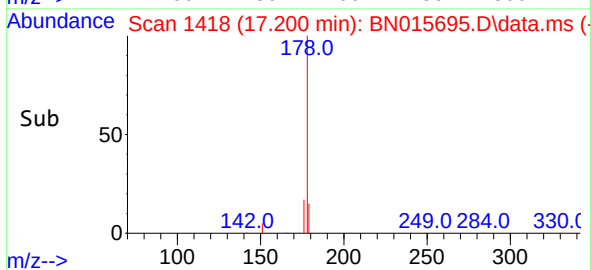






#27
Fluoranthene-d10
Concen: 3.441 ng
RT: 19.112 min Scan# 1706
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:212 Resp: 588940
Ion Ratio Lower Upper
212 100
106 14.5 11.5 17.3
104 7.9 6.3 9.5

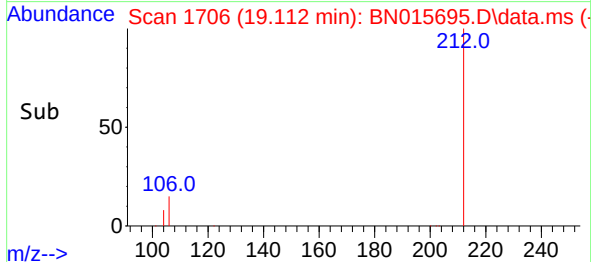

#28
Fluoranthene
Concen: 3.257 ng
RT: 19.142 min Scan# 1712
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:202 Resp: 680488
Ion Ratio Lower Upper
202 100
101 11.9 9.4 14.2
203 17.4 13.8 20.8


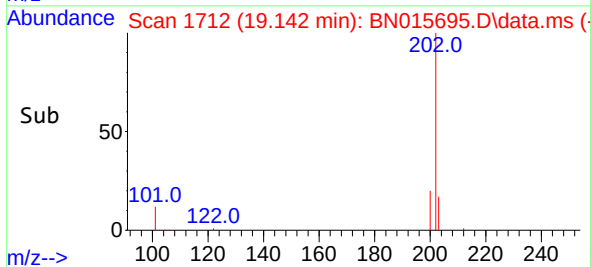

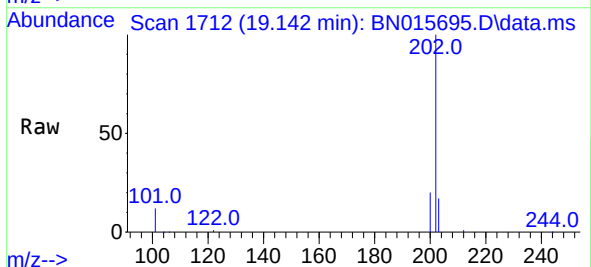




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.280 min Scan# 2006
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:240 Resp: 62632
Ion Ratio Lower Upper
240 100
120 6.3 4.9 7.3
236 25.5 20.4 30.6



#30
Pyrene
Concen: 3.142 ng
RT: 19.509 min Scan# 1786
Delta R.T. 0.005 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:202 Resp: 706784
Ion Ratio Lower Upper
202 100
200 20.7 16.4 24.6
203 17.6 13.9 20.9


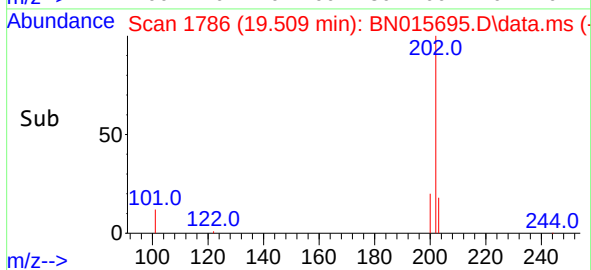






#31
Terphenyl-d14
Concen: 3.056 ng
RT: 19.718 min Scan# 1828
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:244 Resp: 455505
Ion Ratio Lower Upper
244 100
212 7.8 6.2 9.2
122 14.0 10.9 16.3

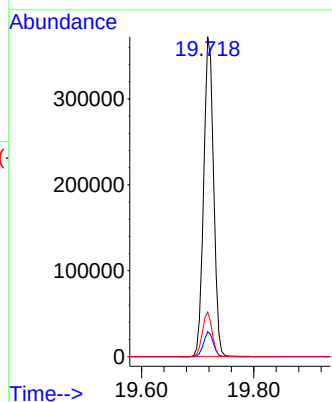

#32
Benzo(a)anthracene
Concen: 3.566 ng
RT: 21.259 min Scan# 2004
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:228 Resp: 699934
Ion Ratio Lower Upper
228 100
226 27.1 21.2 31.8
229 19.6 15.5 23.3






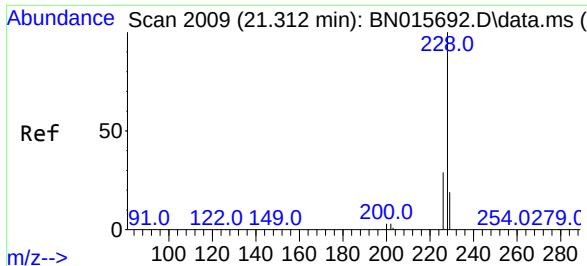


#33
Chrysene
Concen: 3.053 ng
RT: 21.312 min Scan# 2009
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:228 Resp: 663861




Ion	Ratio	Lower	Upper
228	100		
226	29.8	23.4	35.0
229	19.7	15.5	23.3

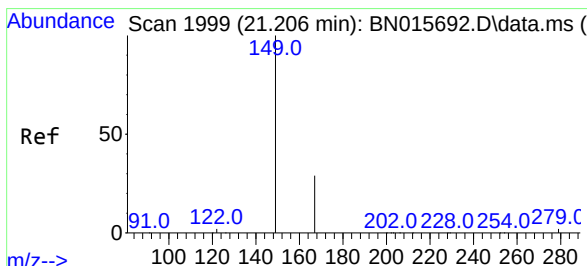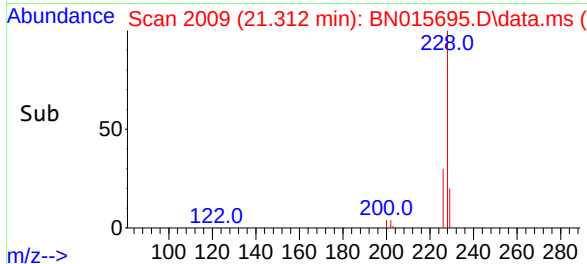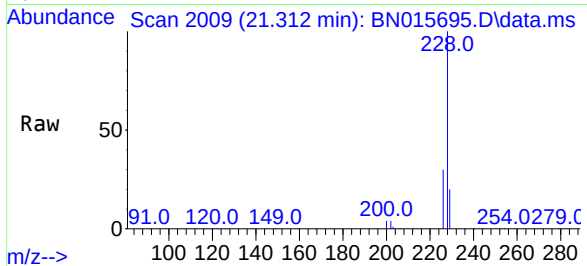


#34
Bis(2-ethylhexyl)phthalate
Concen: 5.422 ng
RT: 21.206 min Scan# 1999
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:149 Resp: 445458

Ion	Ratio	Lower	Upper
149	100		
167	28.6	22.6	34.0
279	3.7	2.8	4.2

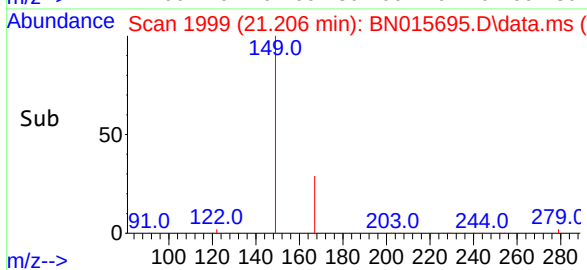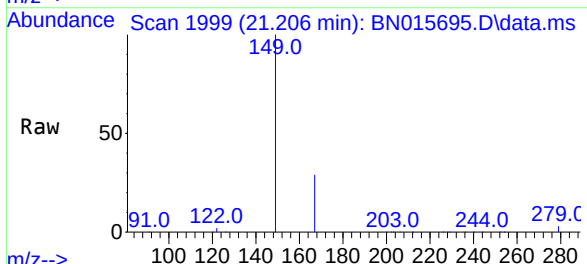







#35
Perylene-d12
Concen: 0.400 ng
RT: 23.563 min Scan# 2450
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:264 Resp: 61618




Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.8	29.8
265	23.2	19.0	28.6

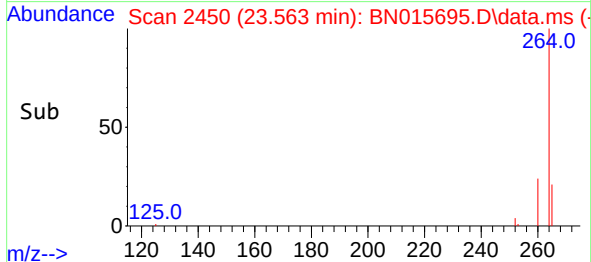


#36
Indeno(1,2,3-cd)pyrene
Concen: 3.374 ng
RT: 25.897 min Scan# 3132
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:276 Resp: 753204

Ion	Ratio	Lower	Upper
276	100		
138	27.8	23.0	34.4
277	25.1	20.0	30.0


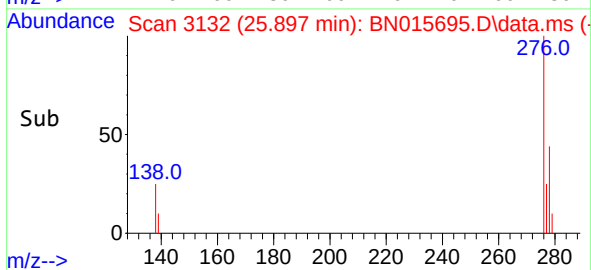






#37
Benzo(b)fluoranthene
Concen: 3.010 ng
RT: 22.875 min Scan# 2249
Delta R.T. 0.003 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 697524
Ion Ratio Lower Upper
252 100
253 21.9 17.5 26.3
125 10.7 8.9 13.3

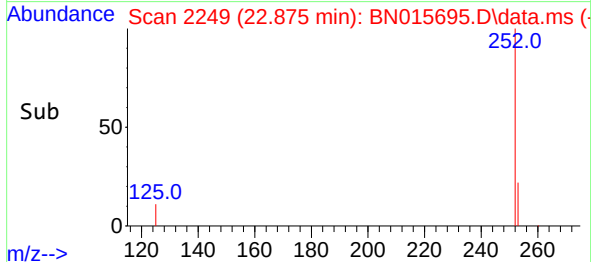

#38
Benzo(k)fluoranthene
Concen: 2.960 ng
RT: 22.919 min Scan# 2262
Delta R.T. 0.003 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02


Tgt Ion:252 Resp: 686854
Ion Ratio Lower Upper
252 100
253 21.9 17.6 26.4
125 10.7 9.4 14.2

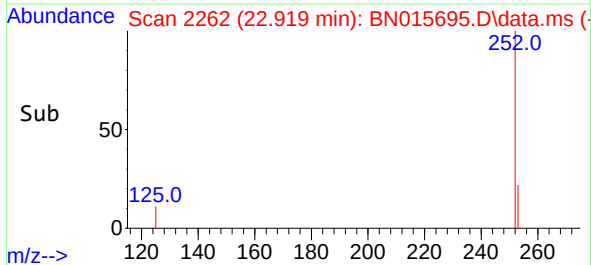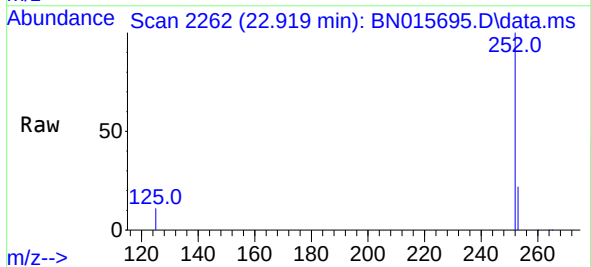






#39
Benzo(a)pyrene
Concen: 3.409 ng
RT: 23.464 min Scan# 2421
Delta R.T. 0.003 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2







Tgt Ion:252 Resp: 640164
Ion Ratio Lower Upper
252 100
253 21.9 17.7 26.5
125 11.9 10.2 15.2

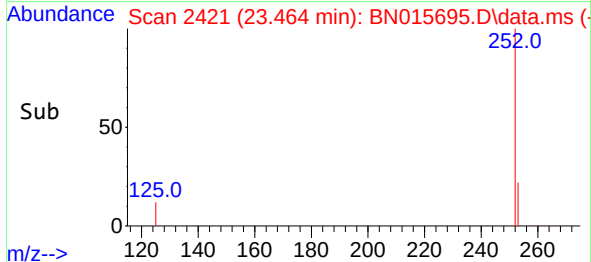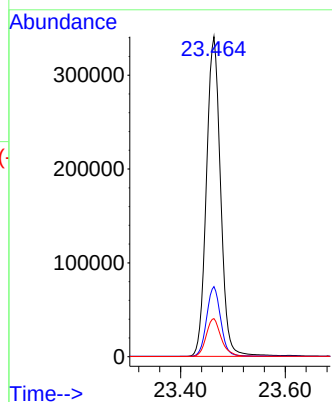

#40
Dibenzo(a,h)anthracene
Concen: 3.499 ng
RT: 25.918 min Scan# 3138
Delta R.T. -0.000 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Tgt Ion:278 Resp: 614276
Ion Ratio Lower Upper
278 100
139 18.4 15.1 22.7
279 23.4 19.0 28.4

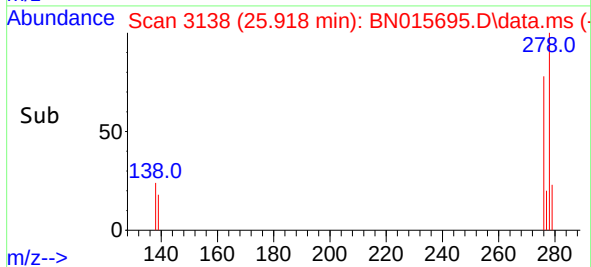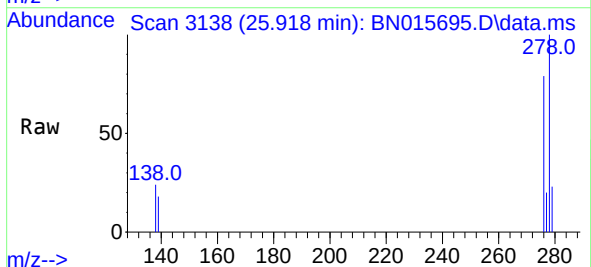

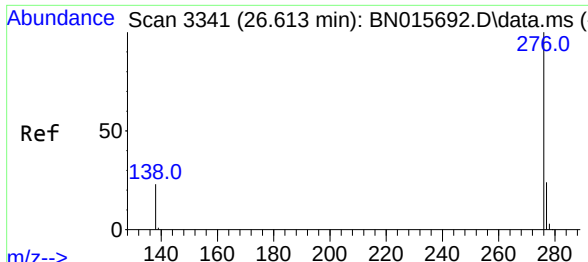

#41
Benzo(g,h,i)perylene
Concen: 3.153 ng
RT: 26.616 min Scan# 3342
Delta R.T. 0.003 min
Lab File: BN015695.D
Acq: 24 Jul 2021 20:02

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:276 Resp: 644489
Ion Ratio Lower Upper
276 100
277 23.6 19.4 29.0
138 23.7 19.0 28.6

